

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
 Data File : PL083248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2023 15:13
 Operator : AR\AJ
 Sample : 03039-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB31A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/07/2023
 Supervised By :Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 20:57:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	2.633	30999998	28787445	10.548	11.089
28)	SA Decachlor...	8.732	7.737	23564865	26458581	11.236	10.641
Target Compounds							
12)	B 4,4'-DDE	5.943	5.062	1090058	817725	0.395	0.337m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
Data File : PL083248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2023 15:13
Operator : AR\AJ
Sample : 03039-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB31A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/07/2023
Supervised By : Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 20:57:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

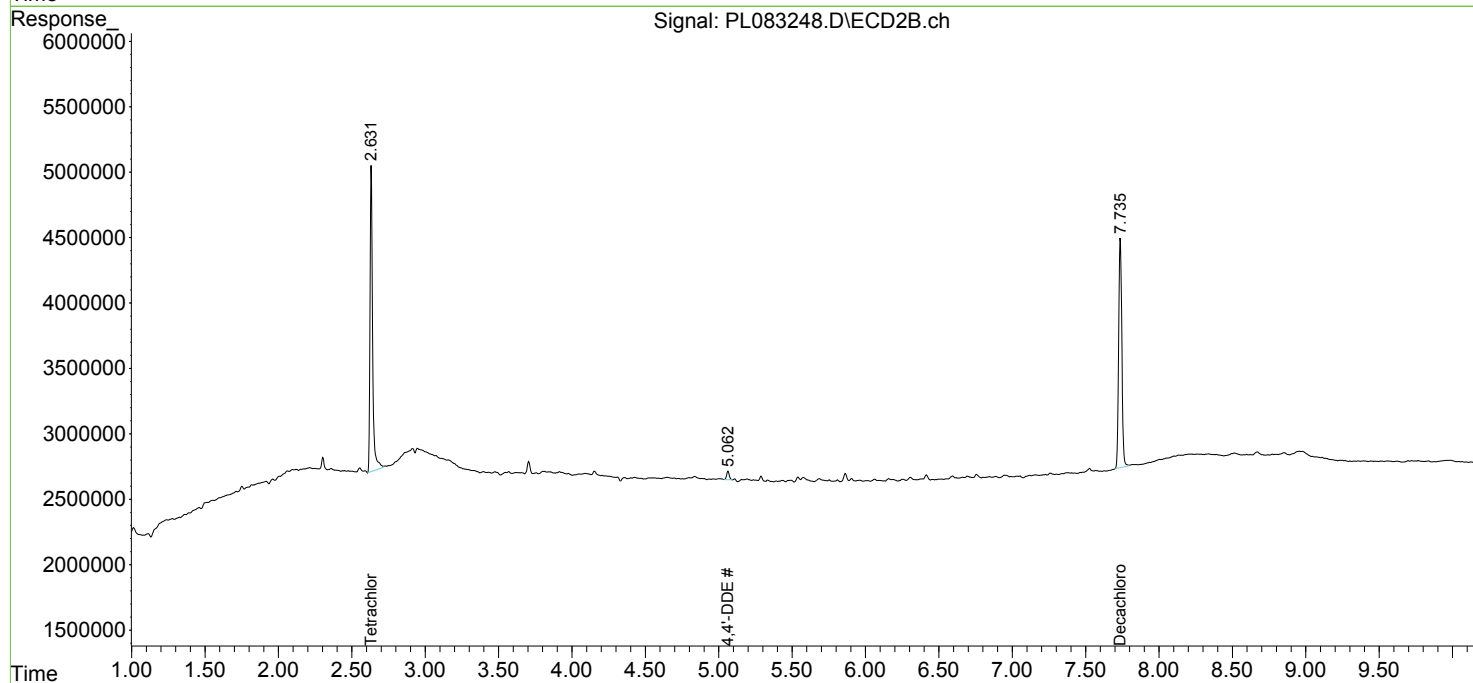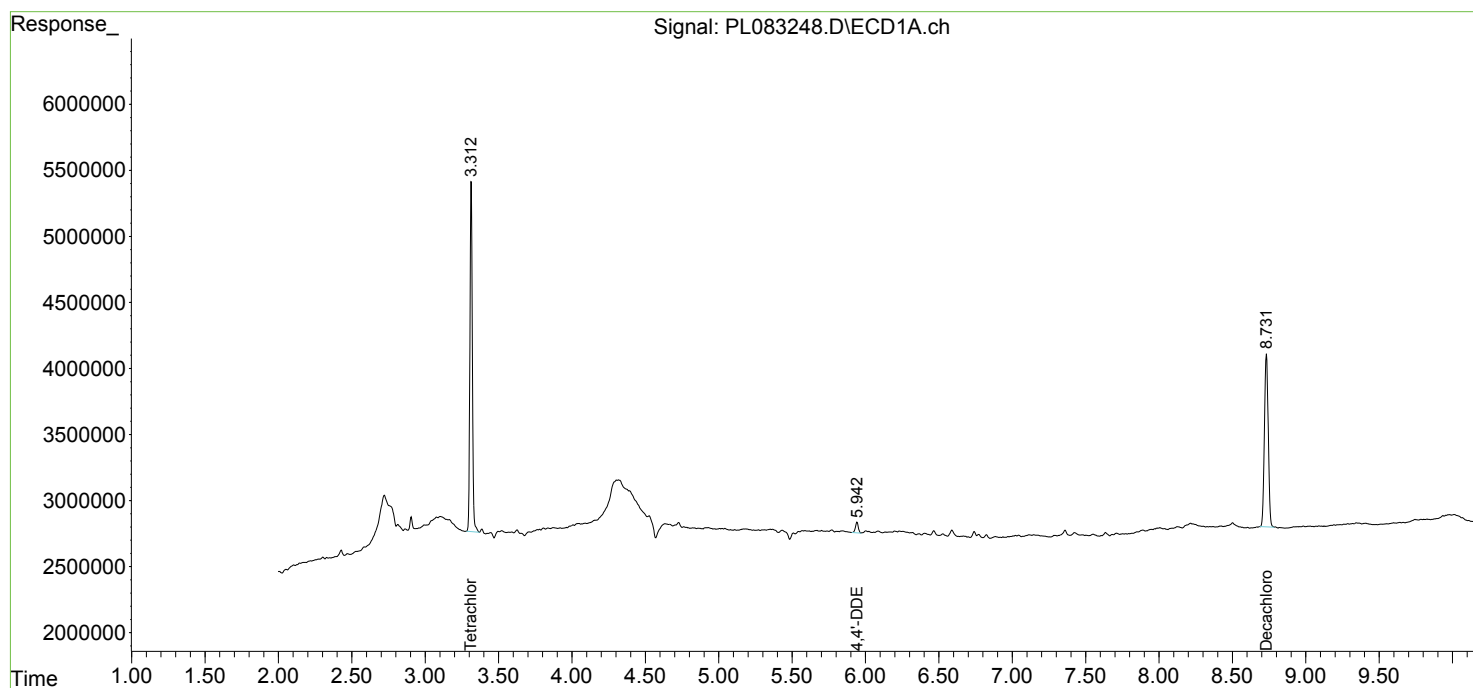

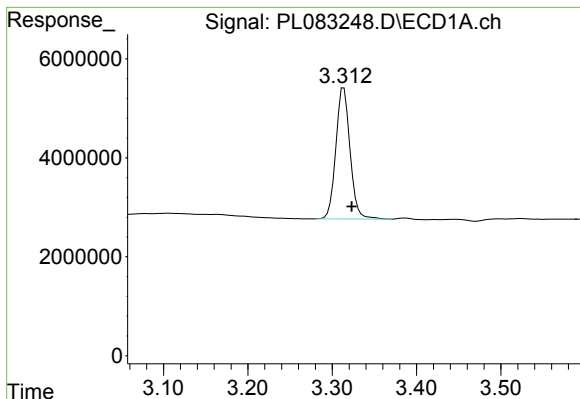


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.009 min
Response: 30999998
Conc: 10.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB31A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

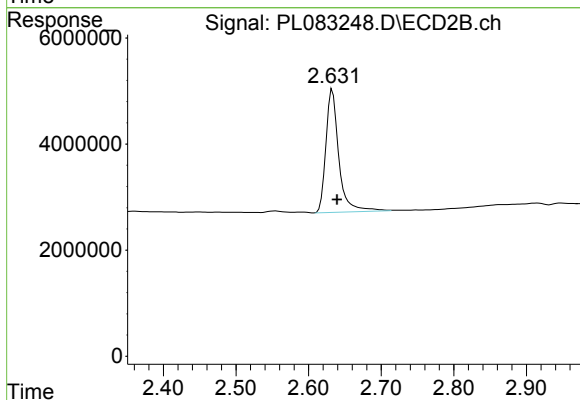


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: -0.006 min
Response: 28787445
Conc: 11.09 ng/ml

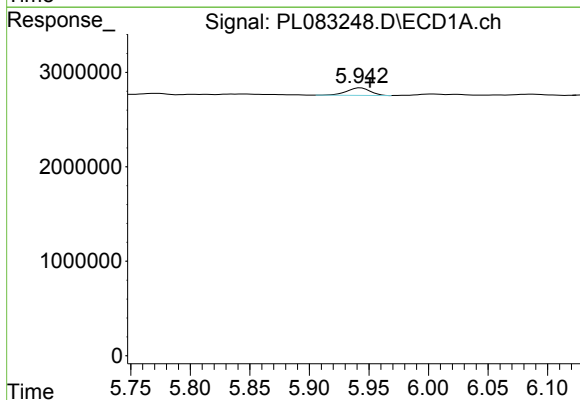


#12 4,4'-DDE

R.T.: 5.943 min
Delta R.T.: -0.008 min
Response: 1090058
Conc: 0.40 ng/ml

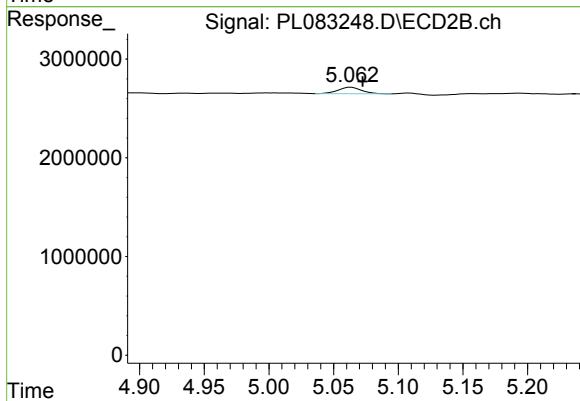

#12 4,4'-DDE

R.T.: 5.062 min
Delta R.T.: -0.010 min
Response: 817725
Conc: 0.34 ng/ml m

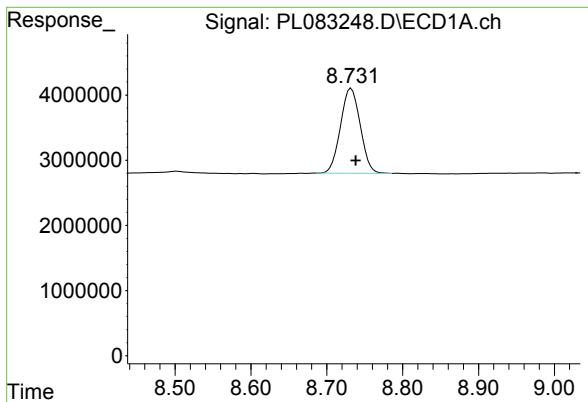


#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.006 min
Response: 23564865
Conc: 11.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB31A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

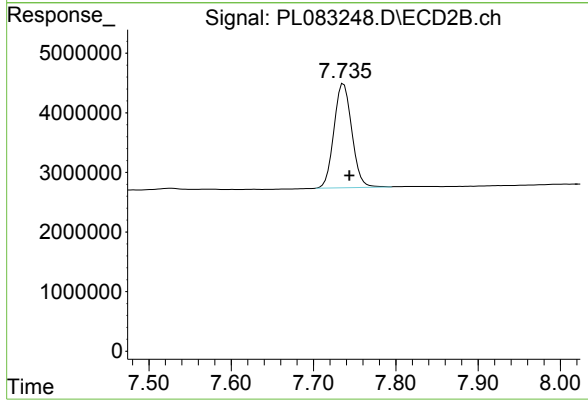

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.007 min
Response: 26458581
Conc: 10.64 ng/ml