

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
 Data File : PL083266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2023 19:53
 Operator : AR\AJ
 Sample : 03046-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3-11-15

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/07/2023
 Supervised By : Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 21:15:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.312	2.633	38940398	43449965	13.249m	16.737 #
28) SA Decachlor...	8.731	7.738	38559441	41970835	18.385m	16.879

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060623\
Data File : PL083266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2023 19:53
Operator : AR\AJ
Sample : 03046-13
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-3-11-15


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/07/2023
Supervised By : Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 21:15:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

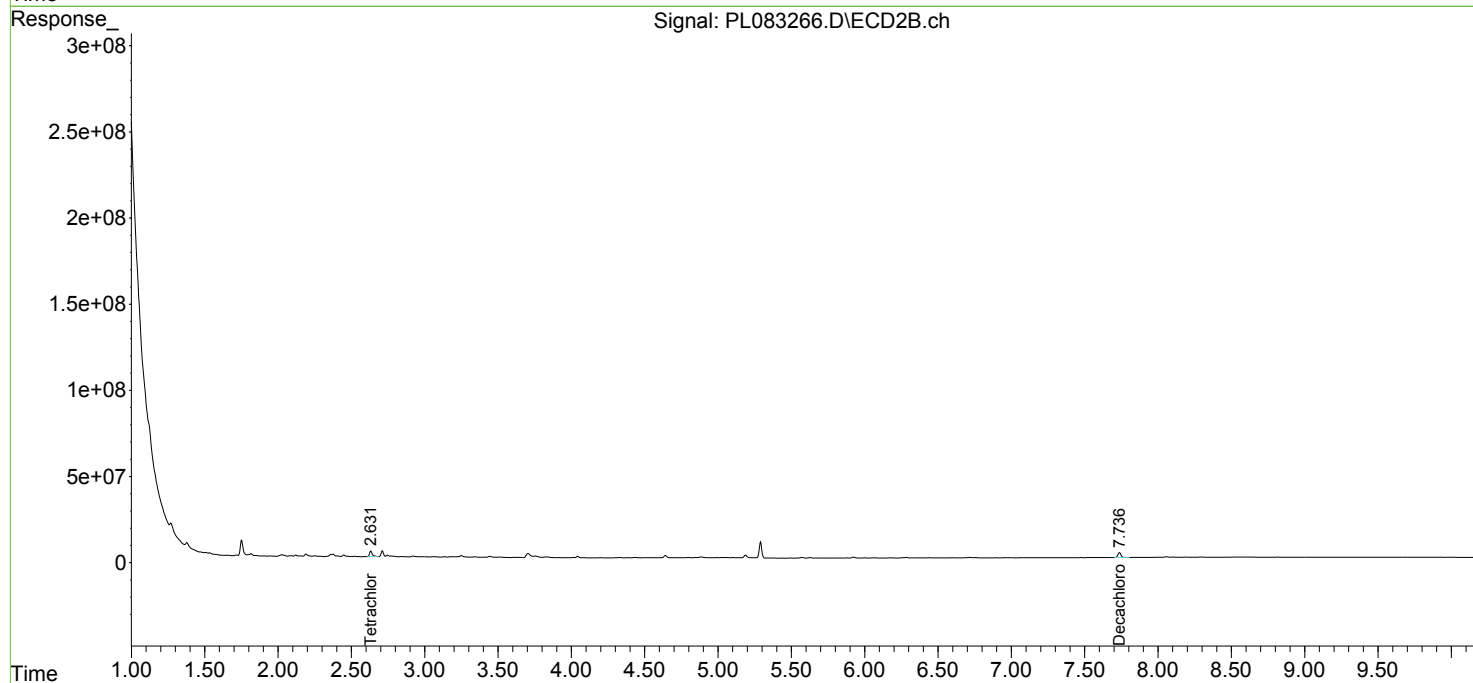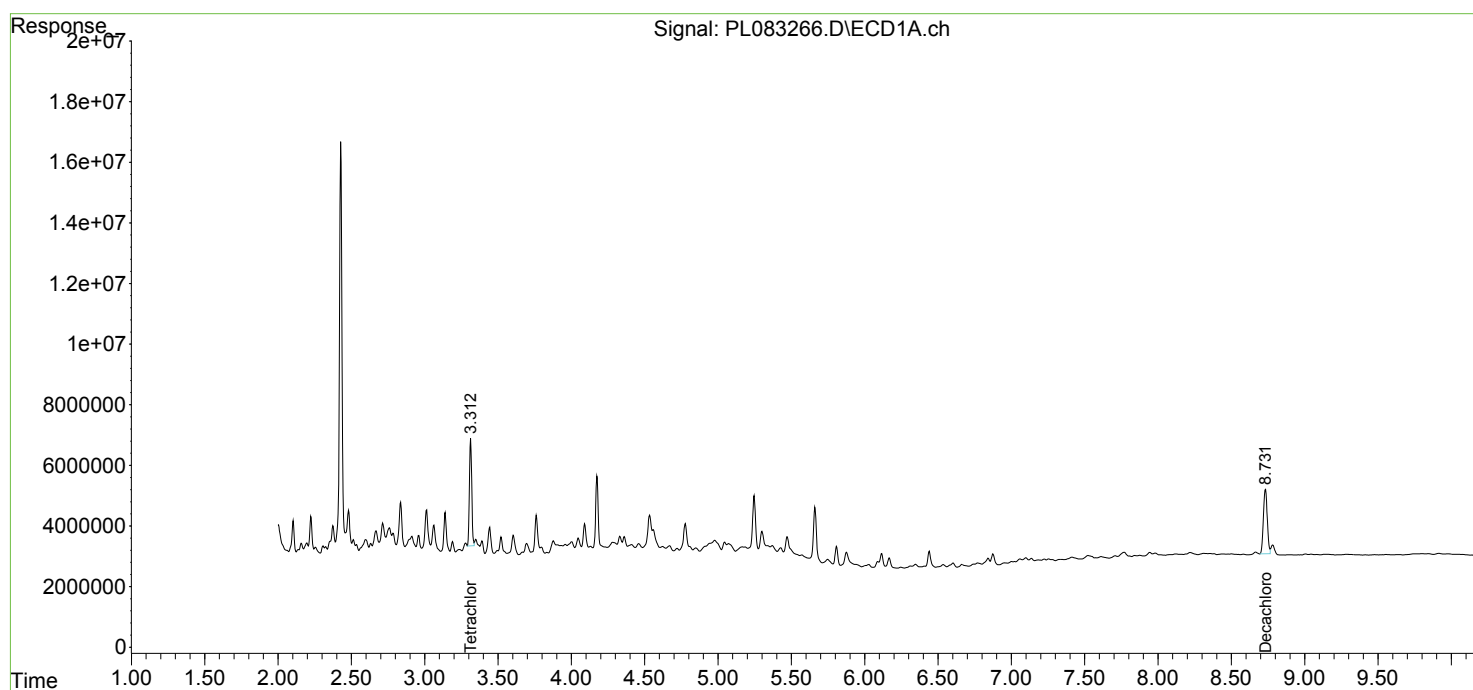

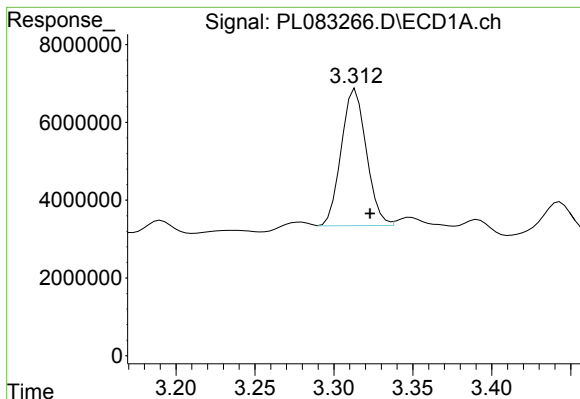


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.011 min
Response: 38940398
Conc: 13.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3-11-15


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

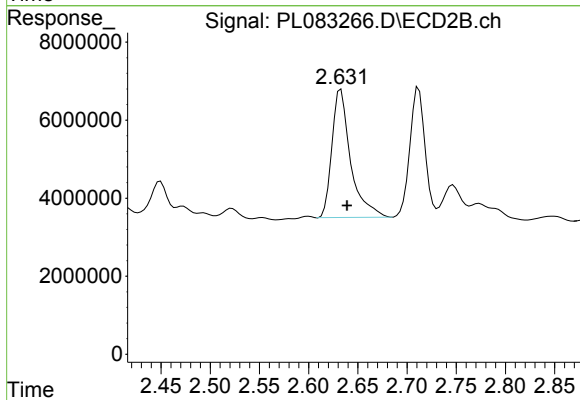


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: -0.006 min
Response: 43449965
Conc: 16.74 ng/ml

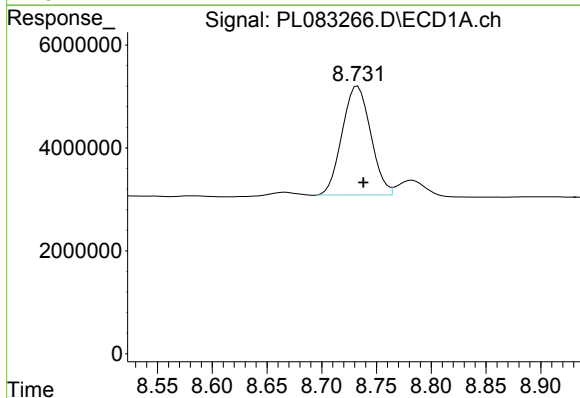

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: -0.007 min
Response: 38559441
Conc: 18.39 ng/ml m

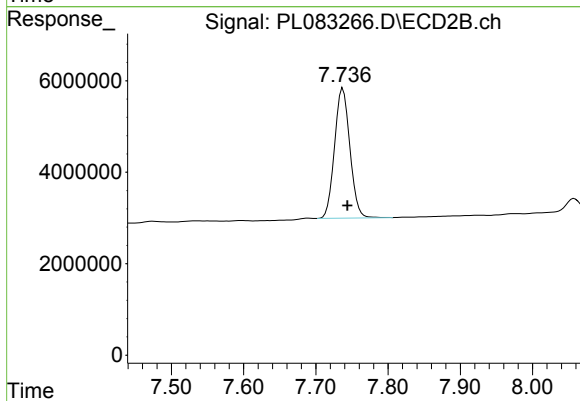

#28 Decachlorobiphenyl

R.T.: 7.738 min
Delta R.T.: -0.006 min
Response: 41970835
Conc: 16.88 ng/ml