

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 08:57
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:18:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.466f	0.000	30787	0	0.075	N.D. #
Target Compounds						
4) MA Heptachlor	5.997f	0.000	634529	0	1.208	N.D. #
6) B beta-BHC	5.997	0.000	634529	0	2.382	N.D. #
19) B Endosulfa...	0.000	9.553f	0	271833	N.D.	0.437 #
21) B Endrin ke...	0.000	10.034	0	360172	N.D.	0.497 #
22) Mirex	9.300	0.000	61755	0	0.107	N.D. #
24) Chlordane-2	6.495	0.000	666922	0	30.519	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 08:57
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:18:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

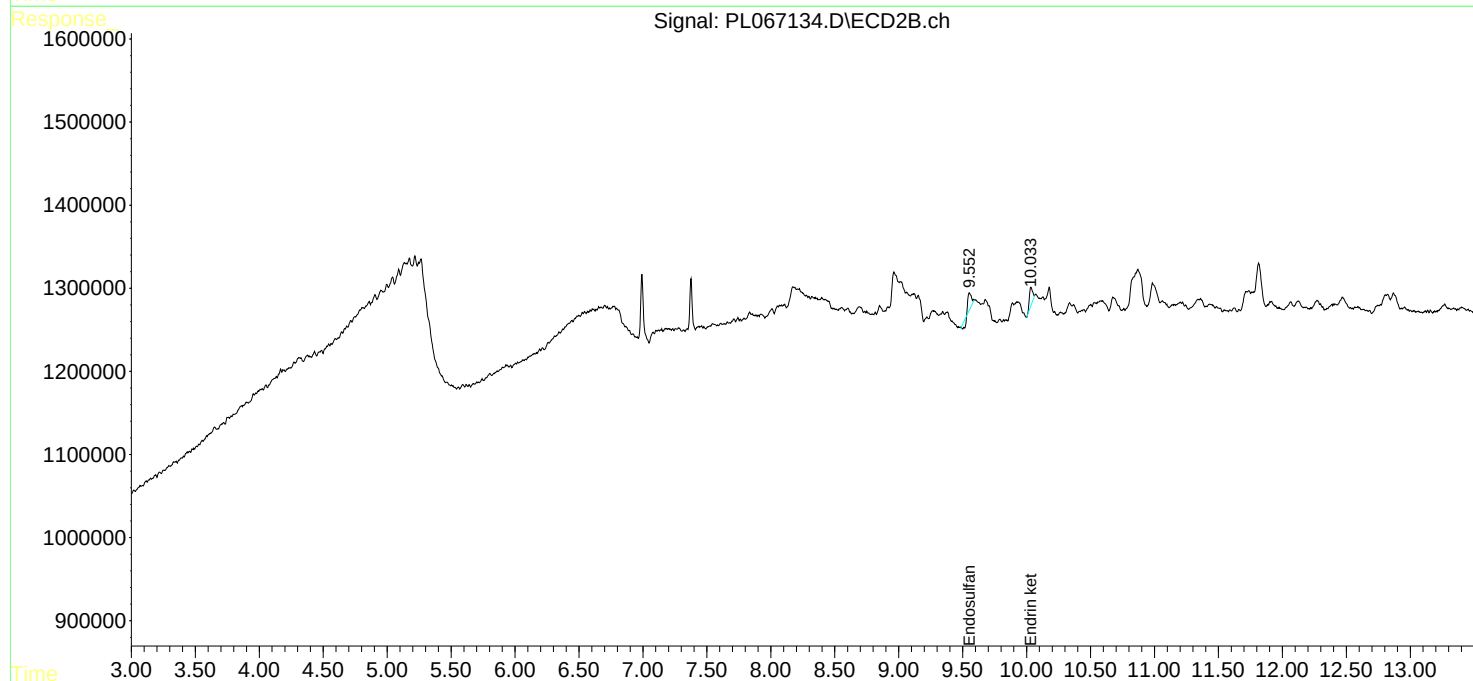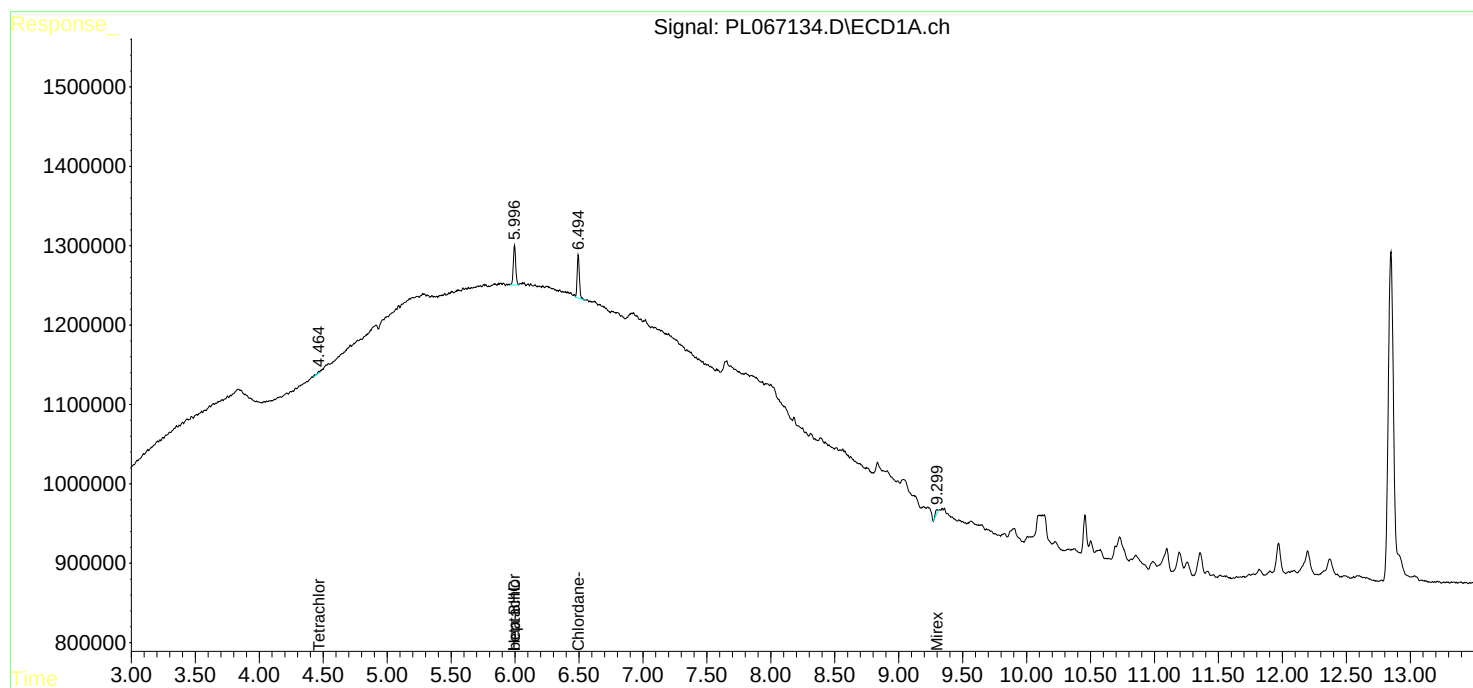


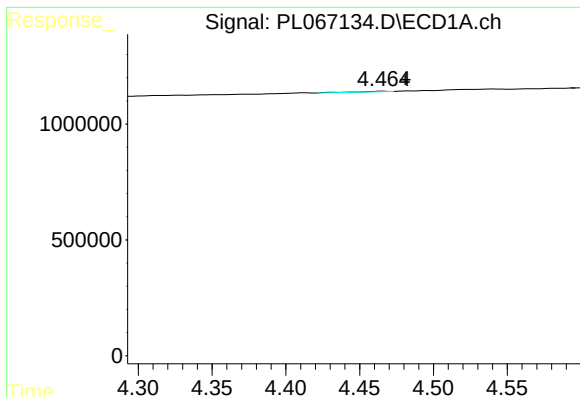

#1 Tetrachloro-m-xylene


R.T.: 4.466 min
Delta R.T.: -0.015 min
Response: 30787
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

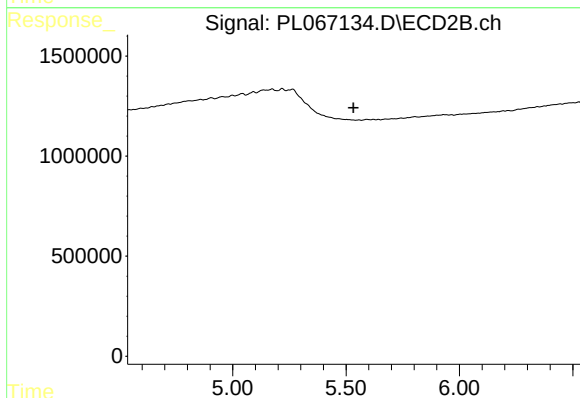


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

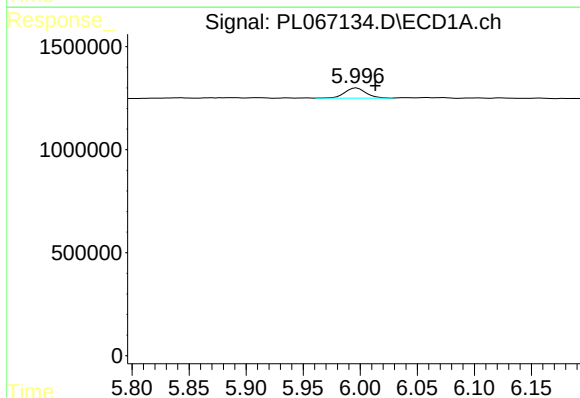


#4 Heptachlor

R.T.: 5.997 min
Delta R.T.: -0.016 min
Response: 634529
Conc: 1.21 ng/ml

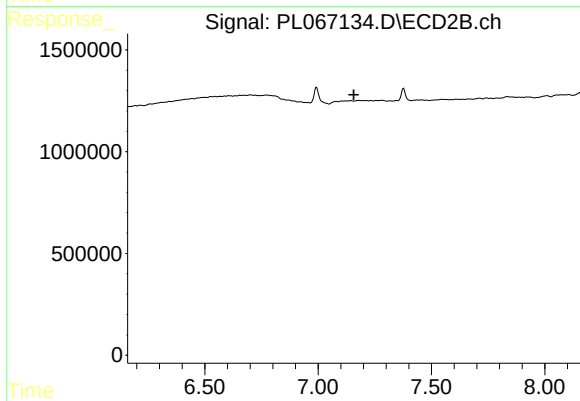

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

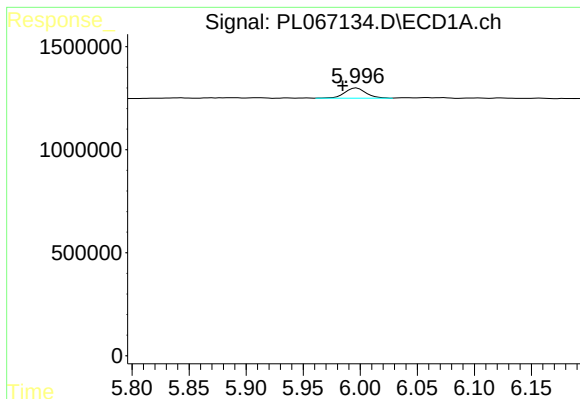

#6 beta-BHC


R.T.: 5.997 min
Delta R.T.: 0.012 min
Response: 634529
Conc: 2.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

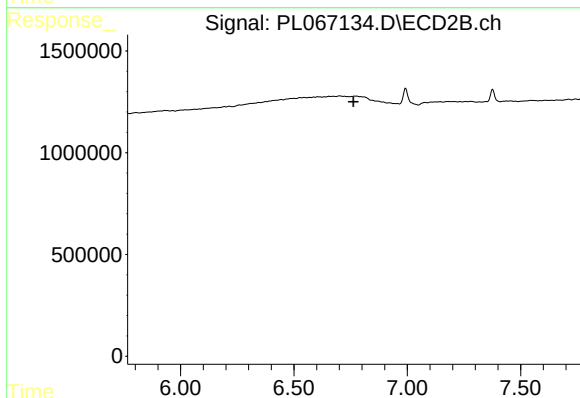


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

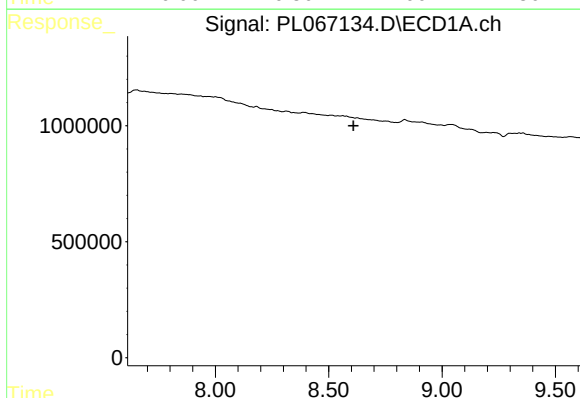


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.610 min
Response: 0
Conc: N.D.

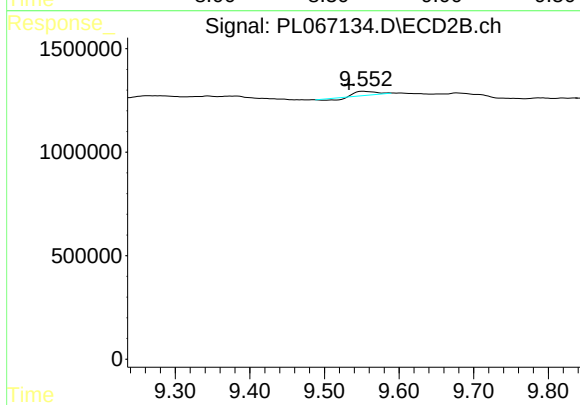

#19 Endosulfan Sulfate


R.T.: 9.553 min
Delta R.T.: 0.020 min
Response: 271833
Conc: 0.44 ng/ml

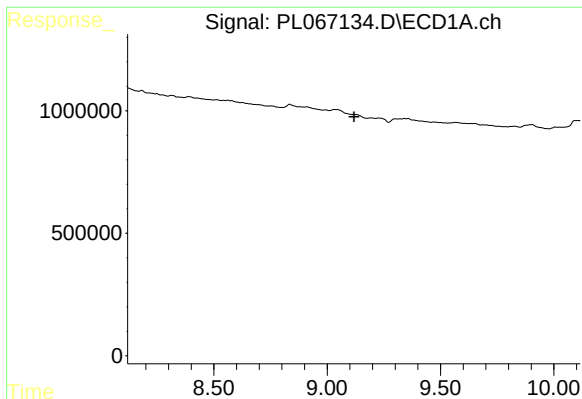

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

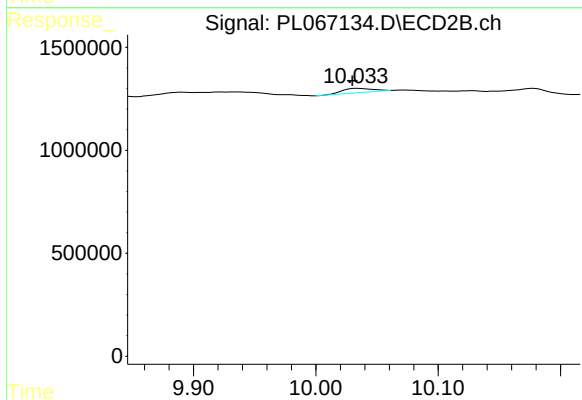


#21 Endrin ketone

R.T.: 10.034 min
Delta R.T.: 0.005 min
Response: 360172
Conc: 0.50 ng/ml

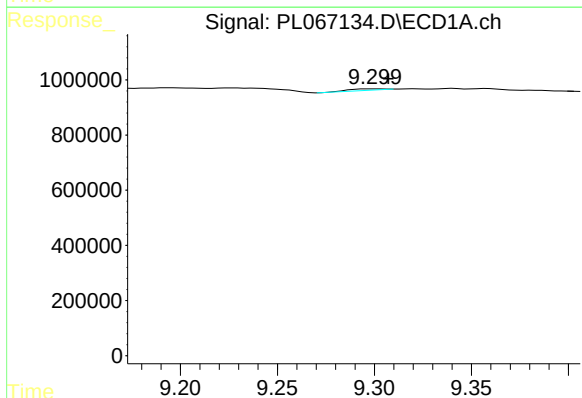


#22 Mirex

R.T.: 9.300 min
Delta R.T.: -0.007 min
Response: 61755
Conc: 0.11 ng/ml

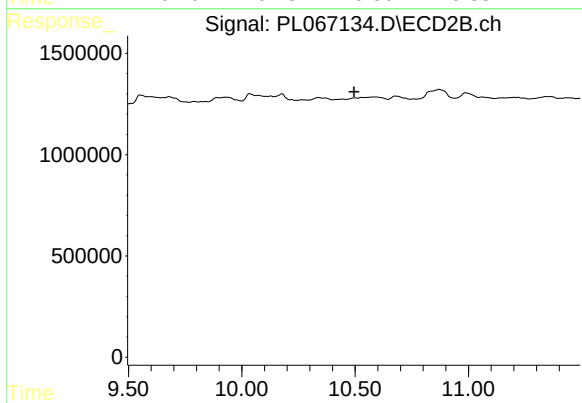

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.496 min
Response: 0
Conc: N.D.

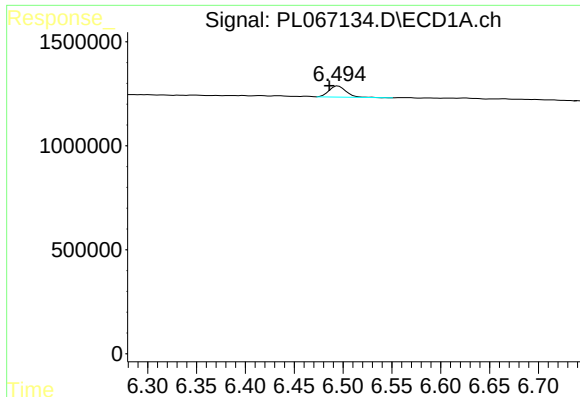

#24 Chlordane-2


R.T.: 6.495 min
Delta R.T.: 0.009 min
Response: 666922
Conc: 30.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

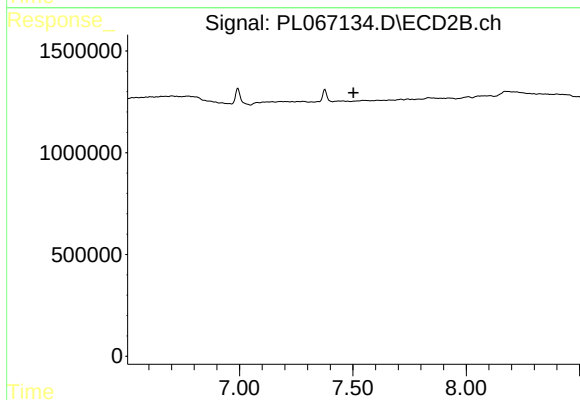


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

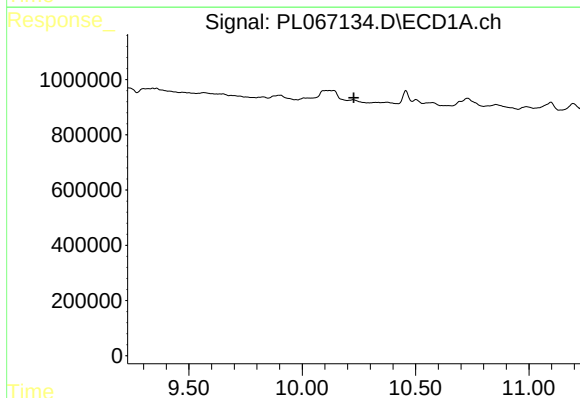

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.228 min
Response: 0
Conc: N.D.

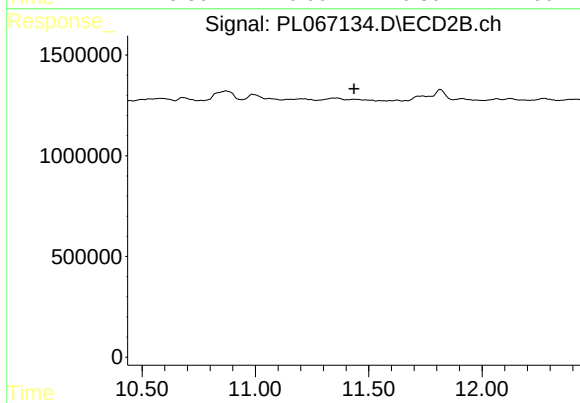

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.435 min
Response: 0
Conc: N.D.