

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 12:33
 Operator : AR\AJ
 Sample : PS136872BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB136872BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:19:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	9046153	15654411	22.091	24.199
28)	SA Decachlor...	10.222	11.427	13560655	19073865	20.971	22.861
Target Compounds							
6)	B beta-BHC	5.965f	0.000	478555	0	1.797	N.D. #
7)	B delta-BHC	0.000	7.001f	0	1498717	N.D.	1.974 #
15)	B Endosulfa...	8.176f	9.177f	2100496	463790	4.054	0.752 #
24)	Chlordane-2	6.484	0.000	1523110	0	69.700	N.D. #
27)	Chlordane-5	8.176f	0.000	2100496	0	111.321	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 12:33
Operator : AR\AJ
Sample : PS136872BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB136872BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:19:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

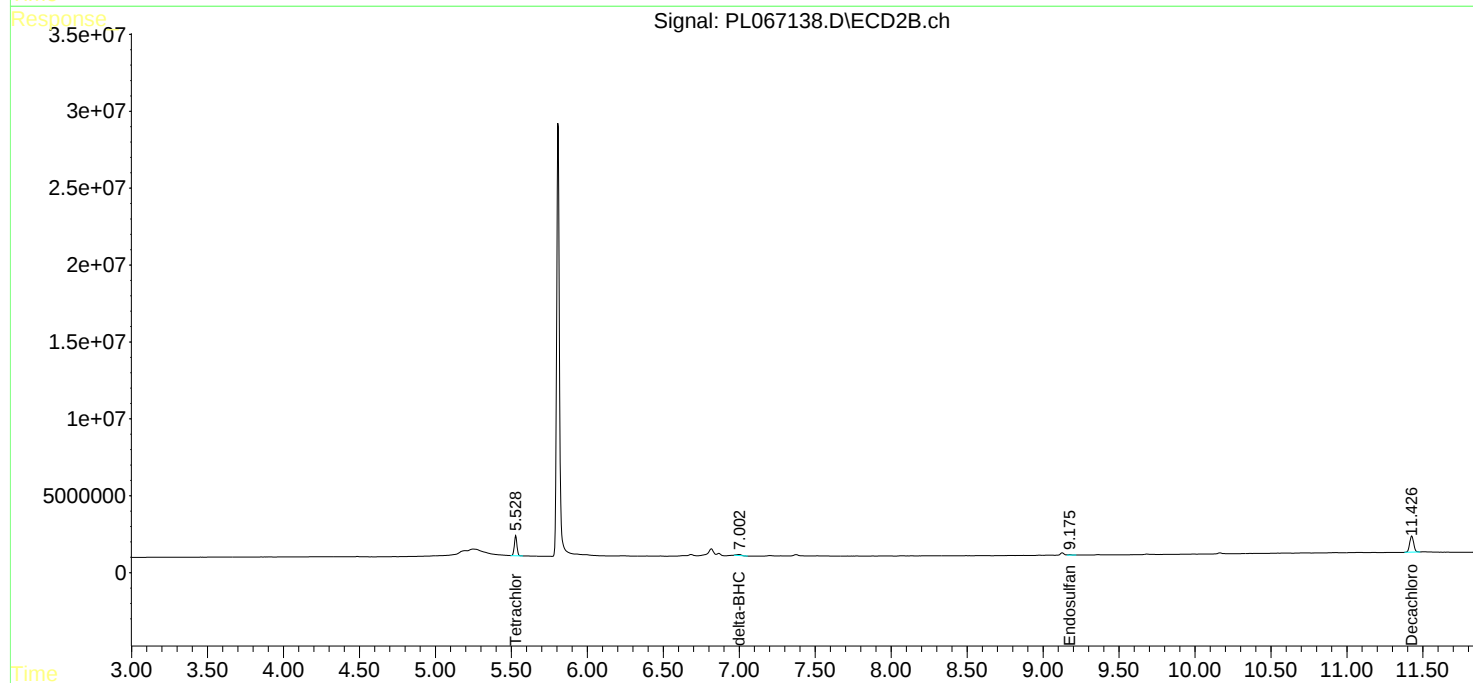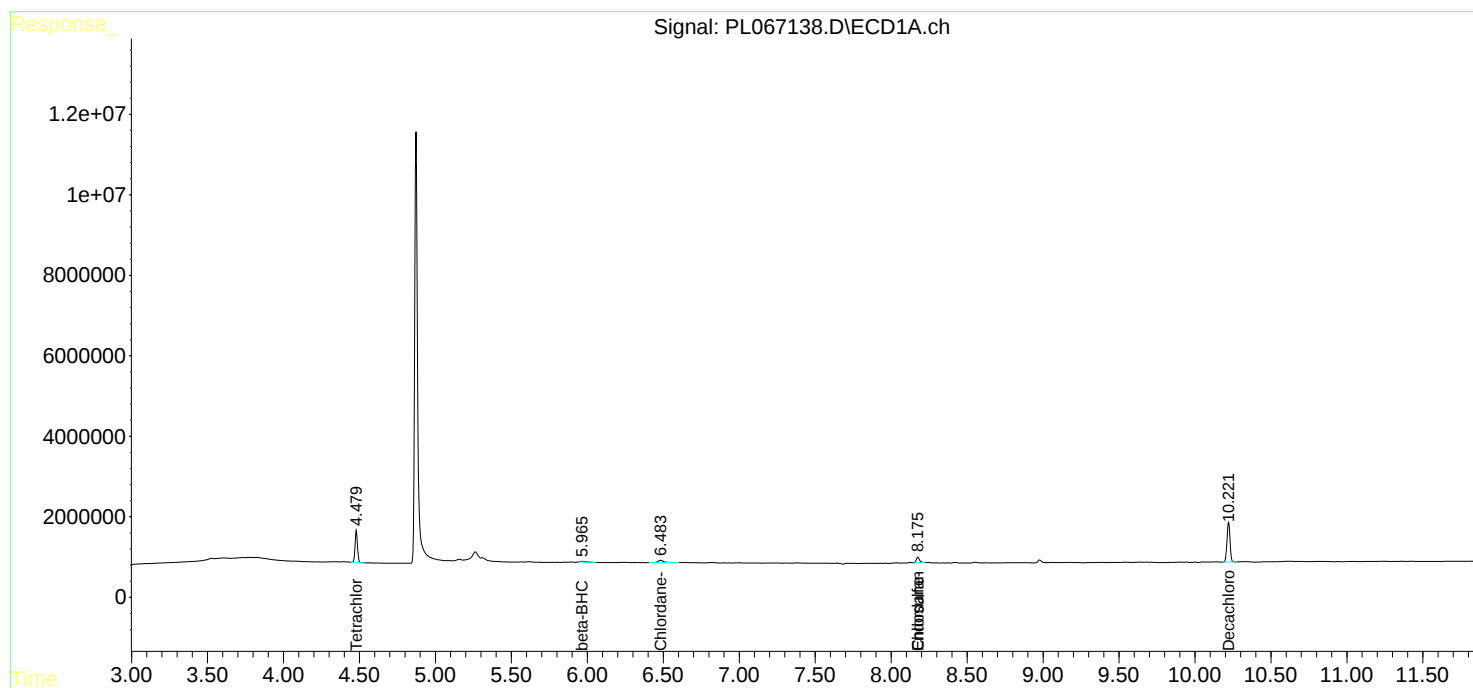


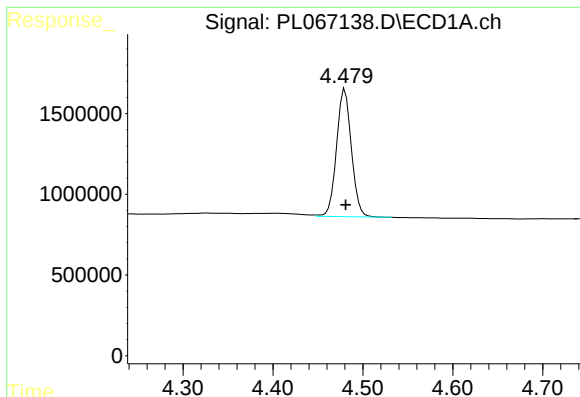

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 9046153
Conc: 22.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136872BL

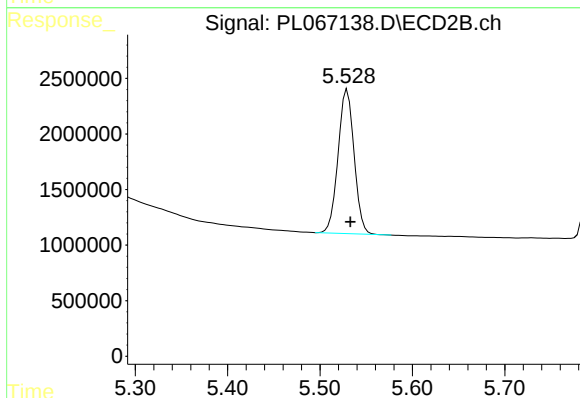


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.003 min
Response: 15654411
Conc: 24.20 ng/ml

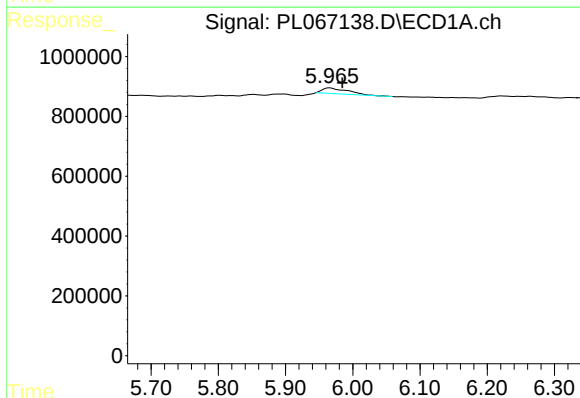


#6 beta-BHC

R.T.: 5.965 min
Delta R.T.: -0.019 min
Response: 478555
Conc: 1.80 ng/ml

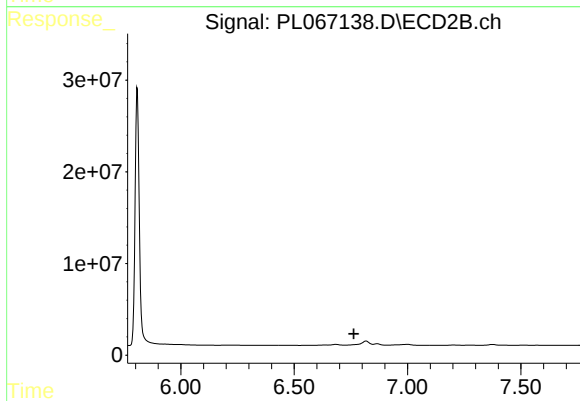

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.763 min
Response: 0
Conc: N.D.

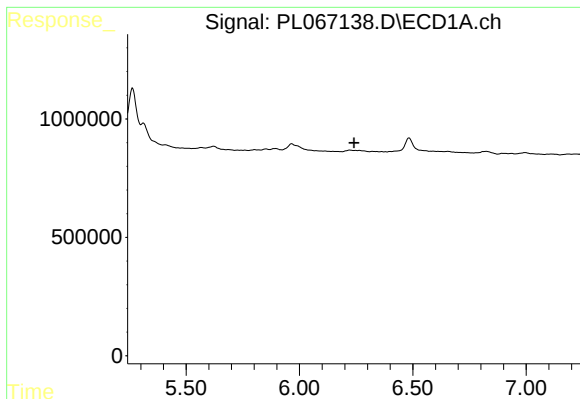

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB136872BL

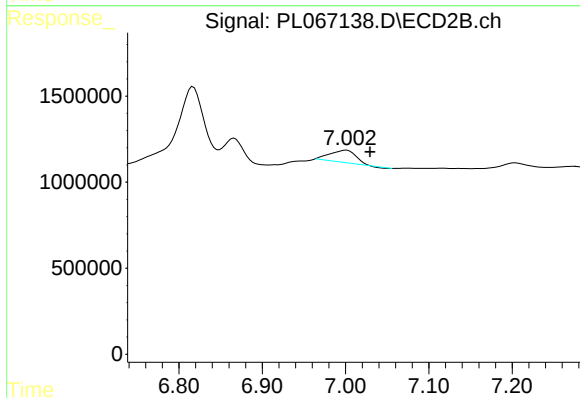


#7 delta-BHC

R.T.: 7.001 min
Delta R.T.: -0.029 min
Response: 1498717
Conc: 1.97 ng/ml

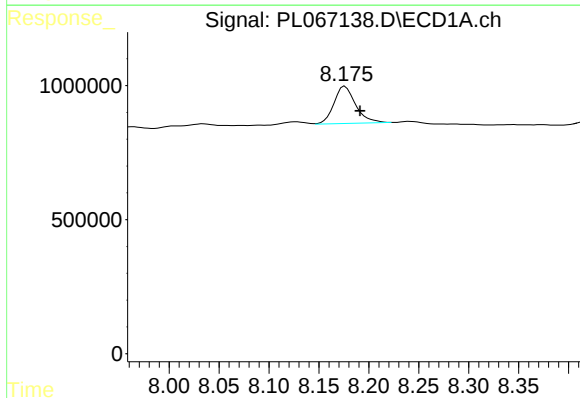


#15 Endosulfan II

R.T.: 8.176 min
Delta R.T.: -0.015 min
Response: 2100496
Conc: 4.05 ng/ml

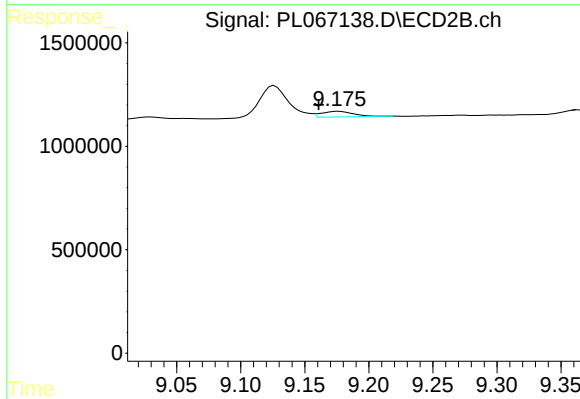

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.016 min
Response: 463790
Conc: 0.75 ng/ml

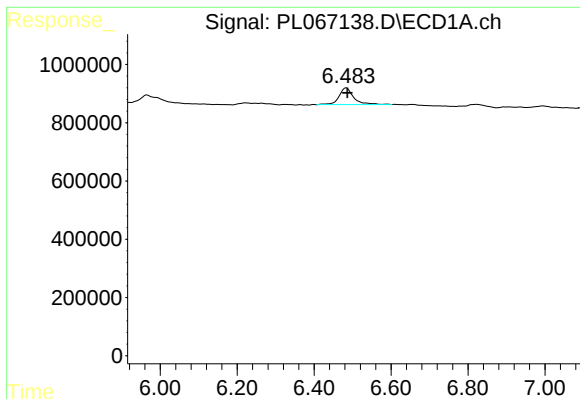

#24 Chlordane-2


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 1523110
Conc: 69.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136872BL

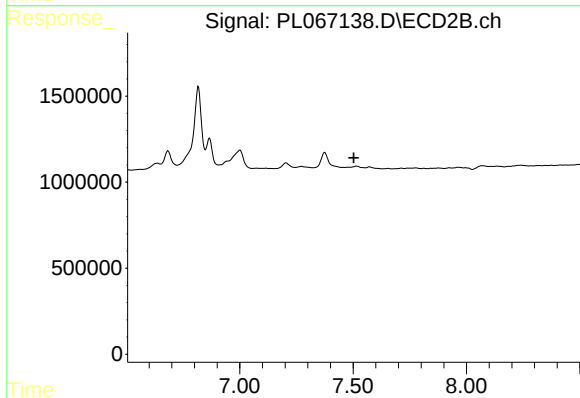


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

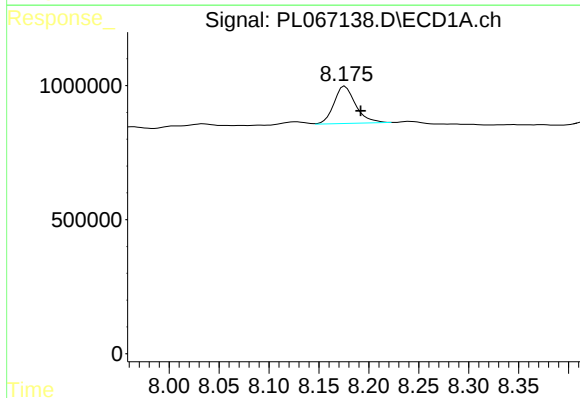


#27 Chlordane-5

R.T.: 8.176 min
Delta R.T.: -0.016 min
Response: 2100496
Conc: 111.32 ng/ml

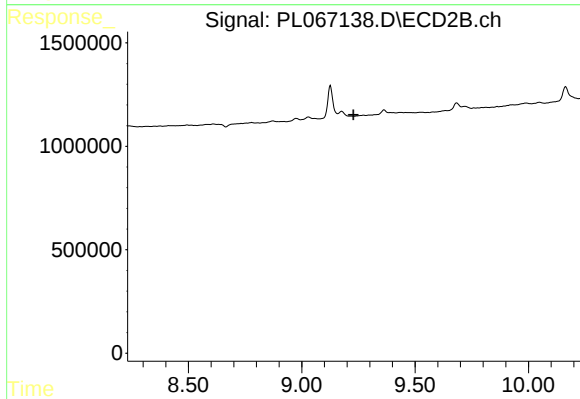

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

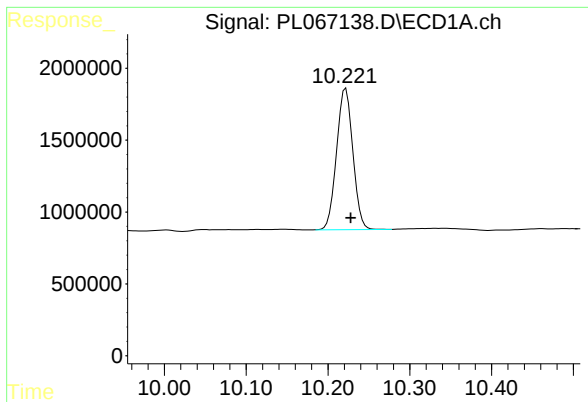

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.006 min
Response: 13560655
Conc: 20.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136872BL

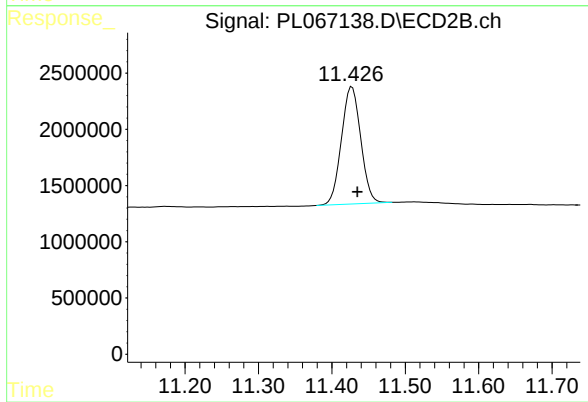

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.008 min
Response: 19073865
Conc: 22.86 ng/ml