

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 14:21
 Operator : AR\AJ
 Sample : M2623-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:20:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	8353620	14511176	20.399	22.432
28)	SA Decachlor...	10.221	11.426	8897261	12626935	13.759	15.134
Target Compounds							
3)	MA gamma-BHC...	5.588	0.000	463078	0	0.831	N.D. #
5)	MB Aldrin	6.341	0.000	397553	0	0.727	N.D. #
15)	B Endosulfa...	8.177	9.176	1090045	468764	2.104	0.760 #
19)	B Endosulfa...	8.591f	0.000	601026	0	1.088	N.D. #
21)	B Endrin ke...	0.000	10.025	0	5294299	N.D.	7.302 #
23)	Chlordane-1	0.000	6.935f	0	384661	N.D.	18.769 #
24)	Chlordane-2	6.483	0.000	1294198	0	59.225	N.D. #
27)	Chlordane-5	8.177	0.000	1090045	0	57.770	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 14:21
Operator : AR\AJ
Sample : M2623-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:20:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

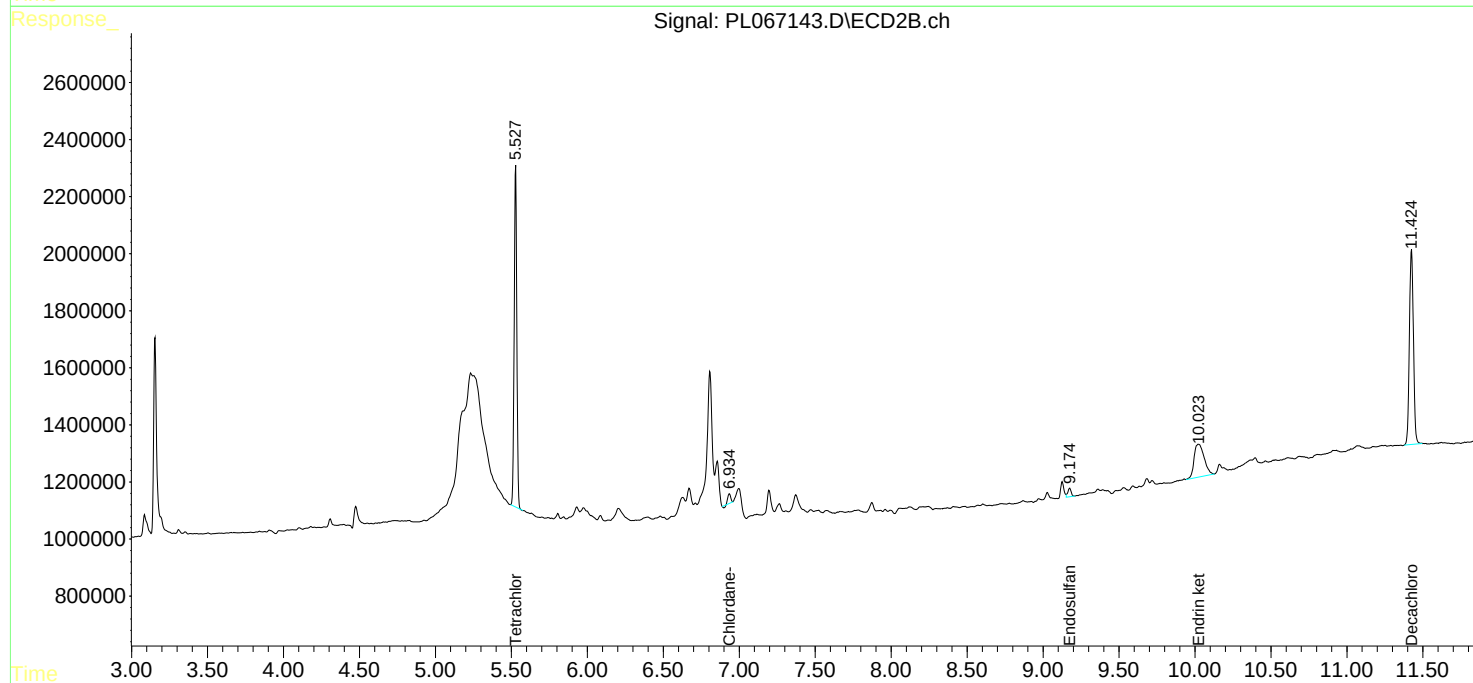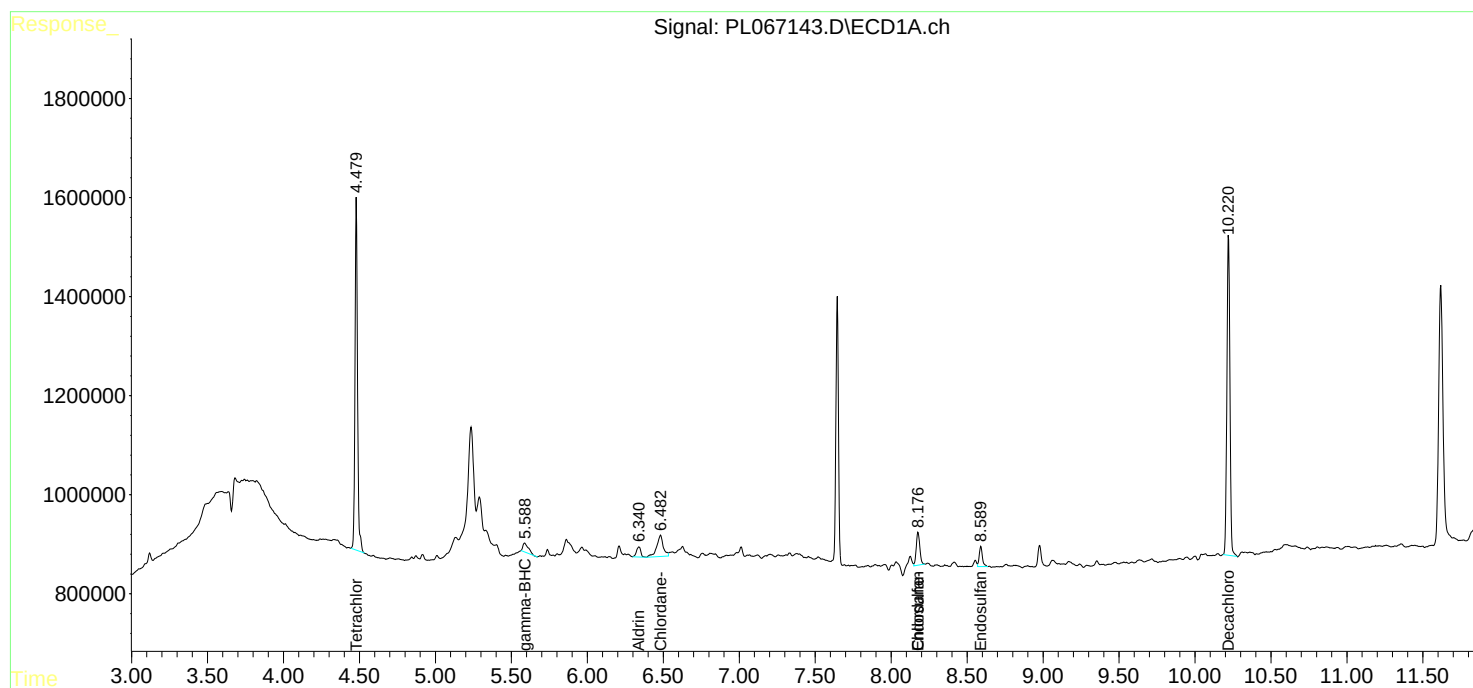


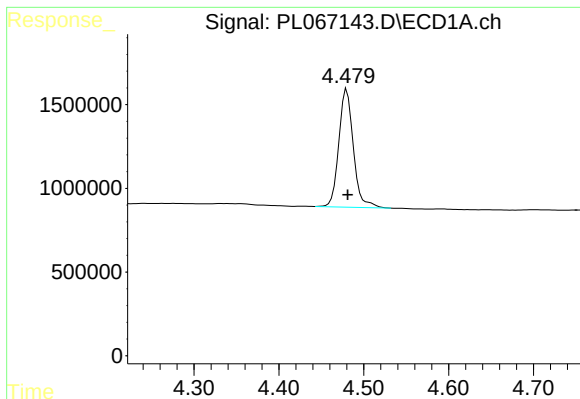

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 8353620
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

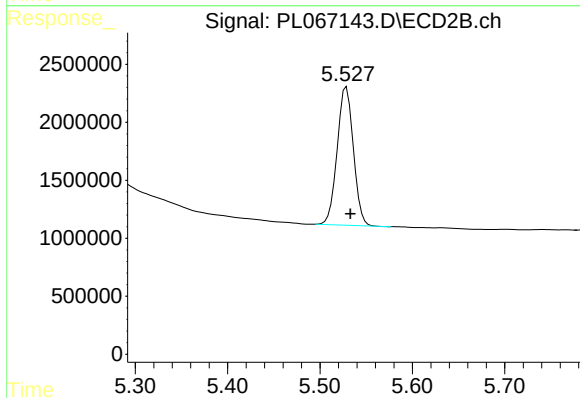


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 14511176
Conc: 22.43 ng/ml

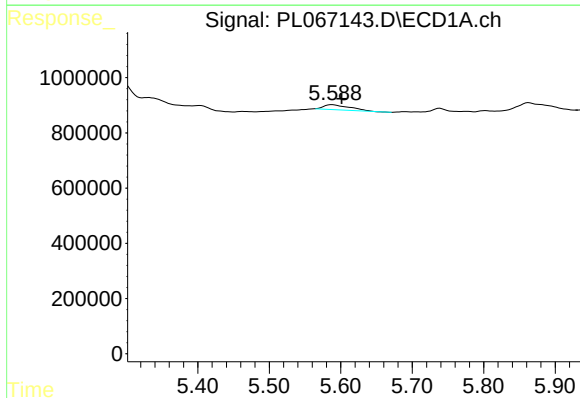


#3 gamma-BHC (Lindane)

R.T.: 5.588 min
Delta R.T.: -0.013 min
Response: 463078
Conc: 0.83 ng/ml

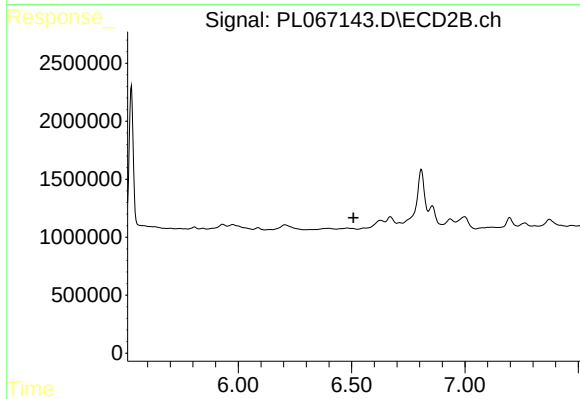

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

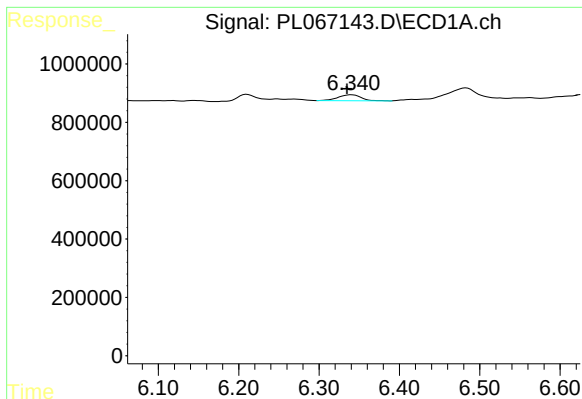

#5 Aldrin


R.T.: 6.341 min
Delta R.T.: 0.006 min
Response: 397553
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

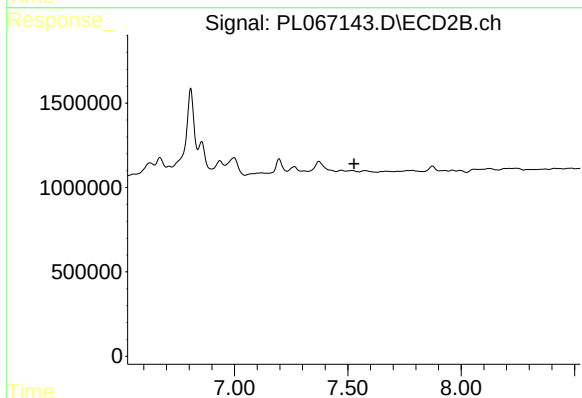


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.527 min
Response: 0
Conc: N.D.

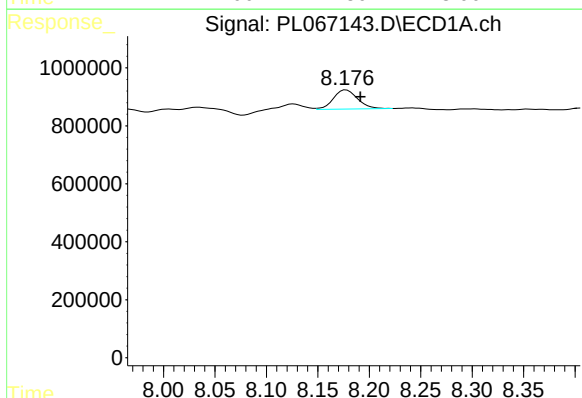


#15 Endosulfan II

R.T.: 8.177 min
Delta R.T.: -0.014 min
Response: 1090045
Conc: 2.10 ng/ml

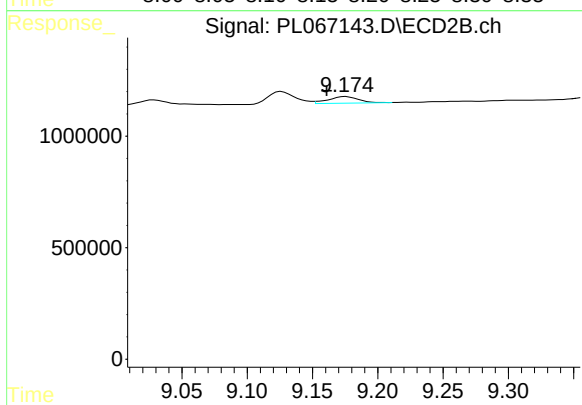

#15 Endosulfan II


R.T.: 9.176 min
Delta R.T.: 0.015 min
Response: 468764
Conc: 0.76 ng/ml

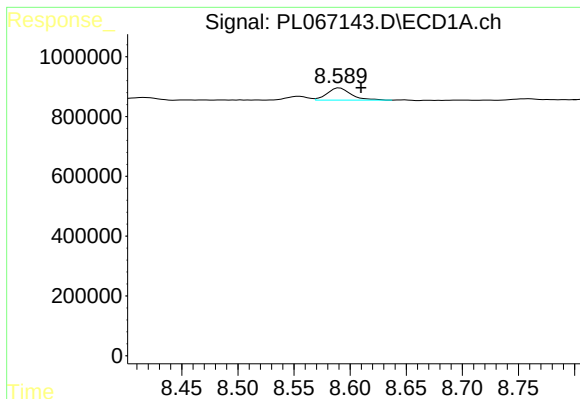

#19 Endosulfan Sulfate


R.T.: 8.591 min
Delta R.T.: -0.019 min
Response: 601026
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

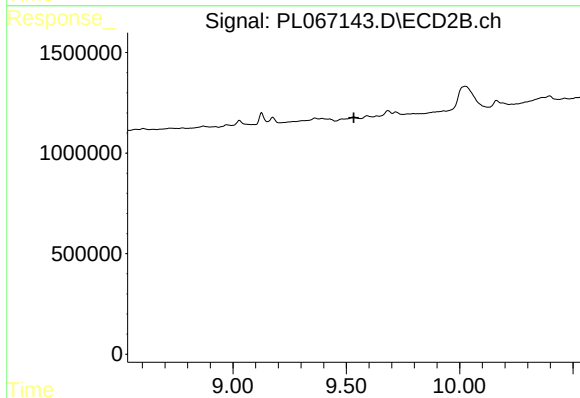


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.533 min
Response: 0
Conc: N.D.

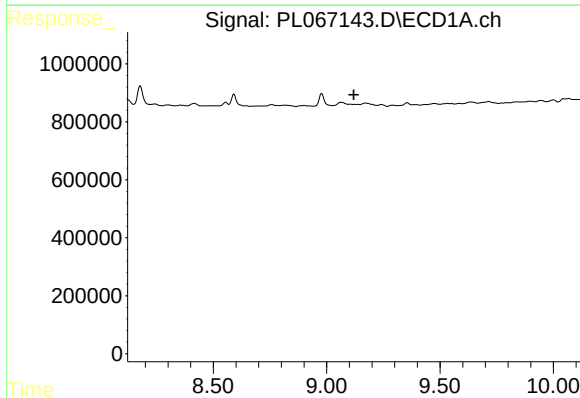


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.119 min
Response: 0
Conc: N.D.

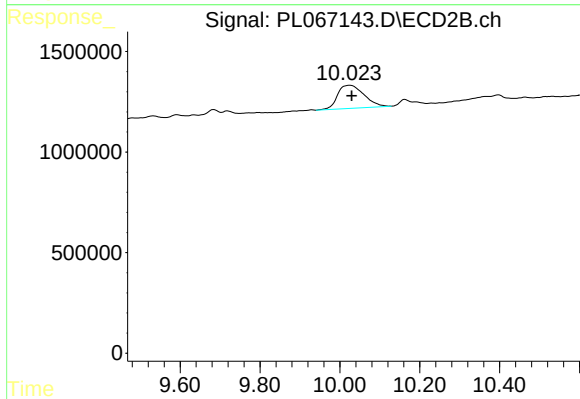

#21 Endrin ketone


R.T.: 10.025 min
Delta R.T.: -0.005 min
Response: 5294299
Conc: 7.30 ng/ml

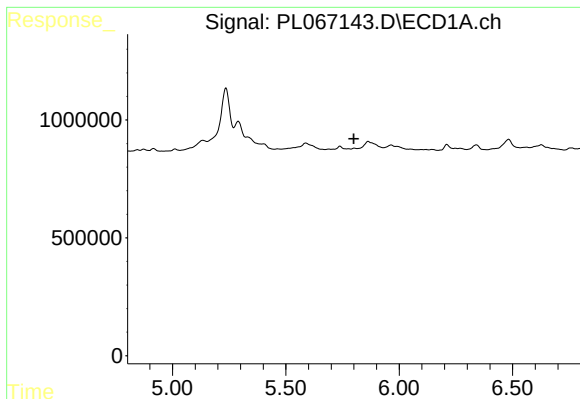

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

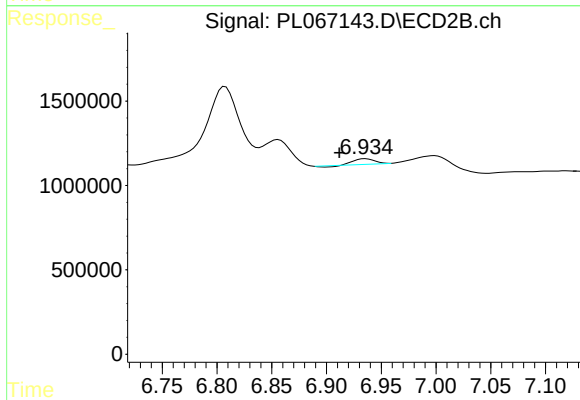


#23 Chlordane-1

R.T.: 6.935 min
Delta R.T.: 0.023 min
Response: 384661
Conc: 18.77 ng/ml

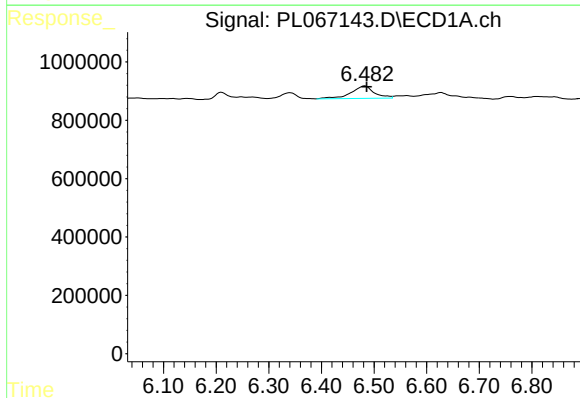


#24 Chlordane-2

R.T.: 6.483 min
Delta R.T.: -0.003 min
Response: 1294198
Conc: 59.22 ng/ml

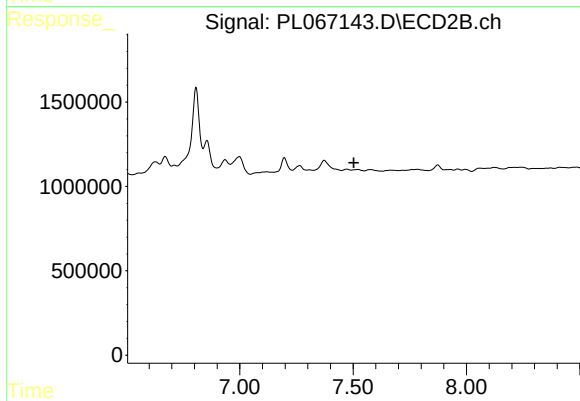

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

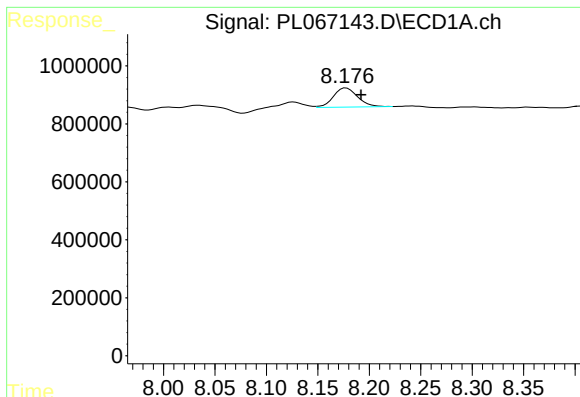

#27 Chlordane-5


R.T.: 8.177 min
Delta R.T.: -0.014 min
Response: 1090045
Conc: 57.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

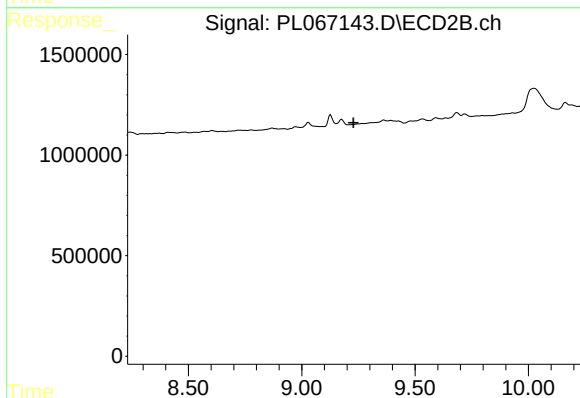


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

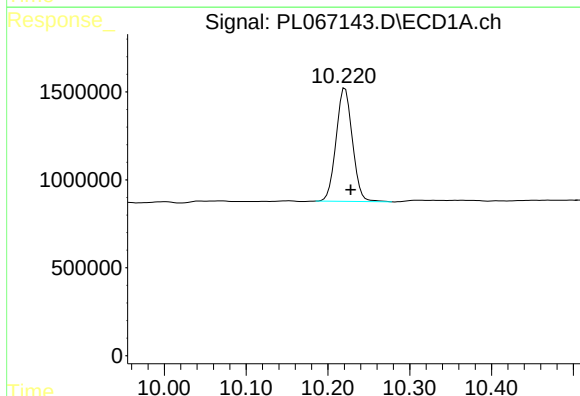

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 8897261
Conc: 13.76 ng/ml

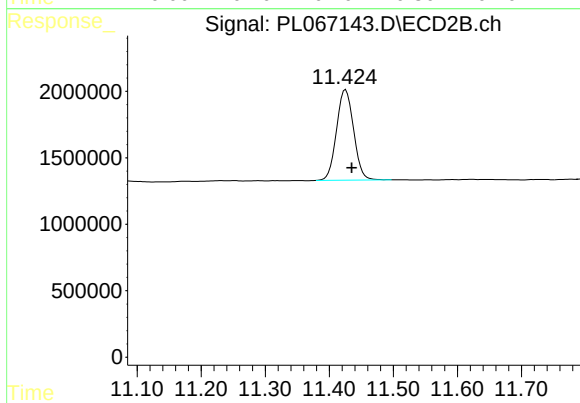

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.009 min
Response: 12626935
Conc: 15.13 ng/ml