

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 14:55
 Operator : AR\AJ
 Sample : M2623-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:21:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	8579956	14931487	20.952	23.082
28)	SA Decachlor...	10.221	11.425	11641952	16565806	18.004	19.855
Target Compounds							
3)	MA gamma-BHC...	5.606	0.000	538310	0	0.966	N.D. #
5)	MB Aldrin	6.337	0.000	309719	0	0.566	N.D. #
7)	B delta-BHC	6.216f	0.000	188939	0	0.356	N.D. #
15)	B Endosulfa...	8.178	9.177f	868029	389431	1.675	0.631 #
18)	B Endrin al...	8.404f	0.000	396041	0	0.860	N.D. #
19)	B Endosulfa...	8.591f	9.534	684451	393986	1.239	0.633 #
20)	A Methoxychlor	8.903	0.000	216480	0	0.726	N.D. #
21)	B Endrin ke...	0.000	10.039	0	12683292	N.D.	17.493 #
23)	Chlordane-1	0.000	6.941f	0	160983	N.D.	7.855 #
24)	Chlordane-2	6.484	0.000	1221863	0	55.914	N.D. #
27)	Chlordane-5	8.178	0.000	868029	0	46.003	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 14:55
Operator : AR\AJ
Sample : M2623-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:21:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

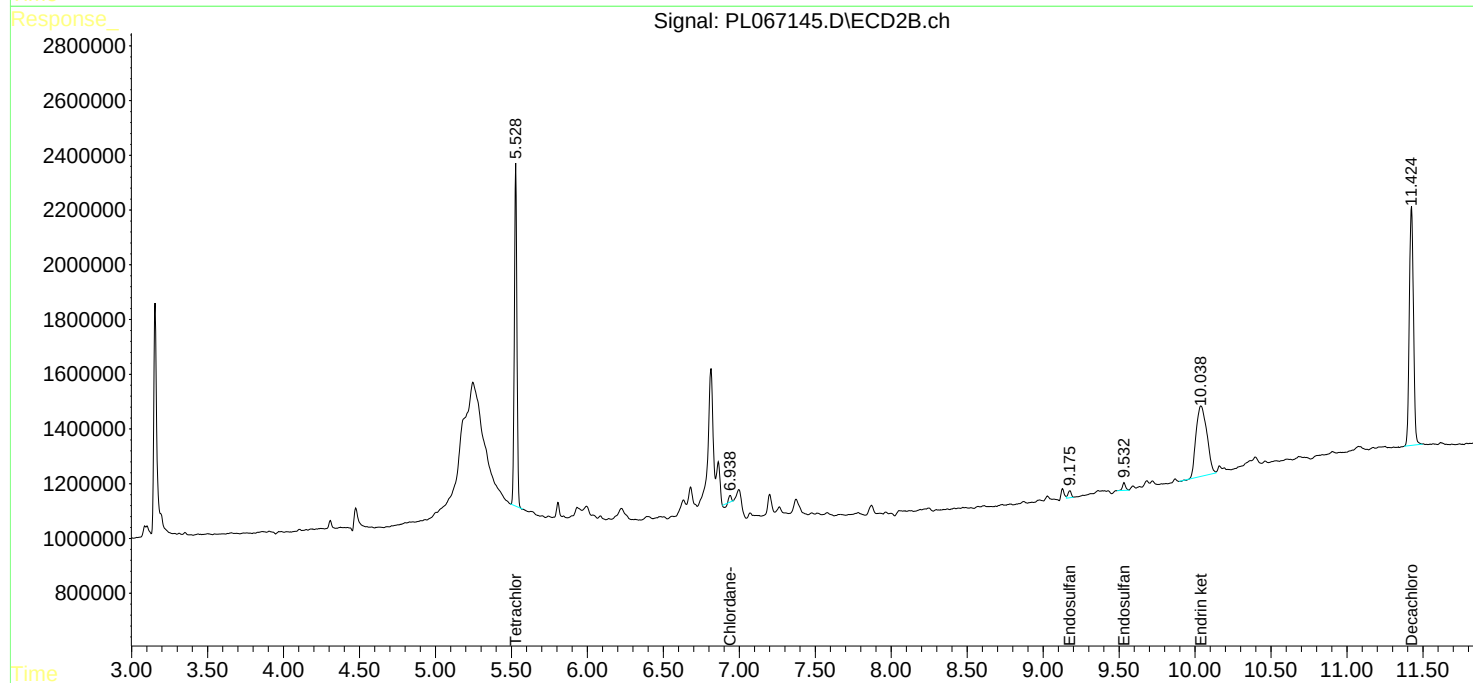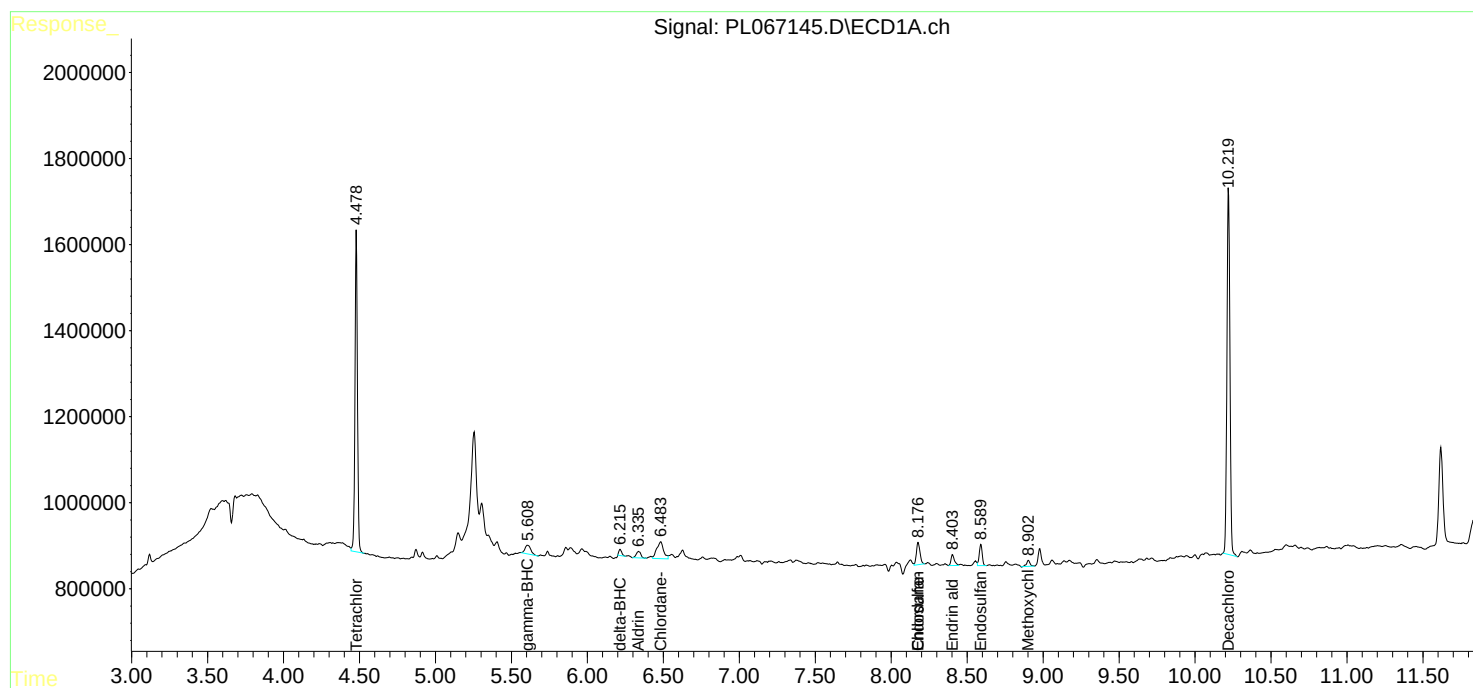


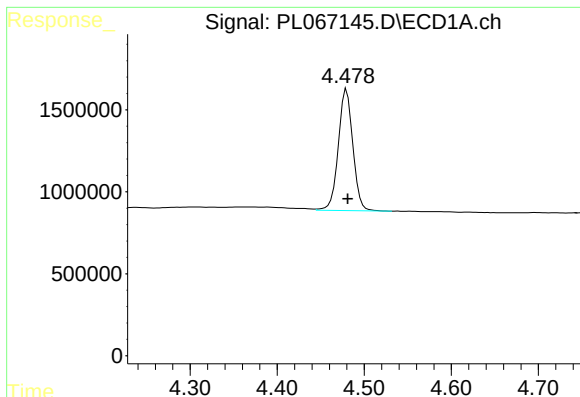

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 8579956
Conc: 20.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

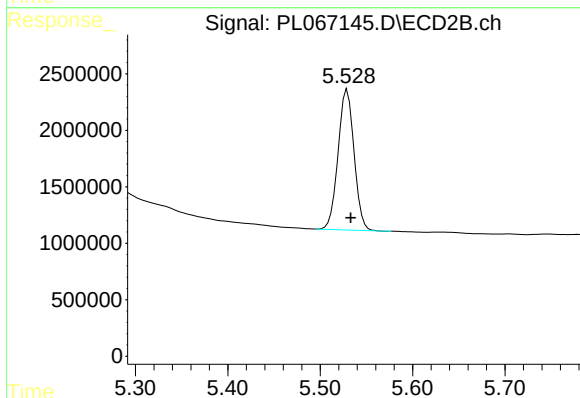


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 14931487
Conc: 23.08 ng/ml

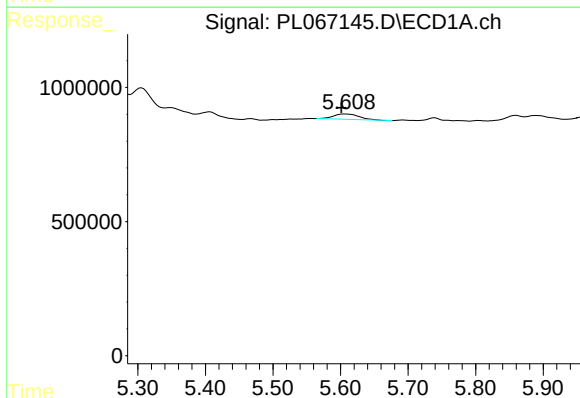


#3 gamma-BHC (Lindane)

R.T.: 5.606 min
Delta R.T.: 0.005 min
Response: 538310
Conc: 0.97 ng/ml

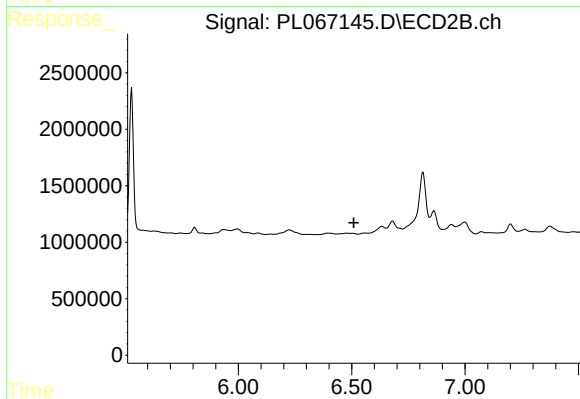

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

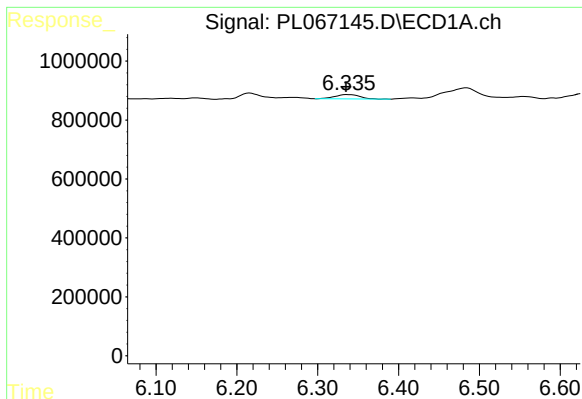

#5 Aldrin


R.T.: 6.337 min
Delta R.T.: 0.002 min
Response: 309719
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

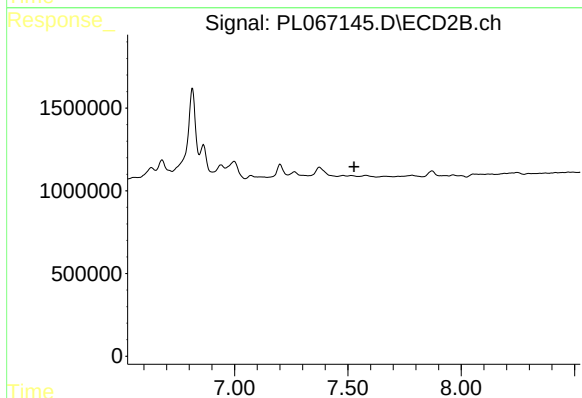


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.527 min
Response: 0
Conc: N.D.

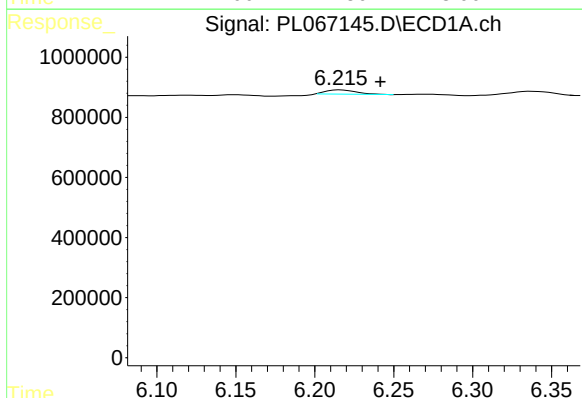


#7 delta-BHC

R.T.: 6.216 min
Delta R.T.: -0.025 min
Response: 188939
Conc: 0.36 ng/ml

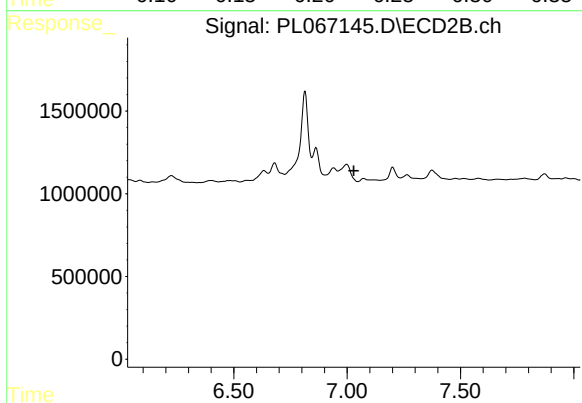

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 7.030 min
Response: 0
Conc: N.D.

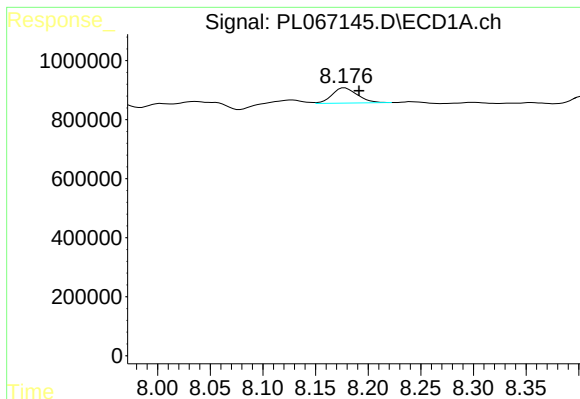

#15 Endosulfan II


R.T.: 8.178 min
Delta R.T.: -0.014 min
Response: 868029
Conc: 1.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

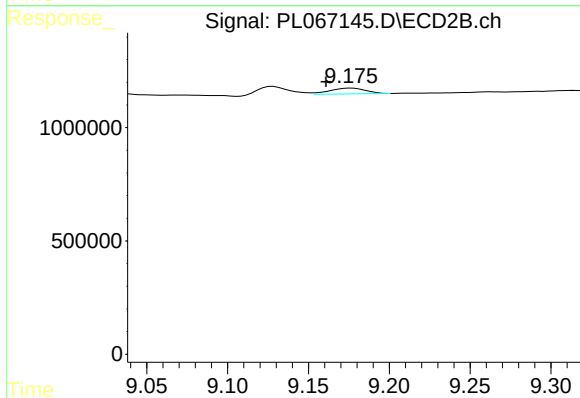


#15 Endosulfan II

R.T.: 9.177 min
Delta R.T.: 0.016 min
Response: 389431
Conc: 0.63 ng/ml

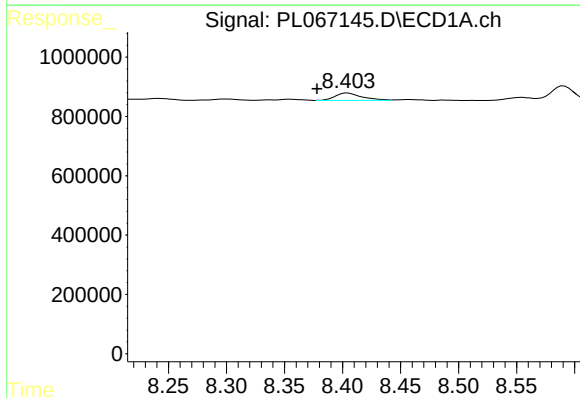


#18 Endrin aldehyde

R.T.: 8.404 min
Delta R.T.: 0.026 min
Response: 396041
Conc: 0.86 ng/ml

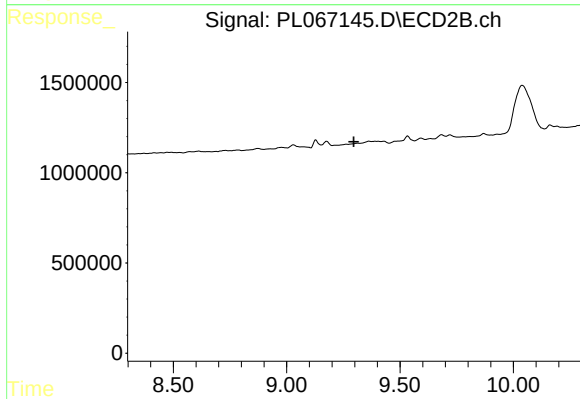

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 9.295 min
Response: 0
Conc: N.D.

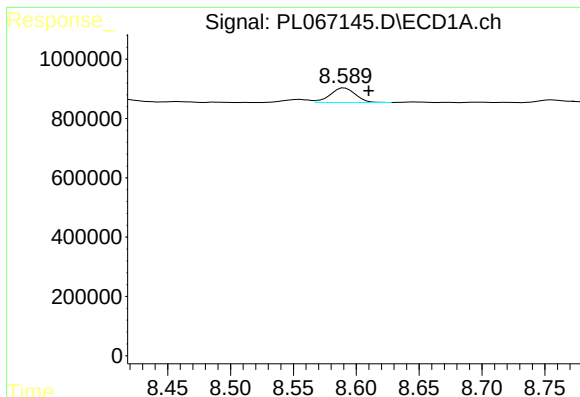

#19 Endosulfan Sulfate


R.T.: 8.591 min
Delta R.T.: -0.019 min
Response: 684451
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

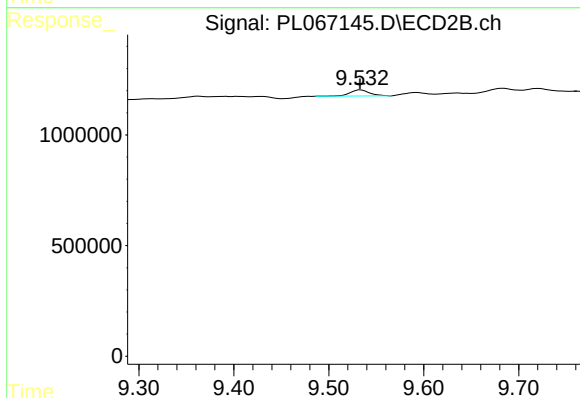


#19 Endosulfan Sulfate

R.T.: 9.534 min
Delta R.T.: 0.000 min
Response: 393986
Conc: 0.63 ng/ml

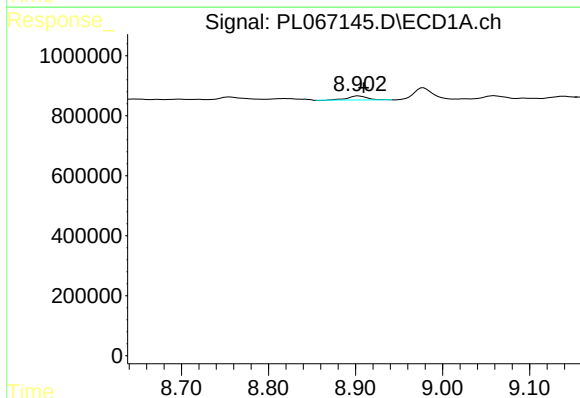


#20 Methoxychlor

R.T.: 8.903 min
Delta R.T.: -0.006 min
Response: 216480
Conc: 0.73 ng/ml

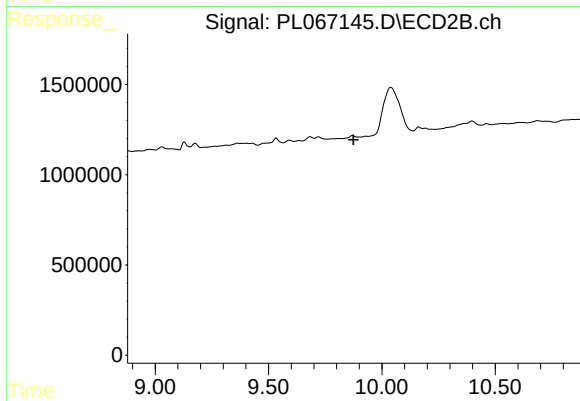

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.875 min
Response: 0
Conc: N.D.

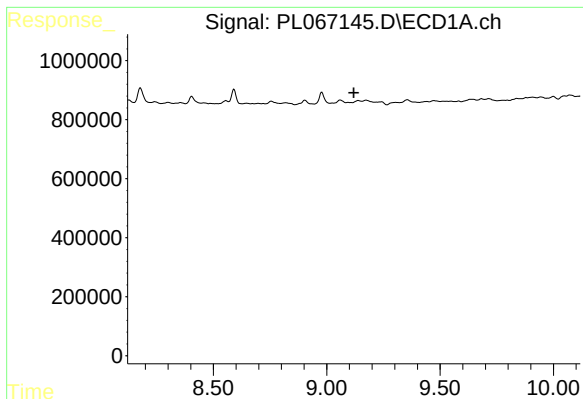

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-6

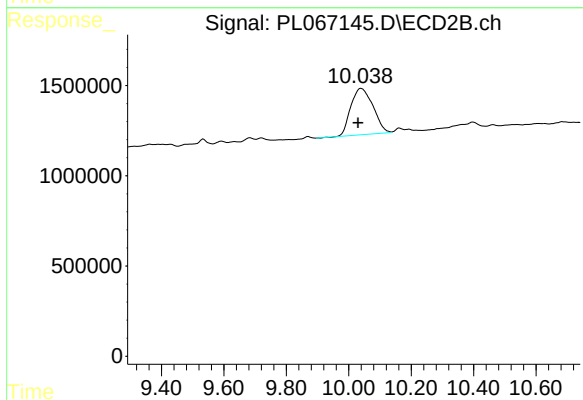


#21 Endrin ketone

R.T.: 10.039 min
Delta R.T.: 0.009 min
Response: 12683292
Conc: 17.49 ng/ml

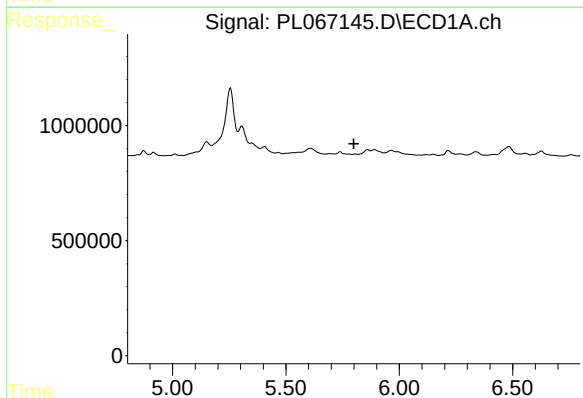


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

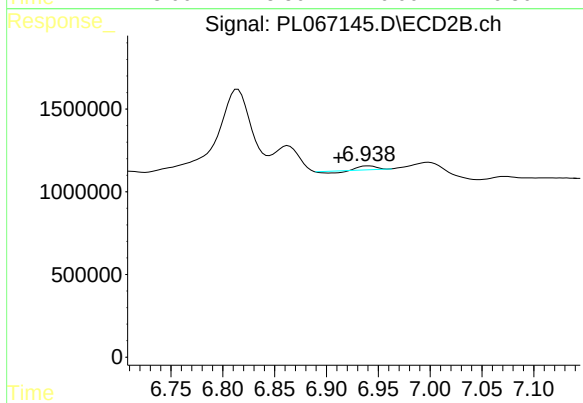

#23 Chlordane-1


R.T.: 6.941 min
Delta R.T.: 0.029 min
Response: 160983
Conc: 7.86 ng/ml

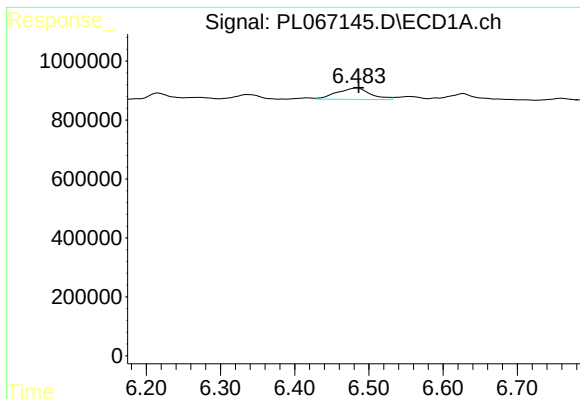

#24 Chlordane-2


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 1221863
Conc: 55.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

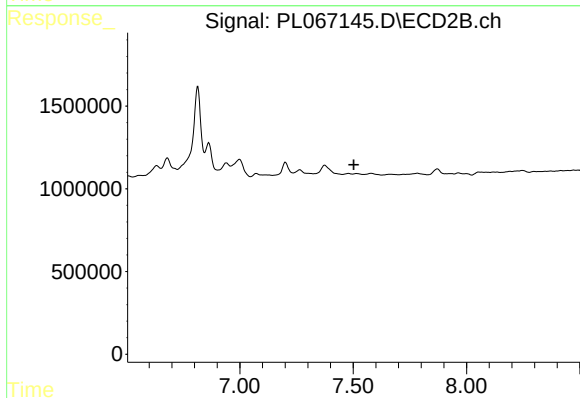


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

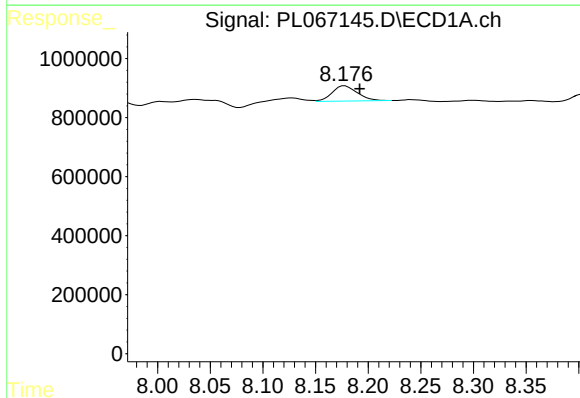


#27 Chlordane-5

R.T.: 8.178 min
Delta R.T.: -0.014 min
Response: 868029
Conc: 46.00 ng/ml

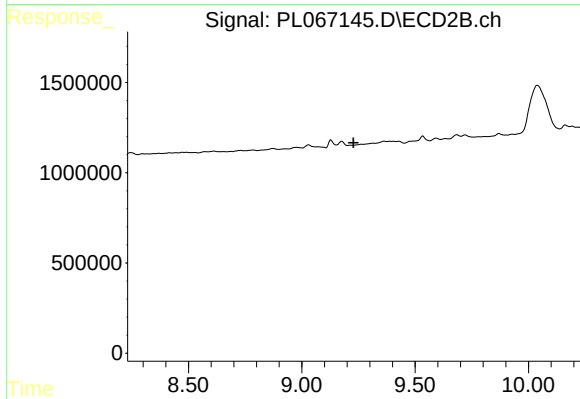

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

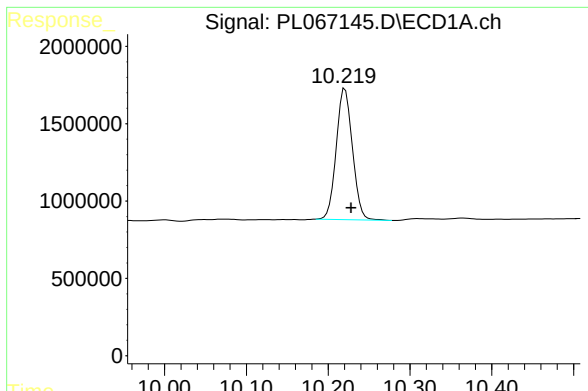

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 11641952
Conc: 18.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-6

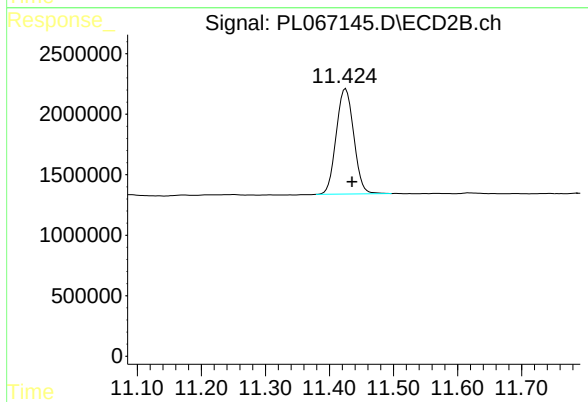

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.010 min
Response: 16565806
Conc: 19.85 ng/ml