

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 15:28
 Operator : AR\AJ
 Sample : M2623-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:22:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	8630204	15345587	21.075	23.722
28)	SA Decachlor...	10.221	11.426	9468328	13371070	14.643	16.026
Target Compounds							
3)	MA gamma-BHC...	5.598	0.000	668574	0	1.200	N.D. #
5)	MB Aldrin	6.341	0.000	1059519	0	1.937	N.D. #
7)	B delta-BHC	6.213f	0.000	199467	0	0.376	N.D. #
15)	B Endosulfa...	8.178	9.178f	838526	626722	1.618	1.016 #
19)	B Endosulfa...	8.592f	0.000	247659	0	0.448	N.D. #
21)	B Endrin ke...	0.000	10.049f	0	2309102	N.D.	3.185 #
23)	Chlordane-1	0.000	6.939f	0	268128	N.D.	13.083 #
24)	Chlordane-2	6.483	0.000	1146302	0	52.457	N.D. #
27)	Chlordane-5	8.178	0.000	838526	0	44.440	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 15:28
Operator : AR\AJ
Sample : M2623-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:22:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

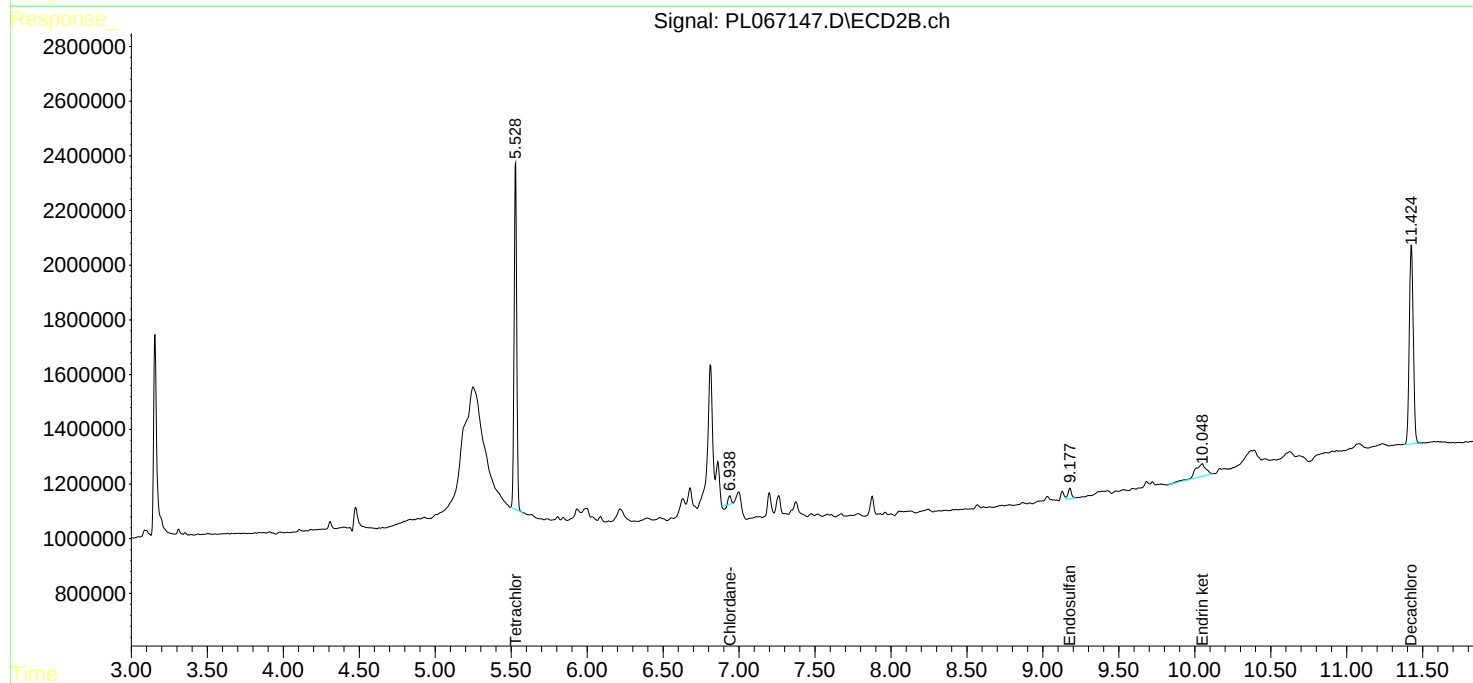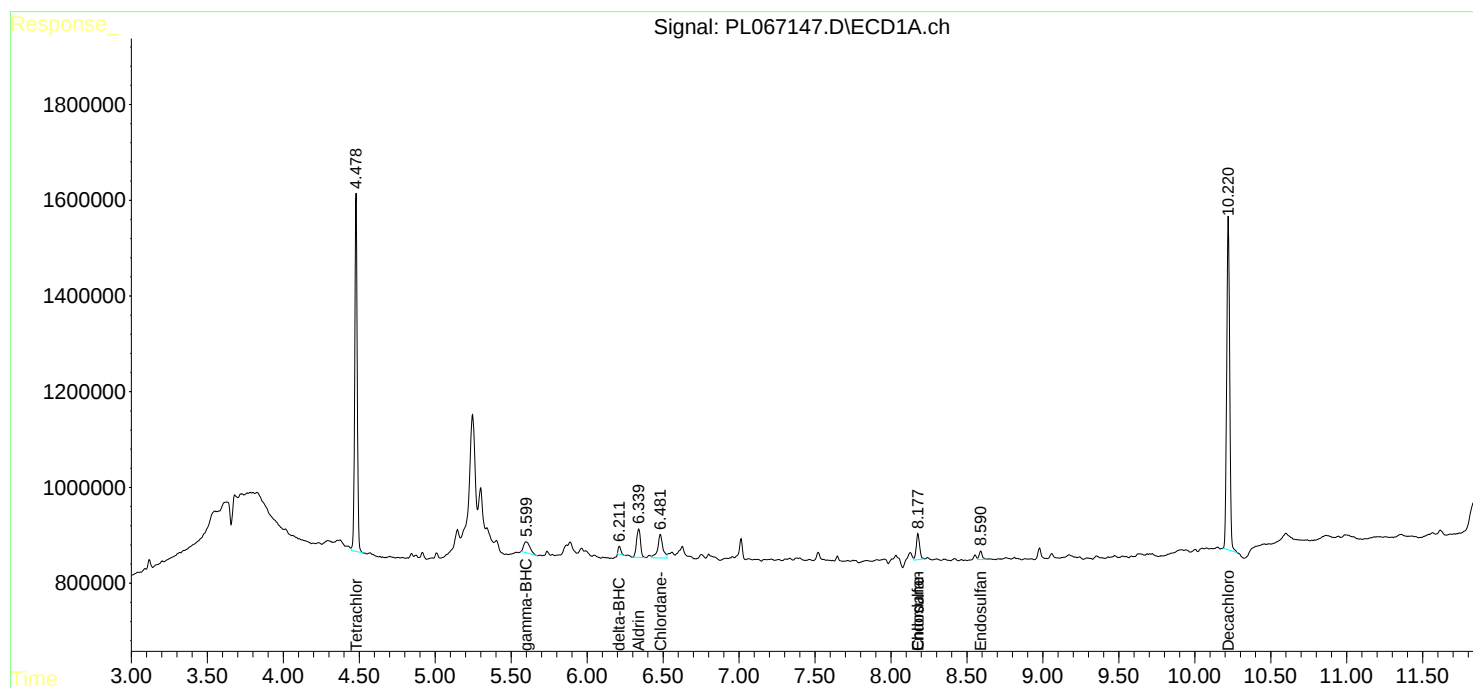


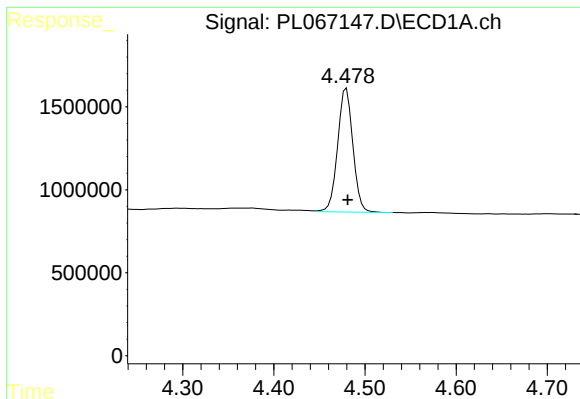

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 8630204
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-8

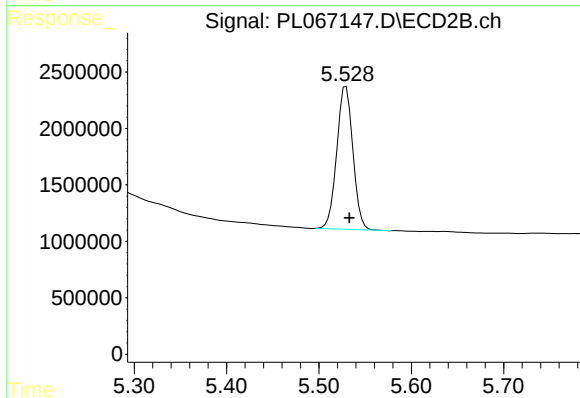


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 15345587
Conc: 23.72 ng/ml

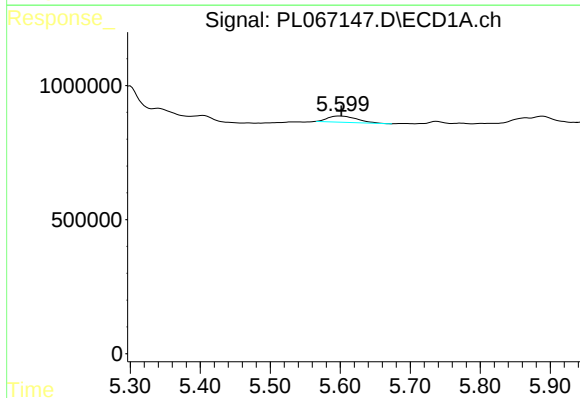


#3 gamma-BHC (Lindane)

R.T.: 5.598 min
Delta R.T.: -0.003 min
Response: 668574
Conc: 1.20 ng/ml

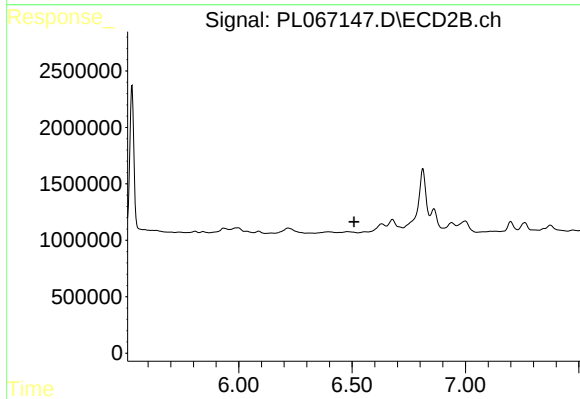

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

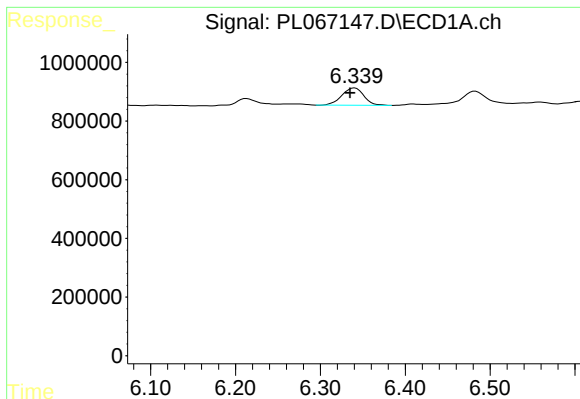

#5 Aldrin


R.T.: 6.341 min
Delta R.T.: 0.006 min
Response: 1059519
Conc: 1.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-8

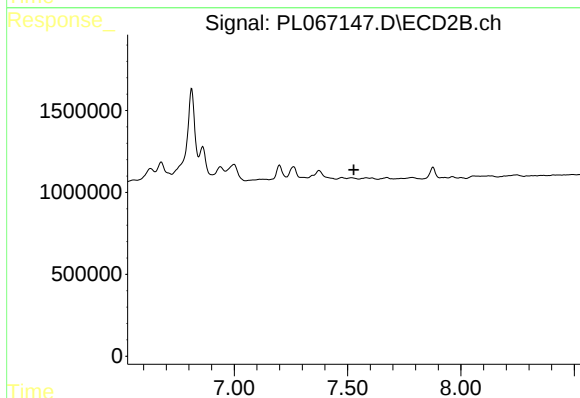


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.527 min
Response: 0
Conc: N.D.

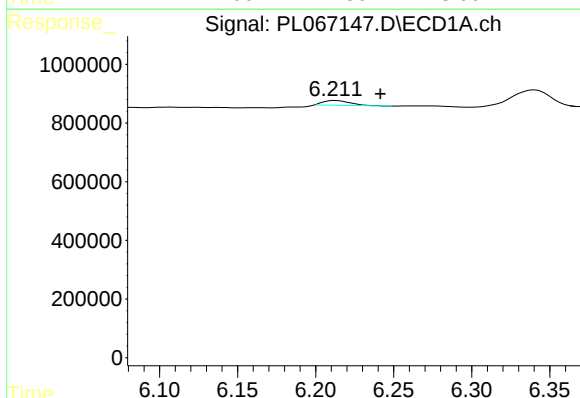


#7 delta-BHC

R.T.: 6.213 min
Delta R.T.: -0.029 min
Response: 199467
Conc: 0.38 ng/ml

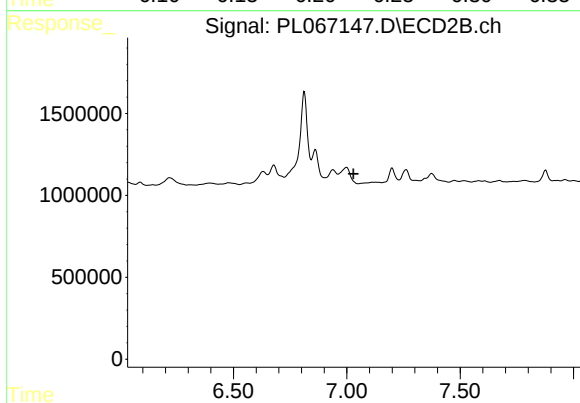

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 7.030 min
Response: 0
Conc: N.D.

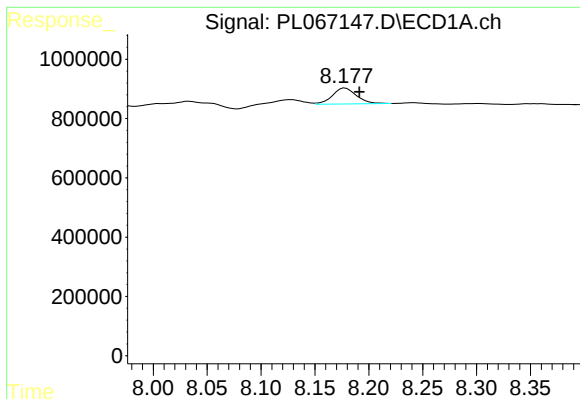

#15 Endosulfan II


R.T.: 8.178 min
Delta R.T.: -0.013 min
Response: 838526
Conc: 1.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-8

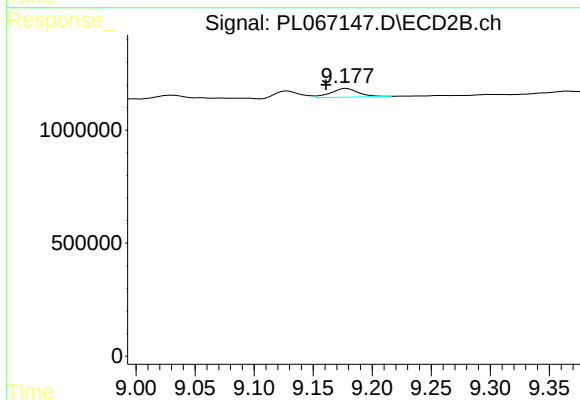


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 626722
Conc: 1.02 ng/ml

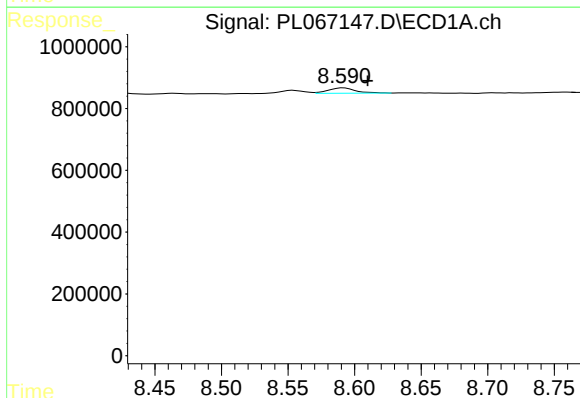


#19 Endosulfan Sulfate

R.T.: 8.592 min
Delta R.T.: -0.018 min
Response: 247659
Conc: 0.45 ng/ml

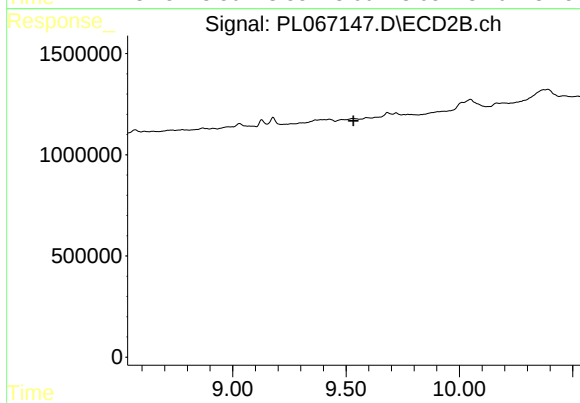

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.533 min
Response: 0
Conc: N.D.

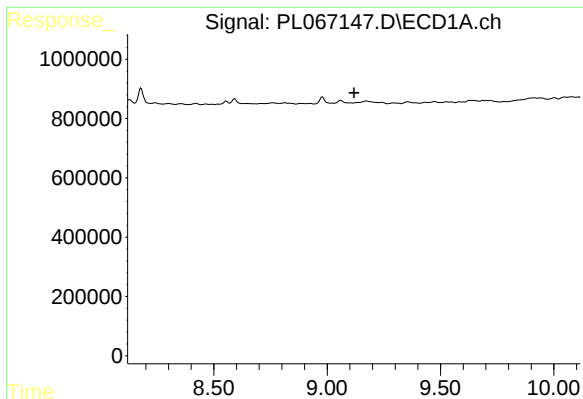

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-8

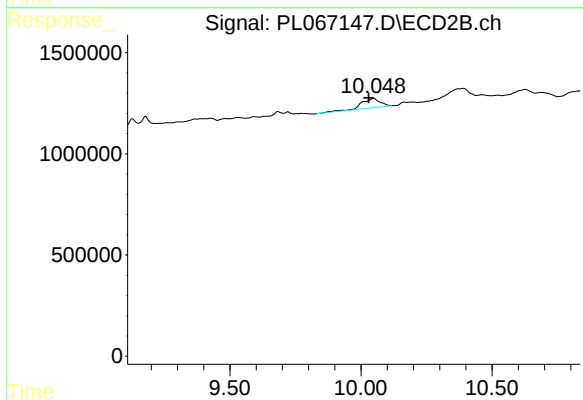


#21 Endrin ketone

R.T.: 10.049 min
Delta R.T.: 0.020 min
Response: 2309102
Conc: 3.18 ng/ml

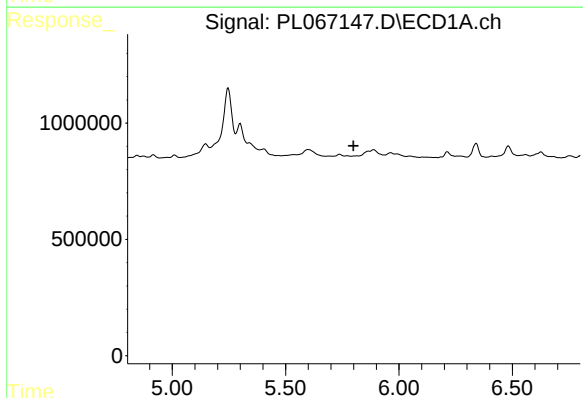


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

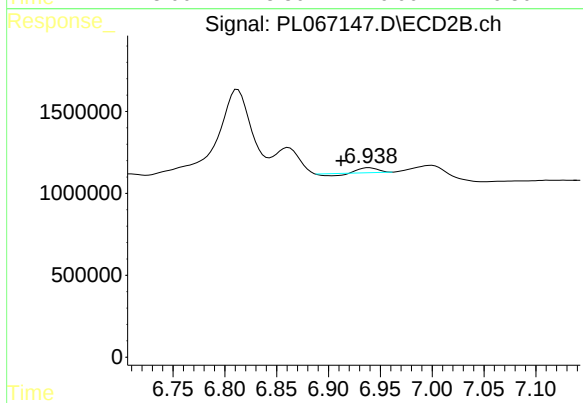

#23 Chlordane-1


R.T.: 6.939 min
Delta R.T.: 0.028 min
Response: 268128
Conc: 13.08 ng/ml

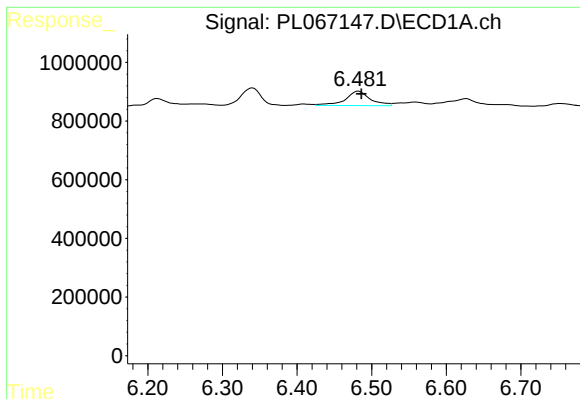

#24 Chlordane-2


R.T.: 6.483 min
Delta R.T.: -0.004 min
Response: 1146302
Conc: 52.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-8

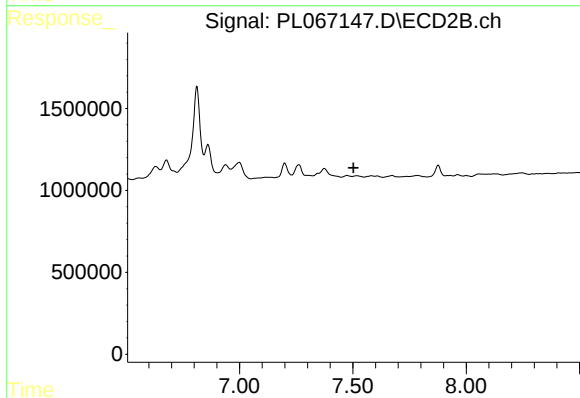


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

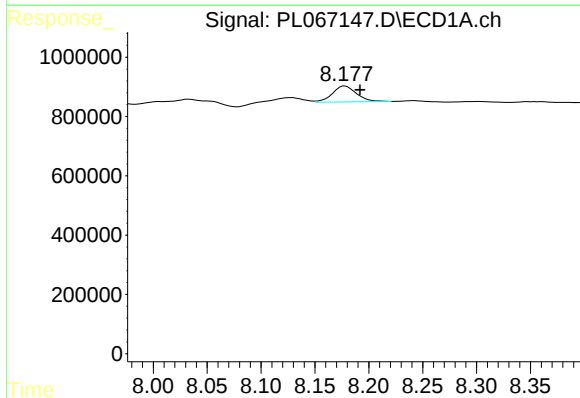


#27 Chlordane-5

R.T.: 8.178 min
Delta R.T.: -0.014 min
Response: 838526
Conc: 44.44 ng/ml

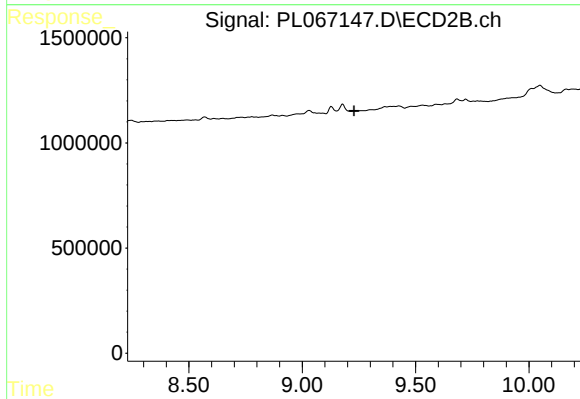

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

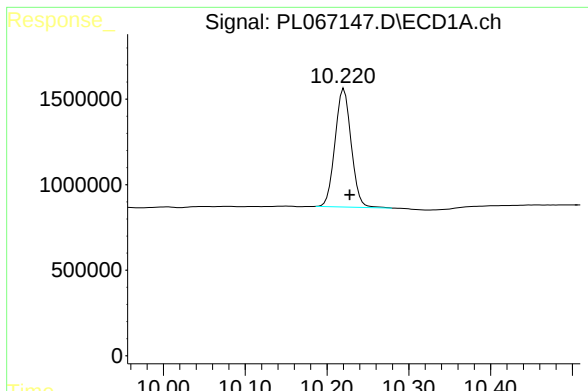

#28 Decachlorobiphenyl


R.T.: 10.221 min

Delta R.T.: -0.007 min

Response: 9468328

Conc: 14.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-8

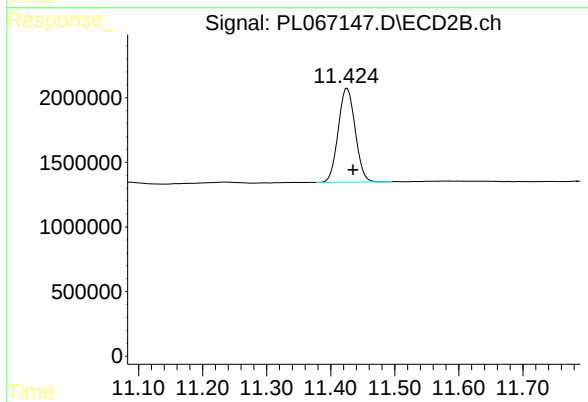

#28 Decachlorobiphenyl

R.T.: 11.426 min

Delta R.T.: -0.009 min

Response: 13371070

Conc: 16.03 ng/ml