

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 16:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:22:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	7656301	13887233	18.697	21.467
28)	SA Decachlor...	10.222	11.427	11663890	17408470	18.038	20.865
Target Compounds							
3)	MA gamma-BHC...	5.597	0.000	640543	0	1.150	N.D. #
4)	MA Heptachlor	5.989f	0.000	261195	0	0.497	N.D. #
6)	B beta-BHC	5.989	0.000	261195	0	0.981	N.D. #
7)	B delta-BHC	6.212f	0.000	192299	0	0.362	N.D. #
15)	B Endosulfa...	8.177	0.000	455890	0	0.880	N.D. #
21)	B Endrin ke...	0.000	10.034	0	3158066	N.D.	4.356 #
23)	Chlordane-1	0.000	6.937f	0	338708	N.D.	16.527 #
24)	Chlordane-2	6.484	0.000	862885	0	39.487	N.D. #
27)	Chlordane-5	8.177f	0.000	455890	0	24.161	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 16:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:22:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

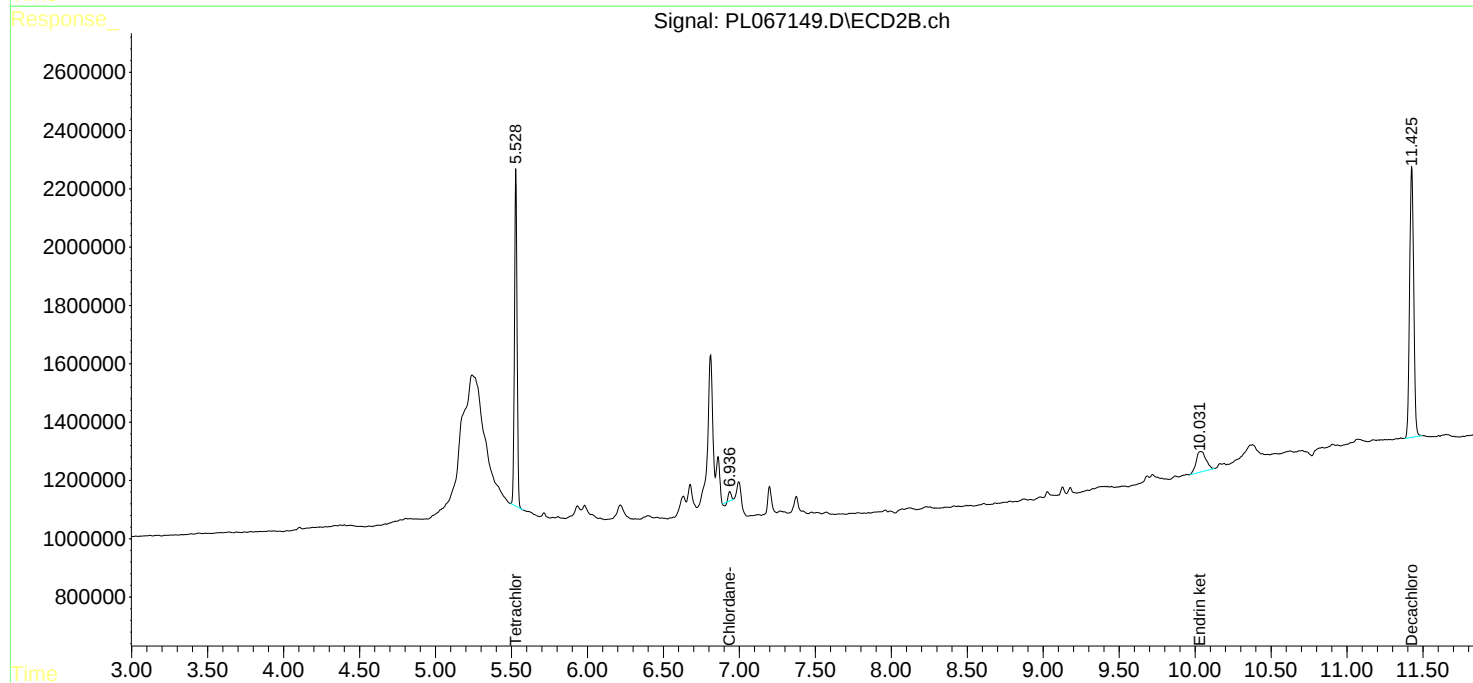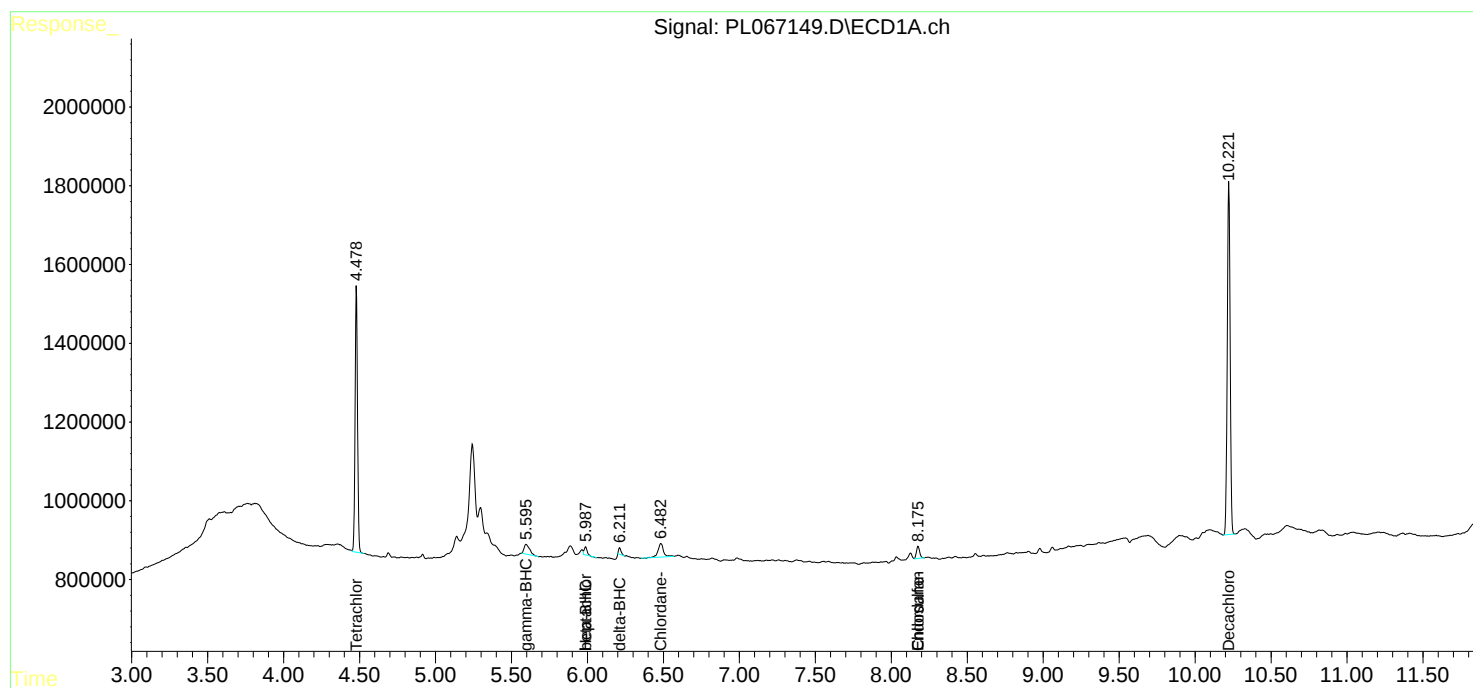


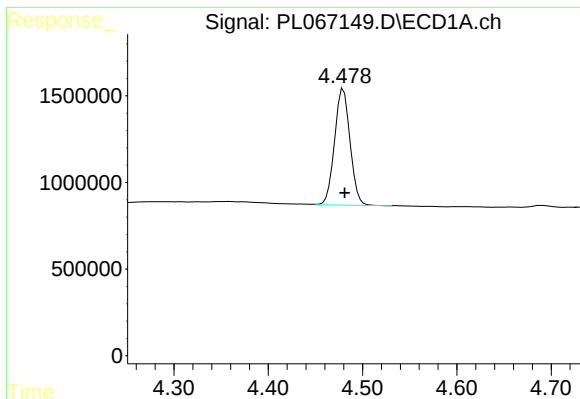

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 7656301
Conc: 18.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

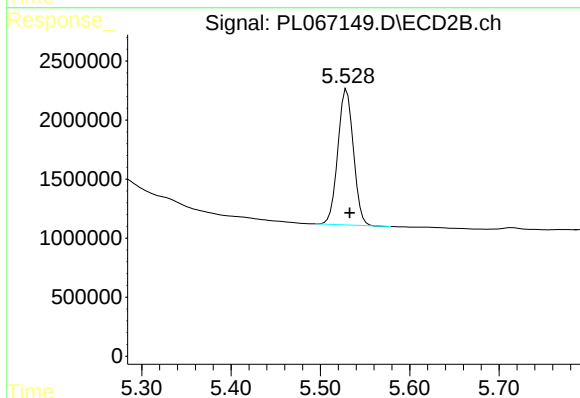


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 13887233
Conc: 21.47 ng/ml

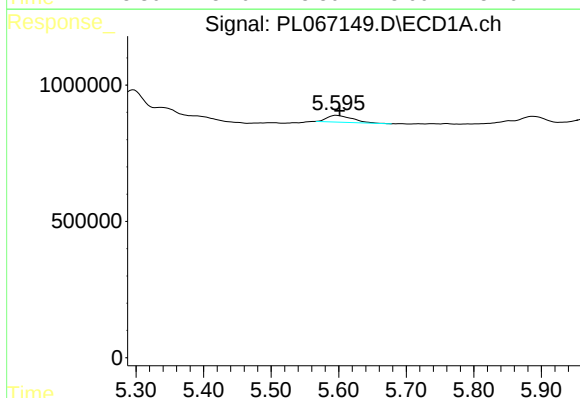


#3 gamma-BHC (Lindane)

R.T.: 5.597 min
Delta R.T.: -0.005 min
Response: 640543
Conc: 1.15 ng/ml

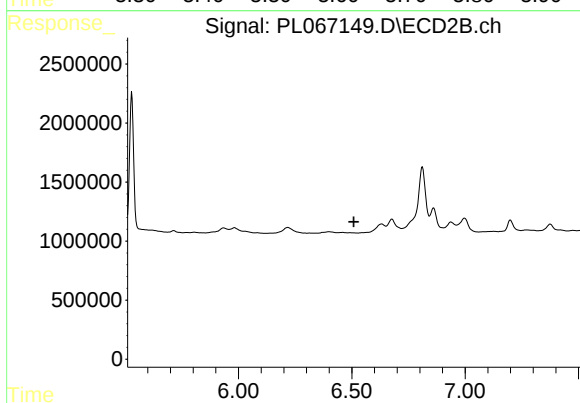

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

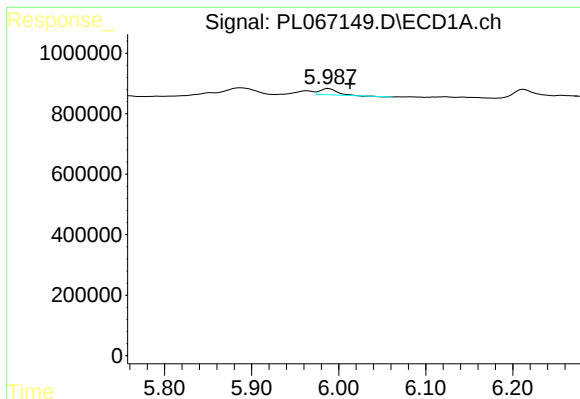

#4 Heptachlor


R.T.: 5.989 min
Delta R.T.: -0.024 min
Response: 261195
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

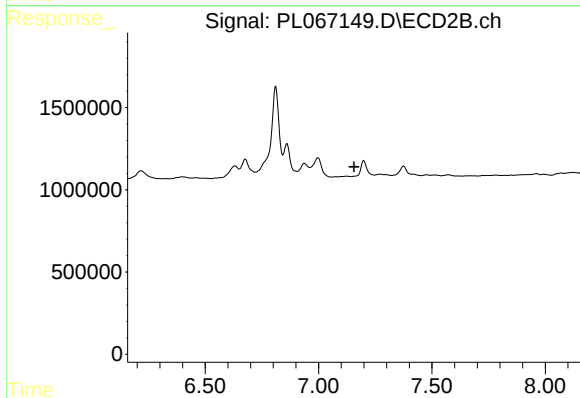


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

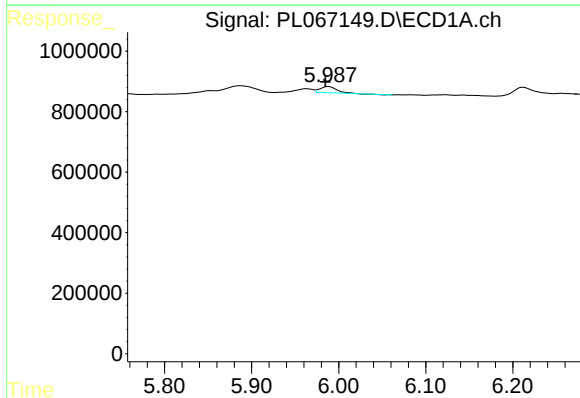


#6 beta-BHC

R.T.: 5.989 min
Delta R.T.: 0.004 min
Response: 261195
Conc: 0.98 ng/ml

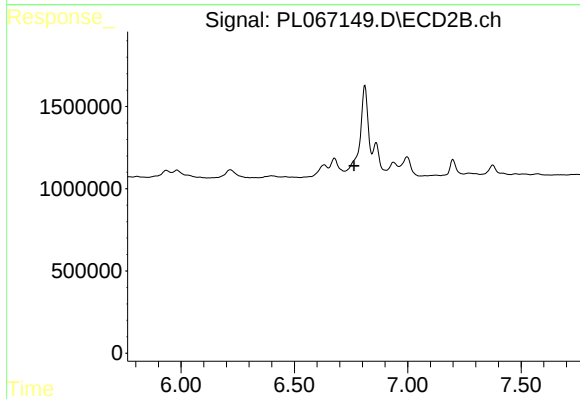

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

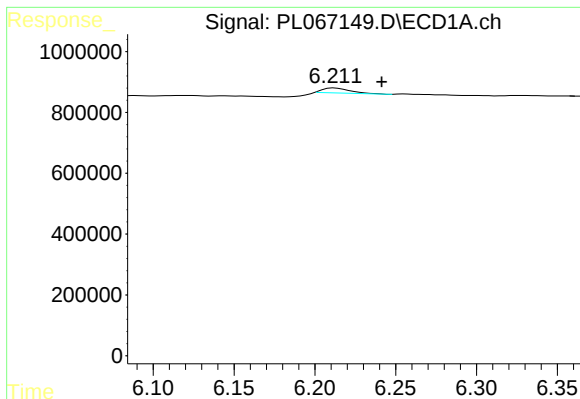

#7 delta-BHC


R.T.: 6.212 min
Delta R.T.: -0.029 min
Response: 192299
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

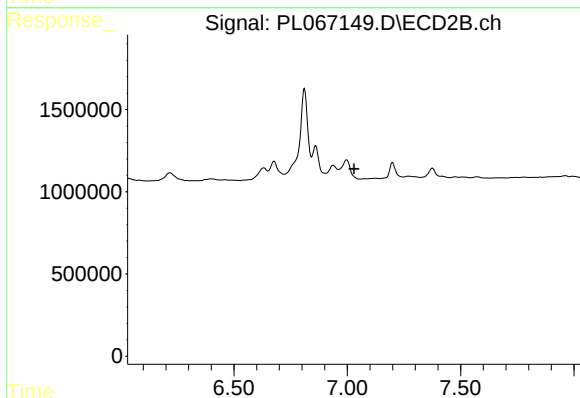


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.030 min
Response: 0
Conc: N.D.

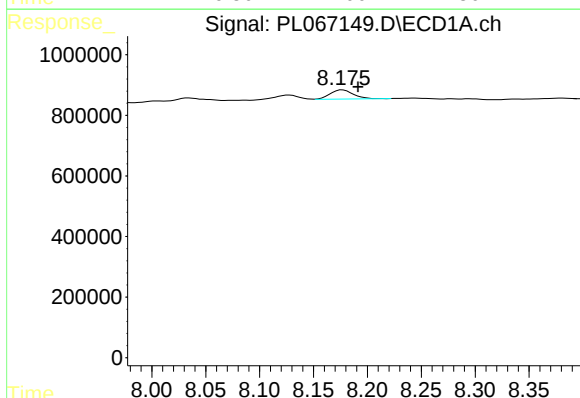


#15 Endosulfan II

R.T.: 8.177 min
Delta R.T.: -0.014 min
Response: 455890
Conc: 0.88 ng/ml

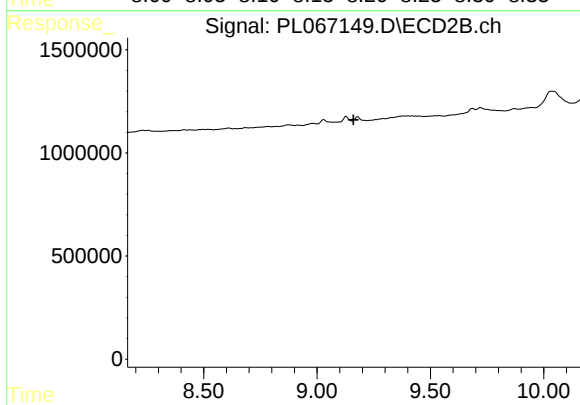

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.161 min
Response: 0
Conc: N.D.

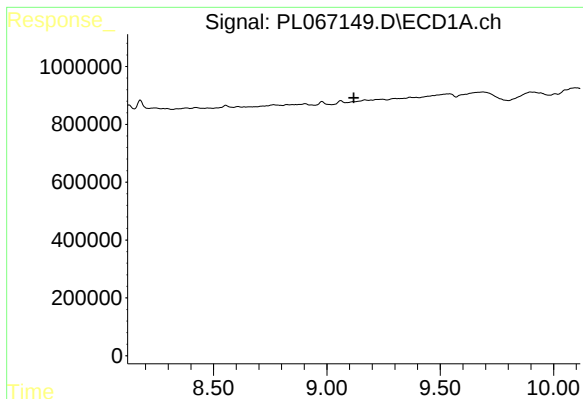

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.119 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

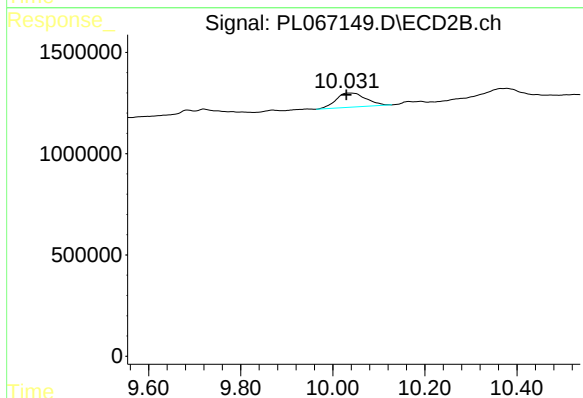


#21 Endrin ketone

R.T.: 10.034 min
Delta R.T.: 0.004 min
Response: 3158066
Conc: 4.36 ng/ml

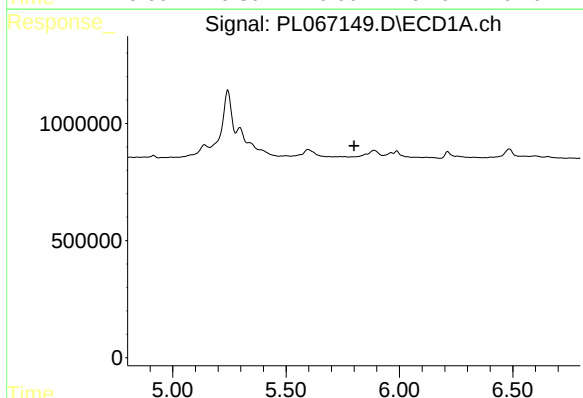


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

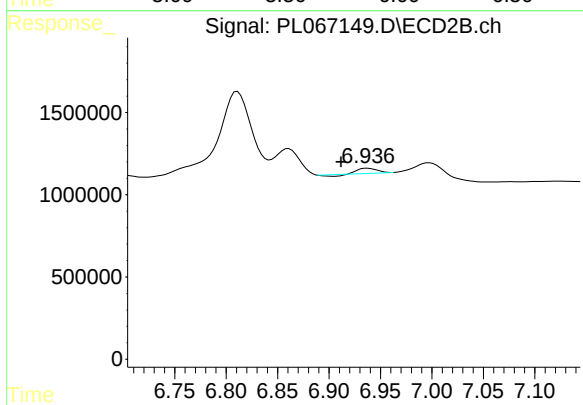

#23 Chlordane-1


R.T.: 6.937 min
Delta R.T.: 0.025 min
Response: 338708
Conc: 16.53 ng/ml

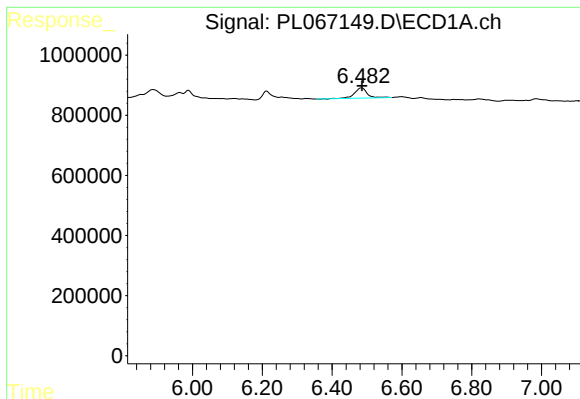

#24 Chlordane-2


R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 862885
Conc: 39.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

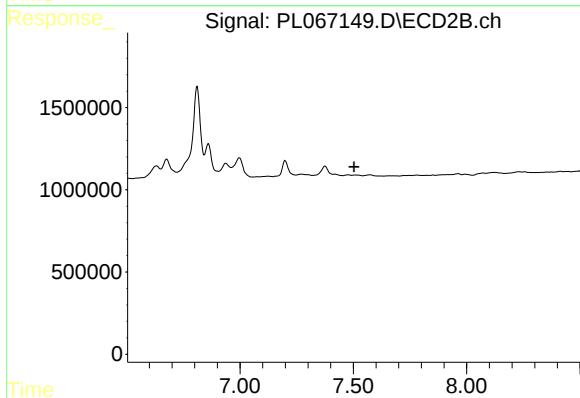


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

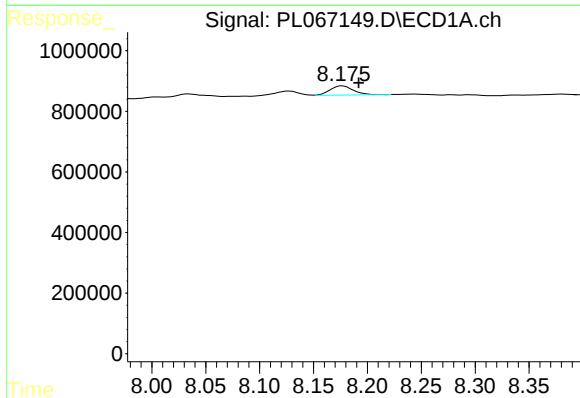


#27 Chlordane-5

R.T.: 8.177 min
Delta R.T.: -0.015 min
Response: 455890
Conc: 24.16 ng/ml

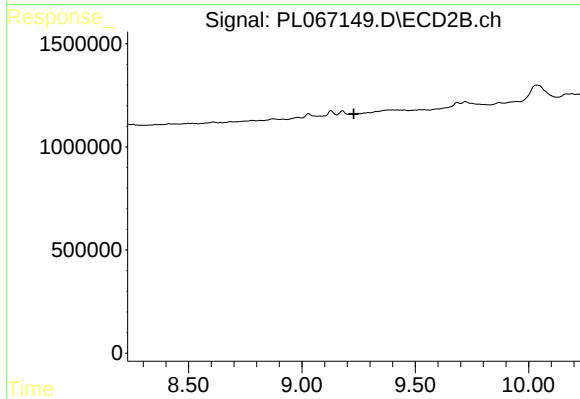

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

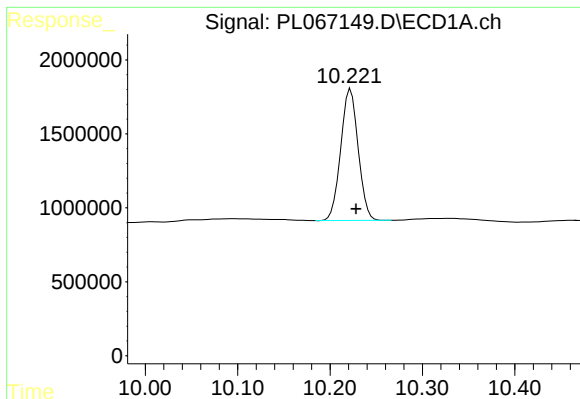

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.006 min
Response: 11663890
Conc: 18.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

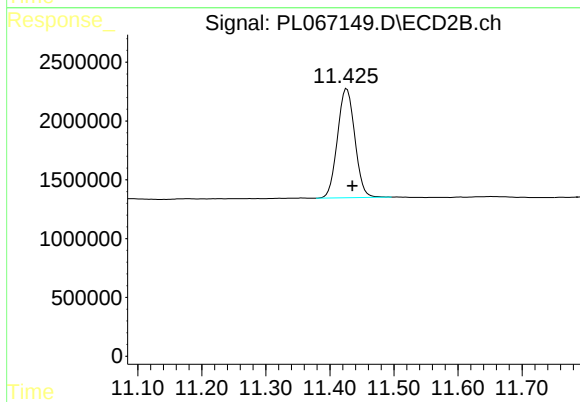

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.008 min
Response: 17408470
Conc: 20.86 ng/ml