

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 21:53
 Operator : AR\AJ
 Sample : M2589-24
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B8(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:25:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	8568874	15544095	20.925	24.029
28)	SA Decachlor...	10.221	11.426	13079921	19476185	20.228	23.343
Target Compounds							
2)	A alpha-BHC	0.000	6.088f	0	438959	N.D.	0.556 #
7)	B delta-BHC	0.000	7.003f	0	1237116	N.D.	1.629 #
11)	B alpha-Chl...	7.255	0.000	336762	0	0.586	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	364969	N.D.	0.592 #
24)	Chlordane-2	6.481	0.000	406110	0	18.584	N.D. #
26)	Chlordane-4	7.255	0.000	336762	0	5.276	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 21:53
Operator : AR\AJ
Sample : M2589-24
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
18-B8(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:25:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

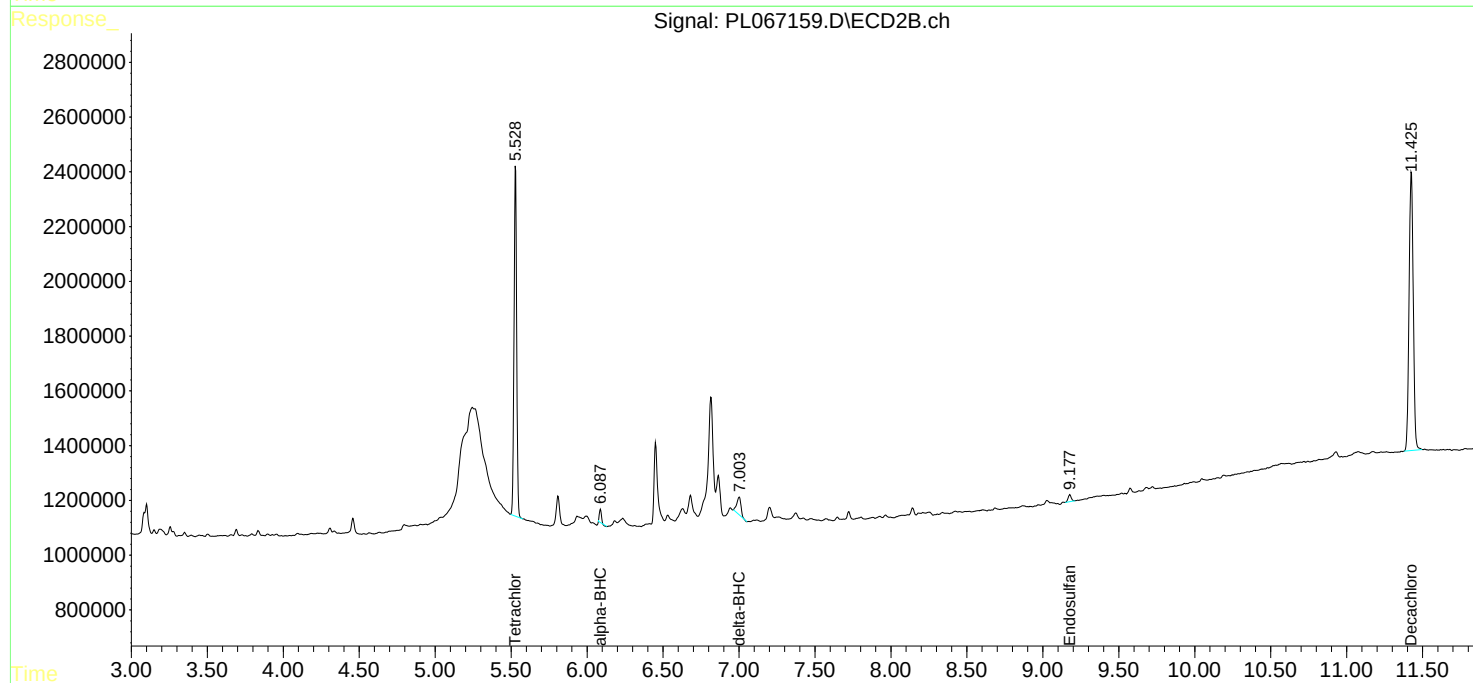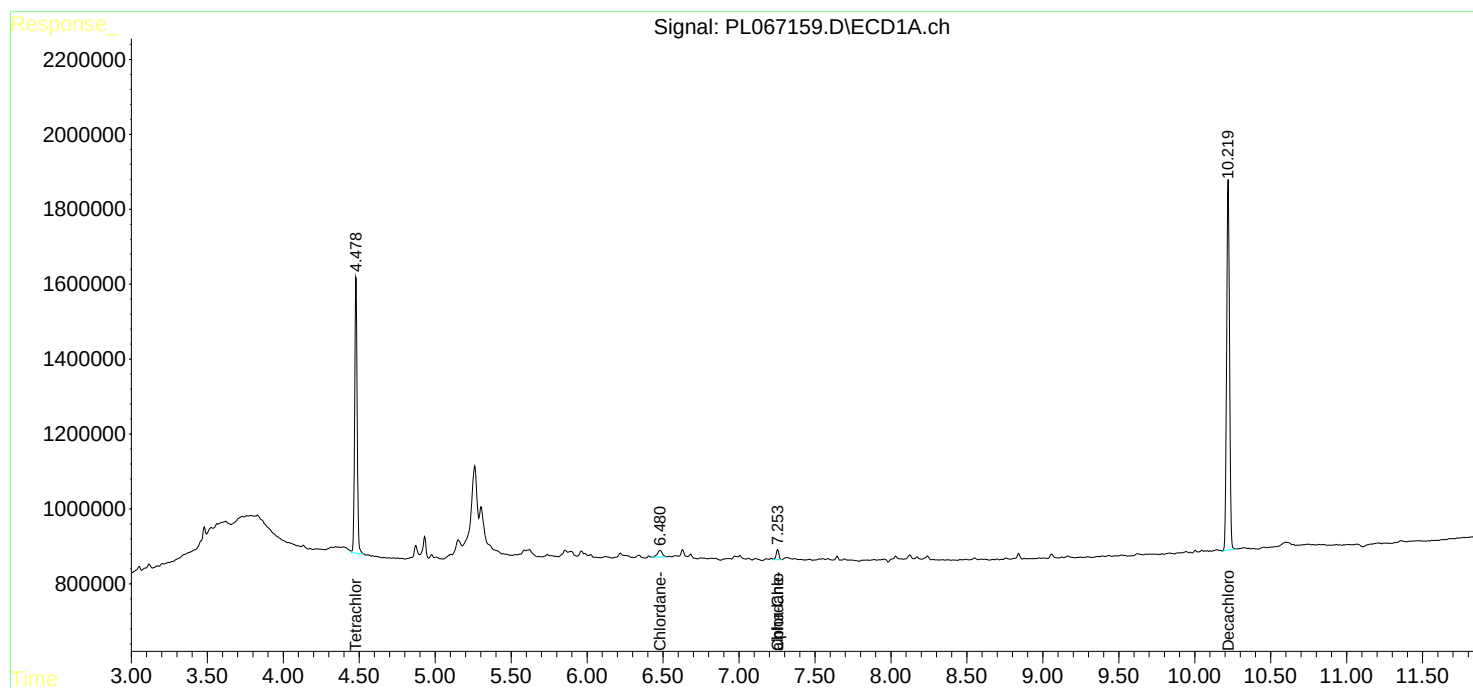


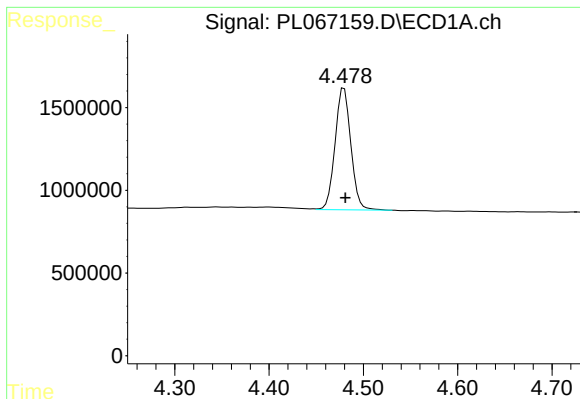

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 8568874
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B8(0-2)

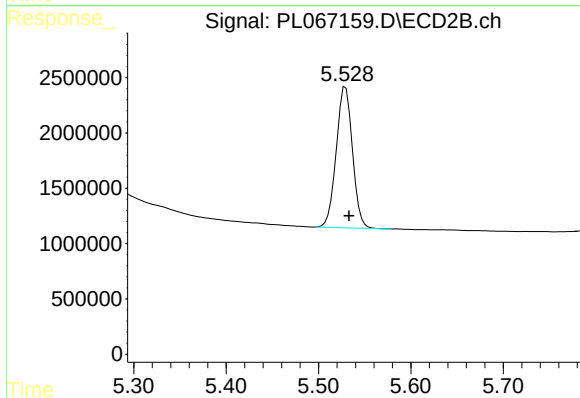


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 15544095
Conc: 24.03 ng/ml

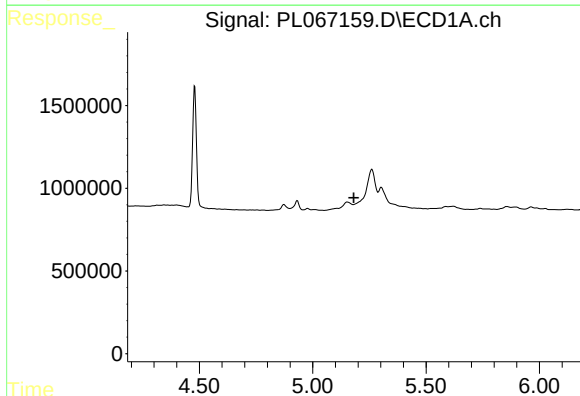


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.182 min
Response: 0
Conc: N.D.

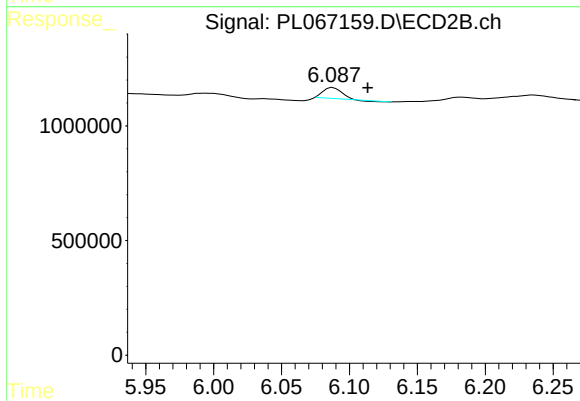

#2 alpha-BHC


R.T.: 6.088 min
Delta R.T.: -0.025 min
Response: 438959
Conc: 0.56 ng/ml

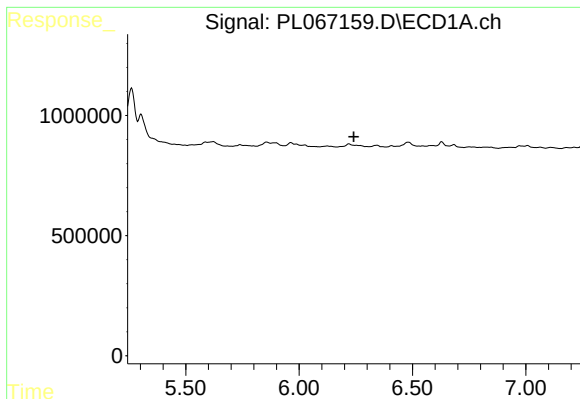

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B8(0-2)

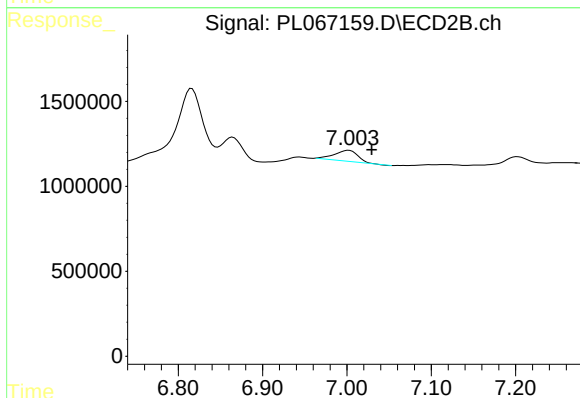


#7 delta-BHC

R.T.: 7.003 min
Delta R.T.: -0.027 min
Response: 1237116
Conc: 1.63 ng/ml

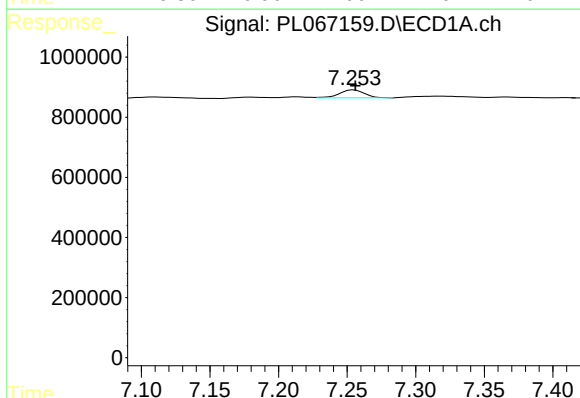


#11 alpha-Chlordane

R.T.: 7.255 min
Delta R.T.: -0.001 min
Response: 336762
Conc: 0.59 ng/ml

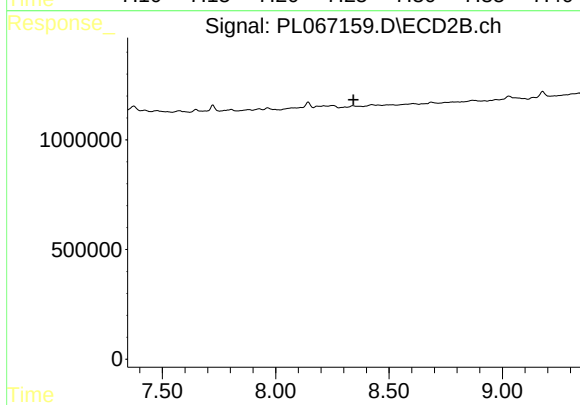

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.344 min
Response: 0
Conc: N.D.

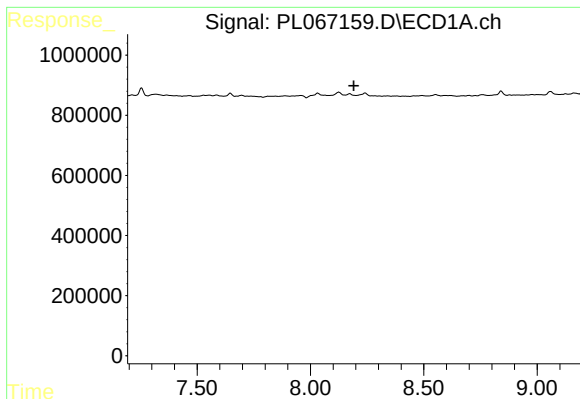

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B8(0-2)

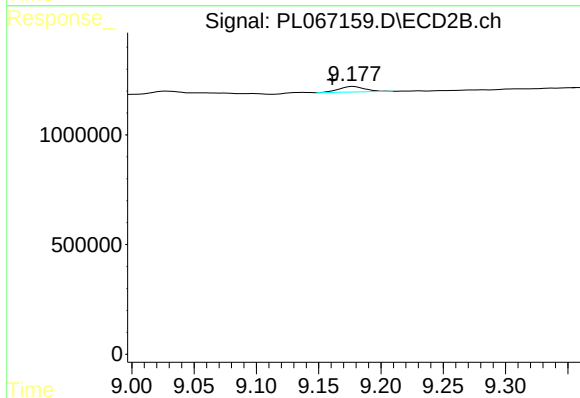


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 364969
Conc: 0.59 ng/ml

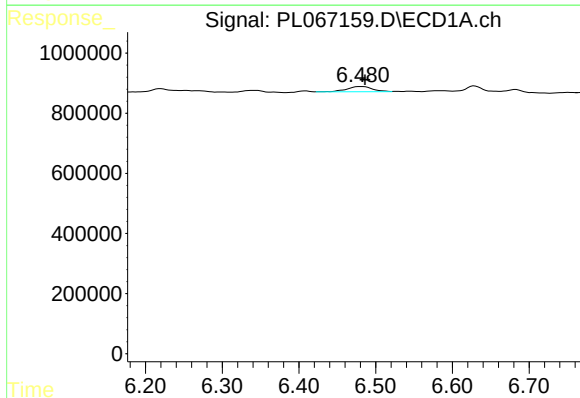


#24 Chlordane-2

R.T.: 6.481 min
Delta R.T.: -0.005 min
Response: 406110
Conc: 18.58 ng/ml

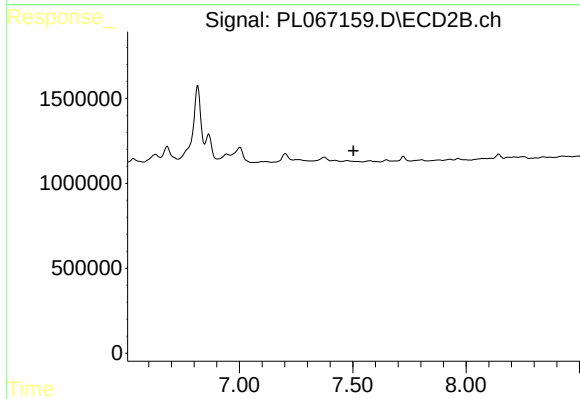

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

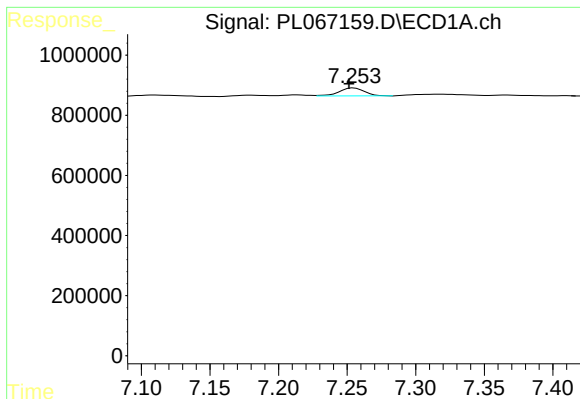

#26 Chlordane-4


R.T.: 7.255 min
Delta R.T.: 0.004 min
Response: 336762
Conc: 5.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B8(0-2)

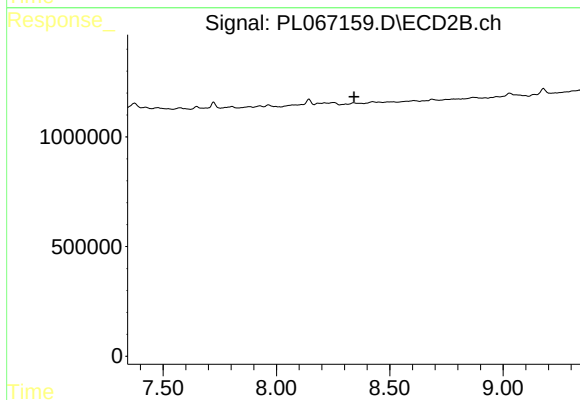


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

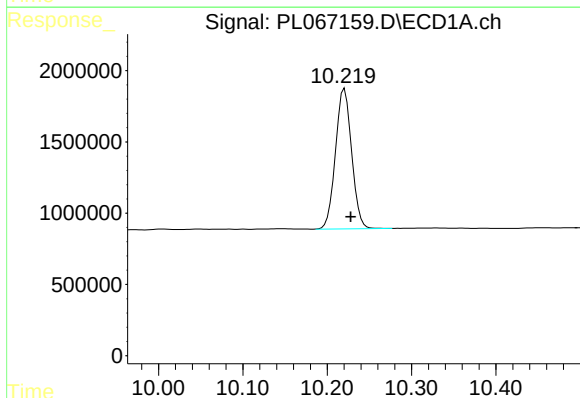

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 13079921
Conc: 20.23 ng/ml

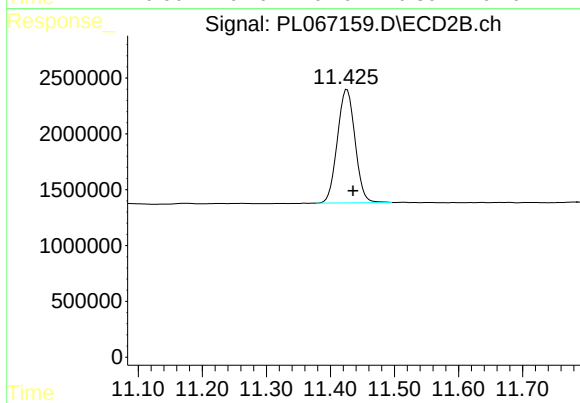

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.009 min
Response: 19476185
Conc: 23.34 ng/ml