

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 22:10
 Operator : AR\AJ
 Sample : M2589-25
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B8(2-4)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:25:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	9304679	16741555	22.722	25.880
28)	SA Decachlor...	10.221	11.425	12592037	18814588	19.473	22.550
Target Compounds							
2)	A alpha-BHC	0.000	6.088f	0	268708	N.D.	0.340 #
3)	MA gamma-BHC...	5.588	0.000	300716	0	0.540	N.D. #
5)	MB Aldrin	0.000	7.531	0	274494	N.D.	0.376 #
7)	B delta-BHC	0.000	7.003f	0	1059241	N.D.	1.395 #
11)	B alpha-Chl...	7.255	0.000	194081	0	0.338	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	748943	N.D.	1.214 #
24)	Chlordane-2	6.479	7.531f	589585	274494	26.980	9.322 #
26)	Chlordane-4	7.255	0.000	194081	0	3.041	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 22:10
Operator : AR\AJ
Sample : M2589-25
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:25:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

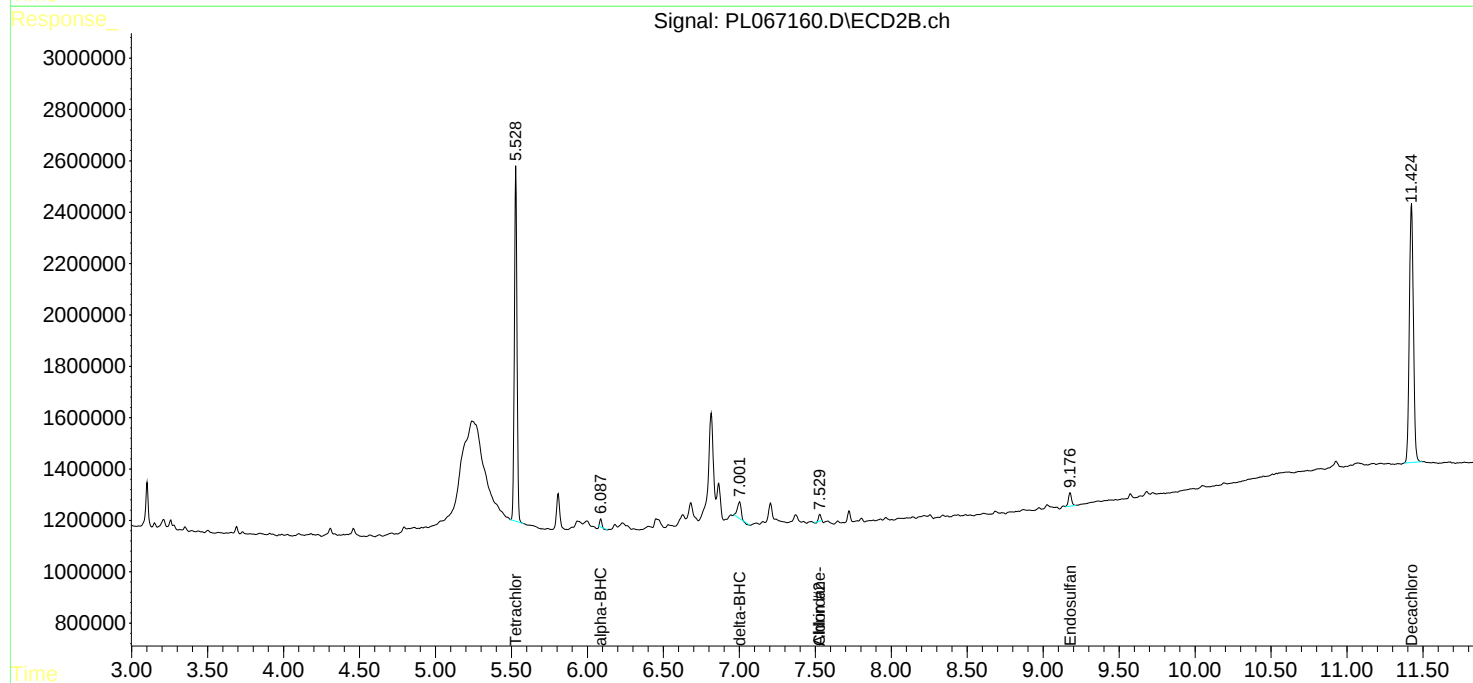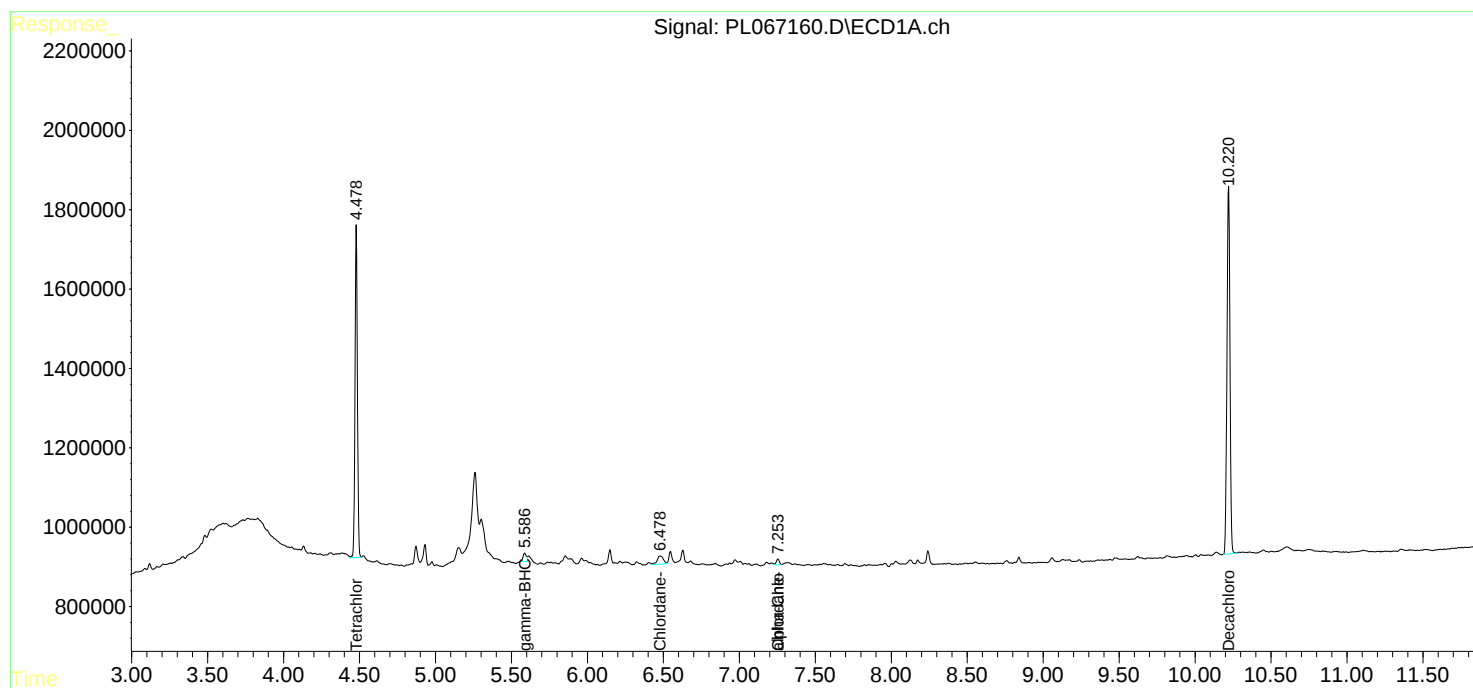


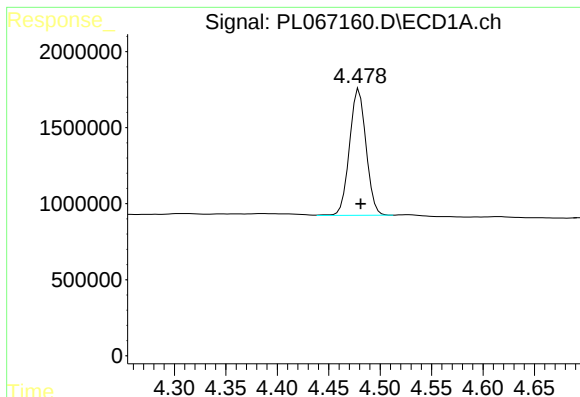

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 9304679
Conc: 22.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

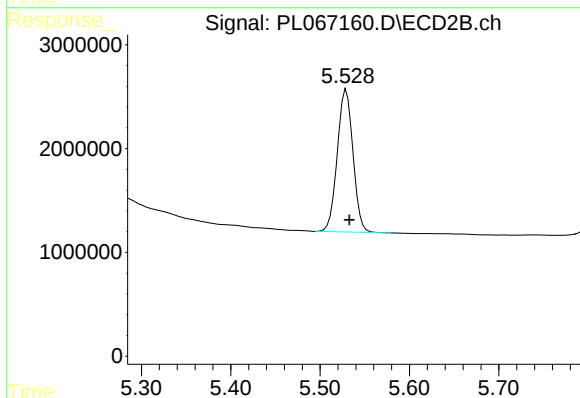


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 16741555
Conc: 25.88 ng/ml

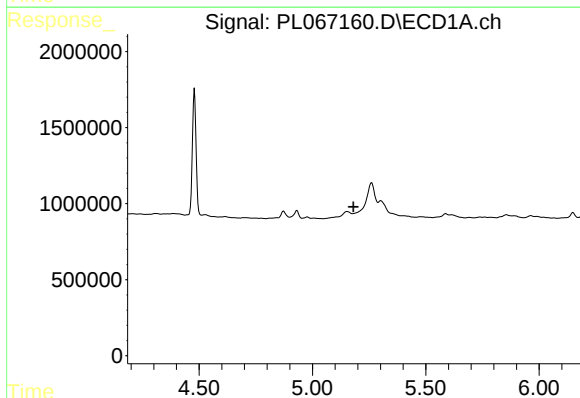


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.182 min
Response: 0
Conc: N.D.

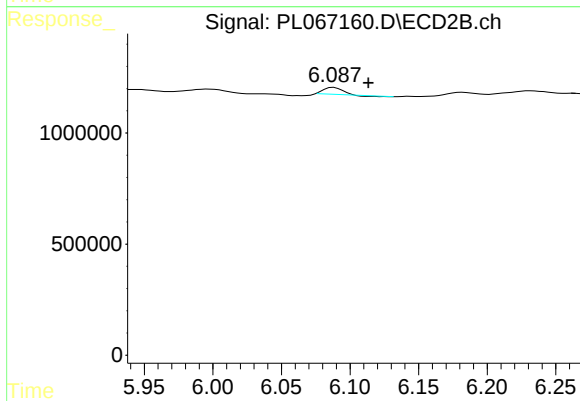

#2 alpha-BHC


R.T.: 6.088 min
Delta R.T.: -0.025 min
Response: 268708
Conc: 0.34 ng/ml

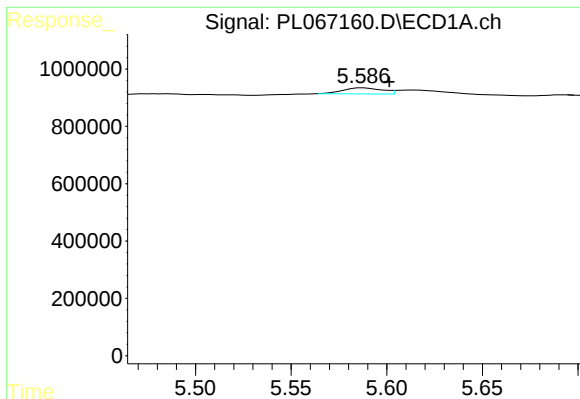

#3 gamma-BHC (Lindane)


R.T.: 5.588 min
Delta R.T.: -0.014 min
Response: 300716
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

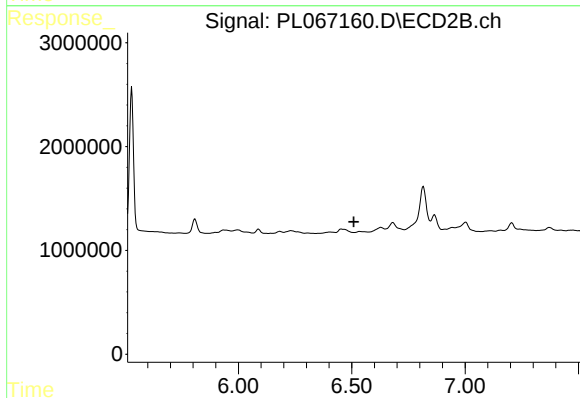


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

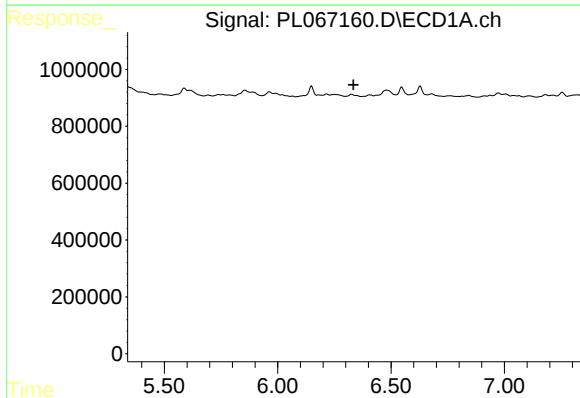


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.335 min
Response: 0
Conc: N.D.

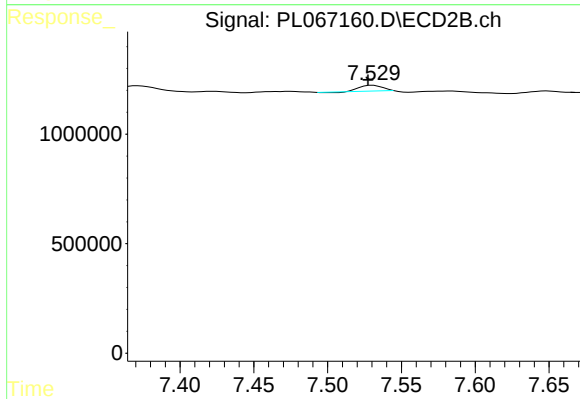

#5 Aldrin


R.T.: 7.531 min
Delta R.T.: 0.003 min
Response: 274494
Conc: 0.38 ng/ml

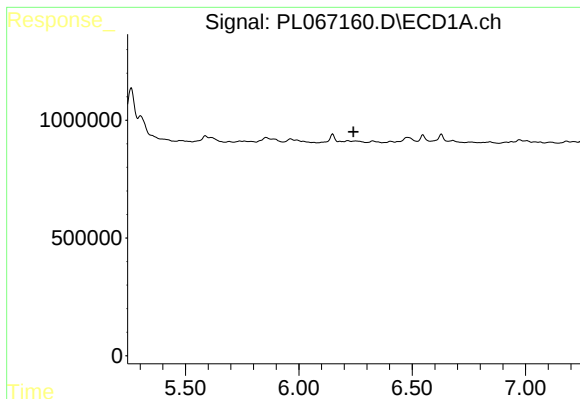

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

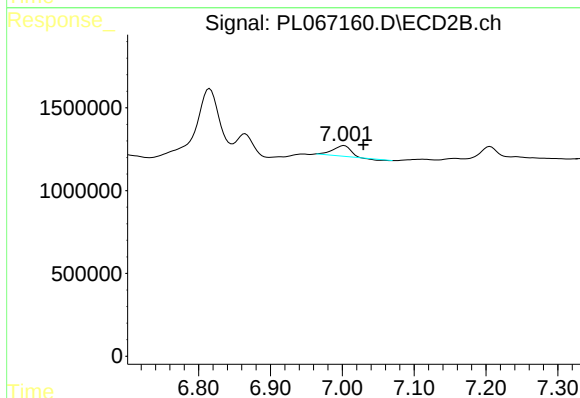


#7 delta-BHC

R.T.: 7.003 min
Delta R.T.: -0.027 min
Response: 1059241
Conc: 1.39 ng/ml

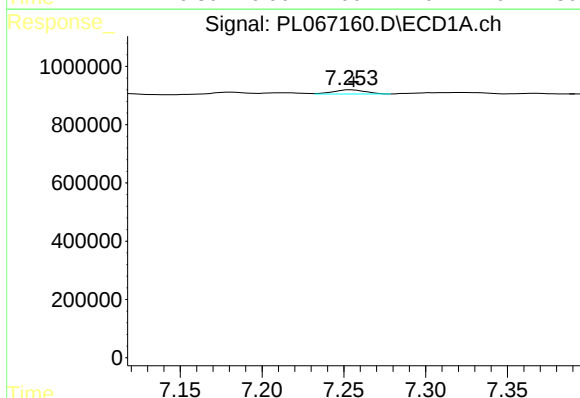


#11 alpha-Chlordane

R.T.: 7.255 min
Delta R.T.: -0.002 min
Response: 194081
Conc: 0.34 ng/ml

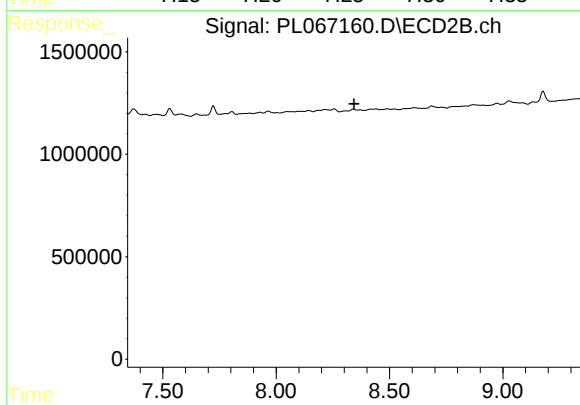

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.344 min
Response: 0
Conc: N.D.

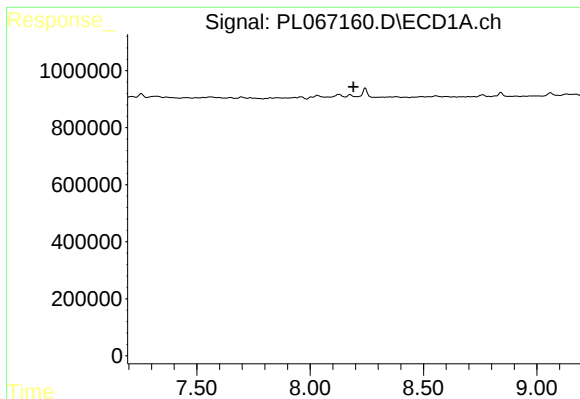

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

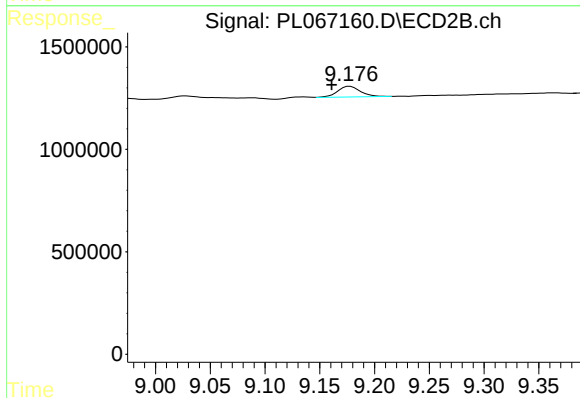


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 748943
Conc: 1.21 ng/ml

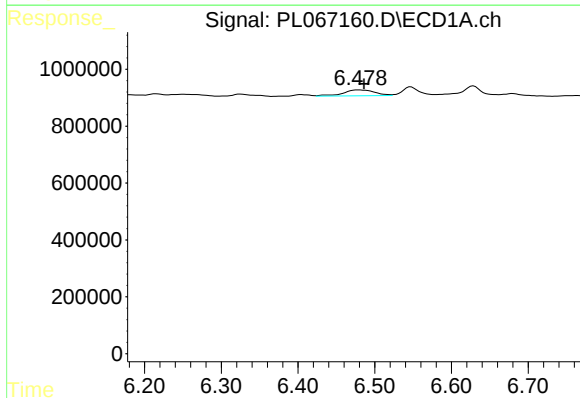


#24 Chlordane-2

R.T.: 6.479 min
Delta R.T.: -0.007 min
Response: 589585
Conc: 26.98 ng/ml

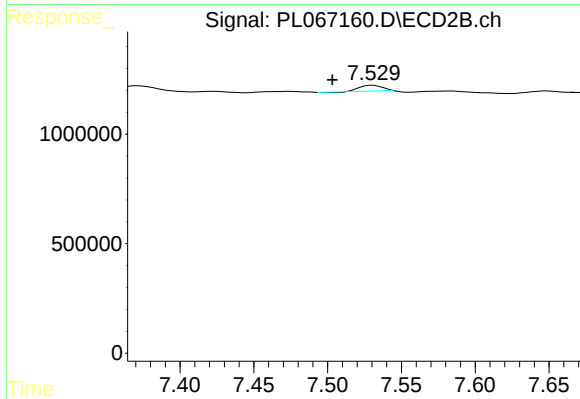

#24 Chlordane-2


R.T.: 7.531 min
Delta R.T.: 0.027 min
Response: 274494
Conc: 9.32 ng/ml

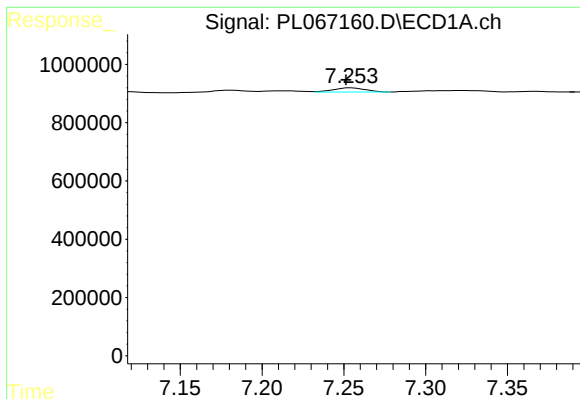

#26 Chlordane-4


R.T.: 7.255 min
Delta R.T.: 0.003 min
Response: 194081
Conc: 3.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B8(2-4)

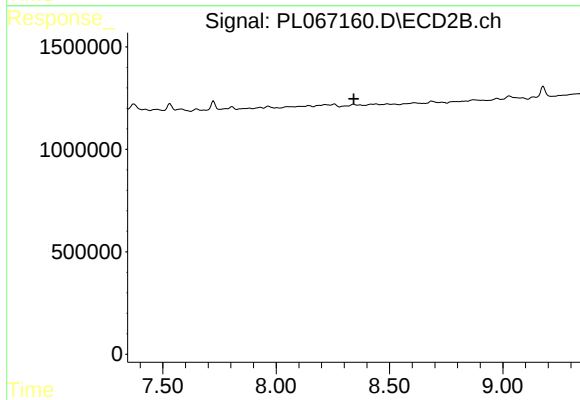


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

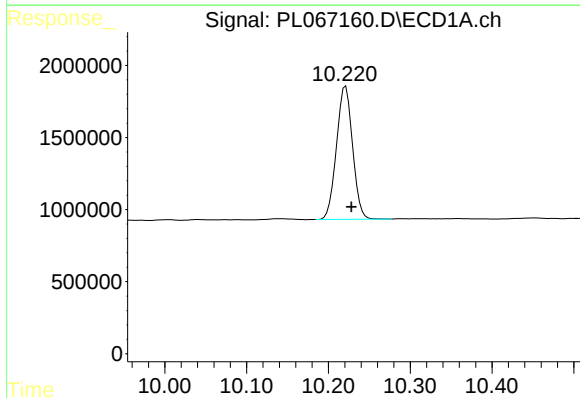

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 12592037
Conc: 19.47 ng/ml

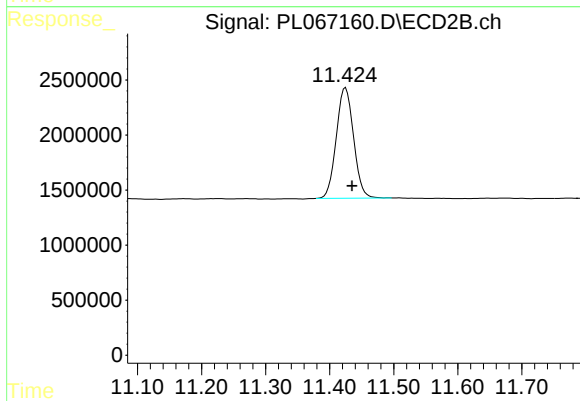

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.010 min
Response: 18814588
Conc: 22.55 ng/ml