

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 23:16
 Operator : AR\AJ
 Sample : M2589-29
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B9(4-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:26:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	9622636	17105438	23.498	26.442
28)	SA Decachlor...	10.221	11.425	14673878	21784694	22.693	26.110
Target Compounds							
3)	MA gamma-BHC...	0.000	6.532f	0	1114379	N.D.	1.471 #
4)	MA Heptachlor	6.024	0.000	232818	0	0.443	N.D. #
7)	B delta-BHC	0.000	7.003f	0	1246473	N.D.	1.642 #
9)	A Endosulfan I	0.000	8.422f	0	400362	N.D.	0.626 #
13)	MA Dieldrin	7.582	8.692	430506	299563	0.772	0.453 #
15)	B Endosulfa...	0.000	9.178f	0	336013	N.D.	0.545 #
21)	B Endrin ke...	0.000	10.048f	0	176899	N.D.	0.244 #
24)	Chlordane-2	6.484	0.000	375615	0	17.189	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 23:16
Operator : AR\AJ
Sample : M2589-29
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
18-B9(4-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:26:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

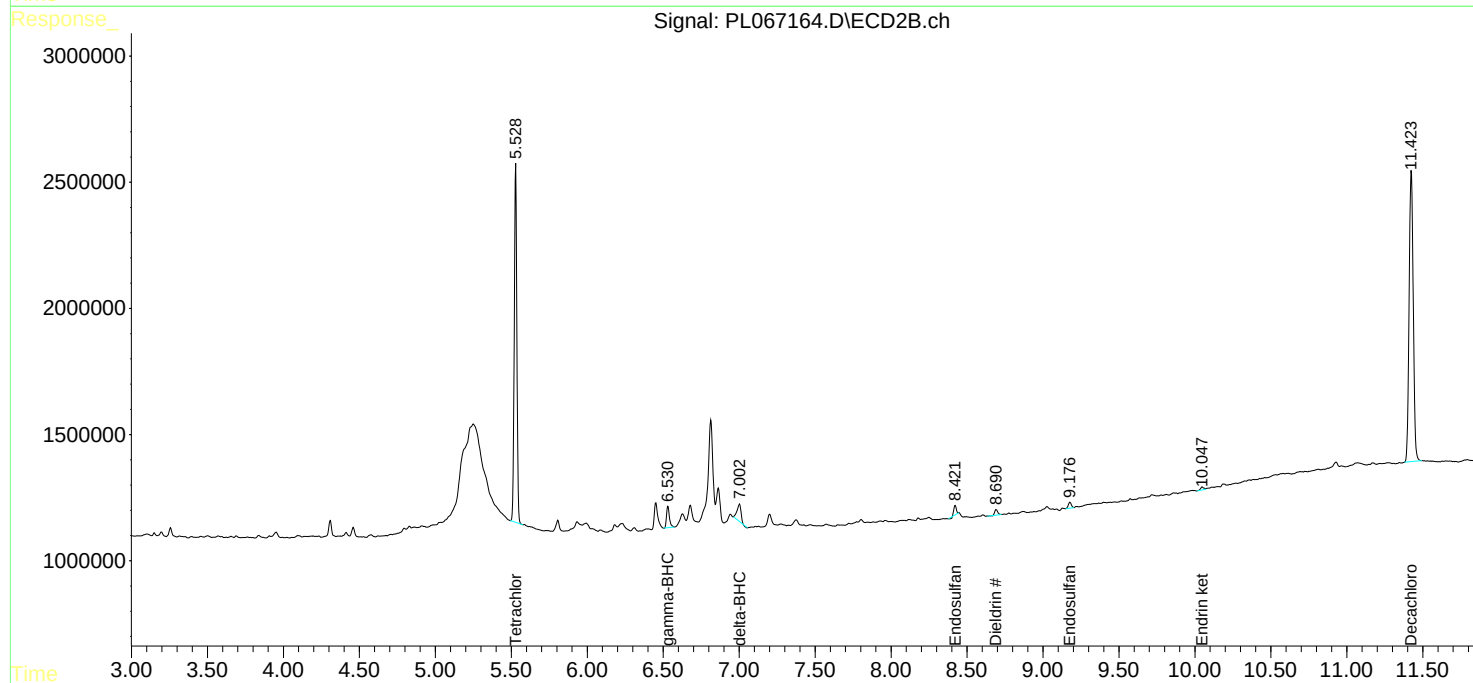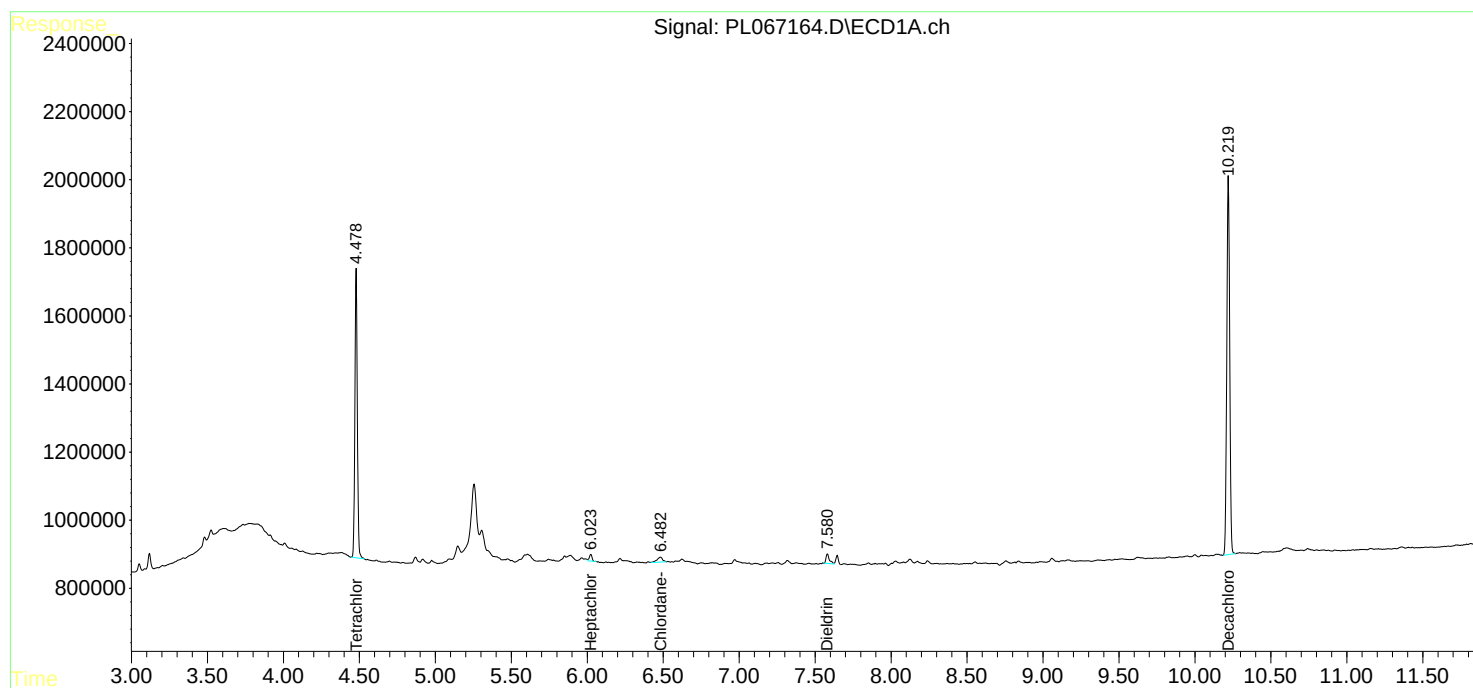


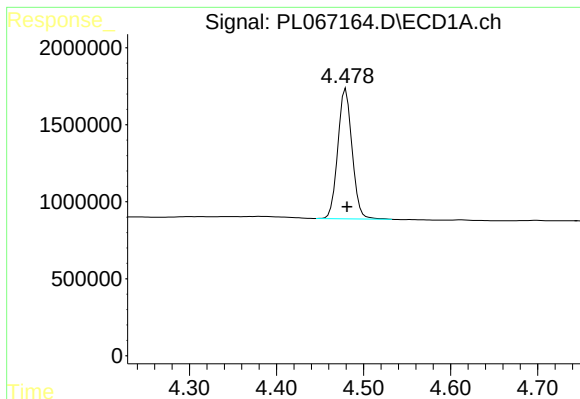

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 9622636
Conc: 23.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B9(4-6)

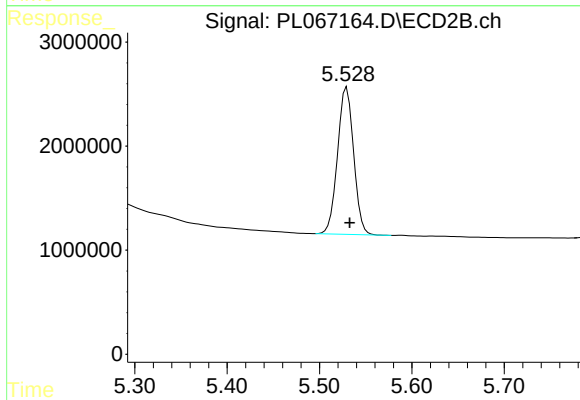


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 17105438
Conc: 26.44 ng/ml

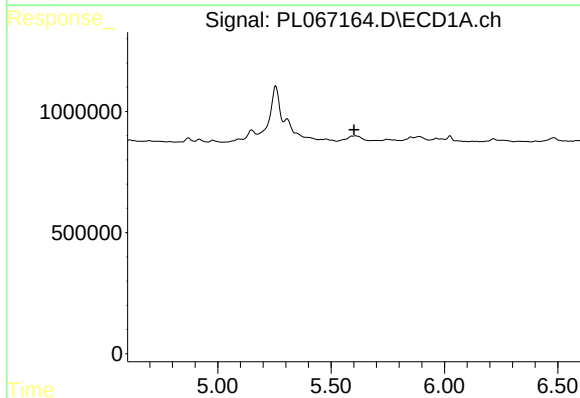


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.601 min
Response: 0
Conc: N.D.

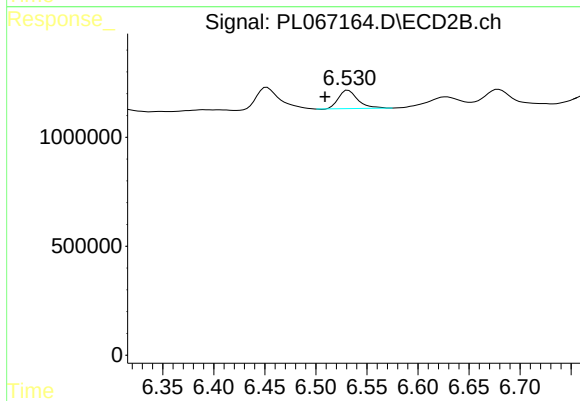

#3 gamma-BHC (Lindane)


R.T.: 6.532 min
Delta R.T.: 0.023 min
Response: 1114379
Conc: 1.47 ng/ml

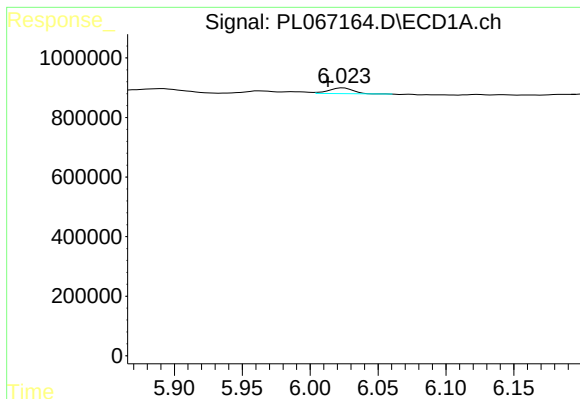

#4 Heptachlor


R.T.: 6.024 min
Delta R.T.: 0.011 min
Response: 232818
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B9(4-6)

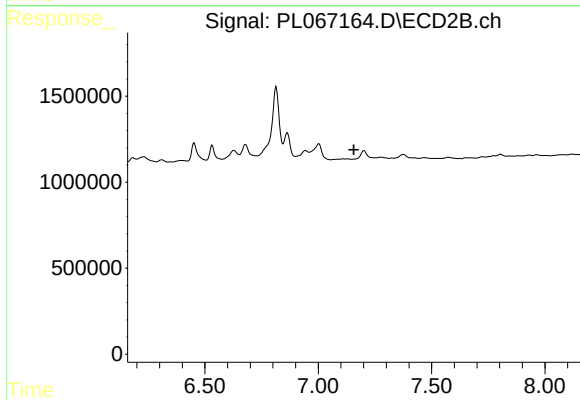


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

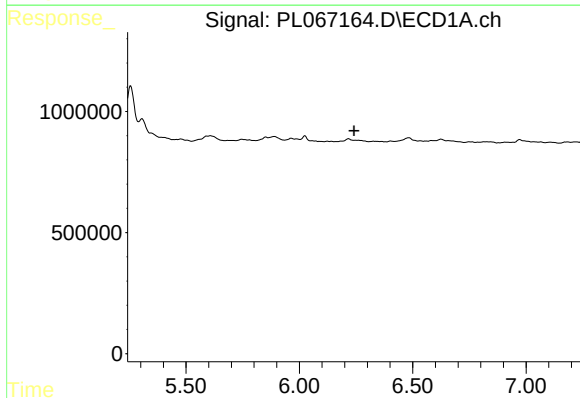


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

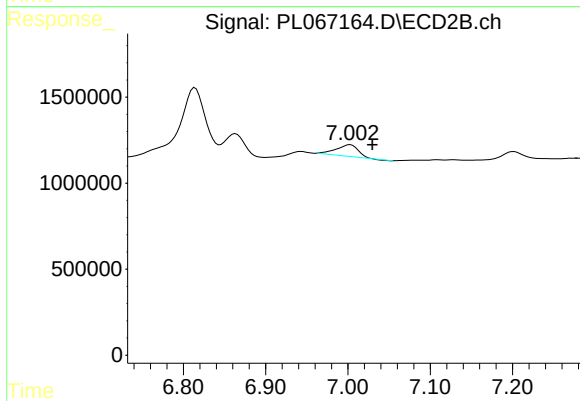

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.027 min
Response: 1246473
Conc: 1.64 ng/ml

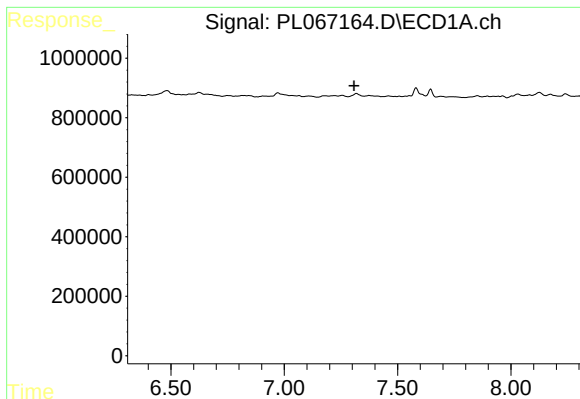

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.308 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B9(4-6)

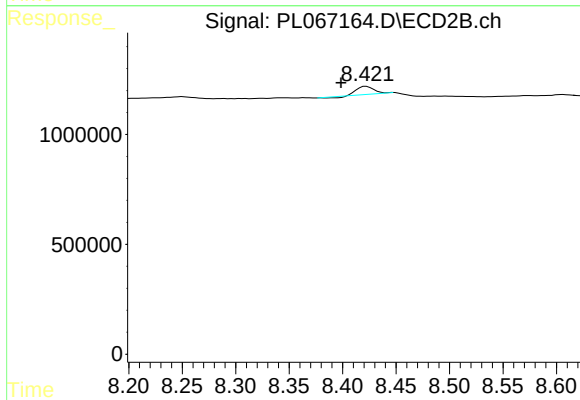


#9 Endosulfan I

R.T.: 8.422 min
Delta R.T.: 0.024 min
Response: 400362
Conc: 0.63 ng/ml

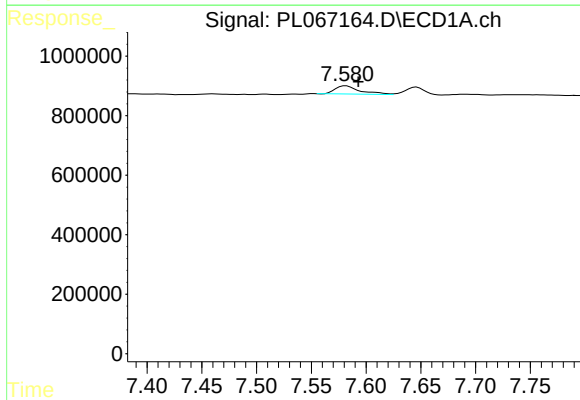


#13 Dieldrin

R.T.: 7.582 min
Delta R.T.: -0.011 min
Response: 430506
Conc: 0.77 ng/ml

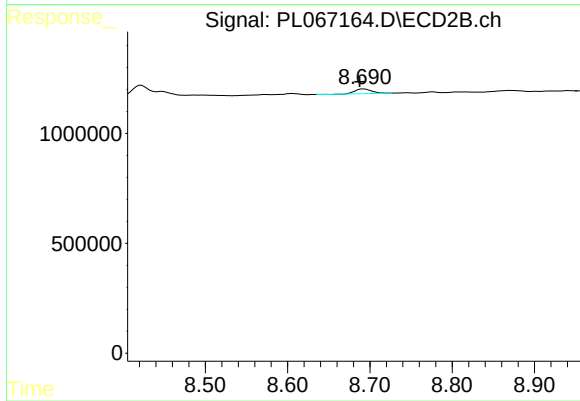

#13 Dieldrin


R.T.: 8.692 min
Delta R.T.: 0.004 min
Response: 299563
Conc: 0.45 ng/ml

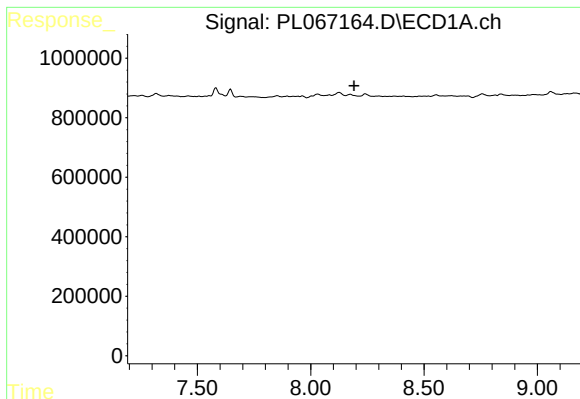

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B9(4-6)

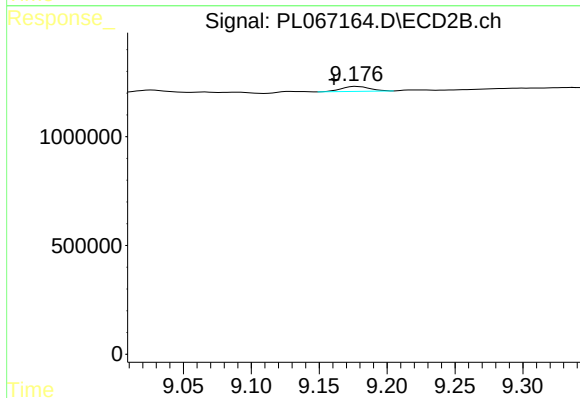


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 336013
Conc: 0.54 ng/ml

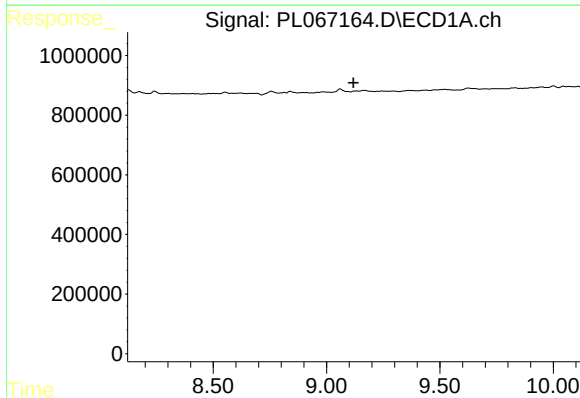


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.119 min
Response: 0
Conc: N.D.

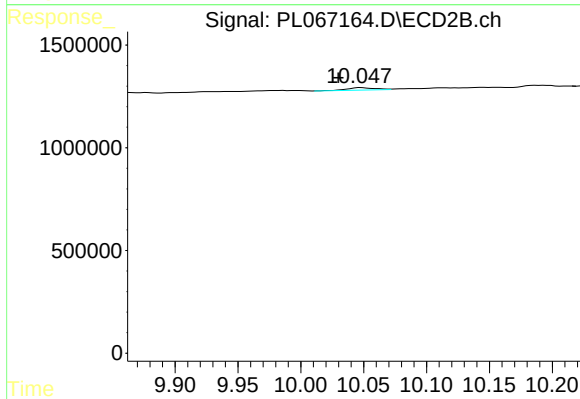

#21 Endrin ketone


R.T.: 10.048 min
Delta R.T.: 0.018 min
Response: 176899
Conc: 0.24 ng/ml

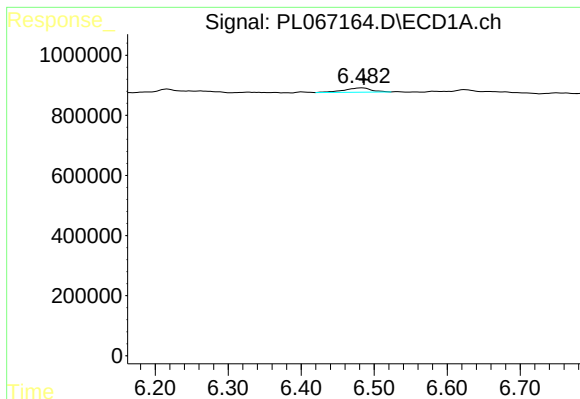

#24 Chlordane-2


R.T.: 6.484 min
Delta R.T.: -0.003 min
Response: 375615
Conc: 17.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B9(4-6)

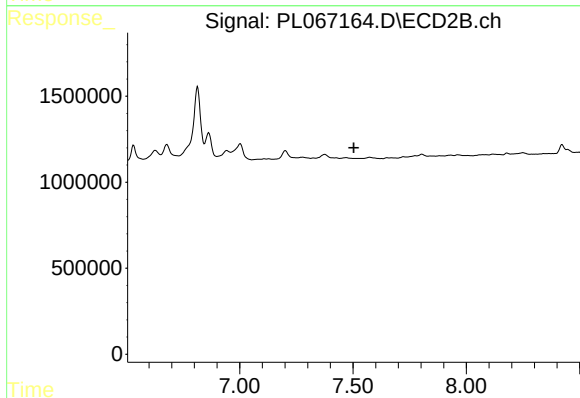


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

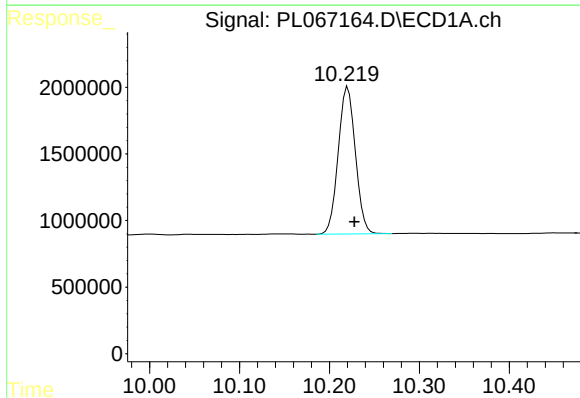

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 14673878
Conc: 22.69 ng/ml

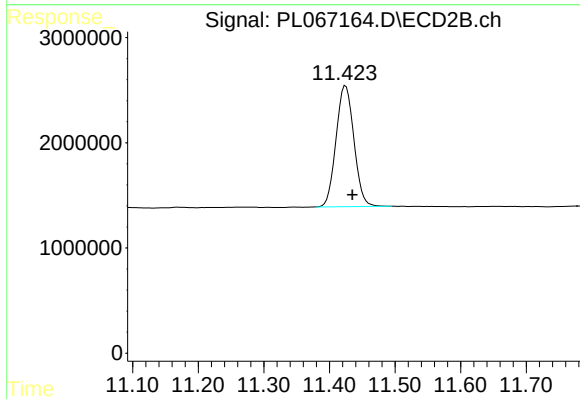

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.010 min
Response: 21784694
Conc: 26.11 ng/ml