

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2021 15:45
 Operator : AR\AJ
 Sample : M2623-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:22:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.529	9132171	15321772	22.301	23.685
28)	SA Decachlor...	10.221	11.426	10038119	14595178	15.524	17.493
Target Compounds							
12)	B 4,4'-DDE	7.469	8.526	331086	322580	0.620	0.493
13)	MA Dieldrin	7.589	8.682	2224502	2845251	3.989	4.304



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2021 15:45
Operator : AR\AJ
Sample : M2623-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:22:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

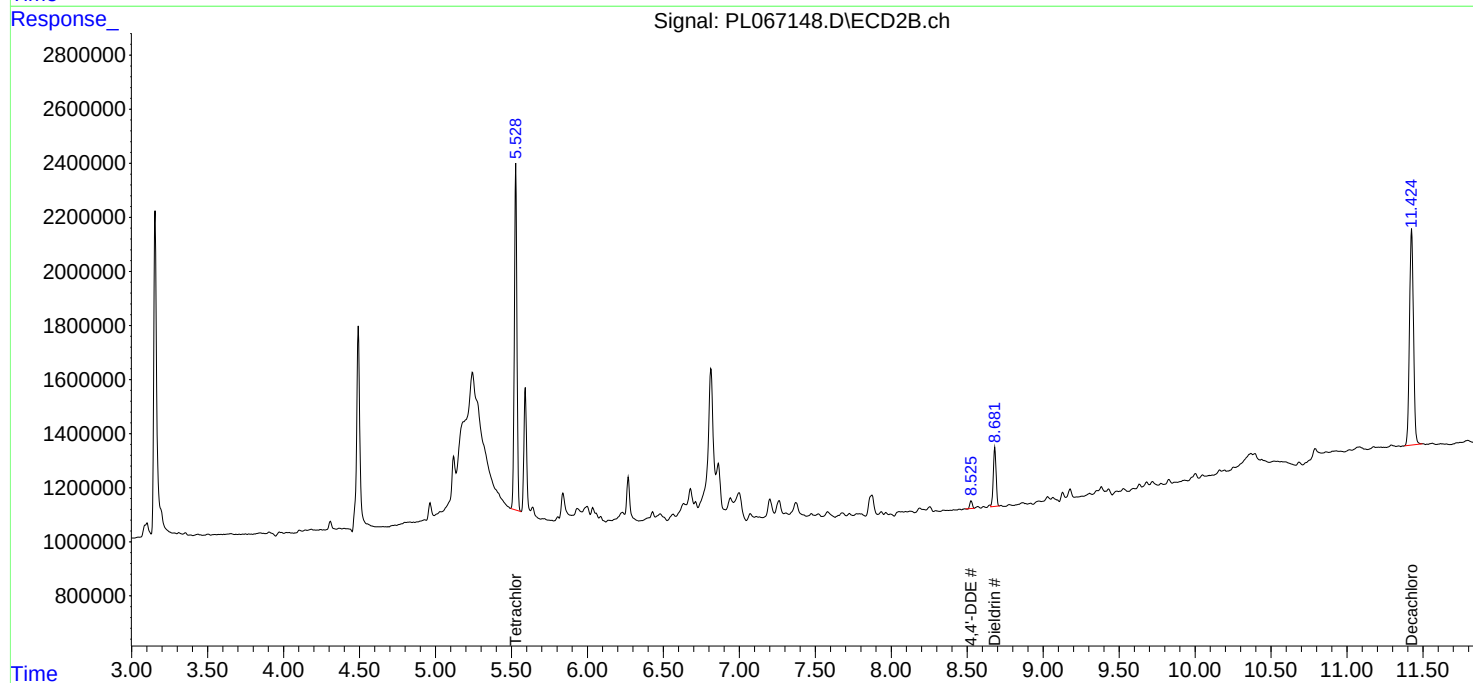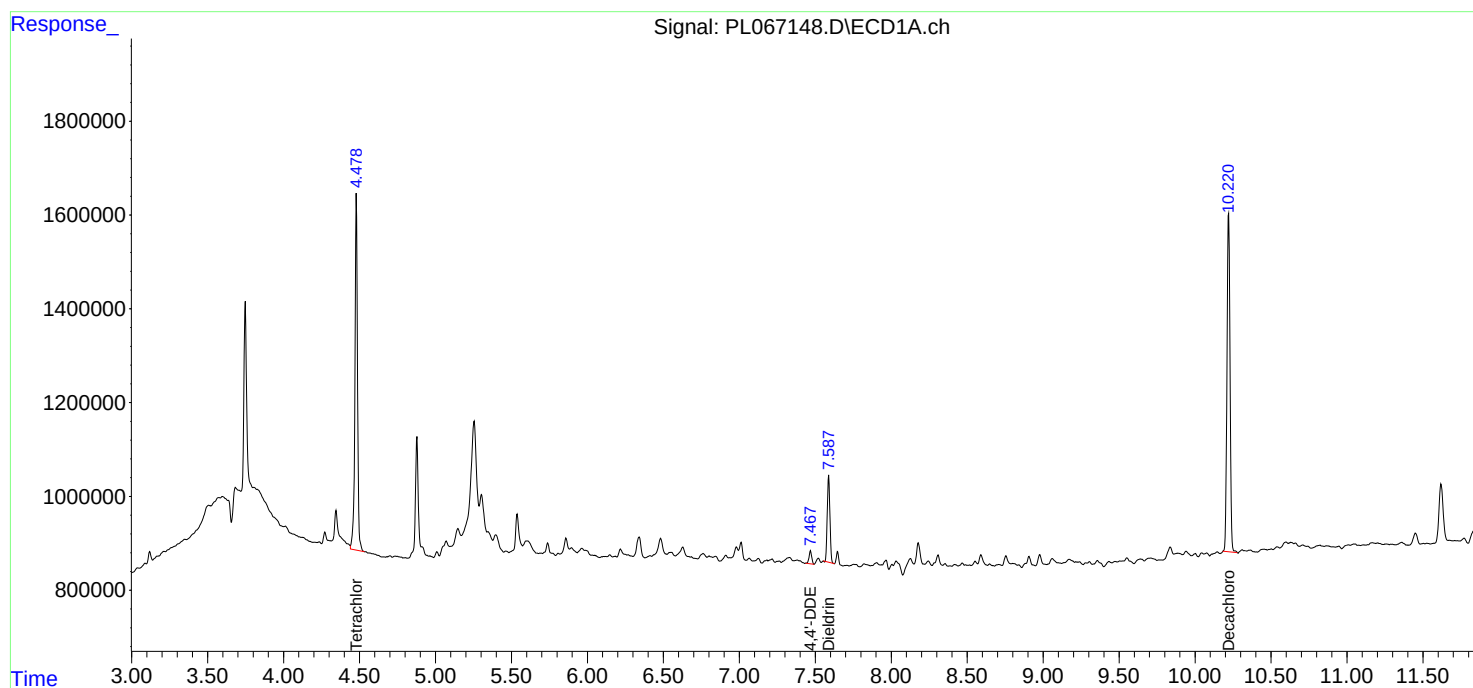


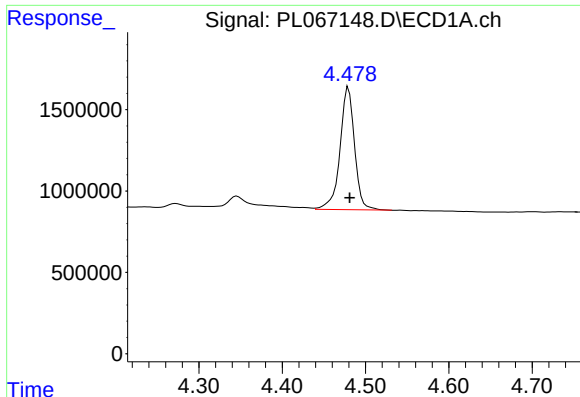

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 9132171
Conc: 22.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-9

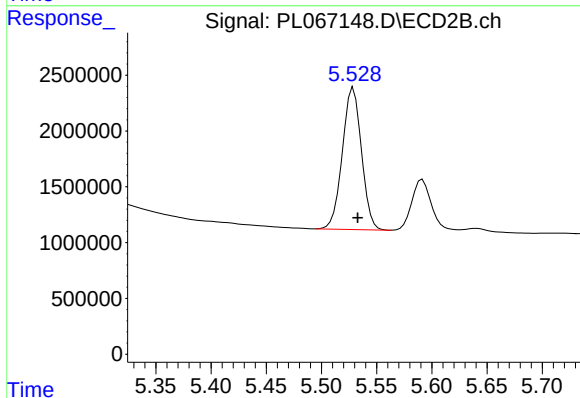


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 15321772
Conc: 23.68 ng/ml

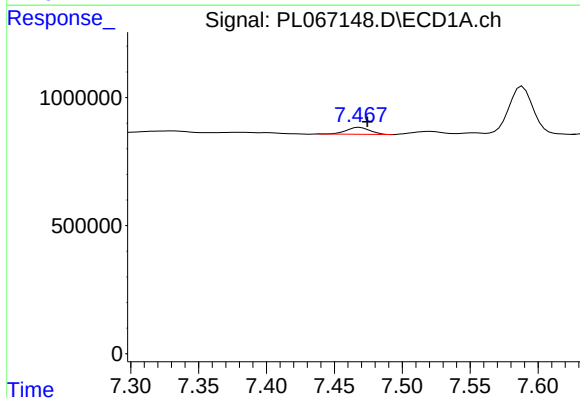


#12 4,4'-DDE

R.T.: 7.469 min
Delta R.T.: -0.006 min
Response: 331086
Conc: 0.62 ng/ml

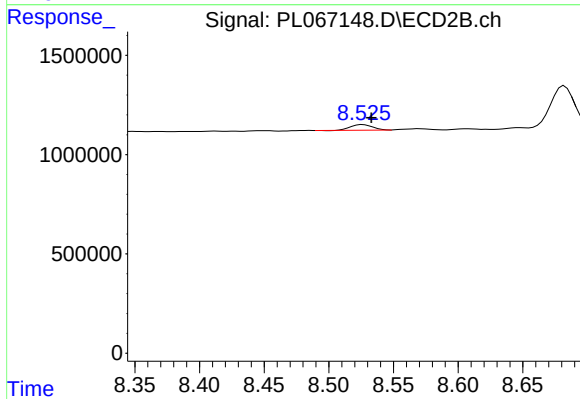

#12 4,4'-DDE


R.T.: 8.526 min
Delta R.T.: -0.006 min
Response: 322580
Conc: 0.49 ng/ml

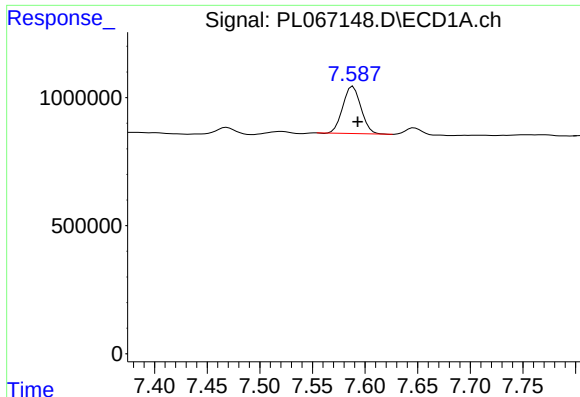

#13 Dieldrin


R.T.: 7.589 min
Delta R.T.: -0.005 min
Response: 2224502
Conc: 3.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-9

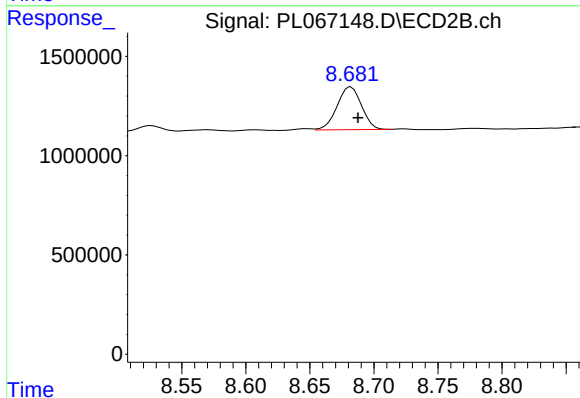


#13 Dieldrin

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 2845251
Conc: 4.30 ng/ml

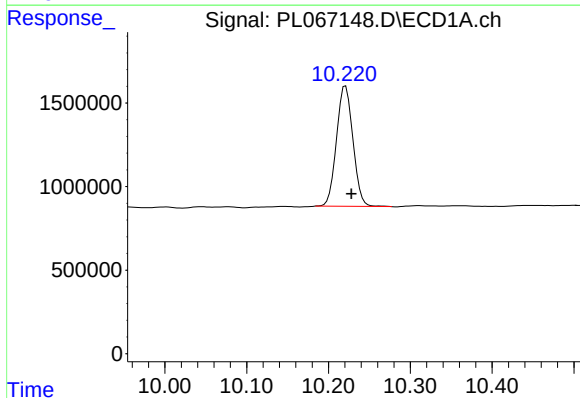

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 10038119
Conc: 15.52 ng/ml

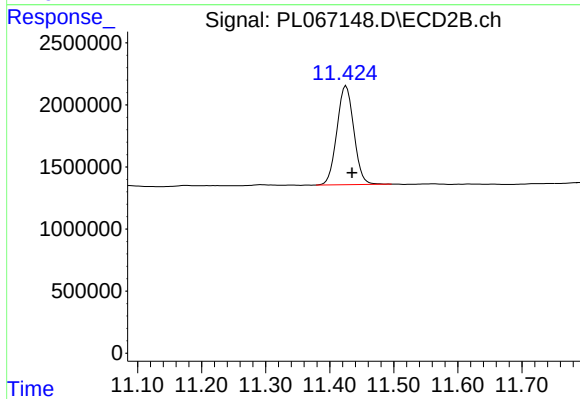

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.009 min
Response: 14595178
Conc: 17.49 ng/ml