

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
 Data File : PL067168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 00:23
 Operator : AR\AJ
 Sample : M2589-33
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B10(4-6)

Manual Integrations
 APPROVED

Ankita
 6/8/2021 11:55:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:27:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	9125056	19067008	22.283	29.474 #
28)	SA Decachlor...	10.221	11.427	15594225	22961686	24.116	27.520
Target Compounds							
12)	B 4,4'-DDE	7.468	8.525	218890	183045	0.410	0.280m#
20)	A Methoxychlor	8.904	9.867	676674	808694	2.270	2.546

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060721\
Data File : PL067168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 00:23
Operator : AR\AJ
Sample : M2589-33
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
18-B10(4-6)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:55:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:27:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

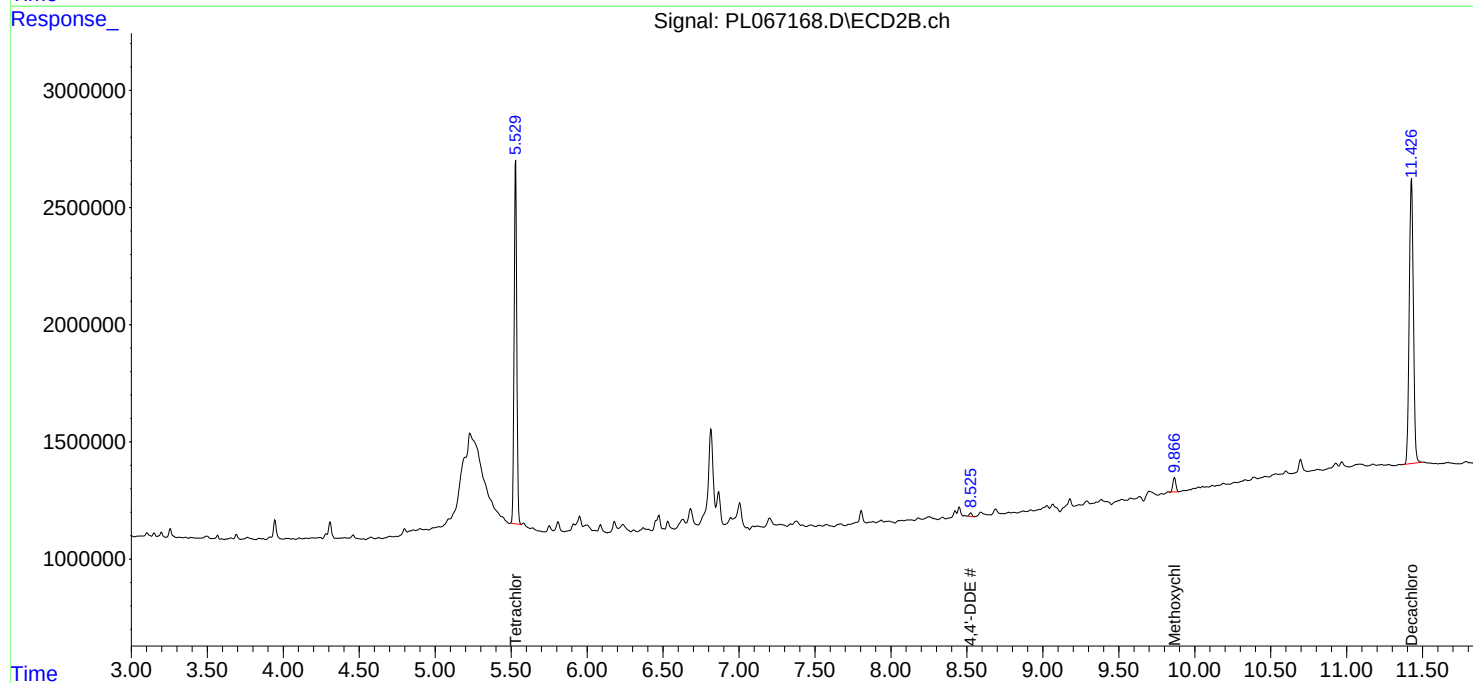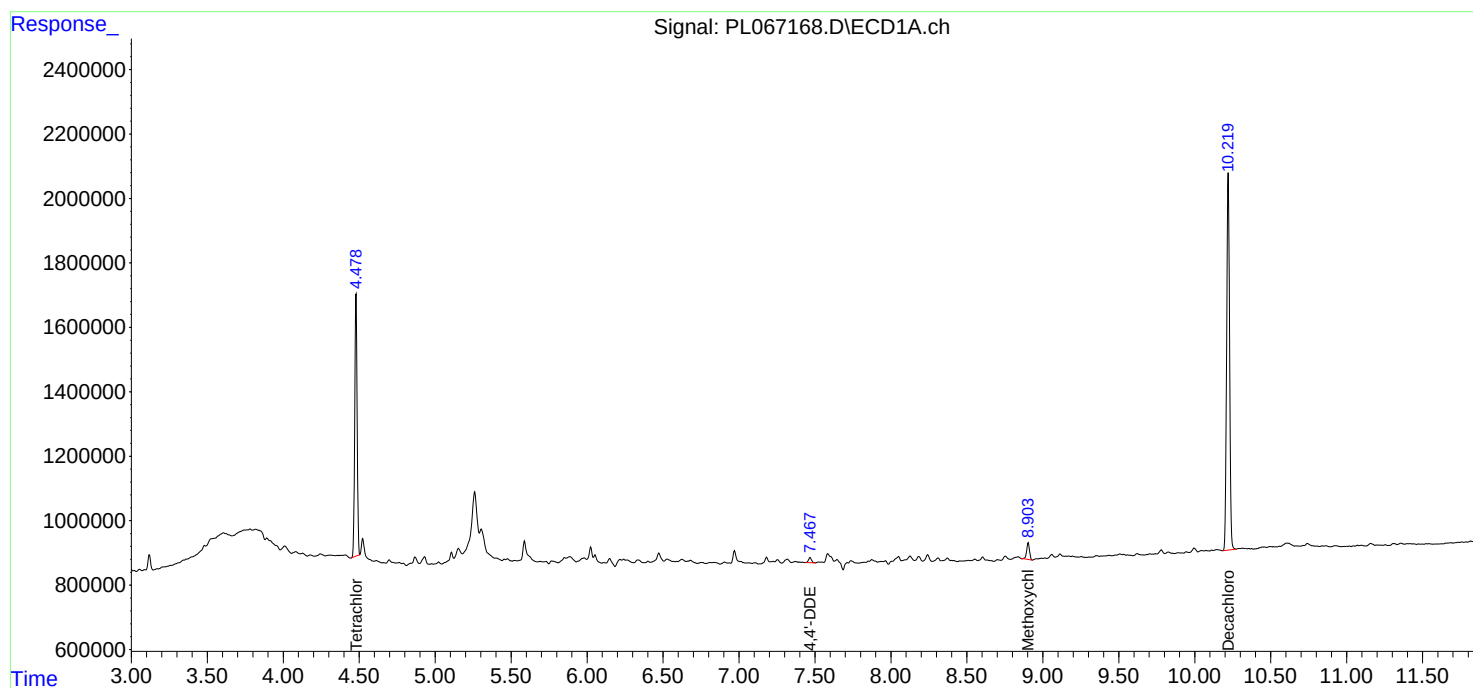

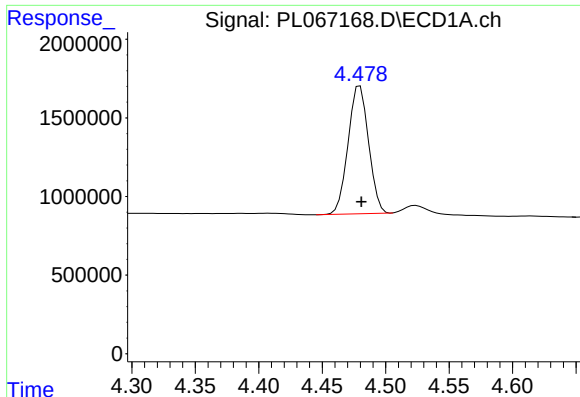


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 9125056
Conc: 22.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B10(4-6)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:55:39 AM

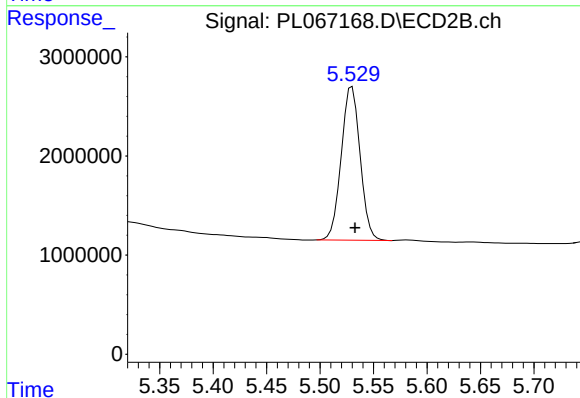


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.003 min
Response: 19067008
Conc: 29.47 ng/ml

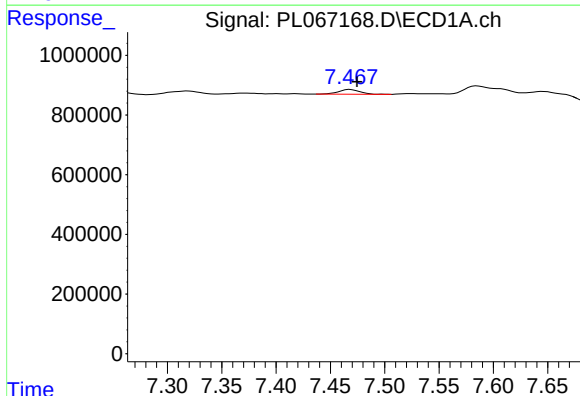


#12 4,4'-DDE

R.T.: 7.468 min
Delta R.T.: -0.006 min
Response: 218890
Conc: 0.41 ng/ml

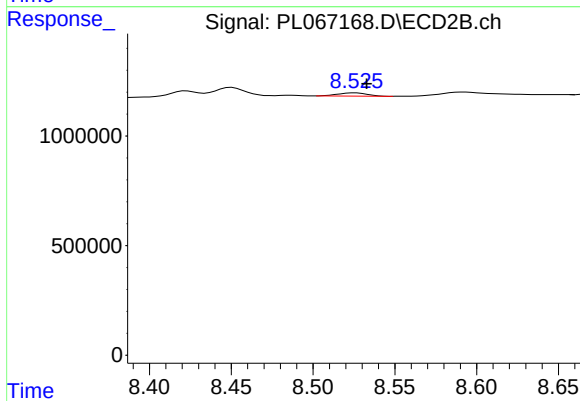

#12 4,4'-DDE

R.T.: 8.525 min
Delta R.T.: -0.008 min
Response: 183045
Conc: 0.28 ng/ml m

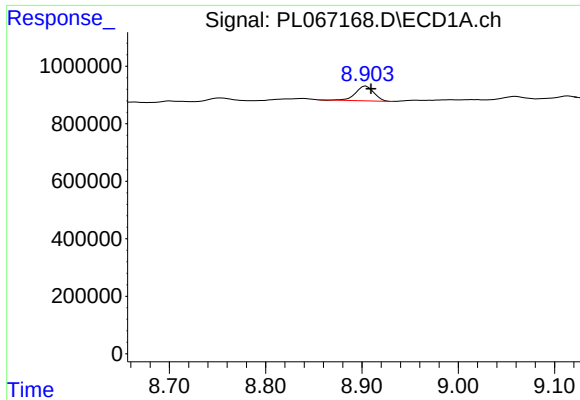


#20 Methoxychlor

R.T.: 8.904 min
Delta R.T.: -0.005 min
Response: 676674
Conc: 2.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B10(4-6)


Manual Integrations
APPROVED

Ankita
6/8/2021 11:55:39 AM

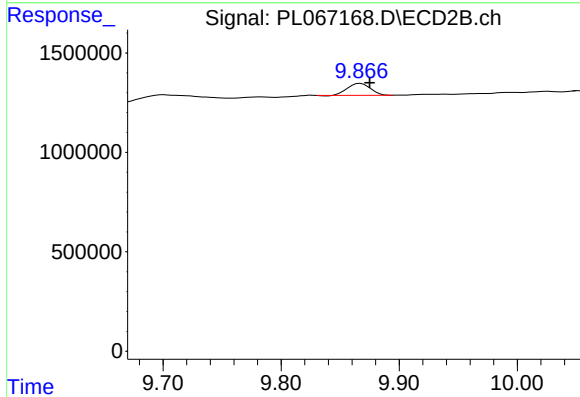


#20 Methoxychlor

R.T.: 9.867 min
Delta R.T.: -0.008 min
Response: 808694
Conc: 2.55 ng/ml

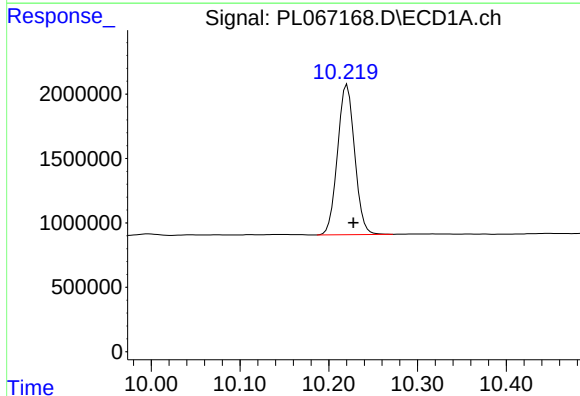

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 15594225
Conc: 24.12 ng/ml

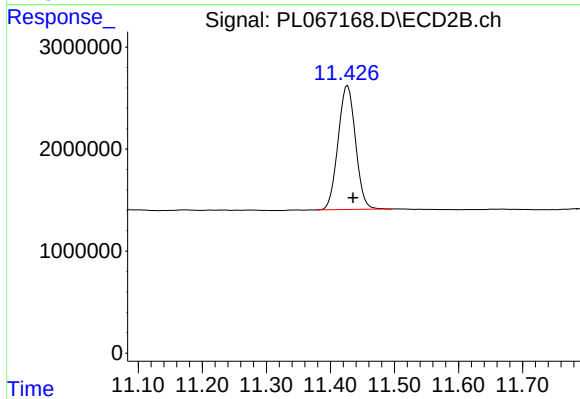

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.008 min
Response: 22961686
Conc: 27.52 ng/ml