

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
 Data File : PL075586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 08:59
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 07:09:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	11.620f	0.000	3580661	0	5.849	N.D. #
Target Compounds							
7)	B delta-BHC	0.000	6.410	0	288770	N.D.	0.135 #
8)	B Heptachlo...	8.126	0.000	4558995	0	5.898	N.D. #
9)	A Endosulfan I	8.537	0.000	546711	0	0.781	N.D. #
10)	B gamma-Chl...	8.382	0.000	2580224	0	3.323	N.D. #
11)	B alpha-Chl...	8.486	7.394f	865372	199017	1.135	0.109 #
13)	MA Dieldrin	0.000	7.757	0	2681510	N.D.	1.584 #
14)	MA Endrin	0.000	8.068f	0	1266062	N.D.	0.926 #
15)	B Endosulfa...	9.304	0.000	263323	0	0.423	N.D. #
21)	B Endrin ke...	10.187f	0.000	729731	0	1.038	N.D. #
25)	Chlordane-3	8.382	0.000	2580224	0	24.989	N.D. #
26)	Chlordane-4	8.486	7.394f	865372	199017	6.832	1.081 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
Data File : PL075586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 08:59
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 07:09:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

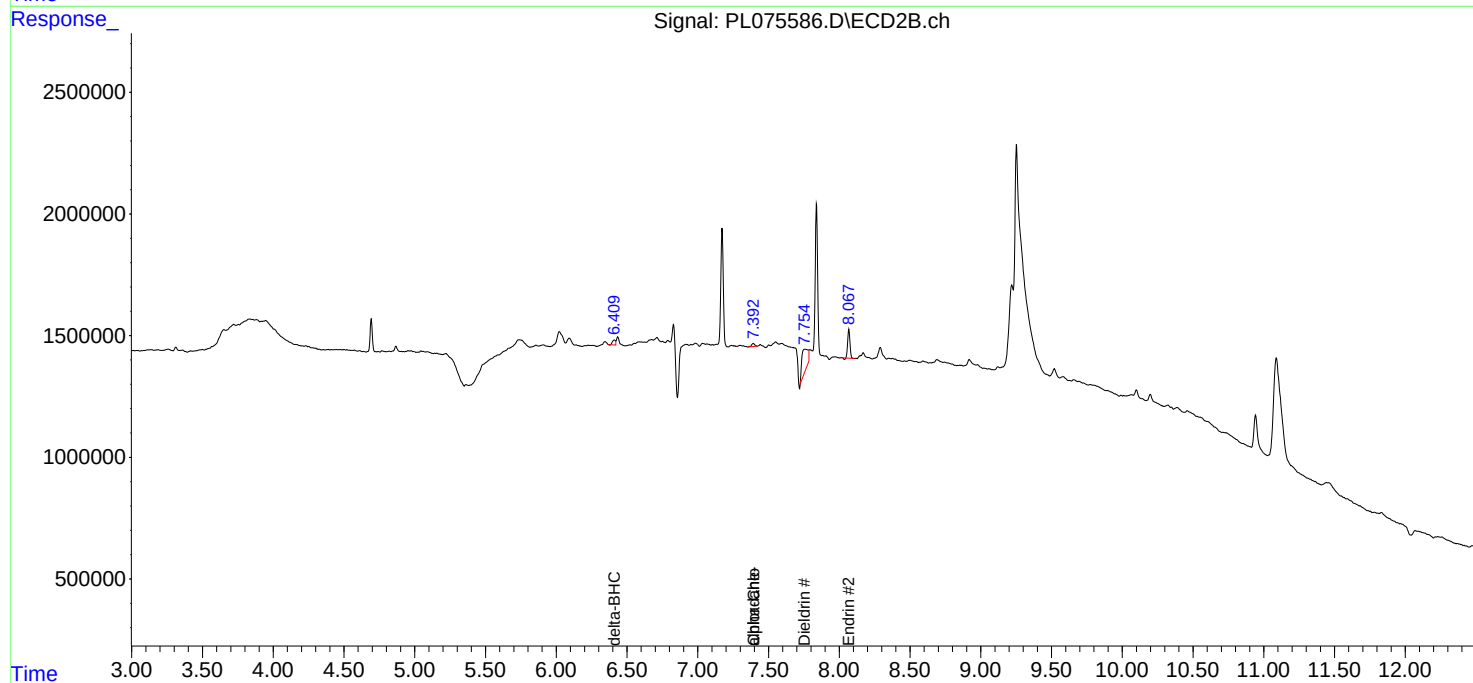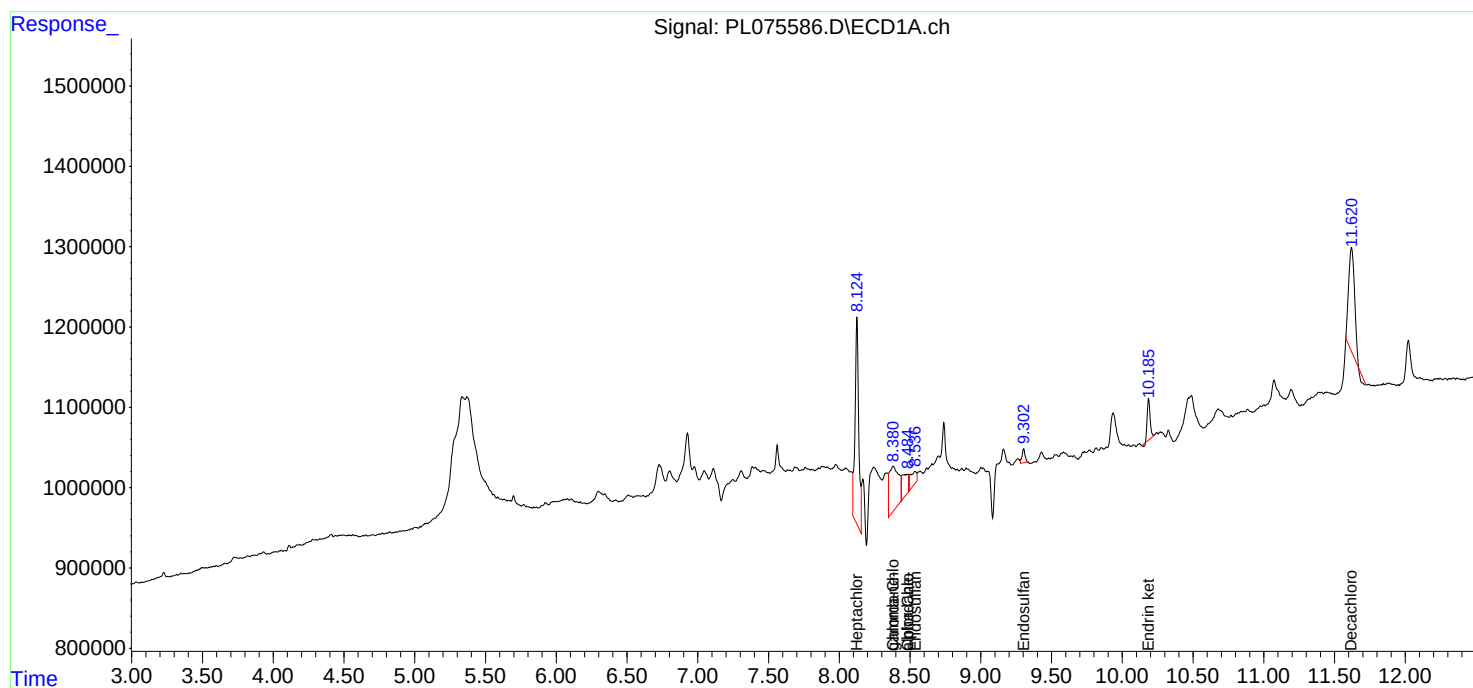


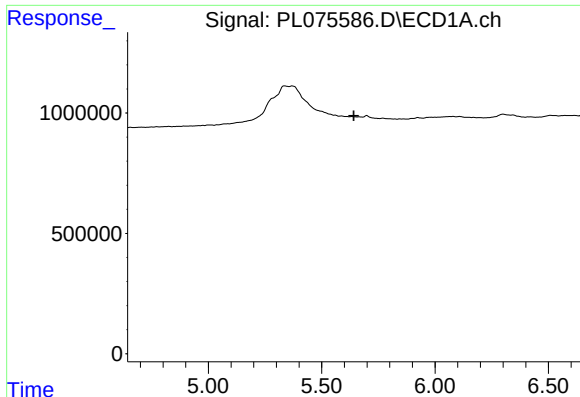

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.641 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

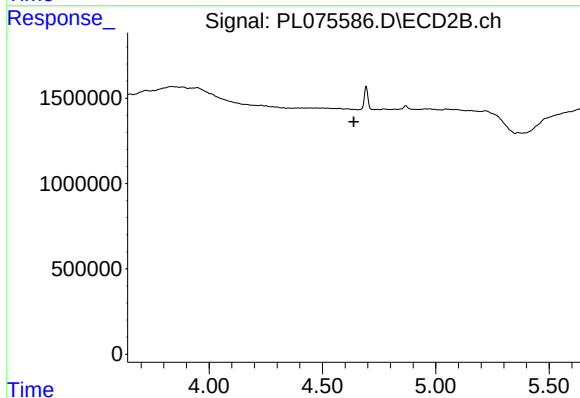


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

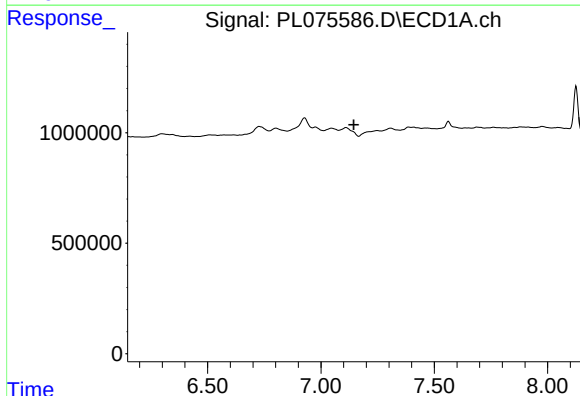


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

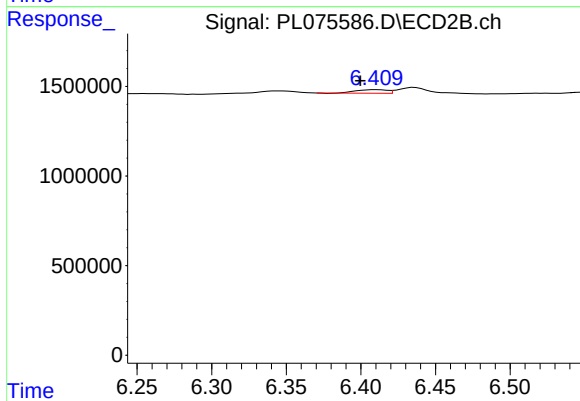

#7 delta-BHC


R.T.: 6.410 min
Delta R.T.: 0.011 min
Response: 288770
Conc: 0.13 ng/ml

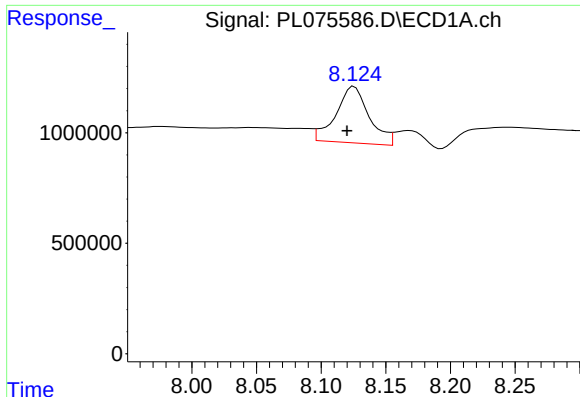

#8 Heptachlor epoxide


R.T.: 8.126 min
Delta R.T.: 0.006 min
Response: 4558995
Conc: 5.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

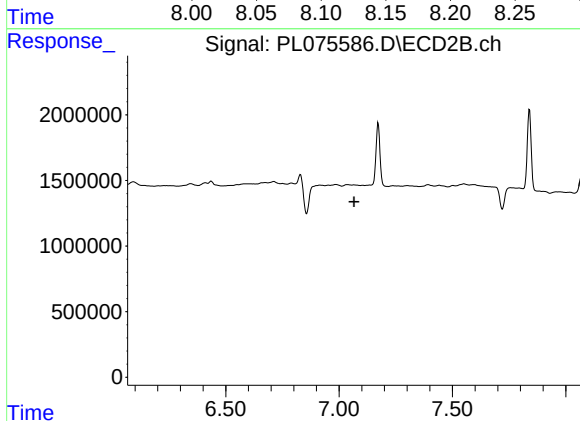


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

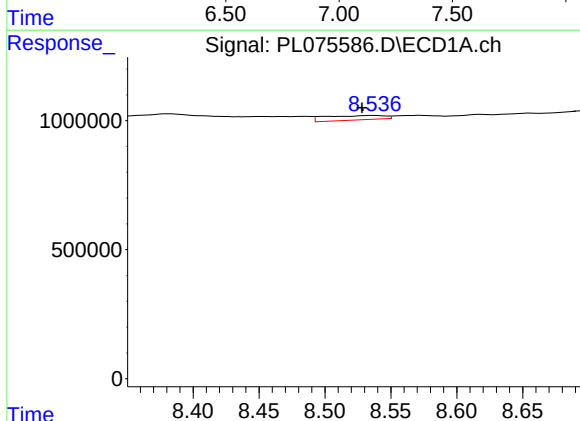


#9 Endosulfan I

R.T.: 8.537 min
Delta R.T.: 0.009 min
Response: 546711
Conc: 0.78 ng/ml

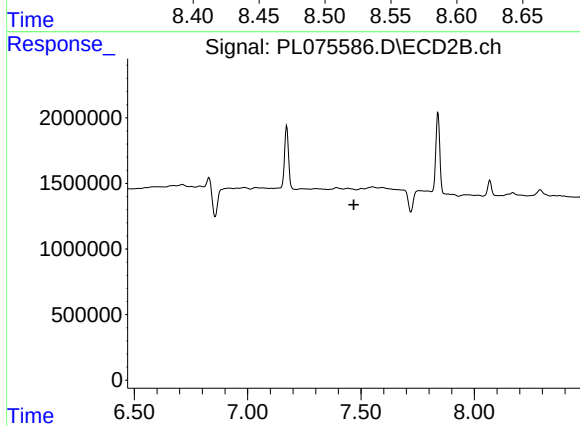

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

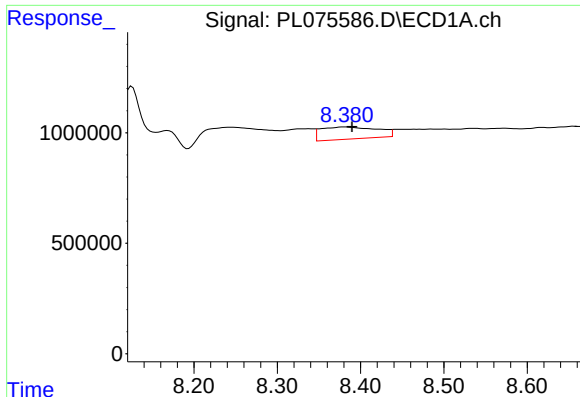

#10 gamma-Chlordane


R.T.: 8.382 min
Delta R.T.: -0.008 min
Response: 2580224
Conc: 3.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

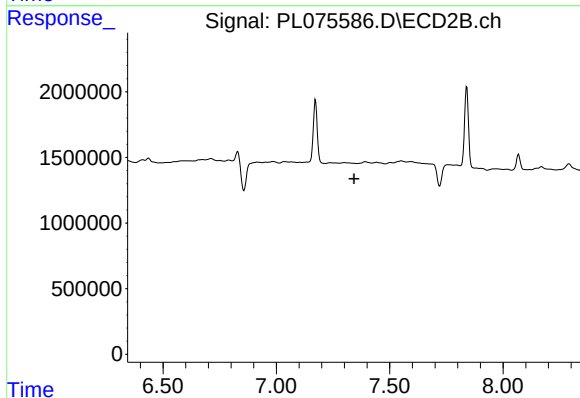


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

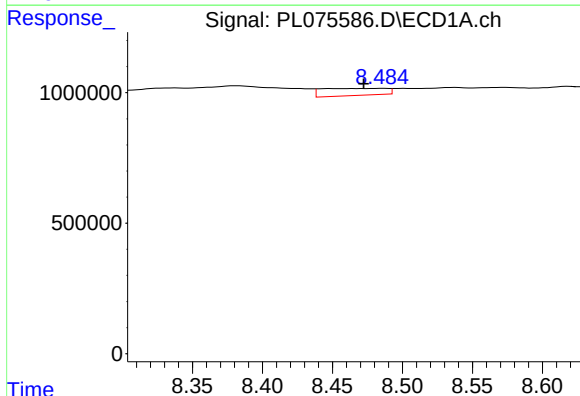


#11 alpha-Chlordane

R.T.: 8.486 min
Delta R.T.: 0.014 min
Response: 865372
Conc: 1.13 ng/ml

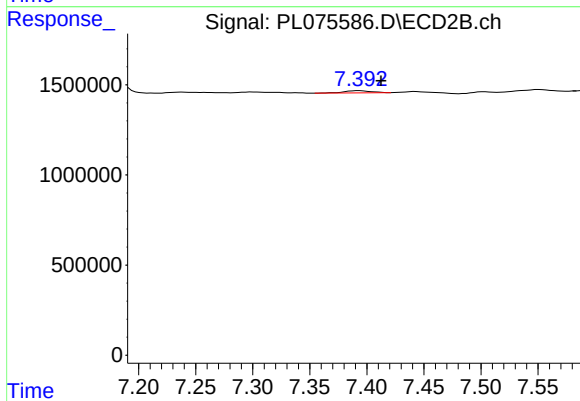

#11 alpha-Chlordane

R.T.: 7.394 min
Delta R.T.: -0.019 min
Response: 199017
Conc: 0.11 ng/ml

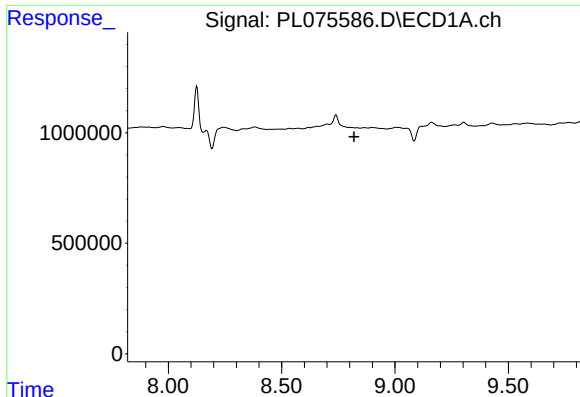

#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#13 Dieldrin


R.T.: 7.757 min
Delta R.T.: 0.003 min
Response: 2681510
Conc: 1.58 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 8.068 min
Delta R.T.: 0.023 min
Response: 1266062
Conc: 0.93 ng/ml

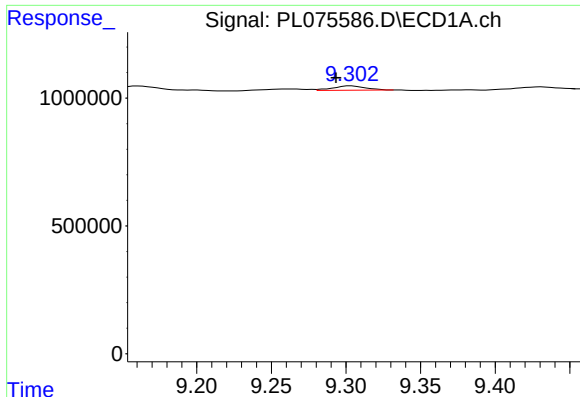

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.010 min
Response: 263323
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

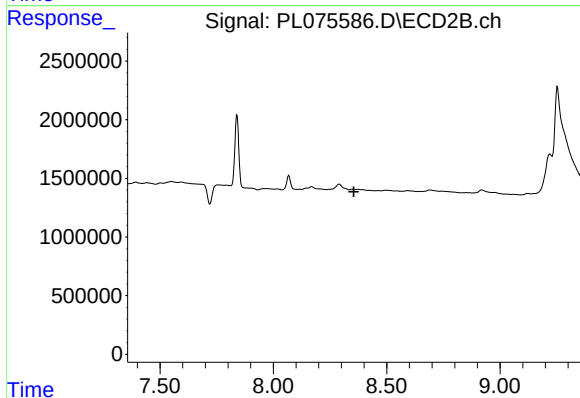


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

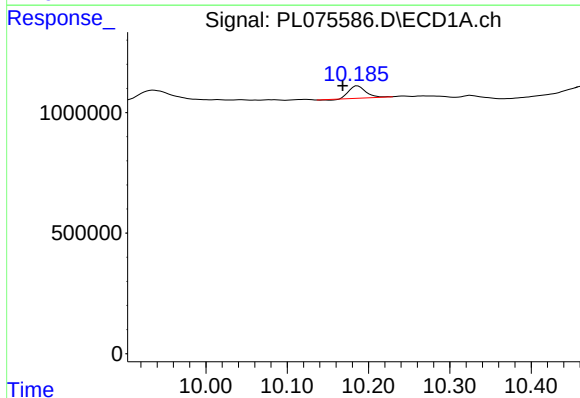


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.018 min
Response: 729731
Conc: 1.04 ng/ml

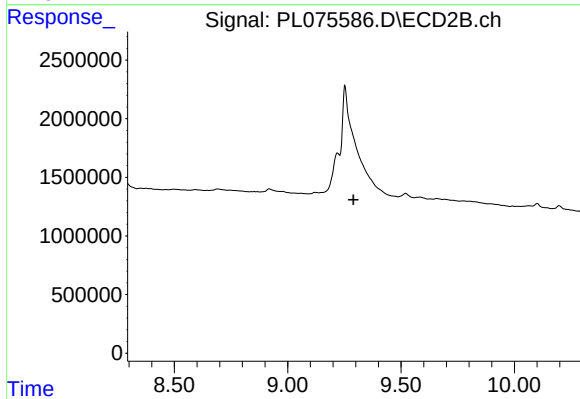

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

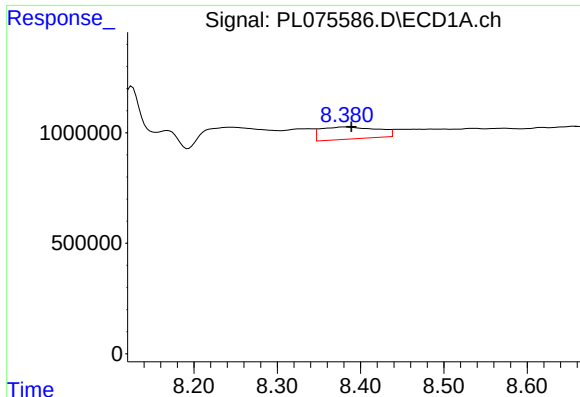

#25 Chlordane-3


R.T.: 8.382 min
Delta R.T.: -0.008 min
Response: 2580224
Conc: 24.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

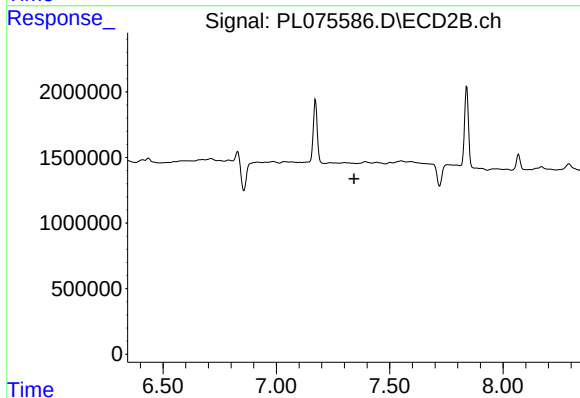


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

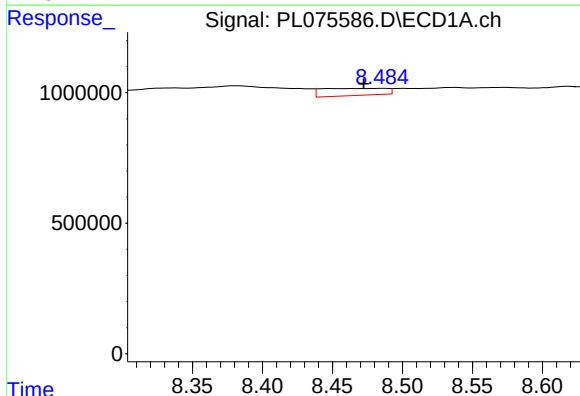


#26 Chlordane-4

R.T.: 8.486 min
Delta R.T.: 0.014 min
Response: 865372
Conc: 6.83 ng/ml

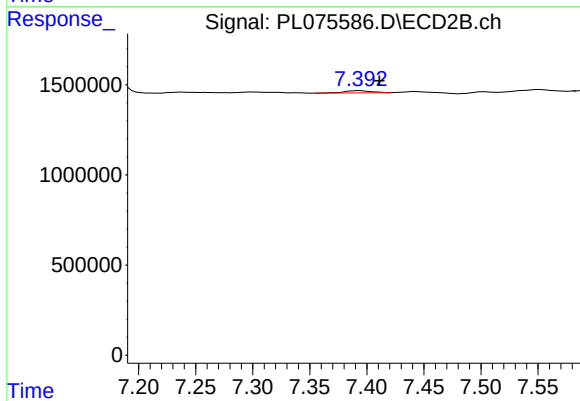

#26 Chlordane-4


R.T.: 7.394 min
Delta R.T.: -0.017 min
Response: 199017
Conc: 1.08 ng/ml

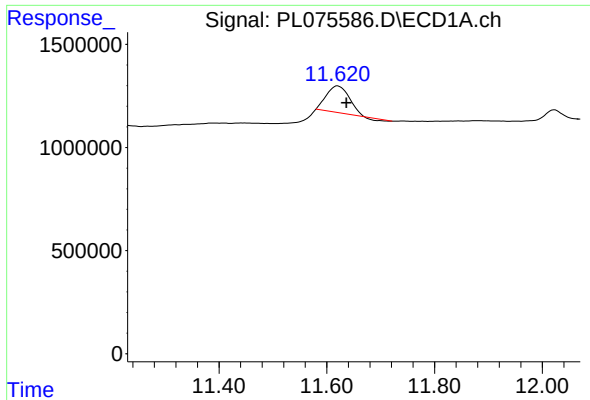

#28 Decachlorobiphenyl

R.T.: 11.620 min
Delta R.T.: -0.016 min
Response: 3580661
Conc: 5.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

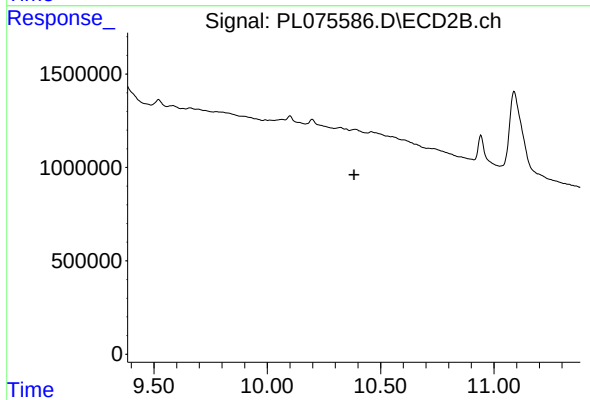

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.383 min
Response: 0
Conc: N.D.