

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
 Data File : PL075593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2022 13:27
 Operator : AR\AJ
 Sample : PB144730BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 07:12:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.638	13284918	31228911	19.685	18.609
28)	SA Decachlor...	11.636	10.382	13584373	29016893	22.189	20.595
Target Compounds							
7)	B delta-BHC	0.000	6.408	0	299687	N.D.	0.140 #
9)	A Endosulfan I	8.535	0.000	46533	0	0.067	N.D. #
10)	B gamma-Chl...	8.383	0.000	1277604	0	1.645	N.D. #
11)	B alpha-Chl...	8.490f	0.000	201288	0	0.264	N.D. #
15)	B Endosulfa...	9.302	0.000	341370	0	0.549	N.D. #
21)	B Endrin ke...	10.185f	0.000	830580	0	1.181	N.D. #
25)	Chlordane-3	8.383	0.000	1277604	0	12.374	N.D. #
26)	Chlordane-4	8.490f	0.000	201288	0	1.589	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
Data File : PL075593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2022 13:27
Operator : AR\AJ
Sample : PB144730BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 07:12:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

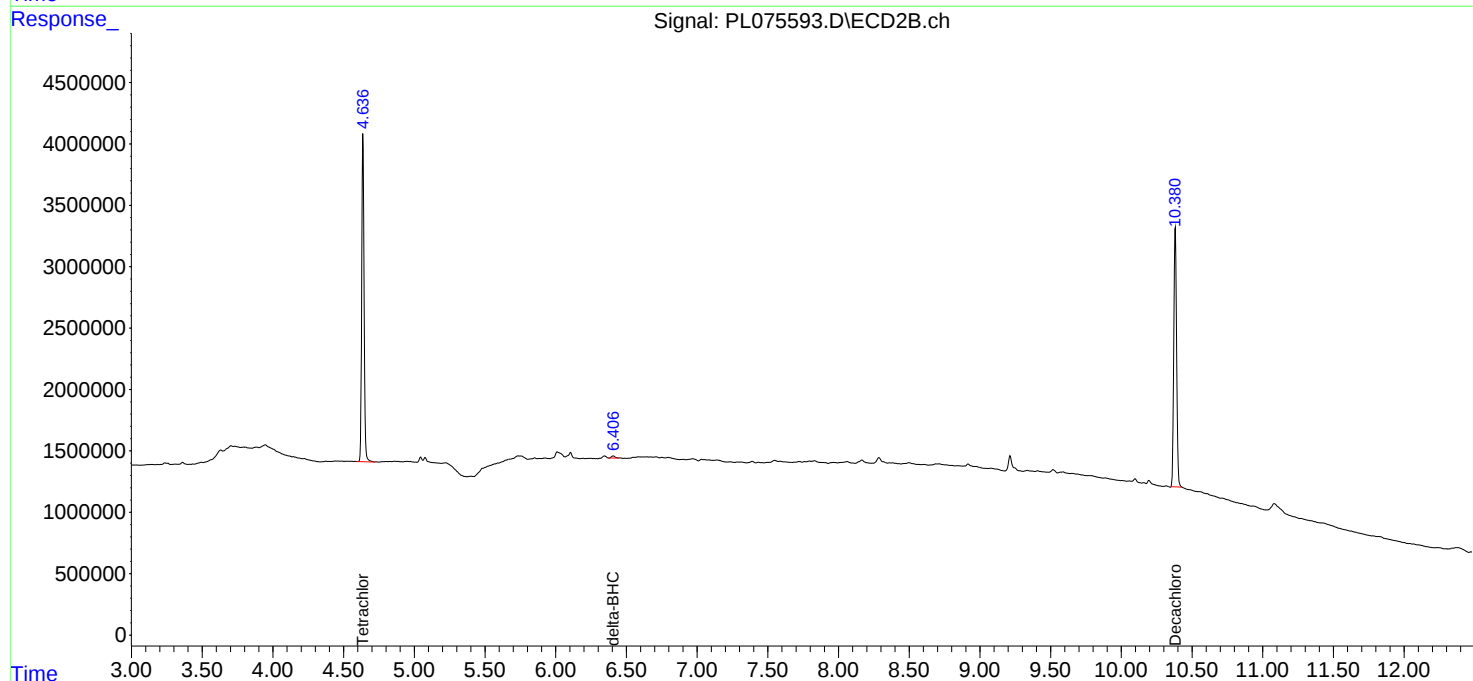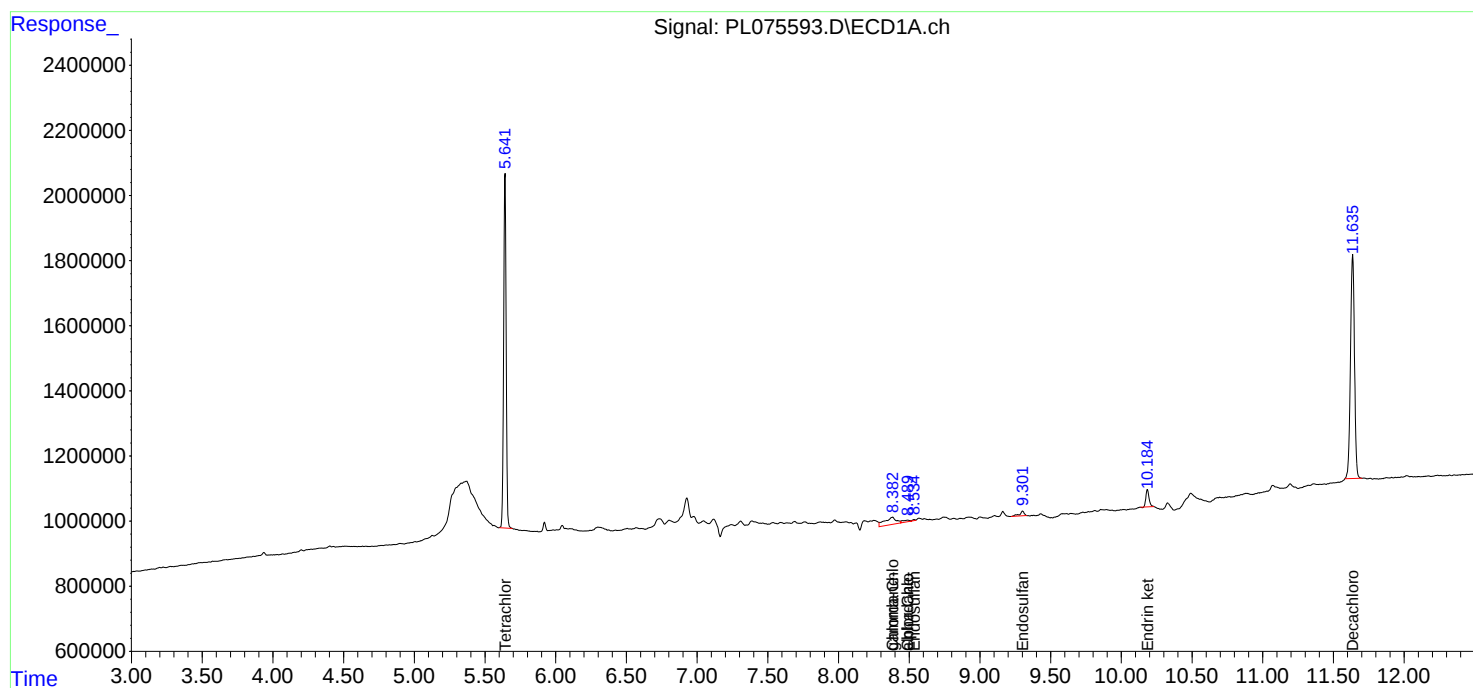


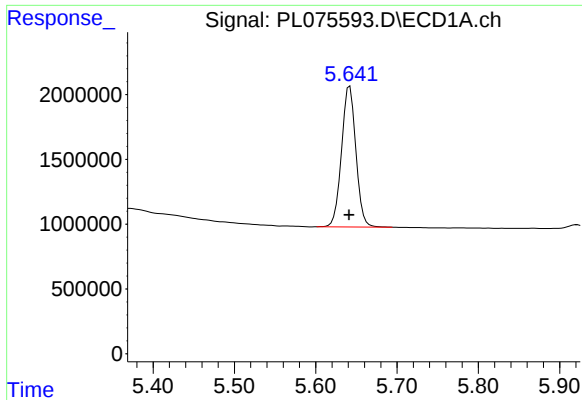

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 13284918
Conc: 19.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

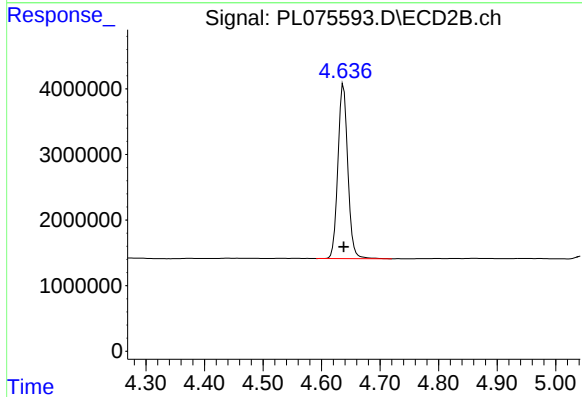


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 31228911
Conc: 18.61 ng/ml

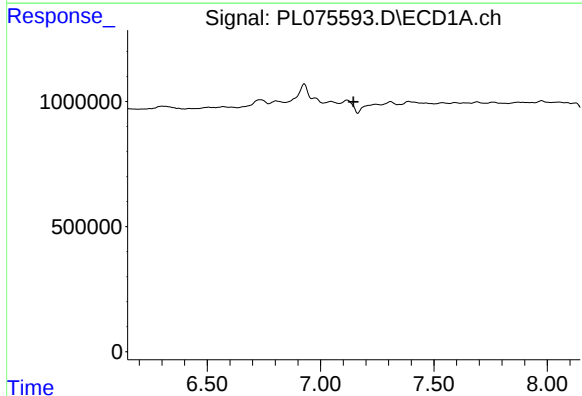


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

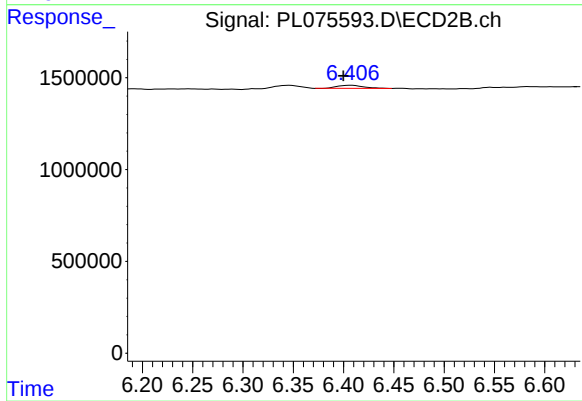

#7 delta-BHC


R.T.: 6.408 min
Delta R.T.: 0.008 min
Response: 299687
Conc: 0.14 ng/ml

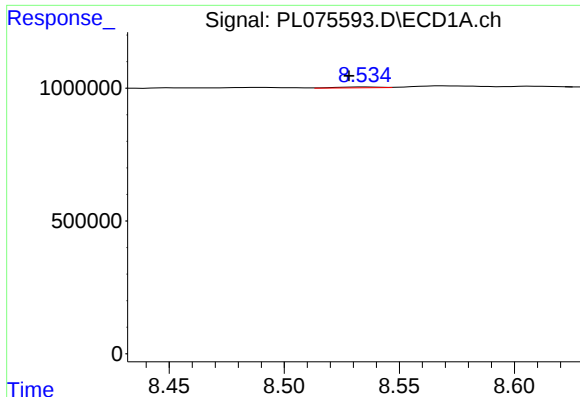

#9 Endosulfan I


R.T.: 8.535 min
Delta R.T.: 0.007 min
Response: 46533
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

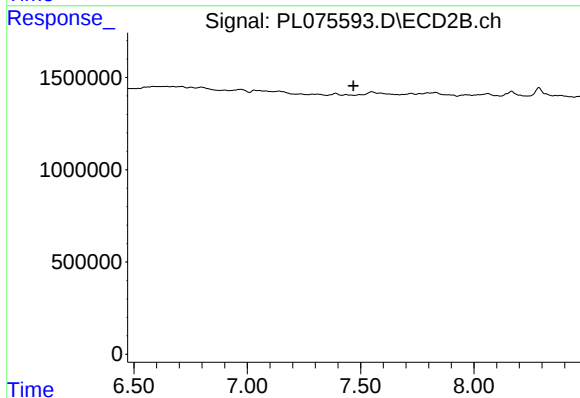


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

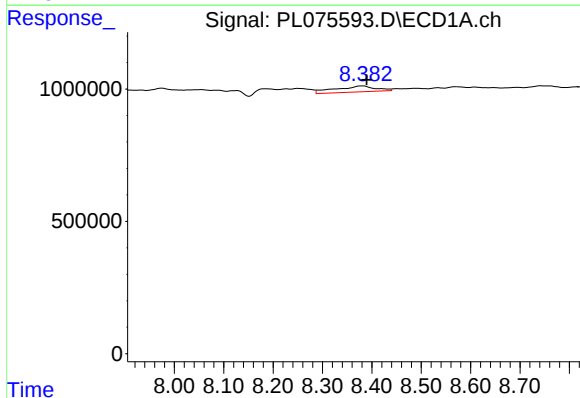


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1277604
Conc: 1.65 ng/ml

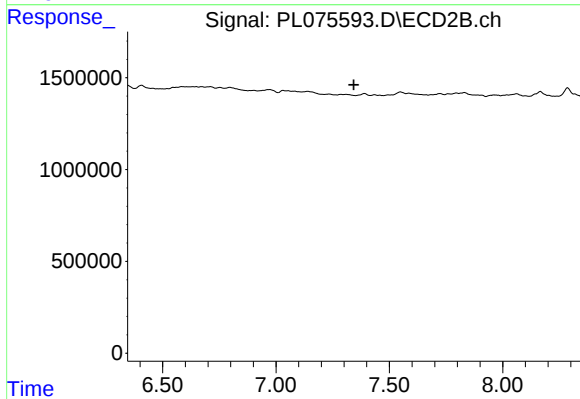

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

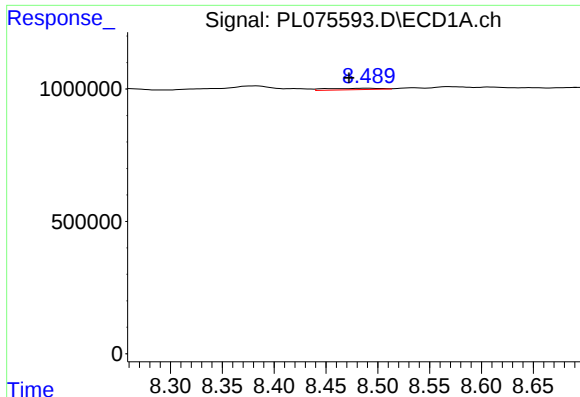

#11 alpha-Chlordane


R.T.: 8.490 min
Delta R.T.: 0.018 min
Response: 201288
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

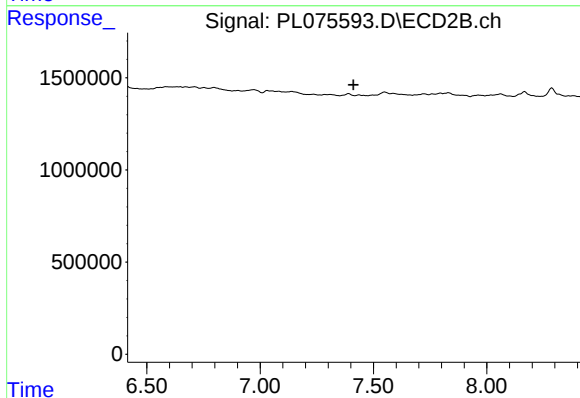


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

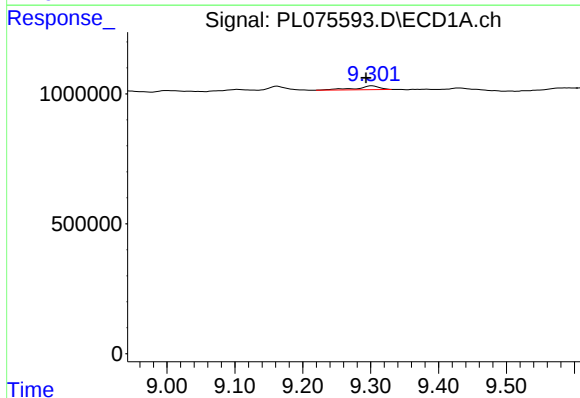


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.009 min
Response: 341370
Conc: 0.55 ng/ml

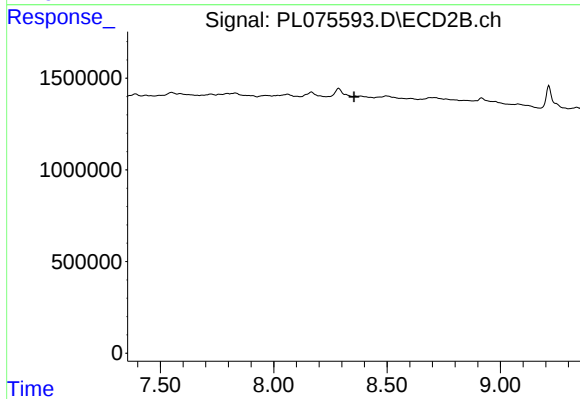

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

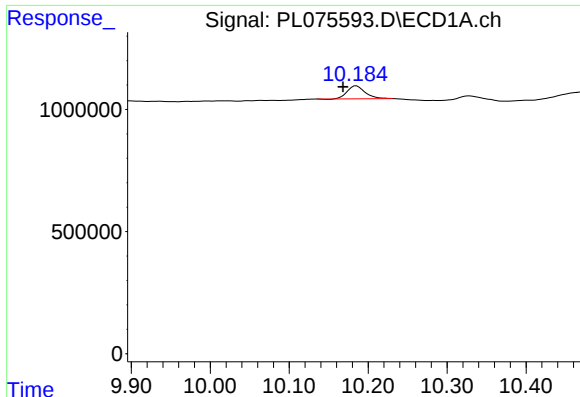

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 830580
Conc: 1.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

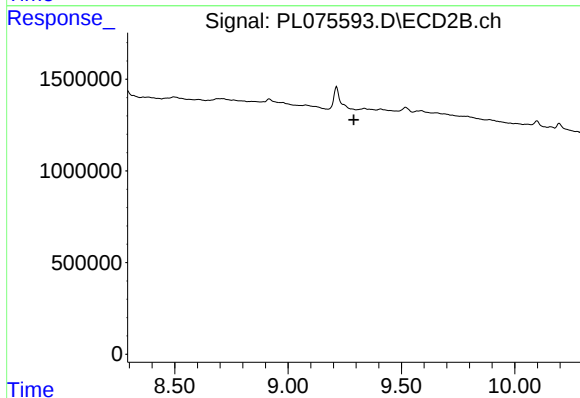


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

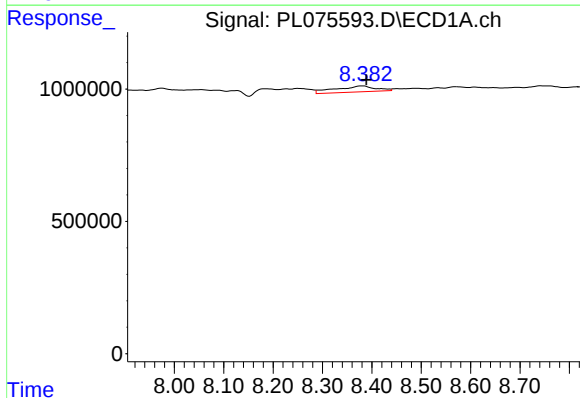


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.006 min
Response: 1277604
Conc: 12.37 ng/ml

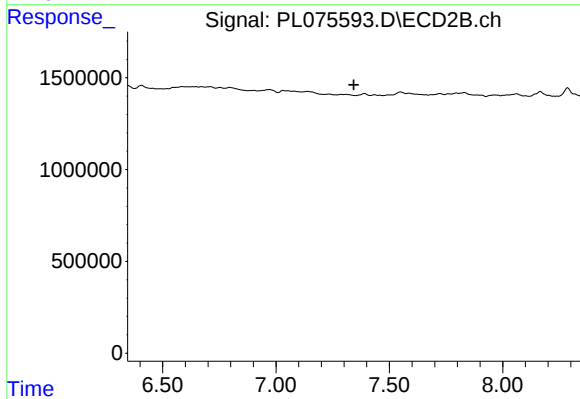

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

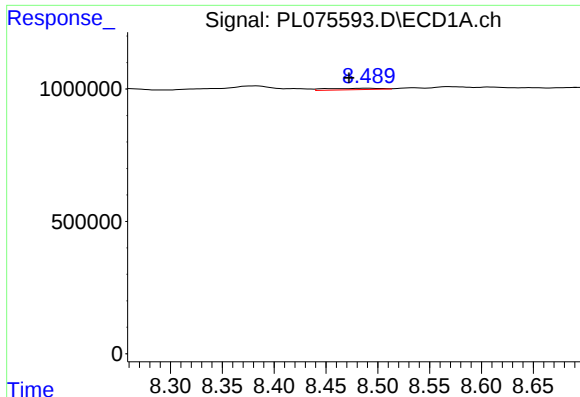

#26 Chlordane-4


R.T.: 8.490 min
Delta R.T.: 0.018 min
Response: 201288
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

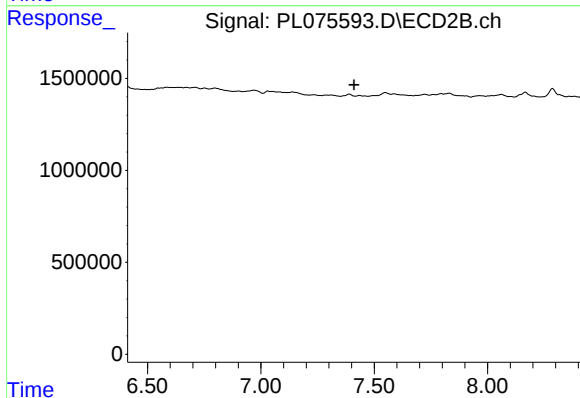


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

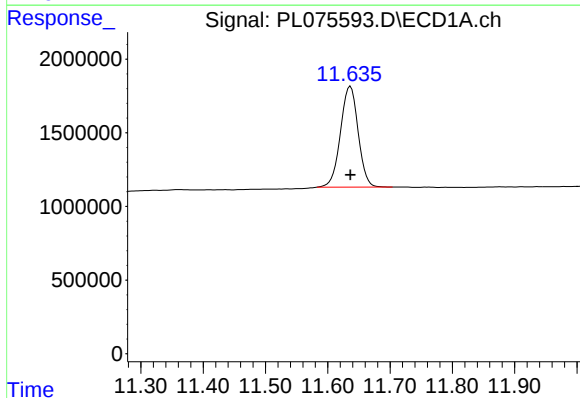

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 13584373
Conc: 22.19 ng/ml

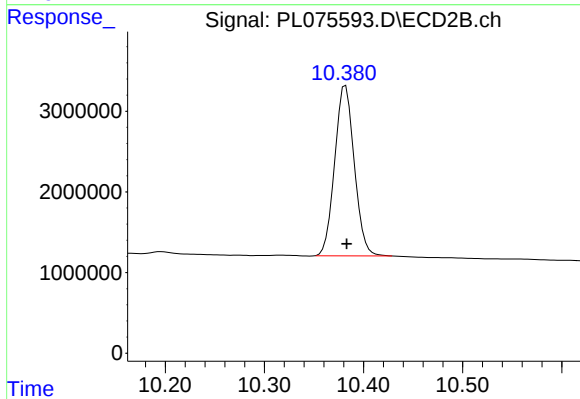

#28 Decachlorobiphenyl

R.T.: 10.382 min
Delta R.T.: -0.001 min
Response: 29016893
Conc: 20.59 ng/ml