

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
 Data File : PL075622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 06:08
 Operator : AR\AJ
 Sample : N3194-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 07:34:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.639	14736362	31042658	21.835	18.498
28)	SA Decachlor...	11.639	10.384	13622267	23104398	22.251	16.398 #
Target Compounds							
4)	MA Heptachlor	7.308f	0.000	252777	0	0.275	N.D. #
7)	B delta-BHC	7.125f	6.403	649973	182721	0.845	0.085 #
9)	A Endosulfan I	8.532	0.000	64023	0	0.092	N.D. #
10)	B gamma-Chl...	8.383	0.000	1871320	0	2.410	N.D. #
11)	B alpha-Chl...	8.471	0.000	220288	0	0.289	N.D. #
15)	B Endosulfa...	9.304	0.000	264510	0	0.425	N.D. #
21)	B Endrin ke...	10.186f	0.000	522250	0	0.743	N.D. #
23)	Chlordane-1	7.044	0.000	251549	0	10.021	N.D. #
25)	Chlordane-3	8.383	0.000	1871320	0	18.124	N.D. #
26)	Chlordane-4	8.471	0.000	220288	0	1.739	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060722\
Data File : PL075622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 06:08
Operator : AR\AJ
Sample : N3194-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 07:34:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

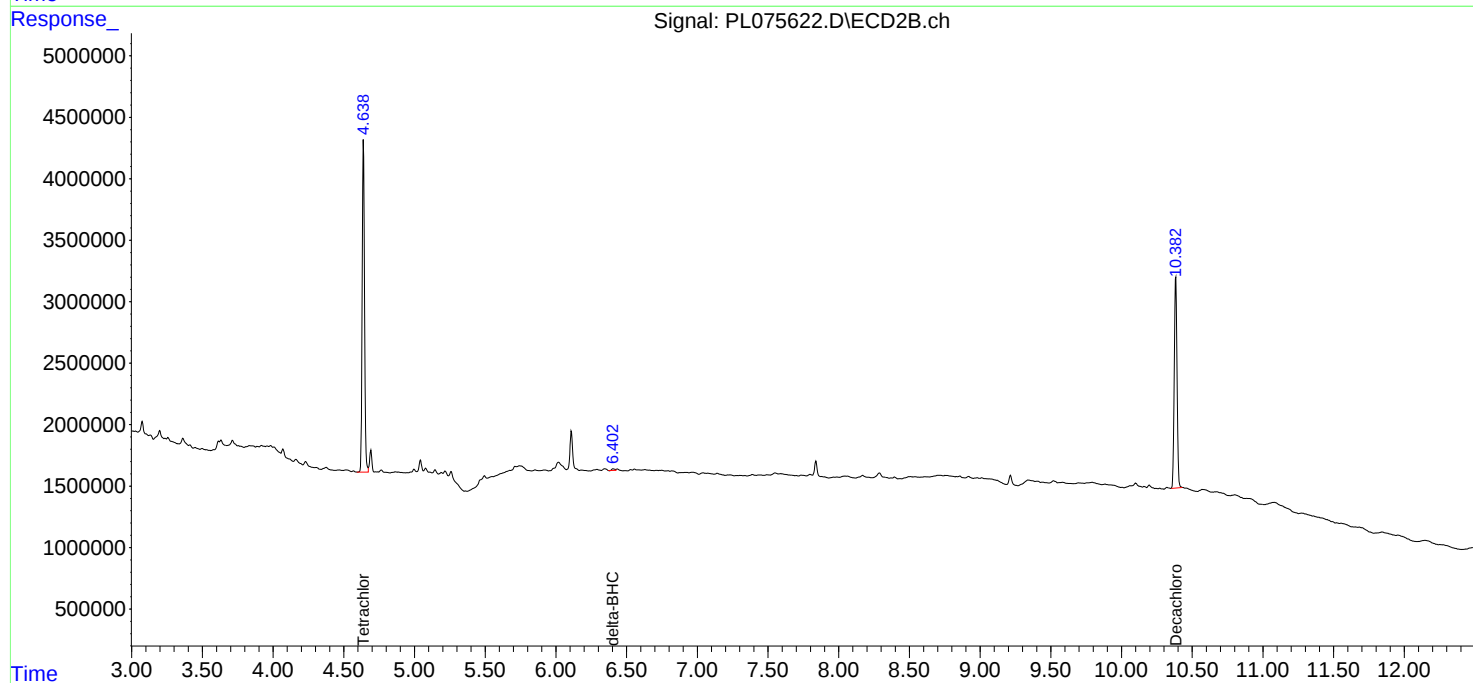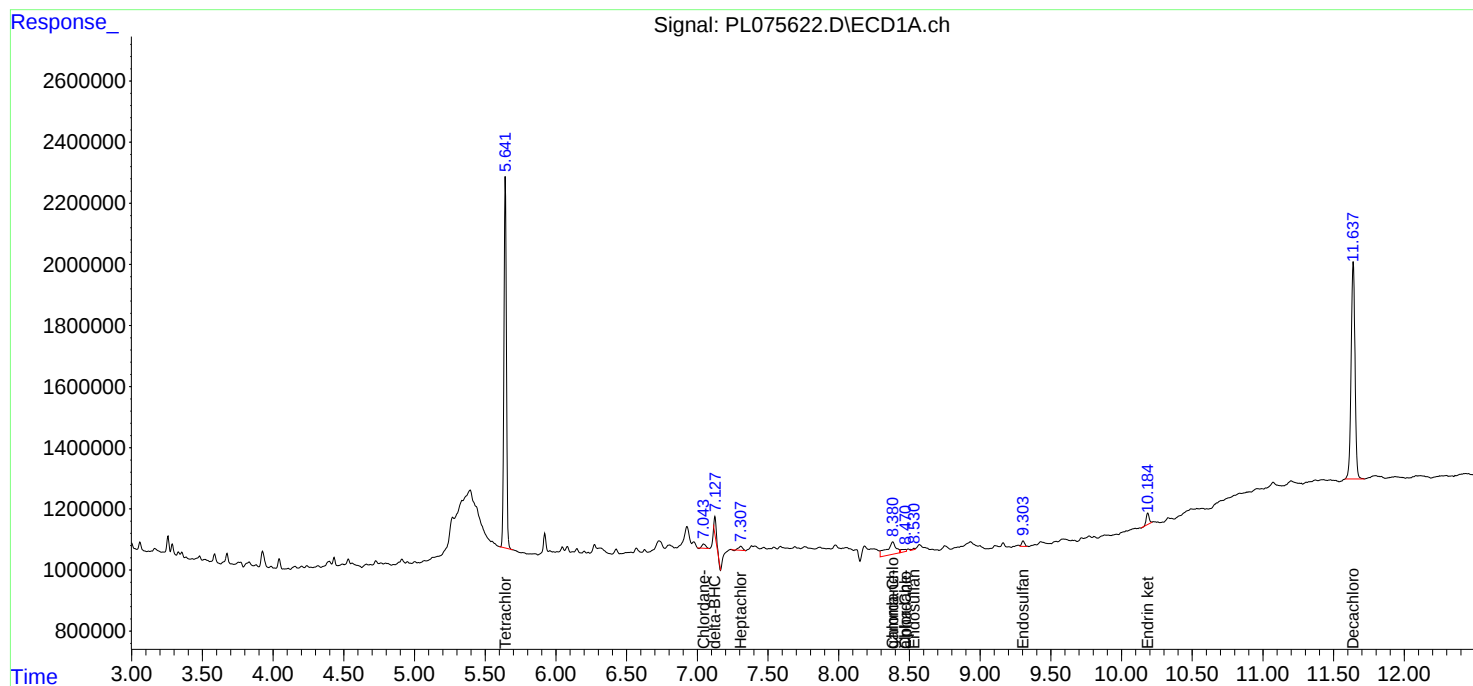


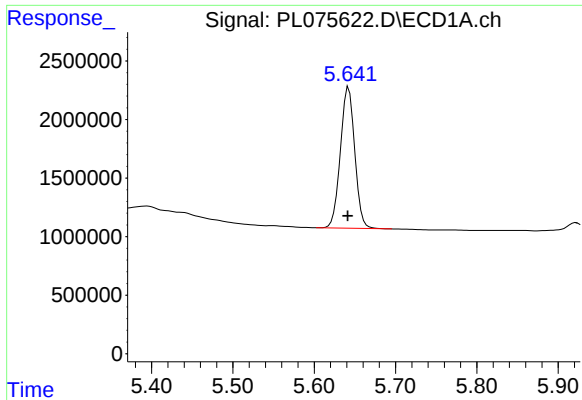

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.001 min
Response: 14736362
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

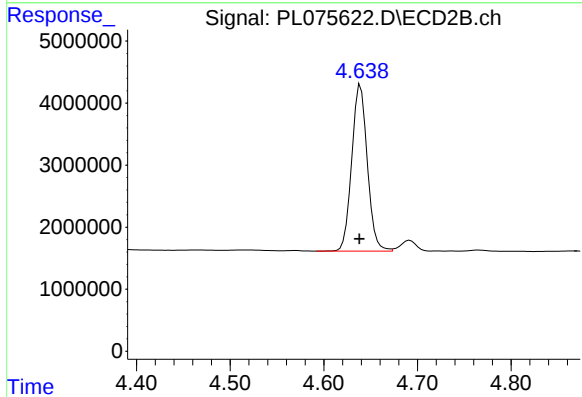


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: 0.002 min
Response: 31042658
Conc: 18.50 ng/ml

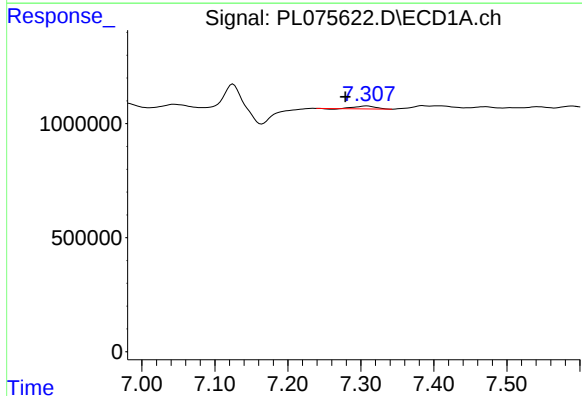


#4 Heptachlor

R.T.: 7.308 min
Delta R.T.: 0.029 min
Response: 252777
Conc: 0.27 ng/ml

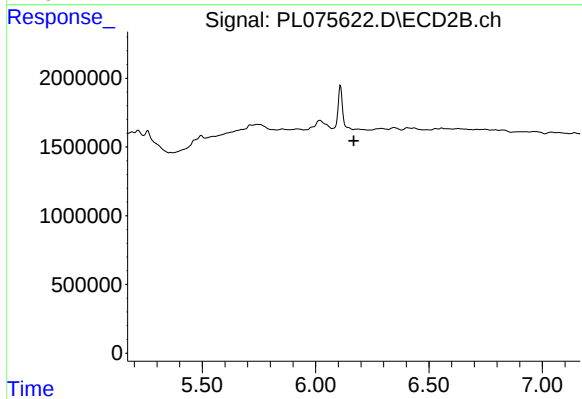

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 6.169 min
Response: 0
Conc: N.D.

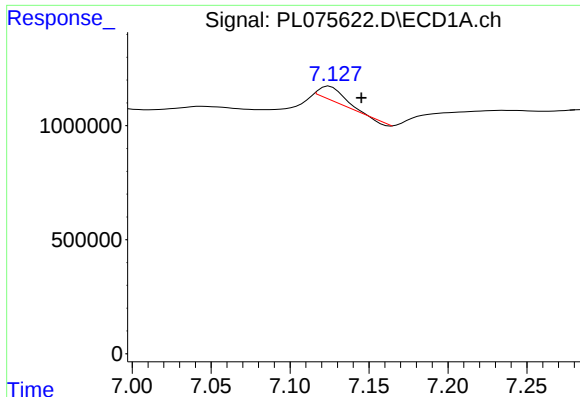

#7 delta-BHC


R.T.: 7.125 min
Delta R.T.: -0.020 min
Response: 649973
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

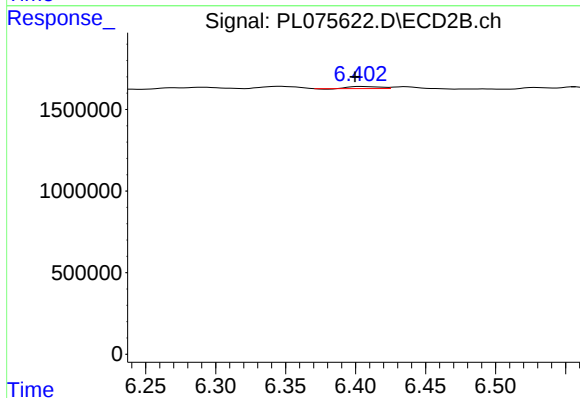


#7 delta-BHC

R.T.: 6.403 min
Delta R.T.: 0.004 min
Response: 182721
Conc: 0.09 ng/ml

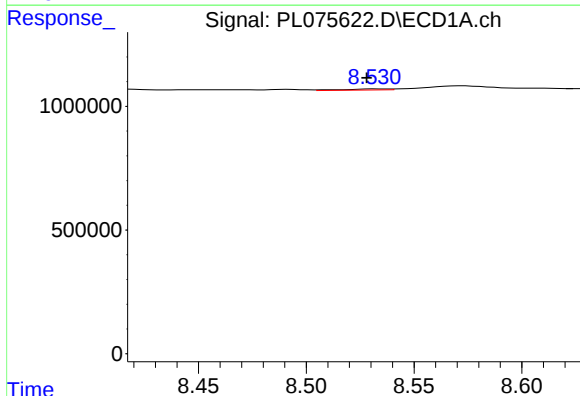


#9 Endosulfan I

R.T.: 8.532 min
Delta R.T.: 0.004 min
Response: 64023
Conc: 0.09 ng/ml

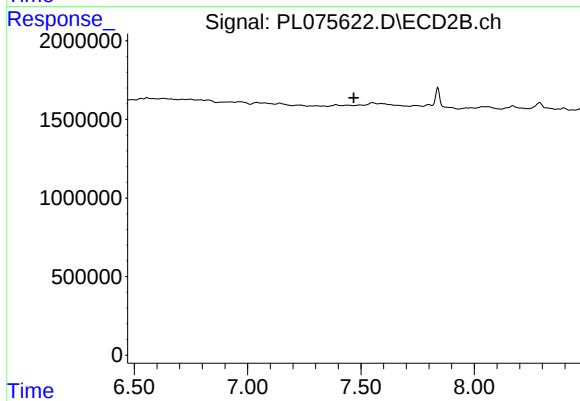

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.469 min
Response: 0
Conc: N.D.

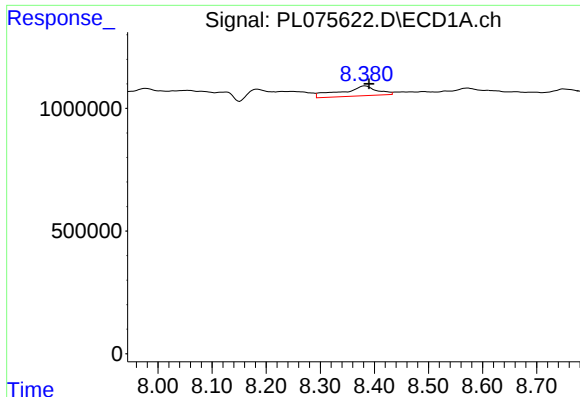

#10 gamma-Chlordane


R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1871320
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

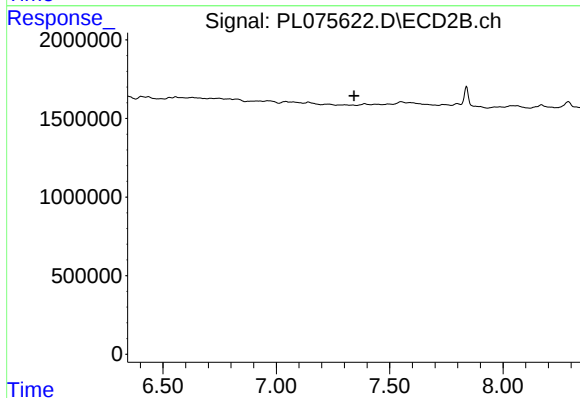


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

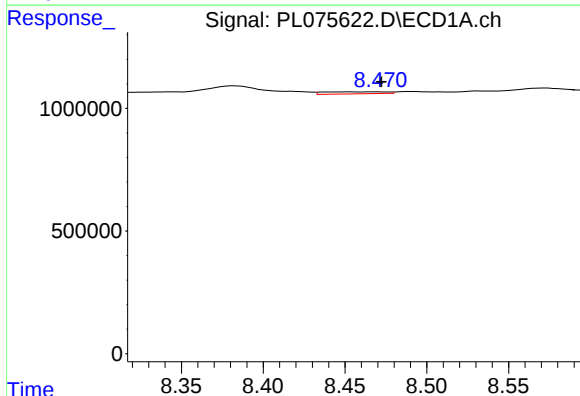


#11 alpha-Chlordane

R.T.: 8.471 min
Delta R.T.: 0.000 min
Response: 220288
Conc: 0.29 ng/ml

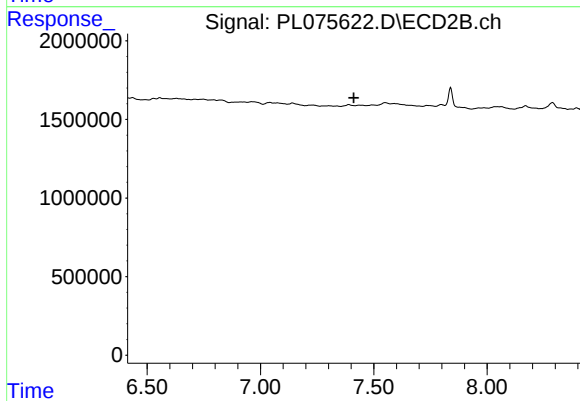

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

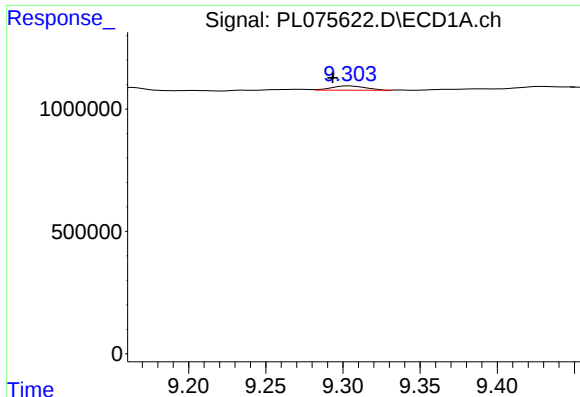

#15 Endosulfan II


R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 264510
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

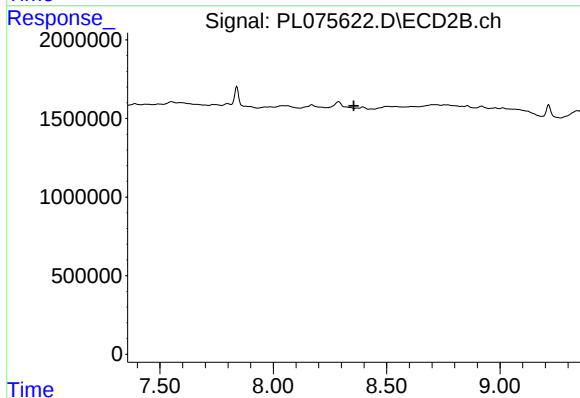


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

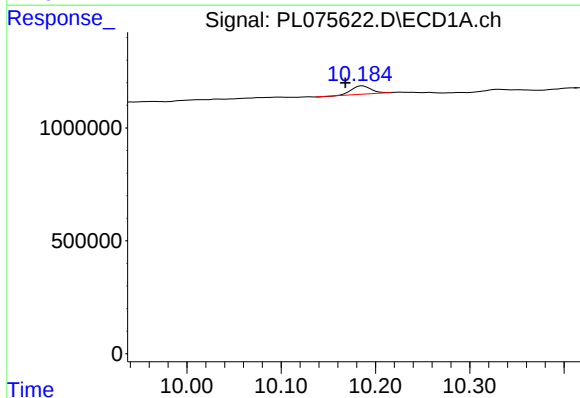


#21 Endrin ketone

R.T.: 10.186 min
Delta R.T.: 0.018 min
Response: 522250
Conc: 0.74 ng/ml

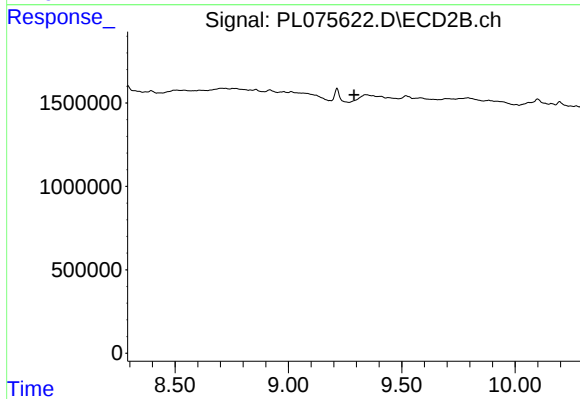

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

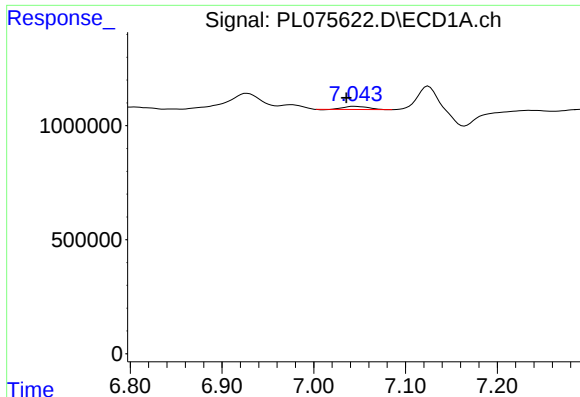

#23 Chlordane-1


R.T.: 7.044 min
Delta R.T.: 0.009 min
Response: 251549
Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

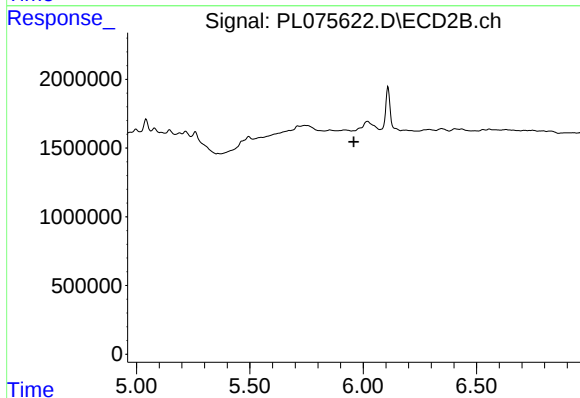


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

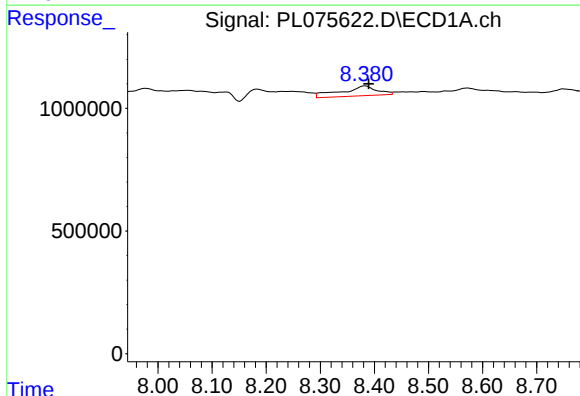


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1871320
Conc: 18.12 ng/ml

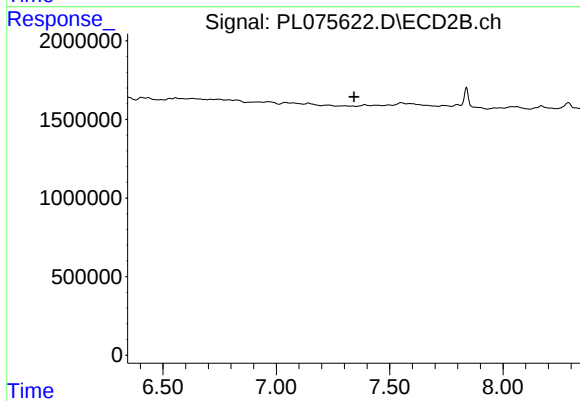

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

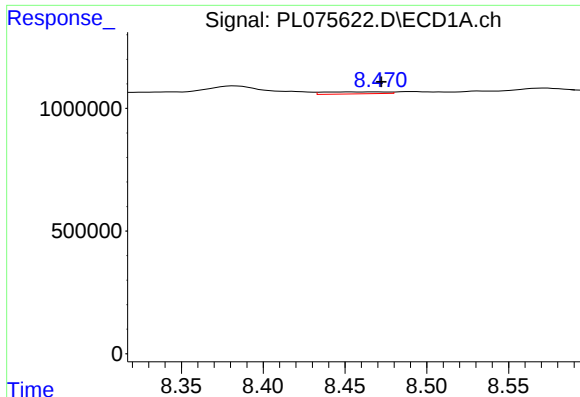

#26 Chlordane-4


R.T.: 8.471 min
Delta R.T.: 0.000 min
Response: 220288
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

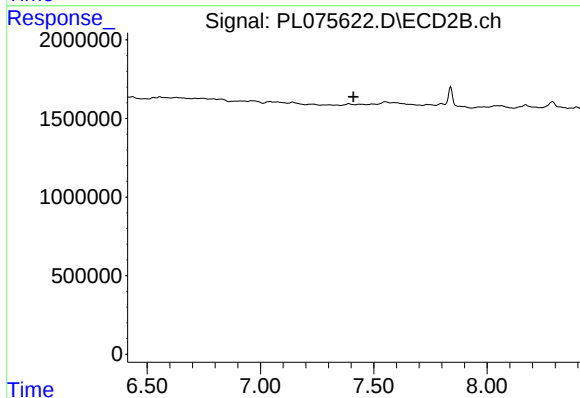


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

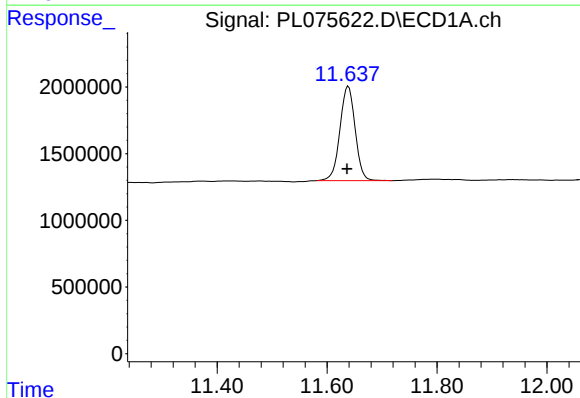

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: 0.003 min
Response: 13622267
Conc: 22.25 ng/ml

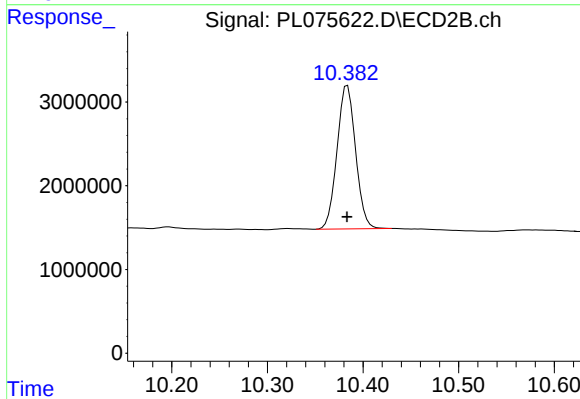

#28 Decachlorobiphenyl

R.T.: 10.384 min
Delta R.T.: 0.000 min
Response: 23104398
Conc: 16.40 ng/ml