

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
 Data File : PL083283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 13:14
 Operator : AR\AJ
 Sample : 03044-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-02-5.0-7.0-DUP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:15:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	2.632	32080222	28893215	10.915	11.130
28)	SA Decachlor...	8.733	7.737	23534494	26141956	11.221	10.513

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
Data File : PL083283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 13:14
Operator : AR\AJ
Sample : 03044-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-02-5.0-7.0-DUP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:15:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

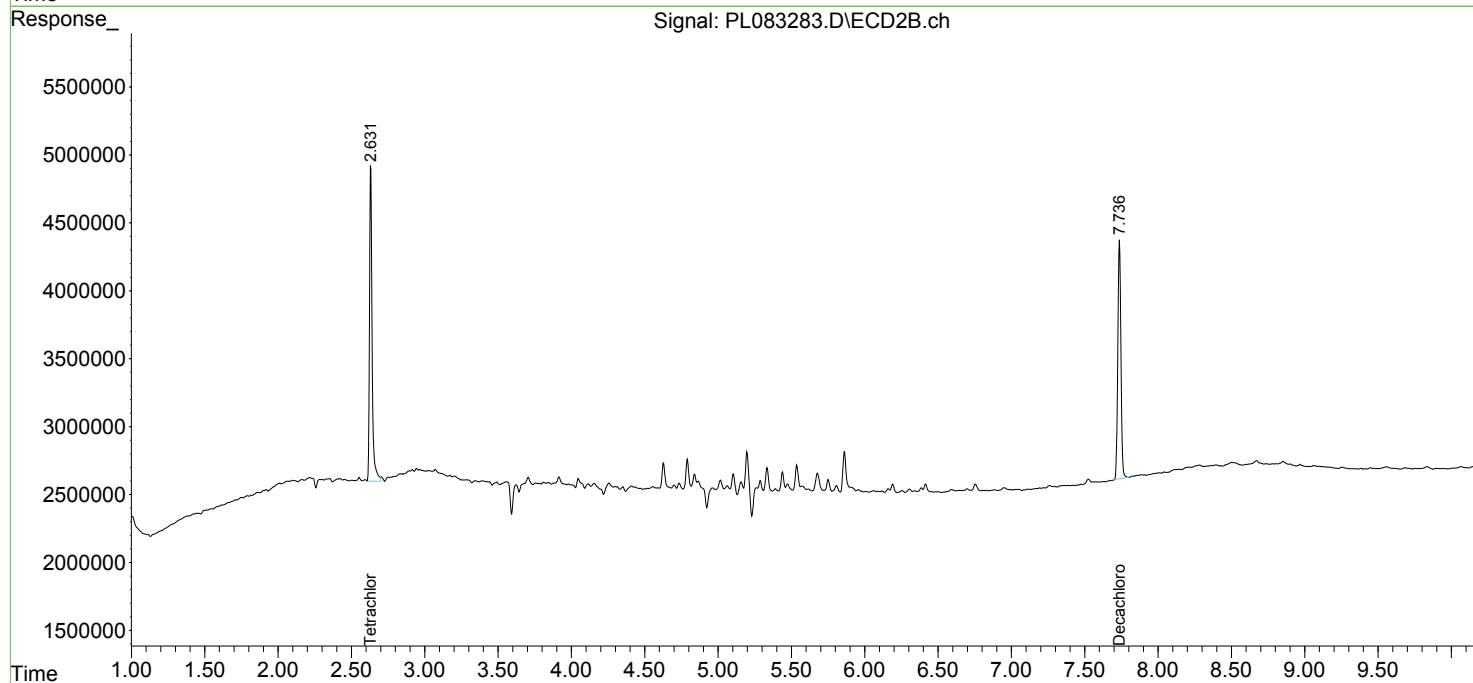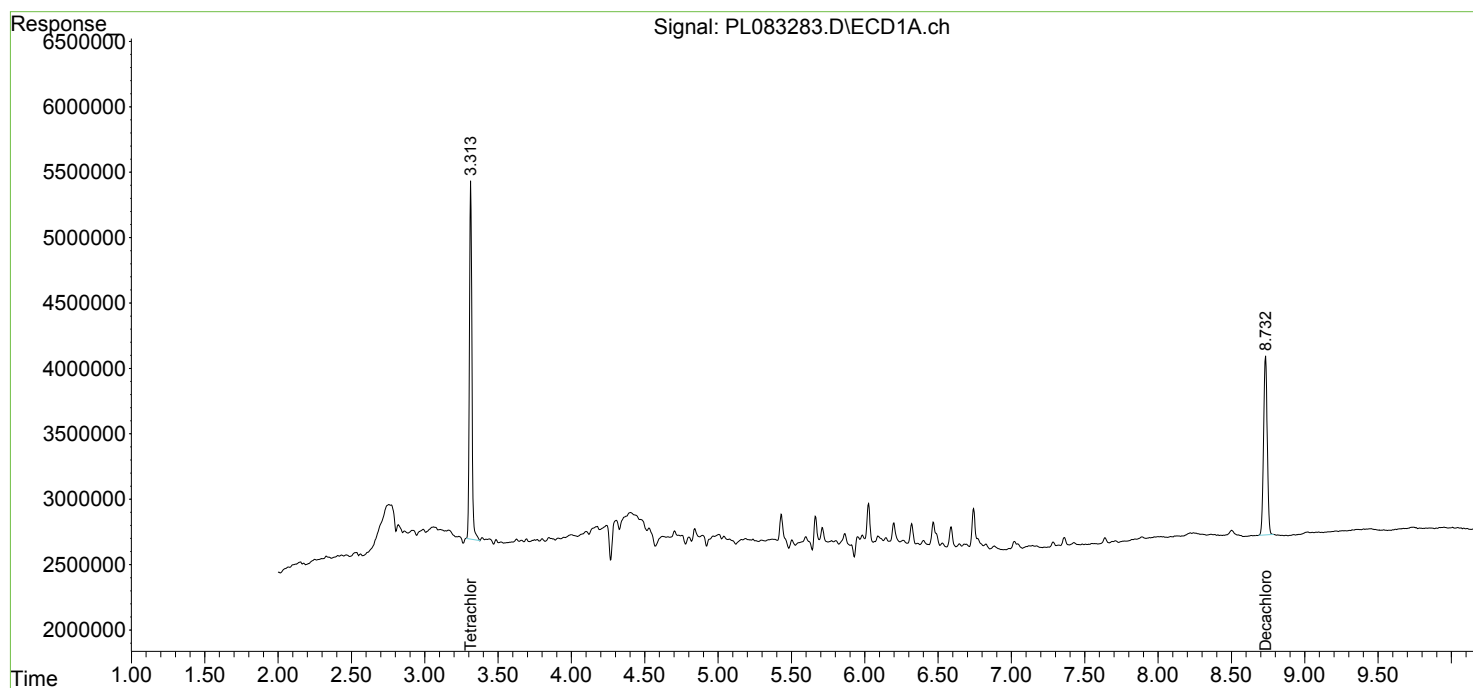


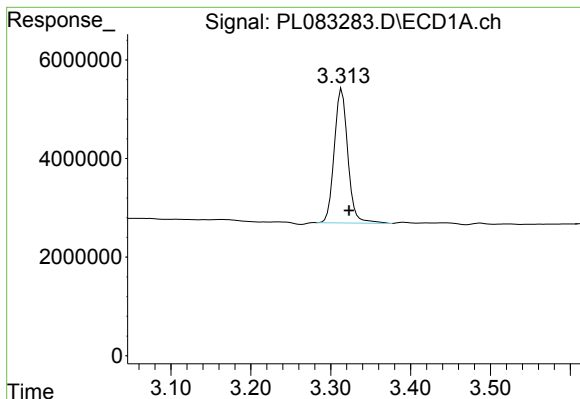

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.009 min
Response: 32080222
Conc: 10.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-02-5.0-7.0-DUP

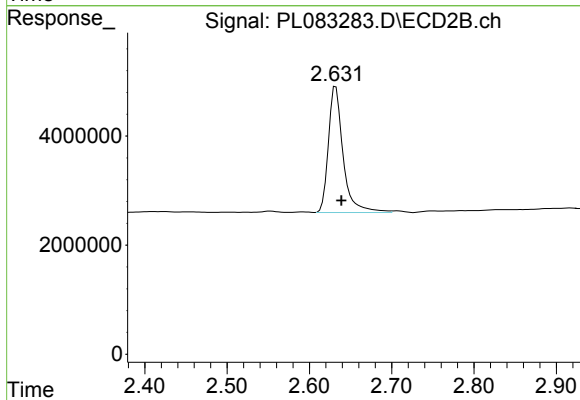


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: -0.007 min
Response: 28893215
Conc: 11.13 ng/ml

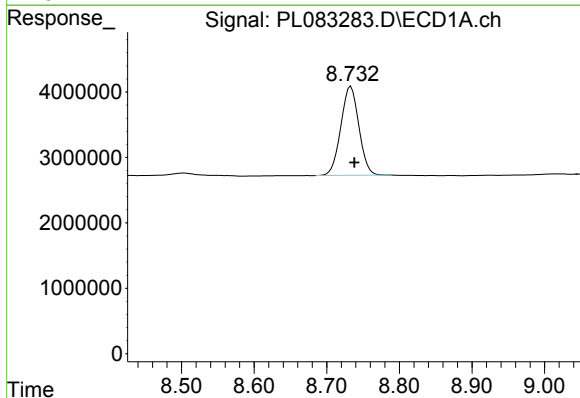

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.005 min
Response: 23534494
Conc: 11.22 ng/ml

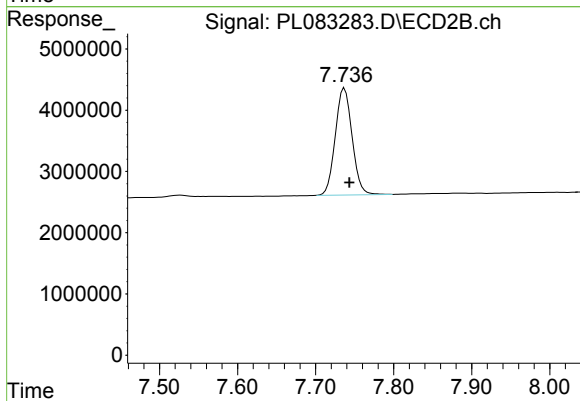

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.006 min
Response: 26141956
Conc: 10.51 ng/ml