

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
 Data File : PL083287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 14:20
 Operator : AR\AJ
 Sample : 03044-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-04-5.0-7.0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/08/2023
 Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:20:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	2.632	32542271	34646694	11.072m	13.346
28)	SA Decachlor...	8.733	7.737	30131915	32193297	14.367	12.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
Data File : PL083287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 14:20
Operator : AR\AJ
Sample : 03044-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/08/2023
Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:20:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

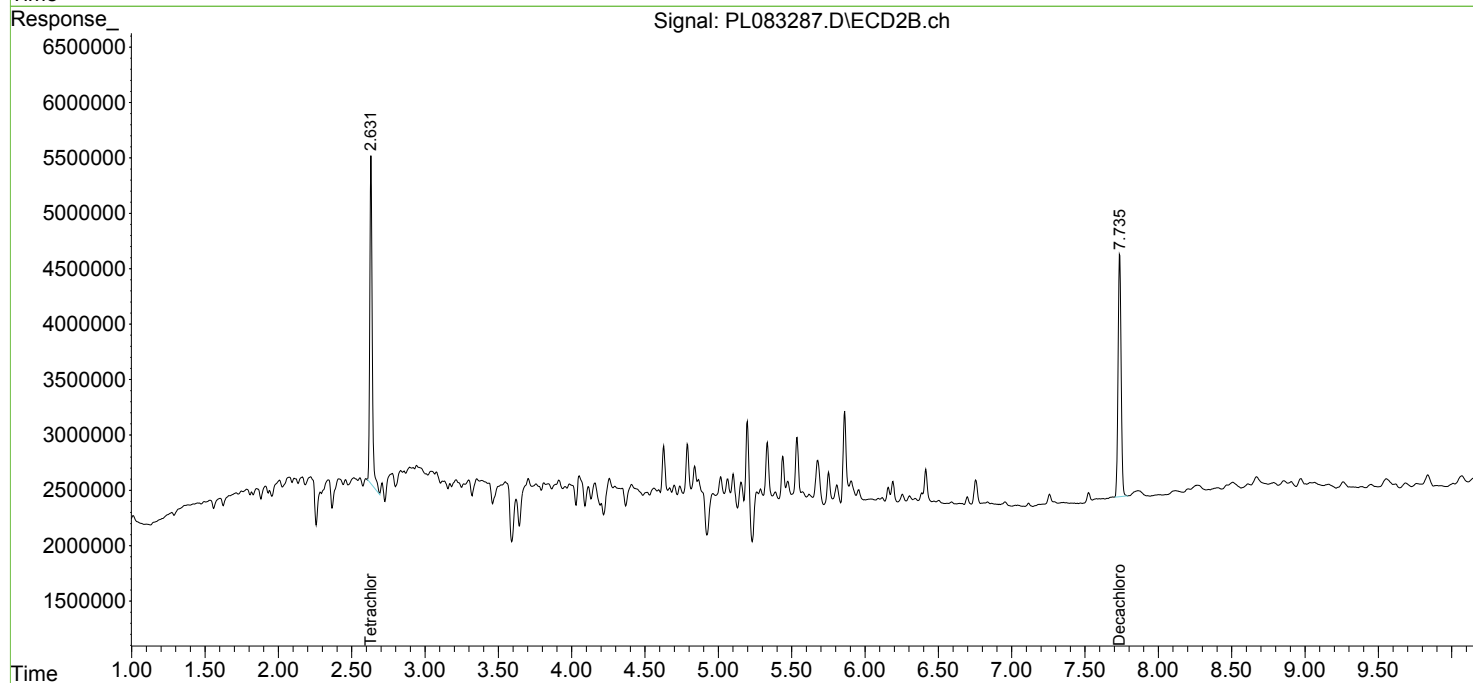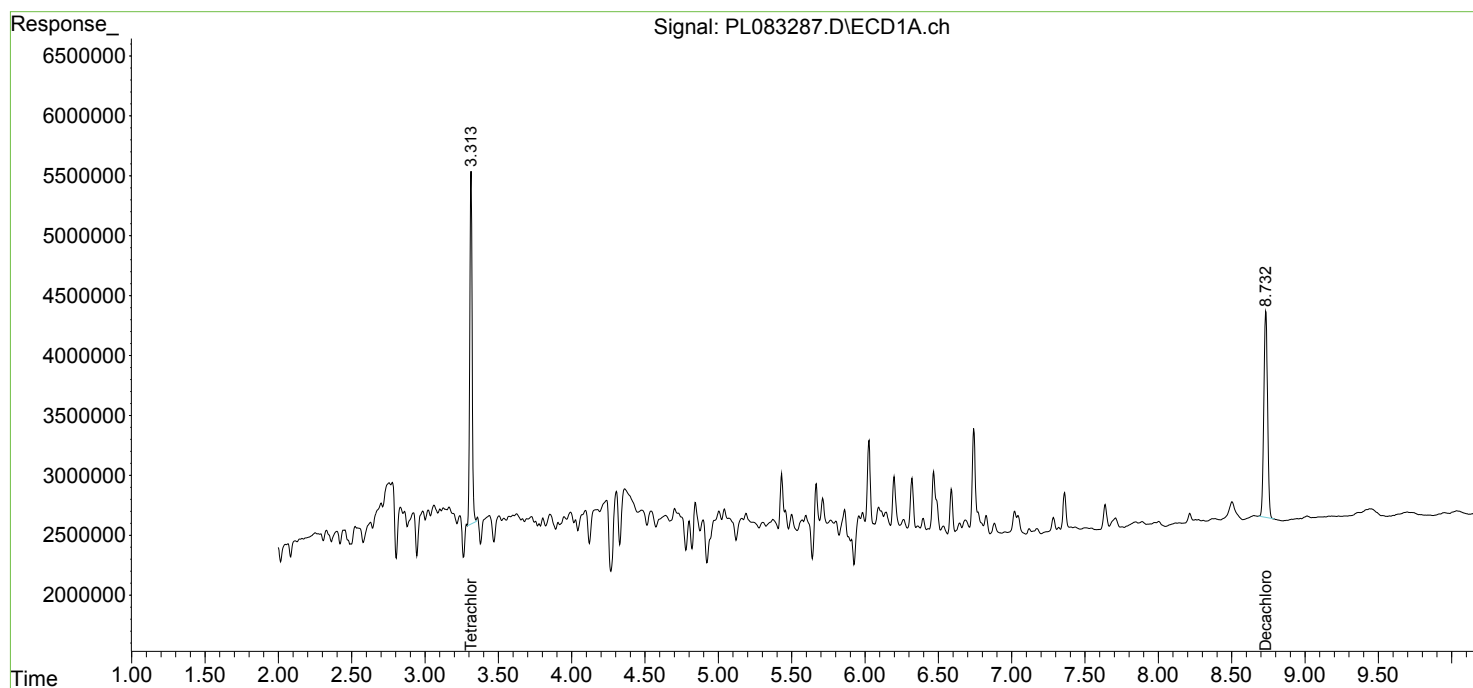

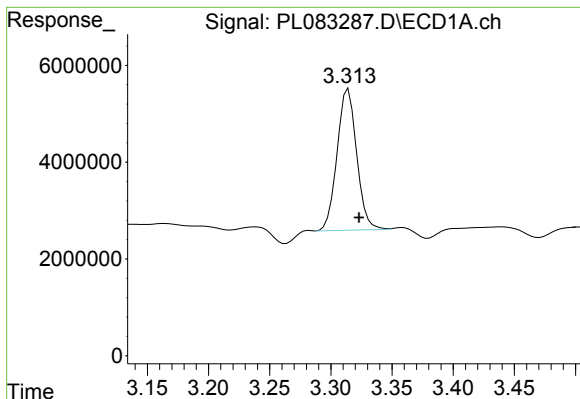


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 32542271
Conc: 11.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-04-5.0-7.0


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

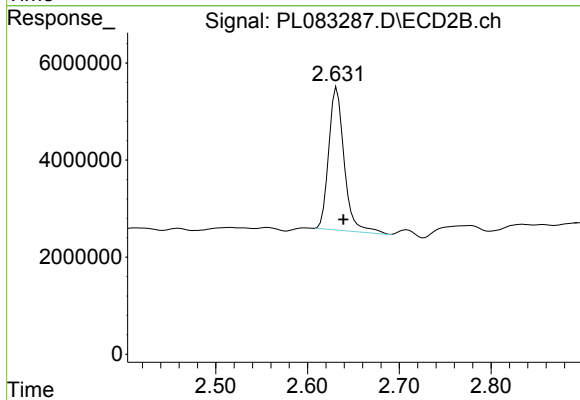


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: -0.007 min
Response: 34646694
Conc: 13.35 ng/ml

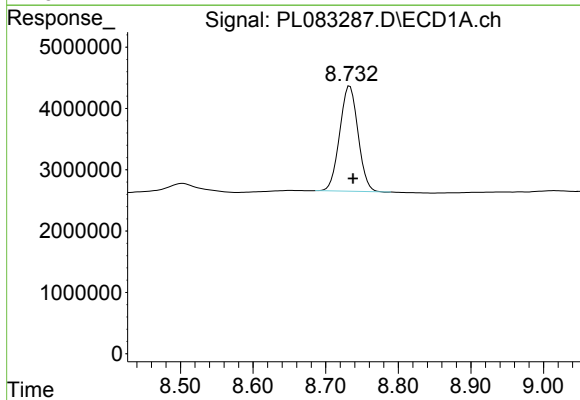

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.005 min
Response: 30131915
Conc: 14.37 ng/ml

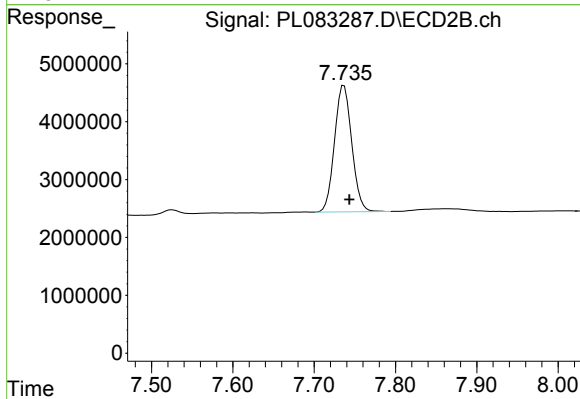

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.007 min
Response: 32193297
Conc: 12.95 ng/ml