

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
 Data File : PL083297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 16:55
 Operator : AR\AJ
 Sample : 03047-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB32A

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/08/2023
 Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:30:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	2.633	46608853	43087034	15.859m	16.597
2)	SA Decachlor...	8.731	7.737	26755936	27586266	12.757	11.094

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
Data File : PL083297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 16:55
Operator : AR\AJ
Sample : 03047-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB32A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/08/2023
Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:30:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

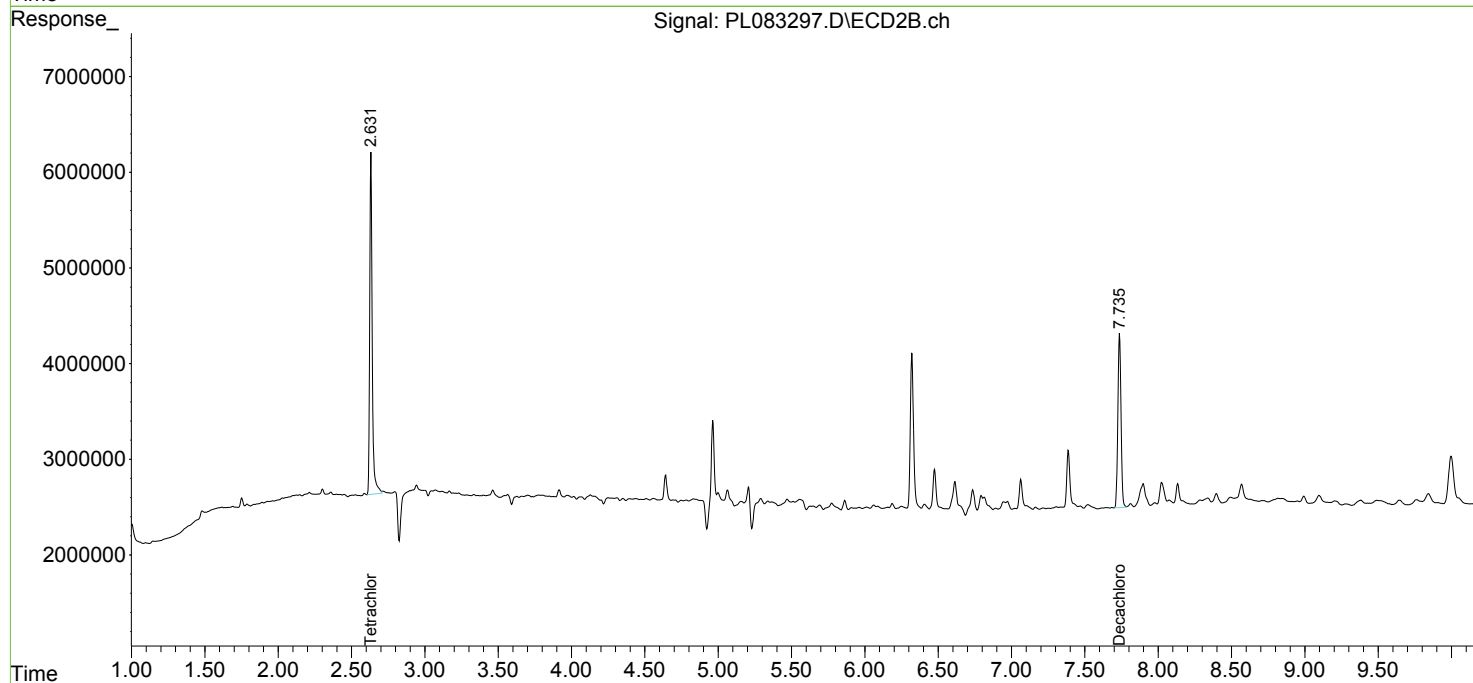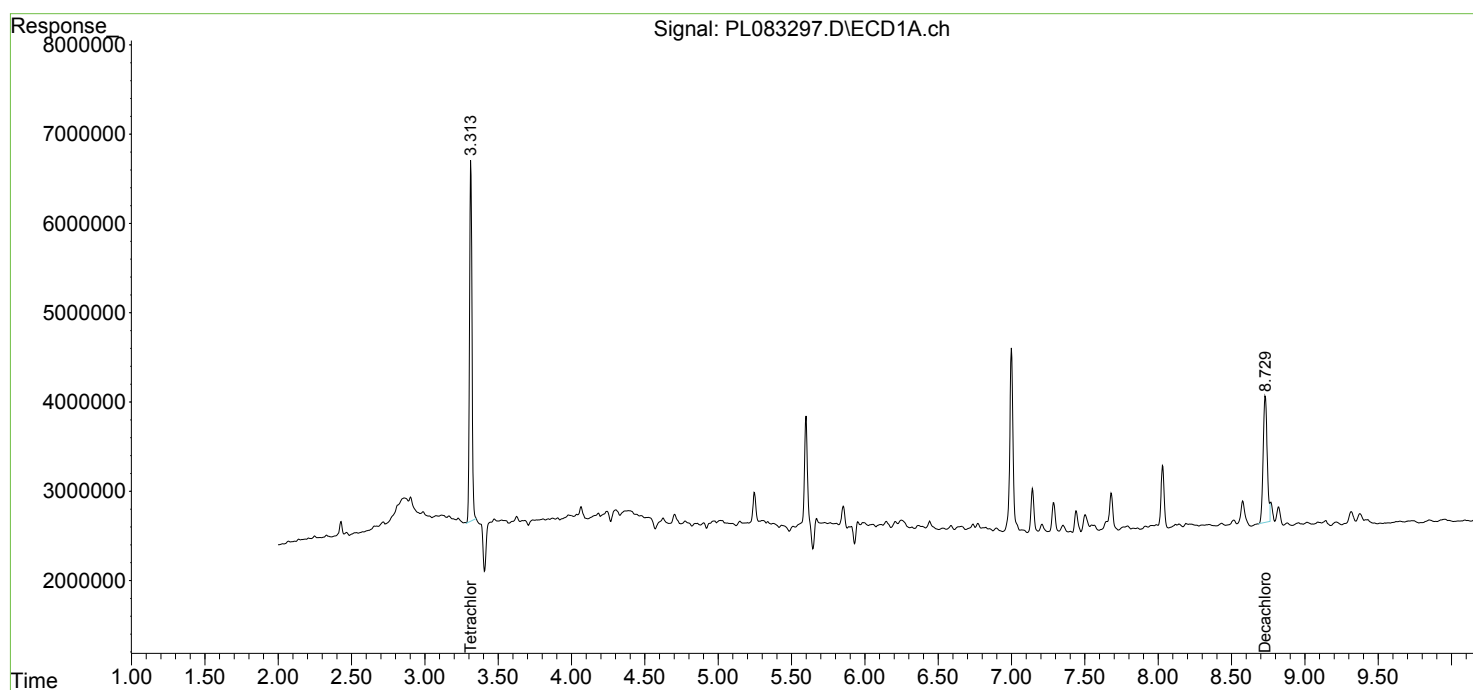

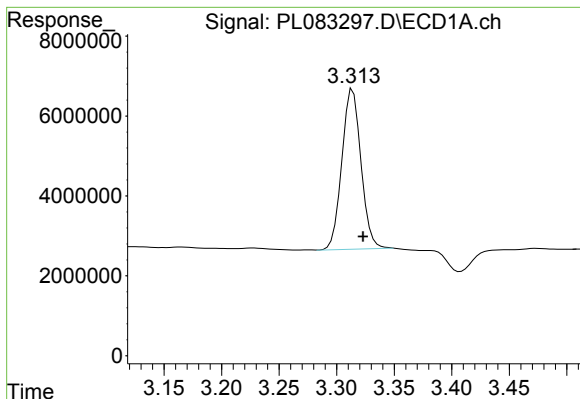


#1 Tetrachloro-m-xylene

R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 46608853
Conc: 15.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB32A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

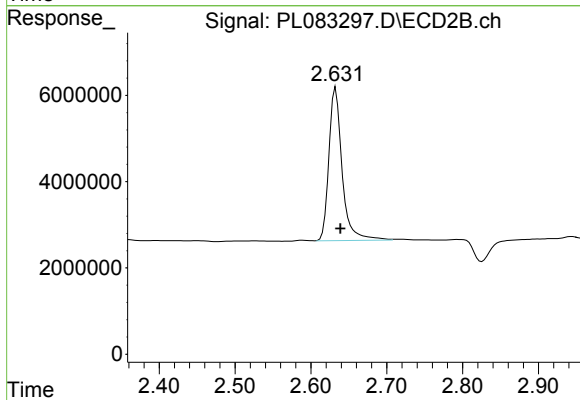


#1 Tetrachloro-m-xylene

R.T.: 2.633 min
Delta R.T.: -0.006 min
Response: 43087034
Conc: 16.60 ng/ml

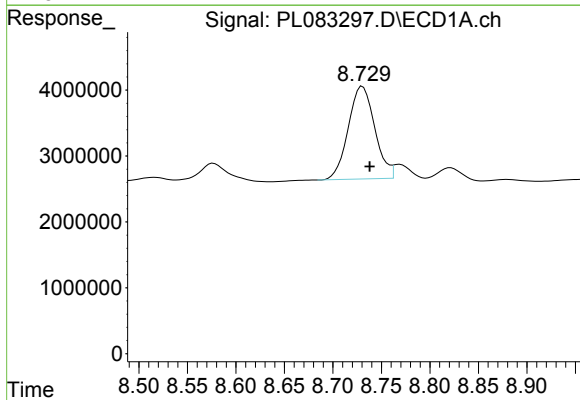

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: -0.007 min
Response: 26755936
Conc: 12.76 ng/ml

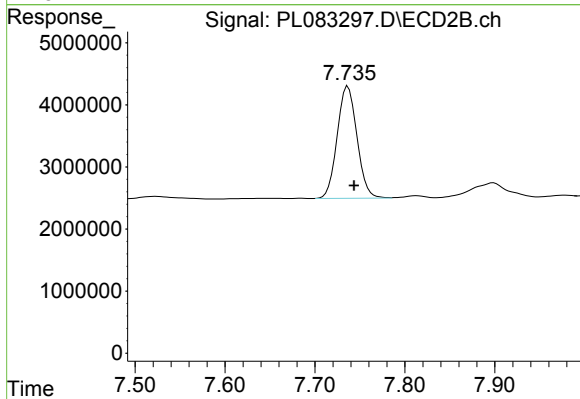

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.007 min
Response: 27586266
Conc: 11.09 ng/ml