

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
 Data File : PL083300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 17:37
 Operator : AR\AJ
 Sample : 03047-02MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB32BMSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/08/2023
 Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:33:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.312	2.632	64628421	57581579	21.990m	22.180
2) SA Decachlor...	8.732	7.736	36129039	41452166	17.226	16.671

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
Data File : PL083300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 17:37
Operator : AR\AJ
Sample : 03047-02MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB32BMSD


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/08/2023
Supervised By : Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:33:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

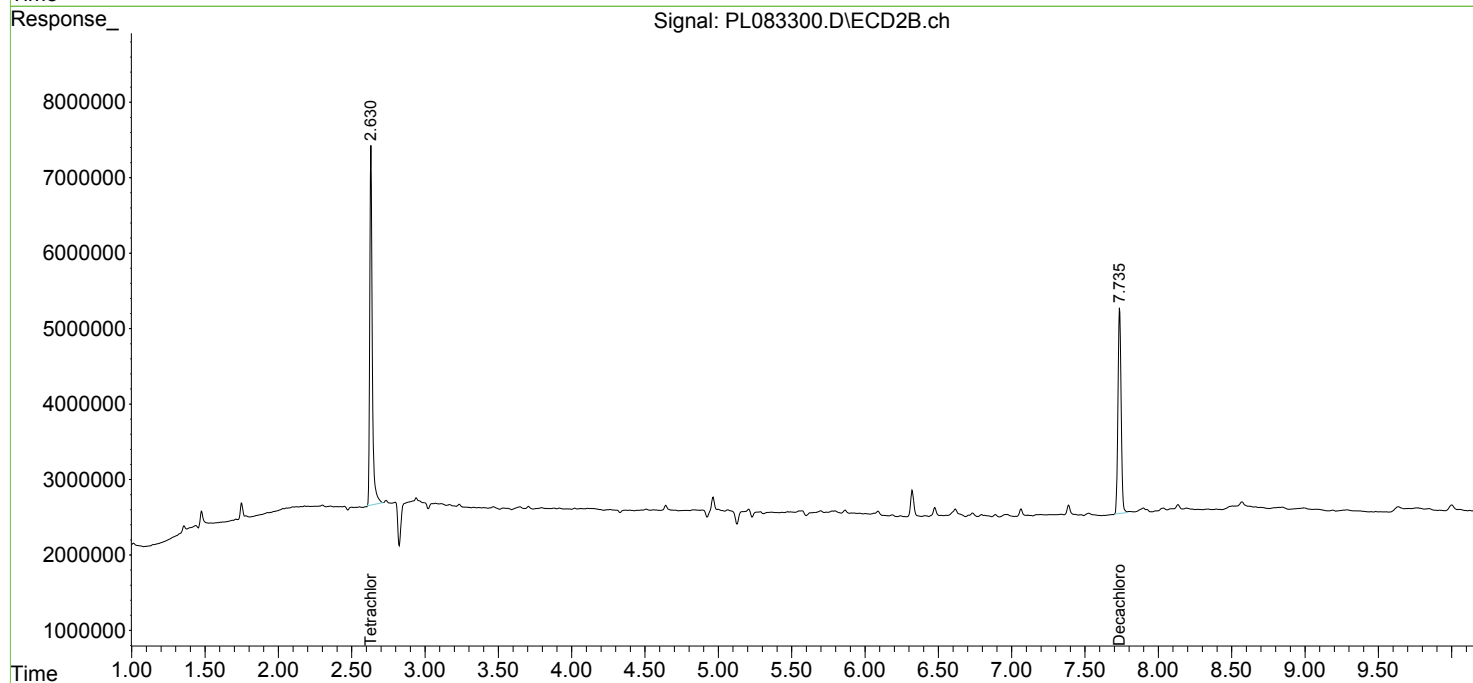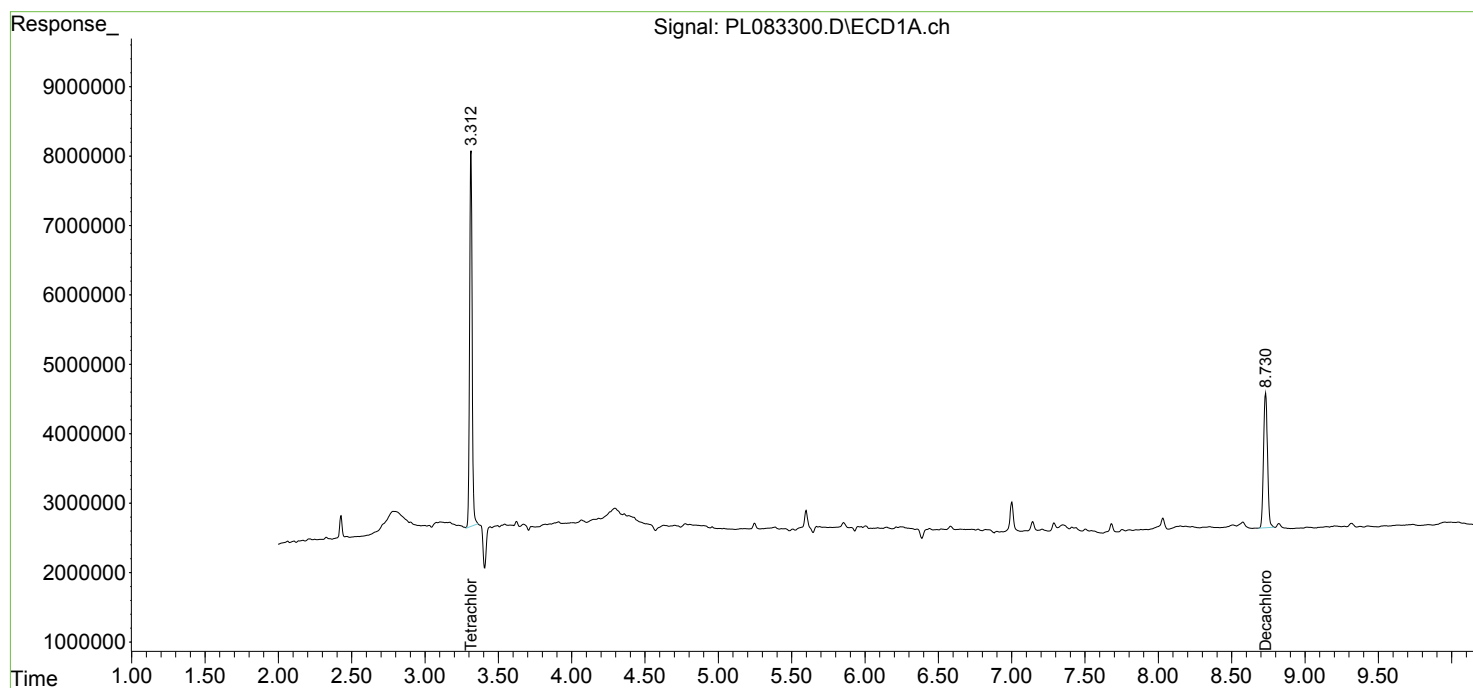

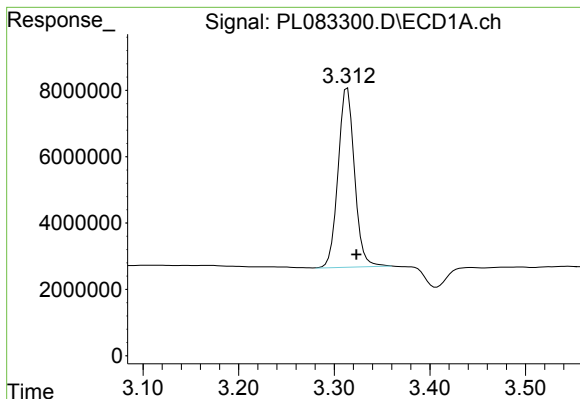


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: -0.011 min
Response: 64628421
Conc: 21.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB32BMSD


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

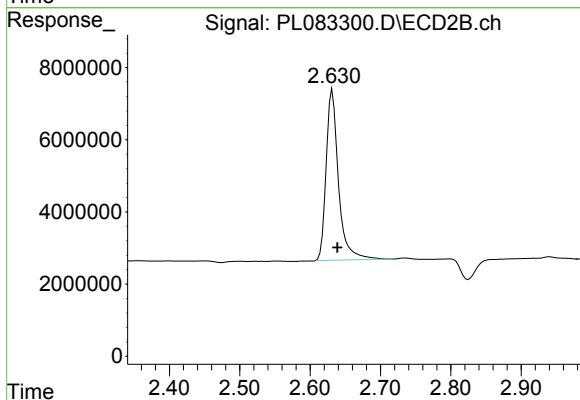


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: -0.007 min
Response: 57581579
Conc: 22.18 ng/ml

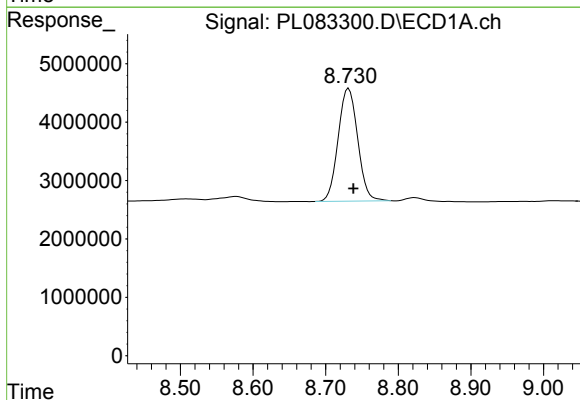

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.006 min
Response: 36129039
Conc: 17.23 ng/ml

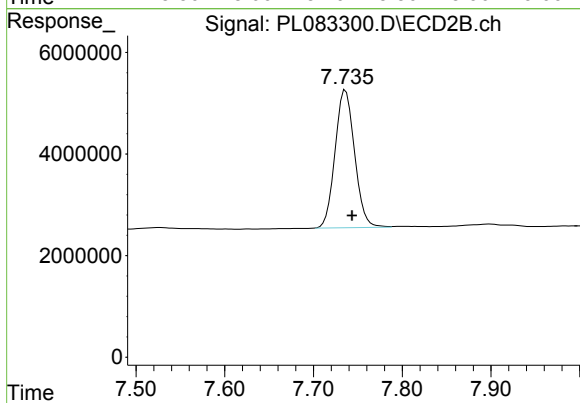

#28 Decachlorobiphenyl

R.T.: 7.736 min
Delta R.T.: -0.007 min
Response: 41452166
Conc: 16.67 ng/ml