

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
 Data File : PL083306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 19:01
 Operator : AR\AJ
 Sample : 03064-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-24236

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:38:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	2.632	21354787	20162614	7.266	7.767
28)	SA Decachlor...	8.732	7.736	20836021	24213465	9.935	9.738
Target Compounds							
12)	B 4,4'-DDE	5.943	5.063	1511695	1266016	0.548	0.521


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060723\
Data File : PL083306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 19:01
Operator : AR\AJ
Sample : 03064-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-24236

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:38:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

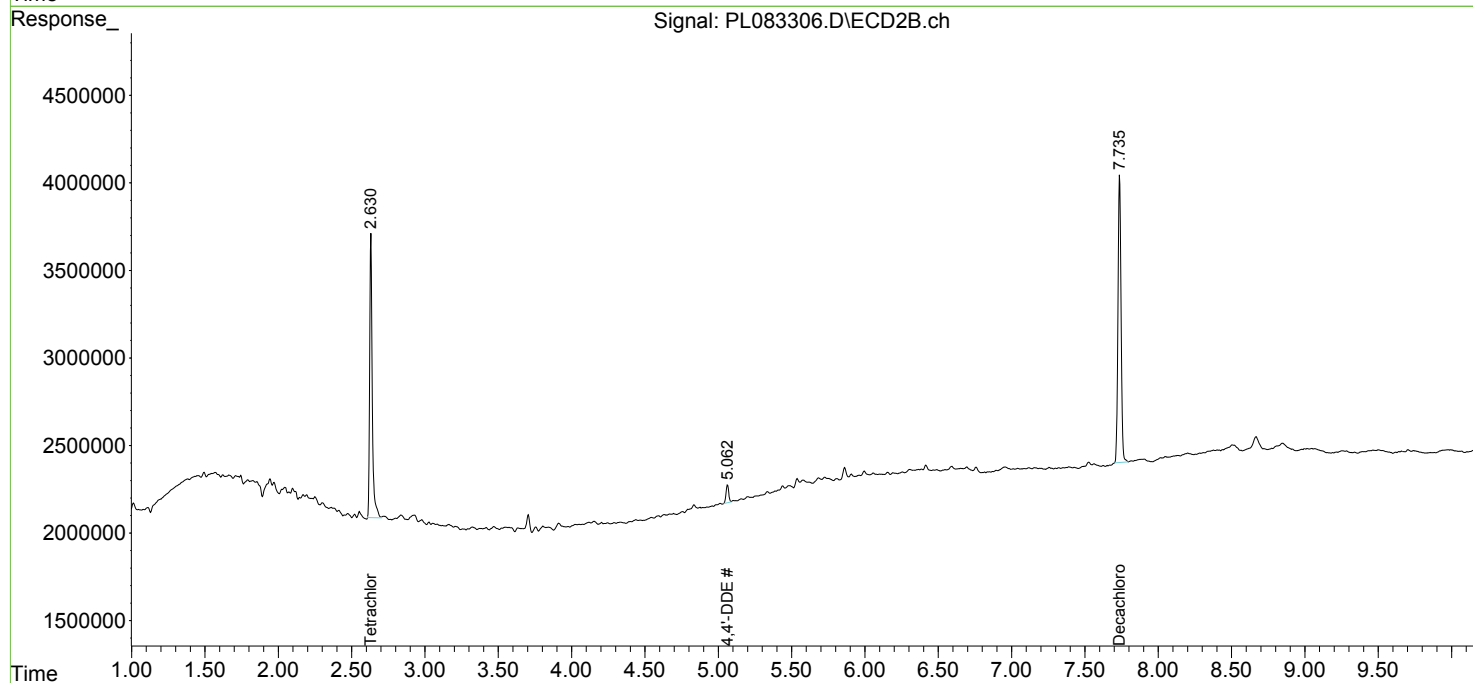


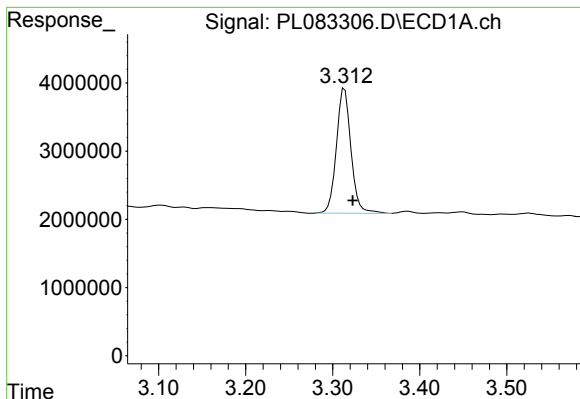

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.009 min
Response: 21354787
Conc: 7.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24236

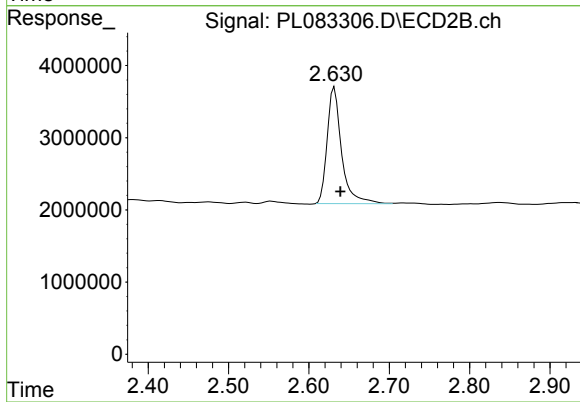


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: -0.007 min
Response: 20162614
Conc: 7.77 ng/ml

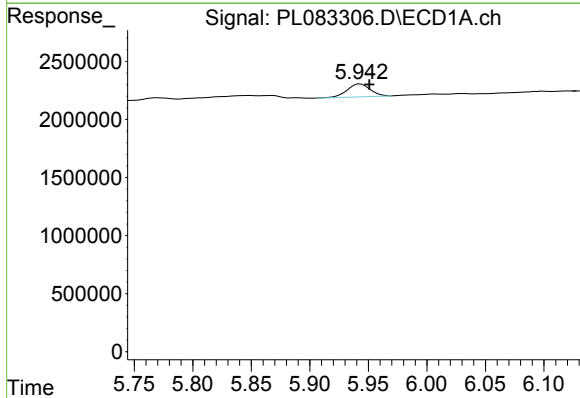


#12 4,4'-DDE

R.T.: 5.943 min
Delta R.T.: -0.008 min
Response: 1511695
Conc: 0.55 ng/ml

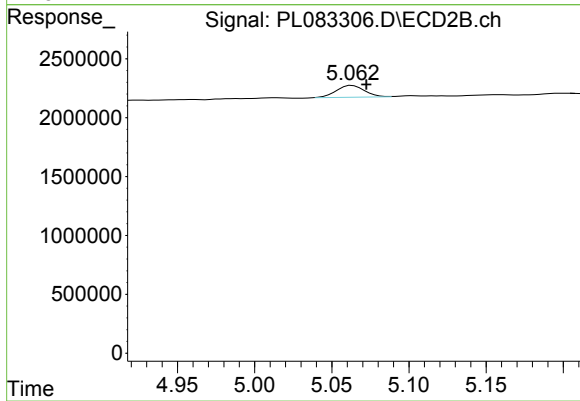

#12 4,4'-DDE

R.T.: 5.063 min
Delta R.T.: -0.009 min
Response: 1266016
Conc: 0.52 ng/ml

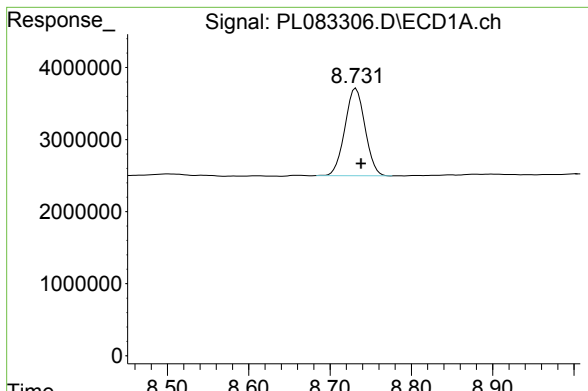

#28 Decachlorobiphenyl


R.T.: 8.732 min

Delta R.T.: -0.006 min

Response: 20836021

Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24236

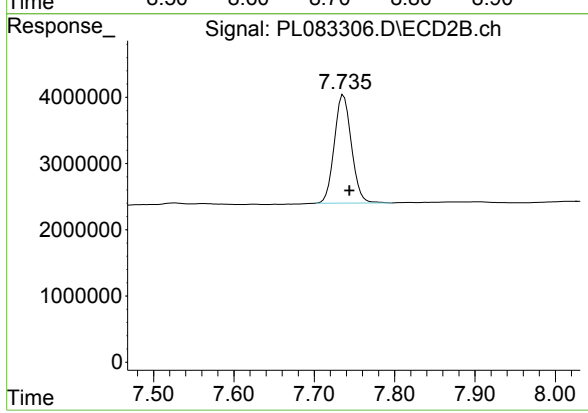

#28 Decachlorobiphenyl

R.T.: 7.736 min

Delta R.T.: -0.007 min

Response: 24213465

Conc: 9.74 ng/ml