

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060820\
 Data File : PL059170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2020 13:14
 Operator : AJ\MA
 Sample : PB129376BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 15:07:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.072	36378356	41820294	21.067	16.073
28)	SA Decachlor...	8.303	9.185	32703310	46546761	19.888	19.636
Target Compounds							
7)	B delta-BHC	0.000	5.167f	0	1062753	N.D.	0.379 #
8)	B Heptachlo...	0.000	5.949	0	283550	N.D.	0.102 #
14)	MA Endrin	0.000	6.798	0	2051993	N.D.	0.824 #
15)	B Endosulfa...	0.000	6.994	0	4519436	N.D.	1.735 #
16)	A 4,4'-DDD	6.210	6.927	2180820	404374	1.650	0.174 #
17)	MA 4,4'-DDT	6.450	7.192f	1001022	28451	0.794	0.012 #
21)	B Endrin ke...	7.242	0.000	42826	0	0.025	N.D. #
22)	Mirex	7.426	8.311f	1509585	102557	1.094	0.052 #
27)	Chlordane-5	0.000	7.088	0	238907	N.D.	3.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060820\
Data File : PL059170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2020 13:14
Operator : AJ\MA
Sample : PB129376BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 15:07:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

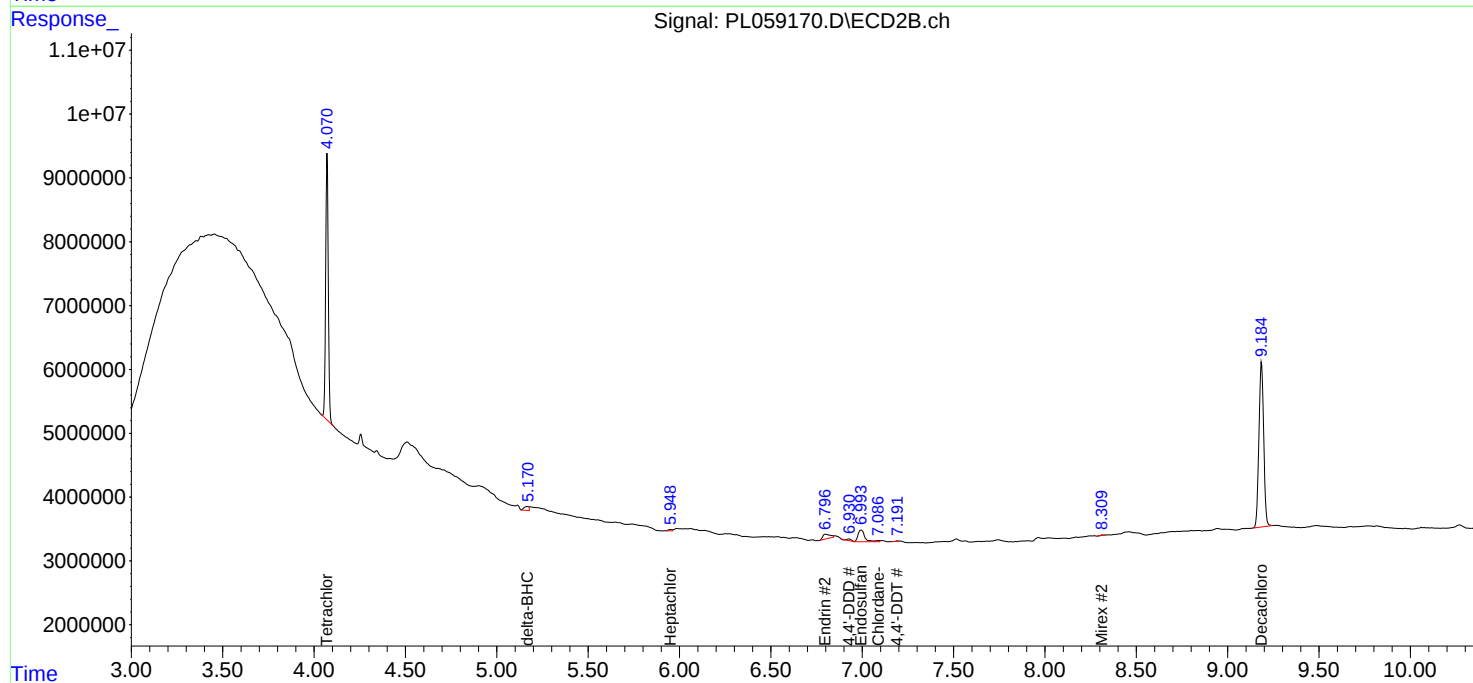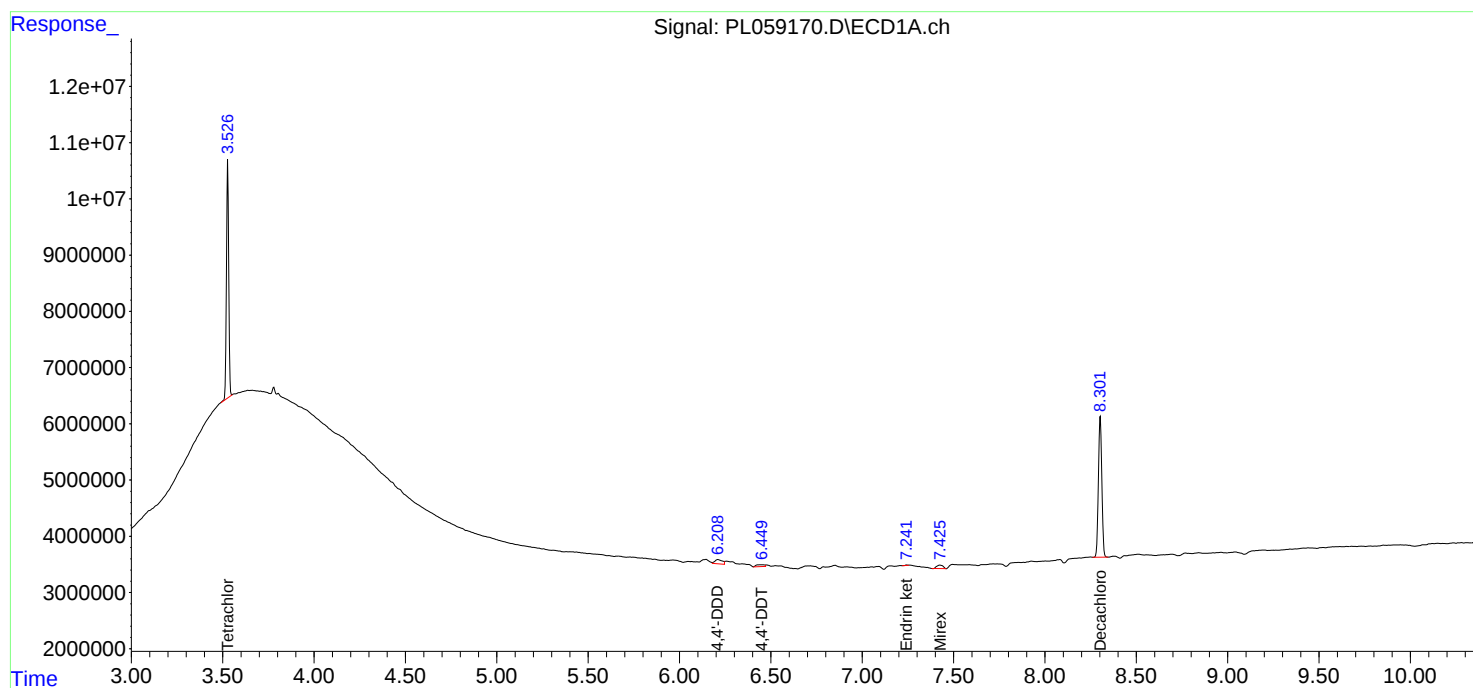


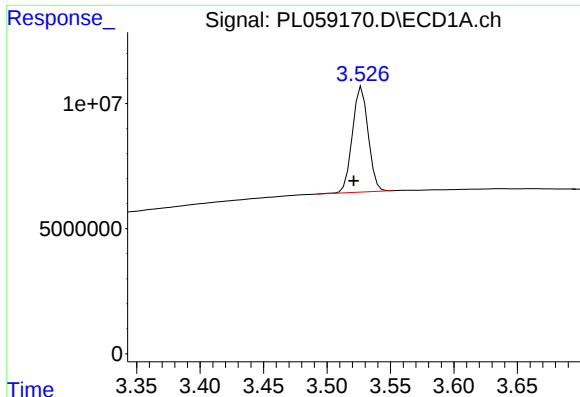

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: 0.007 min
Response: 36378356
Conc: 21.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

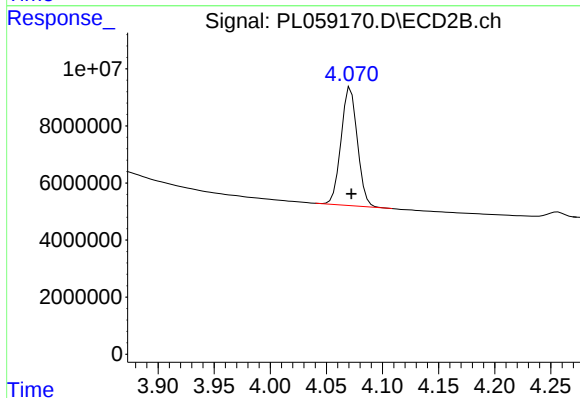


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 41820294
Conc: 16.07 ng/ml

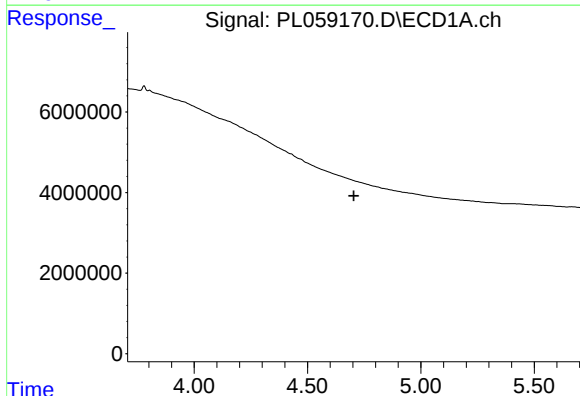


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

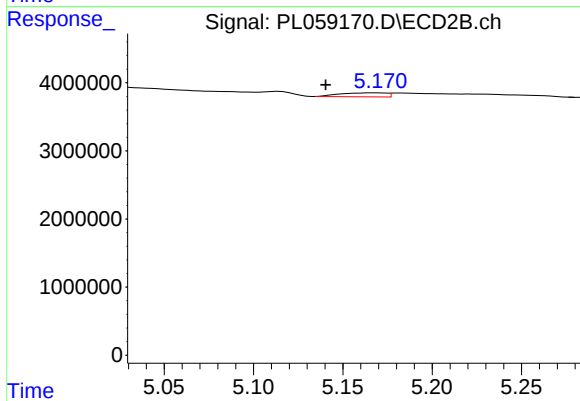

#7 delta-BHC


R.T.: 5.167 min
Delta R.T.: 0.026 min
Response: 1062753
Conc: 0.38 ng/ml

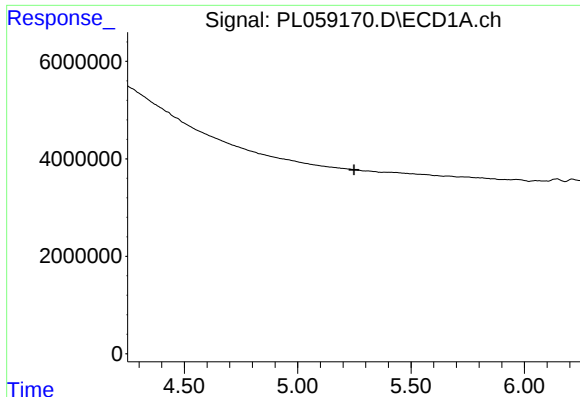

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

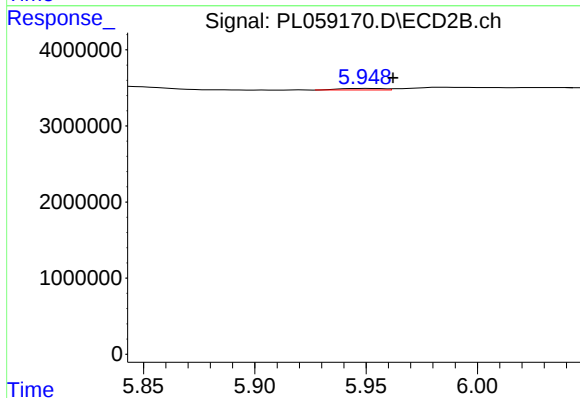


#8 Heptachlor epoxide

R.T.: 5.949 min
Delta R.T.: -0.013 min
Response: 283550
Conc: 0.10 ng/ml

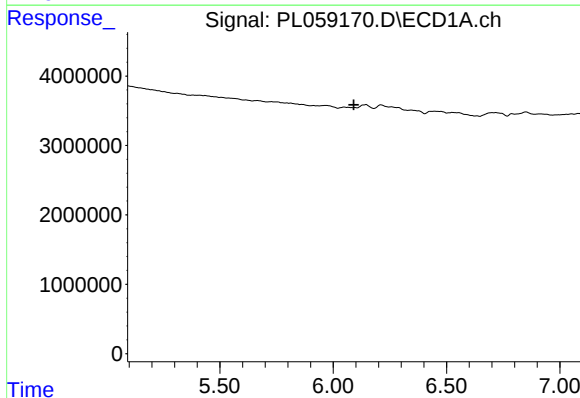


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.091 min
Response: 0
Conc: N.D.

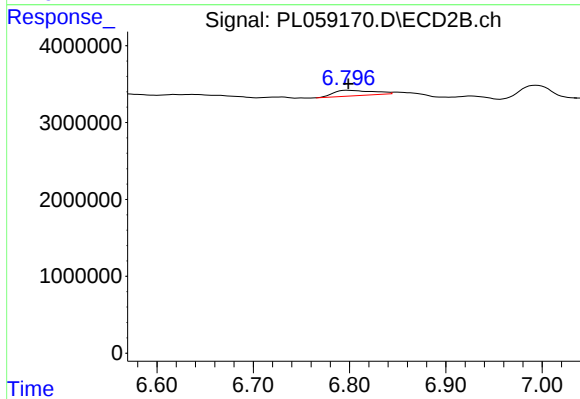

#14 Endrin


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 2051993
Conc: 0.82 ng/ml

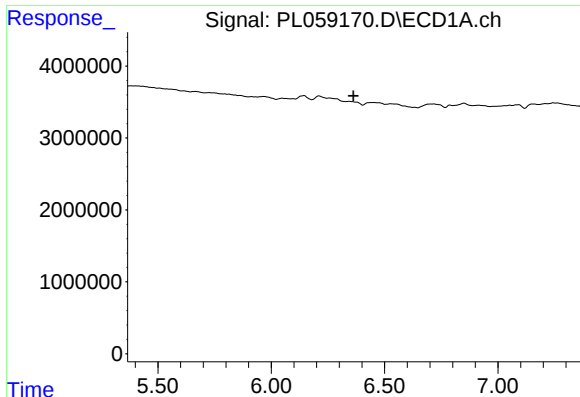

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

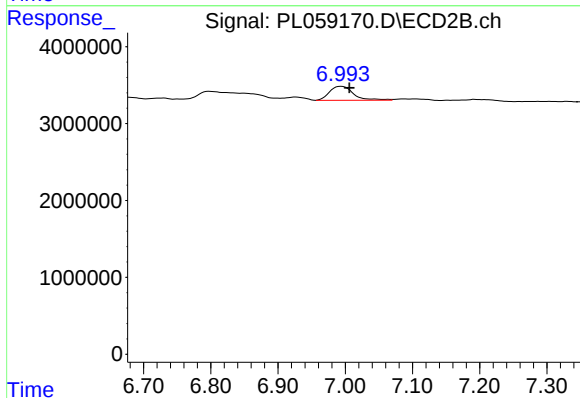


#15 Endosulfan II

R.T.: 6.994 min
Delta R.T.: -0.012 min
Response: 4519436
Conc: 1.73 ng/ml

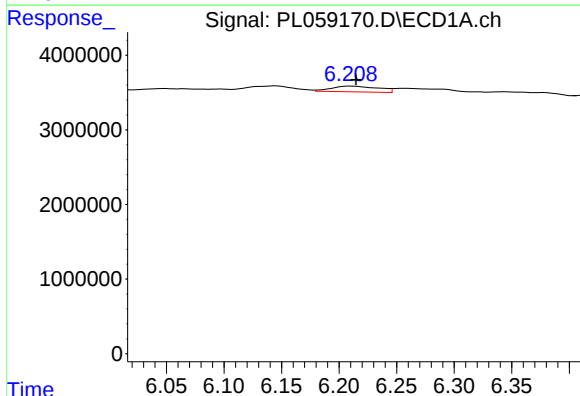


#16 4,4'-DDD

R.T.: 6.210 min
Delta R.T.: -0.005 min
Response: 2180820
Conc: 1.65 ng/ml

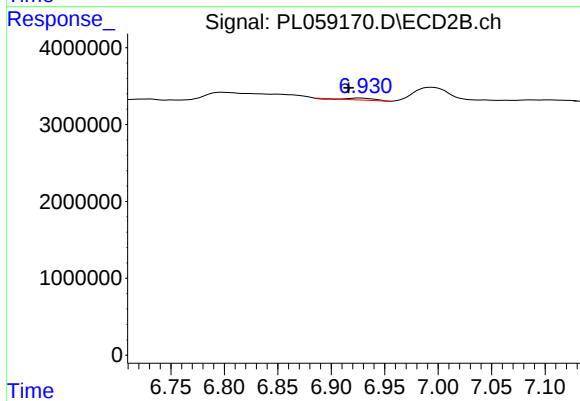

#16 4,4'-DDD


R.T.: 6.927 min
Delta R.T.: 0.011 min
Response: 404374
Conc: 0.17 ng/ml

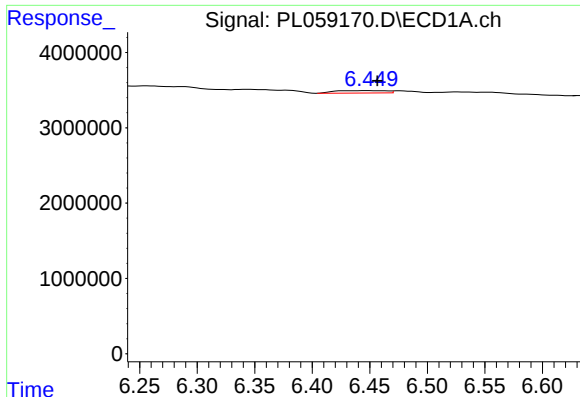

#17 4,4'-DDT


R.T.: 6.450 min
Delta R.T.: -0.006 min
Response: 1001022
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

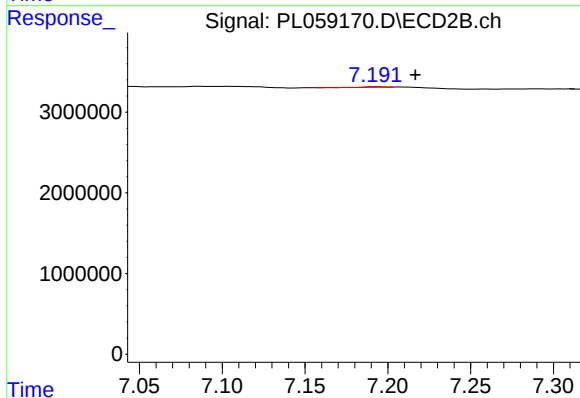


#17 4,4'-DDT

R.T.: 7.192 min
Delta R.T.: -0.024 min
Response: 28451
Conc: 0.01 ng/ml

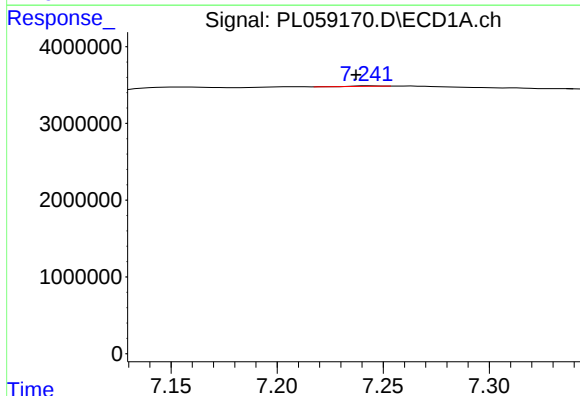


#21 Endrin ketone

R.T.: 7.242 min
Delta R.T.: 0.005 min
Response: 42826
Conc: 0.02 ng/ml

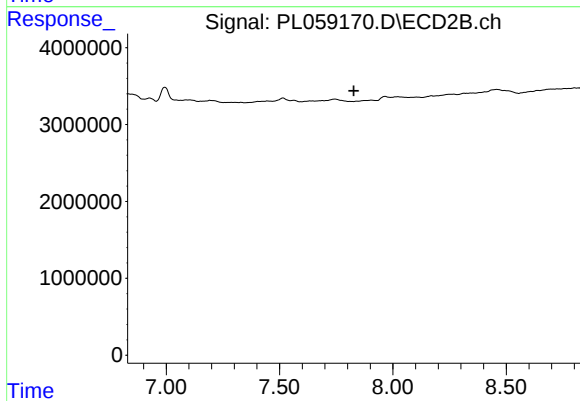

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.828 min
Response: 0
Conc: N.D.

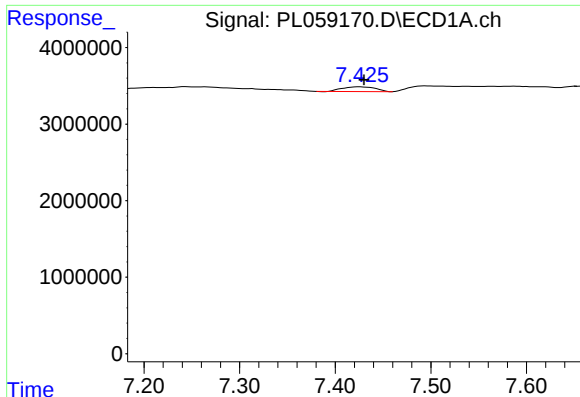

#22 Mirex


R.T.: 7.426 min
Delta R.T.: -0.004 min
Response: 1509585
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

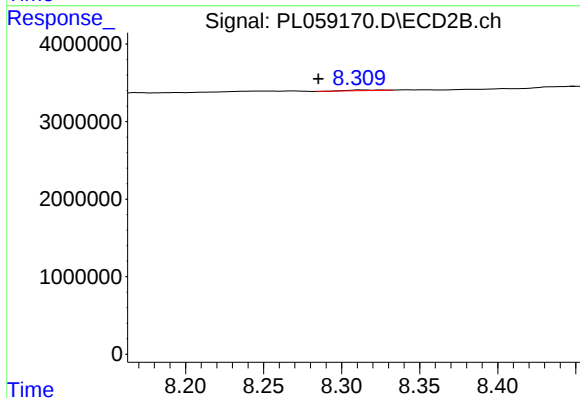


#22 Mirex

R.T.: 8.311 min
Delta R.T.: 0.026 min
Response: 102557
Conc: 0.05 ng/ml

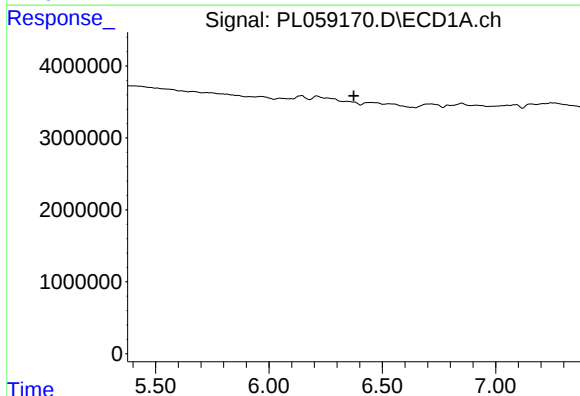


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.374 min
Response: 0
Conc: N.D.

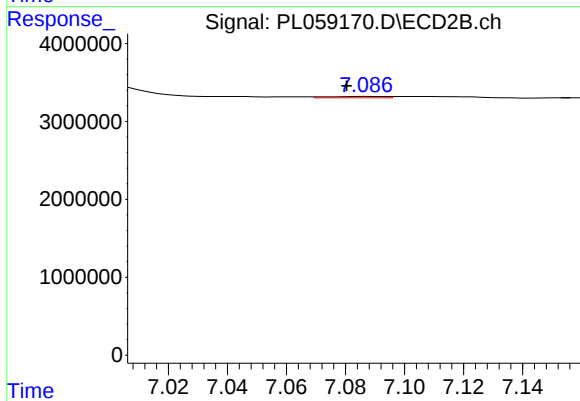

#27 Chlordane-5


R.T.: 7.088 min
Delta R.T.: 0.007 min
Response: 238907
Conc: 3.02 ng/ml

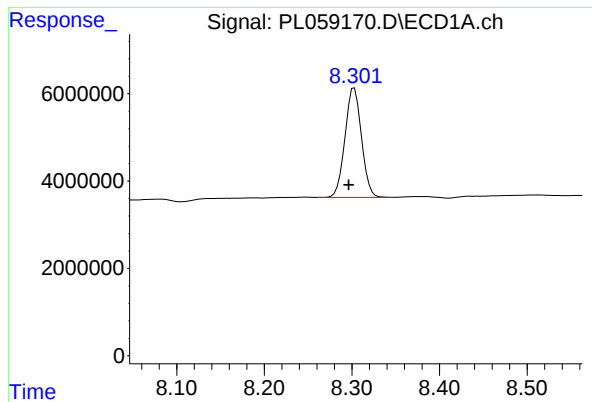

#28 Decachlorobiphenyl

R.T.: 8.303 min
Delta R.T.: 0.006 min
Response: 32703310
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

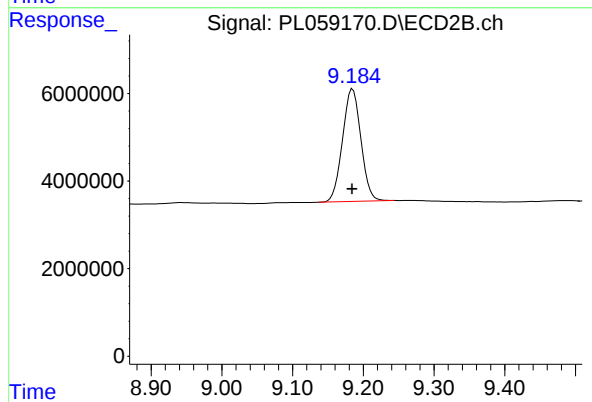

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.000 min
Response: 46546761
Conc: 19.64 ng/ml