

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
 Data File : PL067173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 08:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 05:28:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	5.184	0.000	371957	0	0.703	N.D. #
4) MA	Heptachlor	5.991f	0.000	962287	0	1.832	N.D. #
6) B	beta-BHC	5.991	0.000	962287	0	3.613	N.D. #
8) B	Heptachlo...	0.000	7.996	0	571689	N.D.	0.819 #
22)	Mirex	9.296	0.000	232599	0	0.402	N.D. #
24)	Chlordane-2	6.489	0.000	1489125	0	68.145	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
Data File : PL067173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 08:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 05:28:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

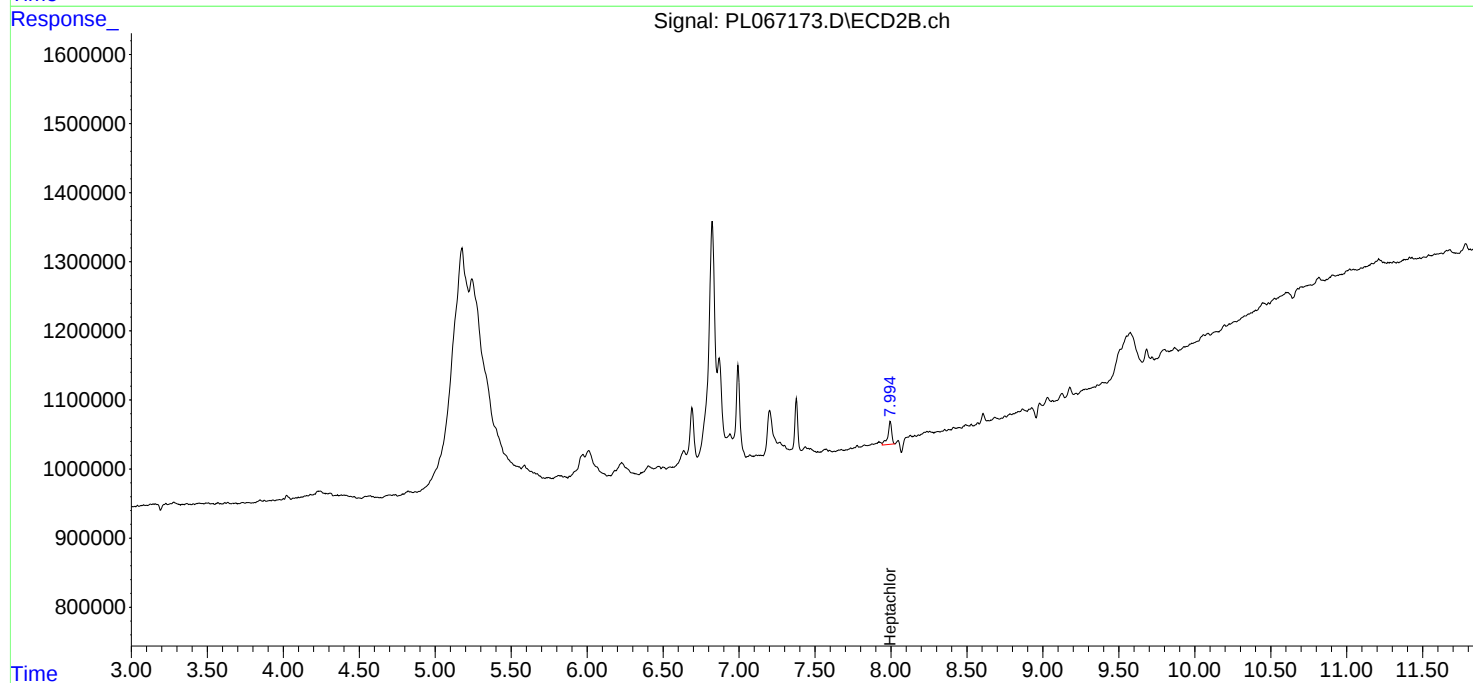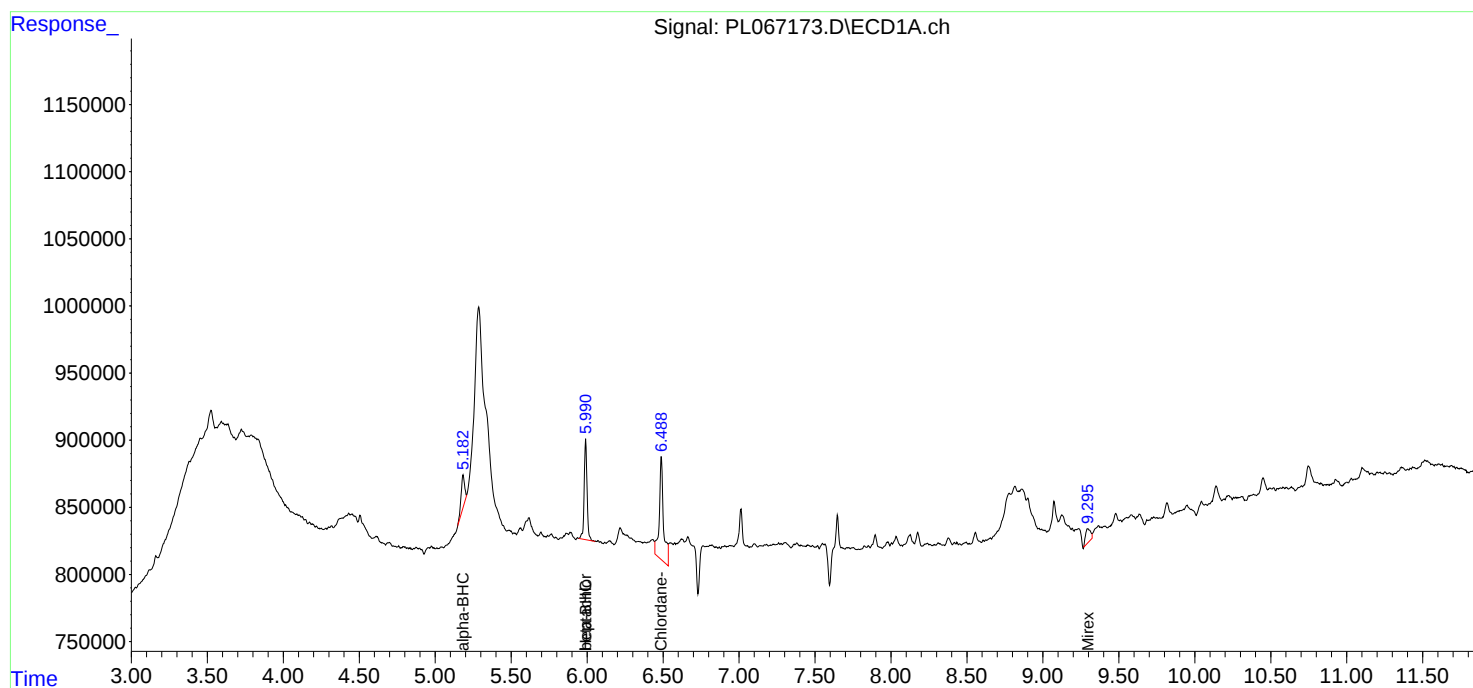


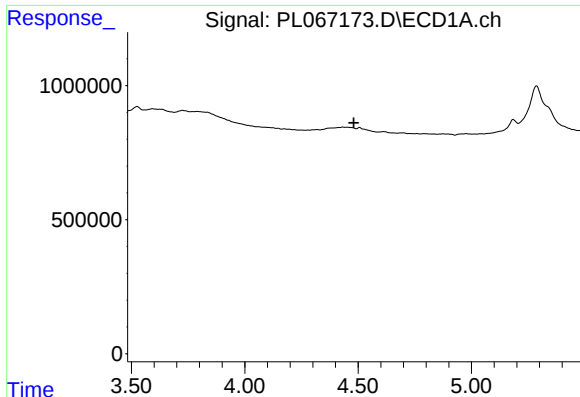

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

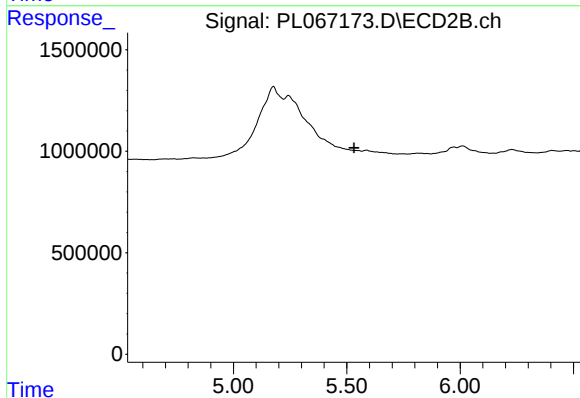


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

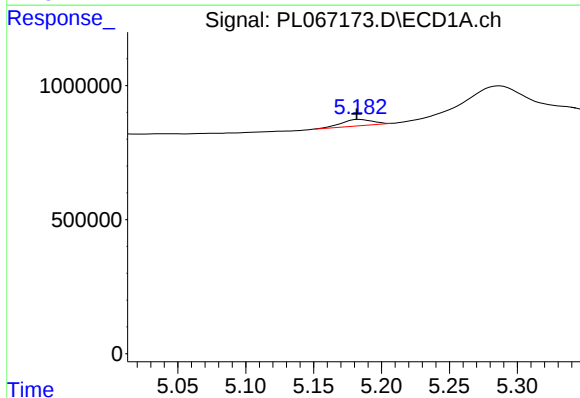


#2 alpha-BHC

R.T.: 5.184 min
Delta R.T.: 0.002 min
Response: 371957
Conc: 0.70 ng/ml

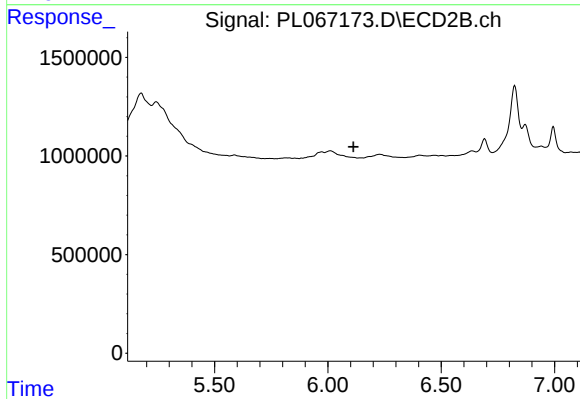

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.113 min
Response: 0
Conc: N.D.

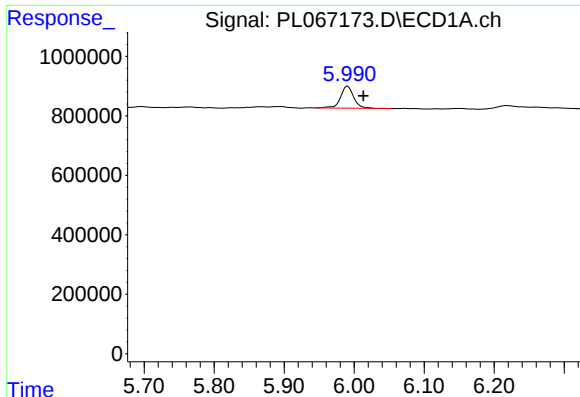

#4 Heptachlor


R.T.: 5.991 min
Delta R.T.: -0.022 min
Response: 962287
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

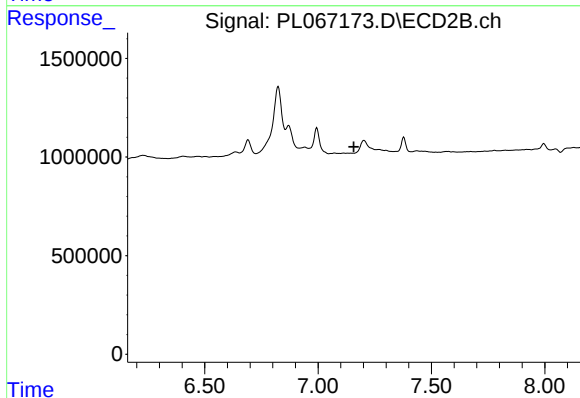


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

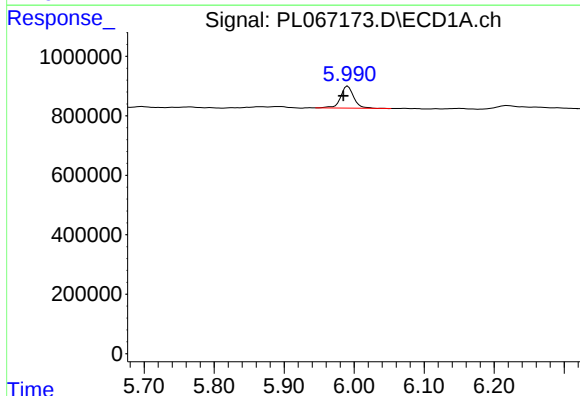


#6 beta-BHC

R.T.: 5.991 min
Delta R.T.: 0.007 min
Response: 962287
Conc: 3.61 ng/ml

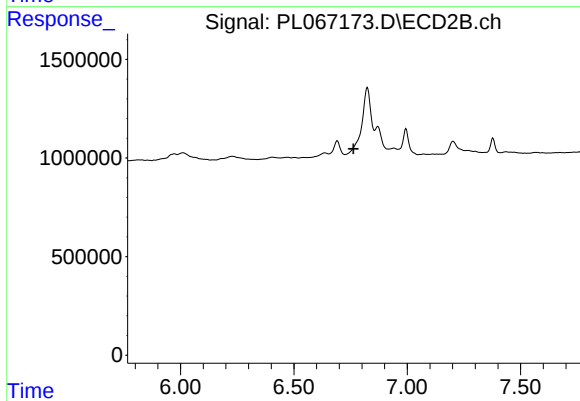

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

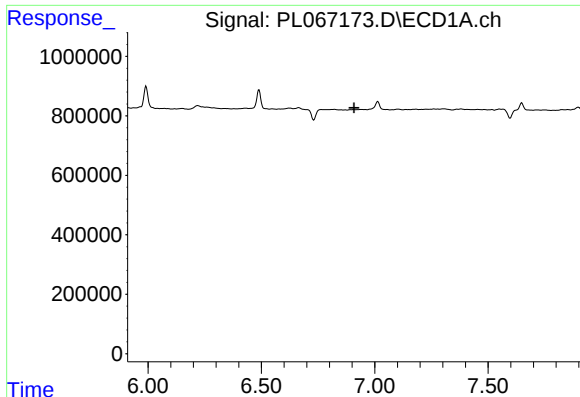

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

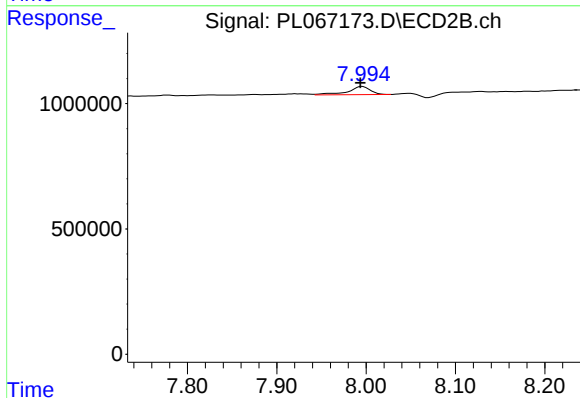


#8 Heptachlor epoxide

R.T.: 7.996 min
Delta R.T.: 0.002 min
Response: 571689
Conc: 0.82 ng/ml

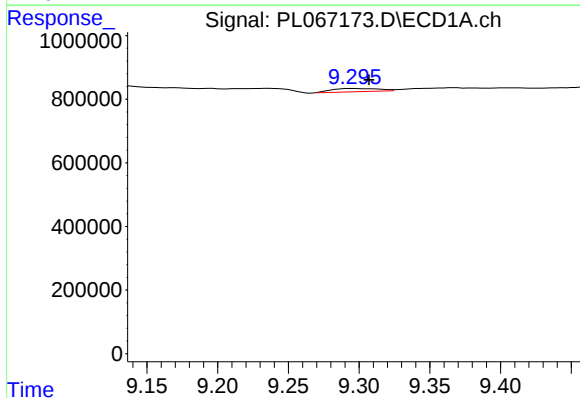


#22 Mirex

R.T.: 9.296 min
Delta R.T.: -0.012 min
Response: 232599
Conc: 0.40 ng/ml

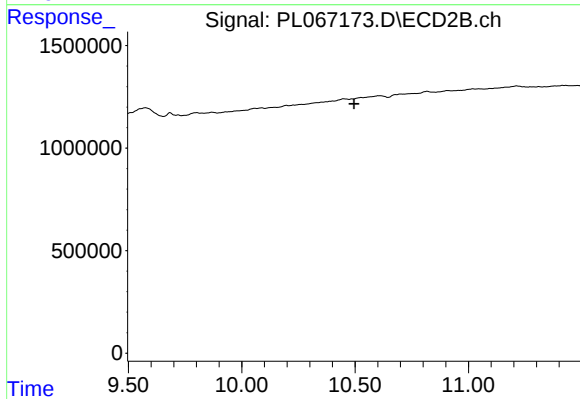

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.496 min
Response: 0
Conc: N.D.

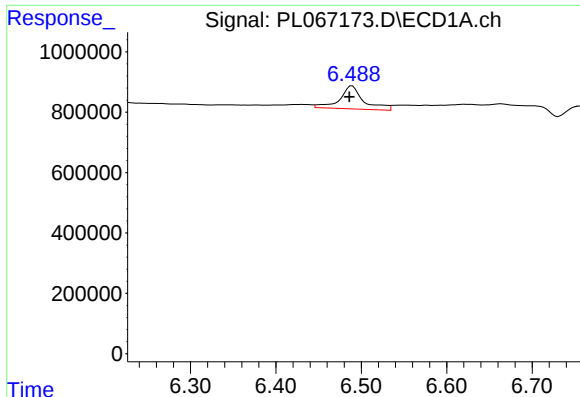

#24 Chlordane-2


R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 1489125
Conc: 68.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

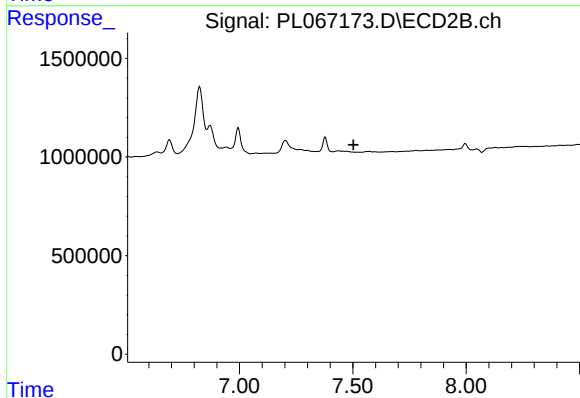


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

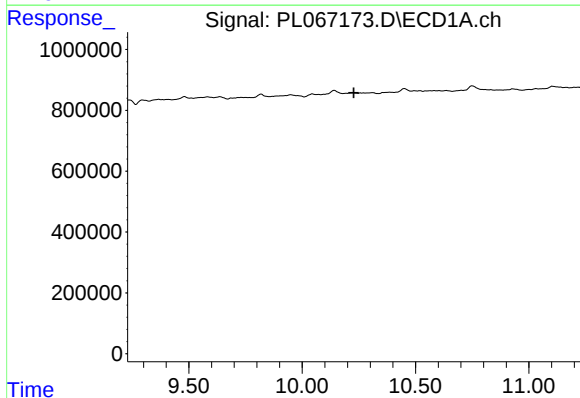

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.228 min
Response: 0
Conc: N.D.

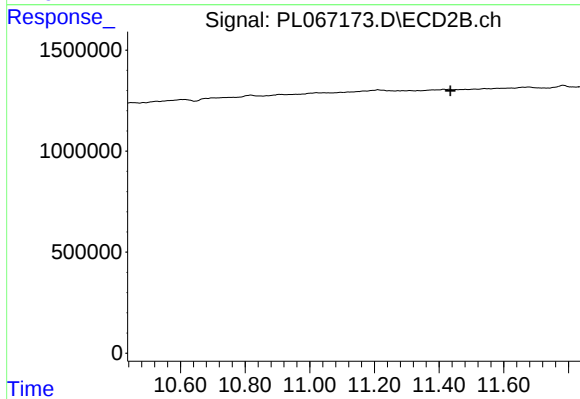

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.435 min
Response: 0
Conc: N.D.