

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
 Data File : PL067183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 12:16
 Operator : AR\AJ
 Sample : M2589-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 05:31:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	10415246	18012529	25.434	27.844
28)	SA Decachlor...	10.220	11.426	14218570	21740497	21.989	26.057
Target Compounds							
3)	MA gamma-BHC...	5.586f	0.000	741215	0	1.331	N.D. #
6)	B beta-BHC	5.965f	0.000	402593	0	1.511	N.D. #
7)	B delta-BHC	0.000	7.005f	0	1697798	N.D.	2.236 #
9)	A Endosulfan I	7.321	0.000	544625	0	1.036	N.D. #
11)	B alpha-Chl...	7.255	0.000	491482	0	0.855	N.D. #
13)	MA Dieldrin	7.592	0.000	225652	0	0.405	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	347426	N.D.	0.563 #
20)	A Methoxychlor	8.911	0.000	222574	0	0.747	N.D. #
26)	Chlordane-4	7.255	0.000	491482	0	7.700	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
Data File : PL067183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 12:16
Operator : AR\AJ
Sample : M2589-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 05:31:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

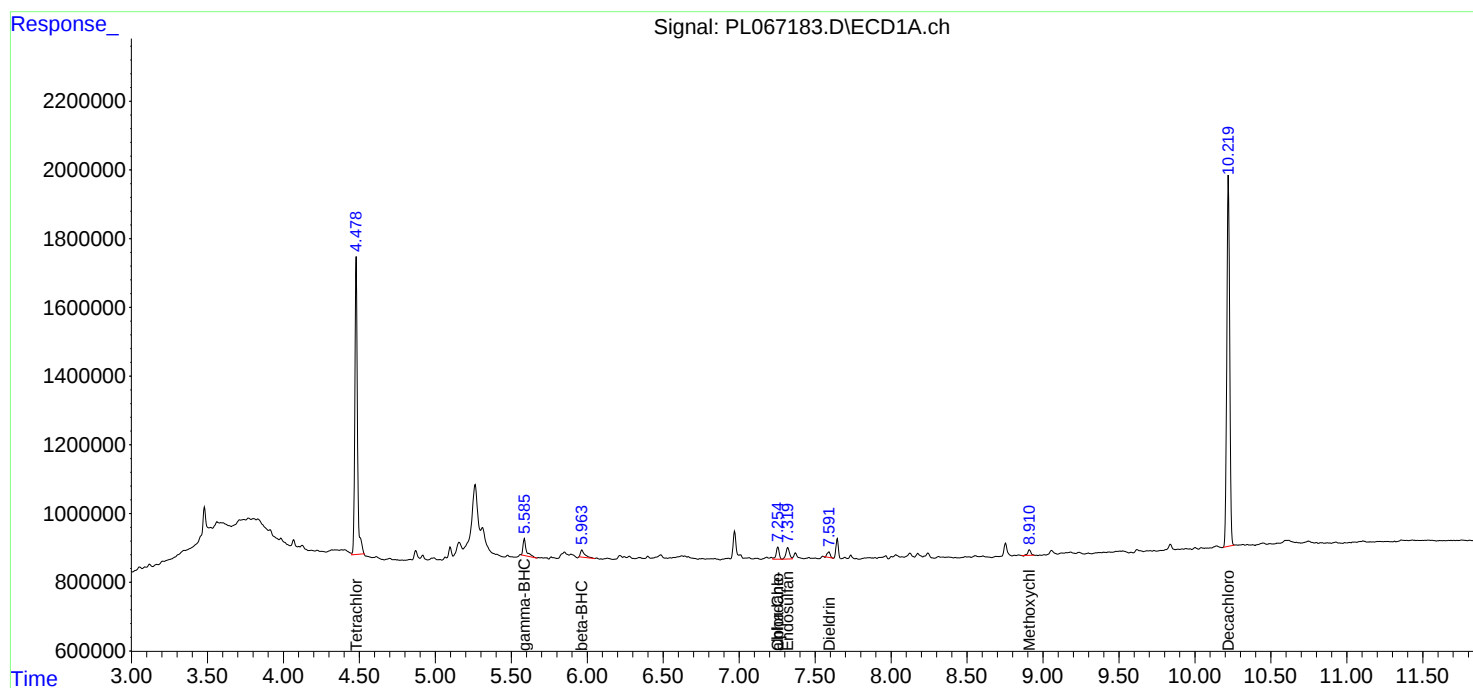


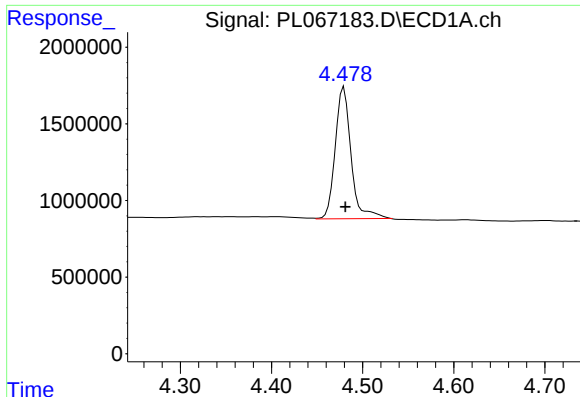

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 10415246
Conc: 25.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

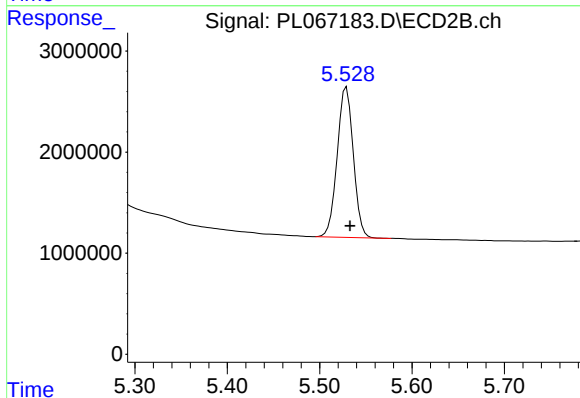


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 18012529
Conc: 27.84 ng/ml

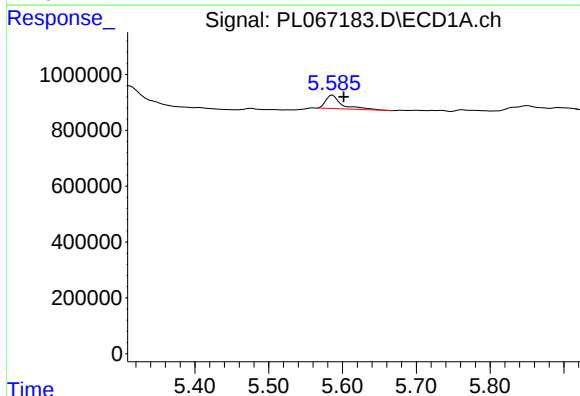


#3 gamma-BHC (Lindane)

R.T.: 5.586 min
Delta R.T.: -0.015 min
Response: 741215
Conc: 1.33 ng/ml

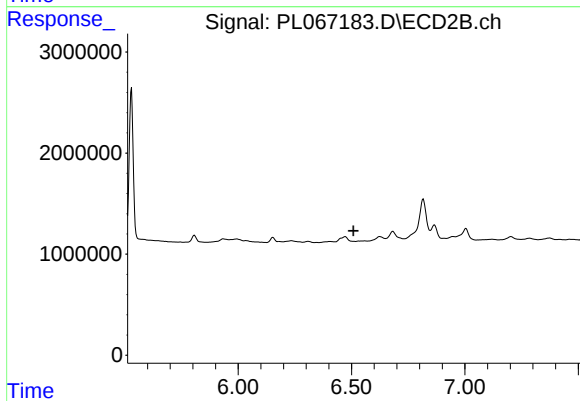

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

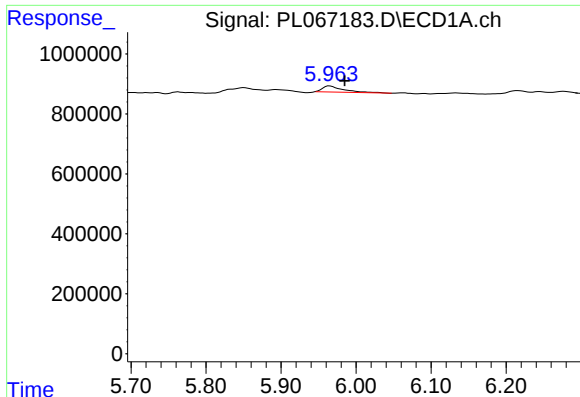

#6 beta-BHC


R.T.: 5.965 min
Delta R.T.: -0.020 min
Response: 402593
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

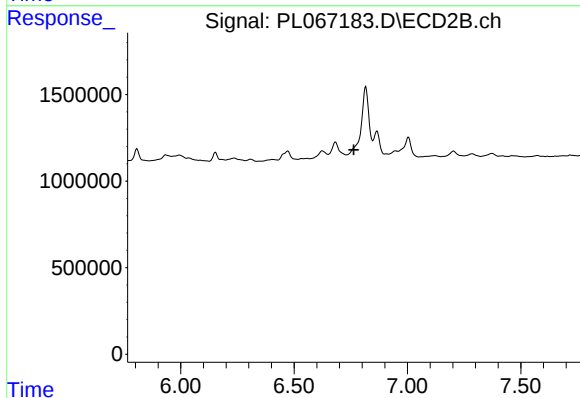


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

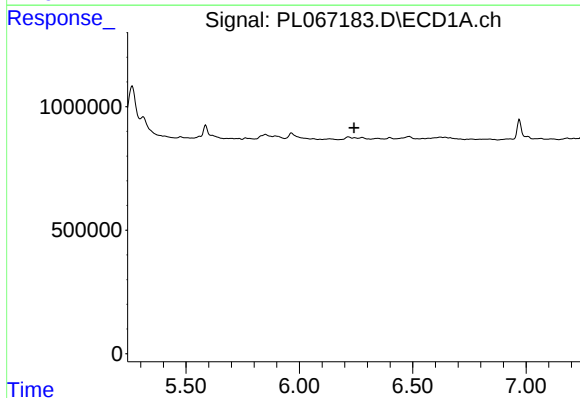


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

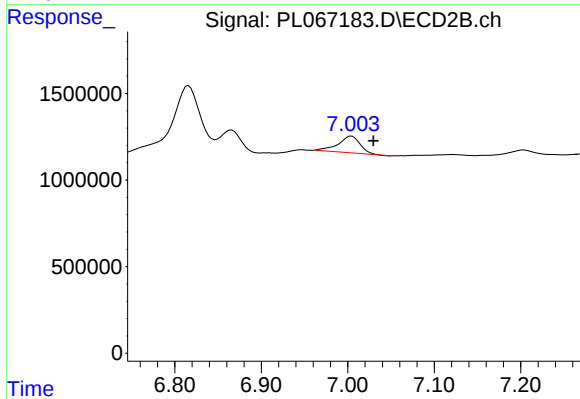

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.025 min
Response: 1697798
Conc: 2.24 ng/ml

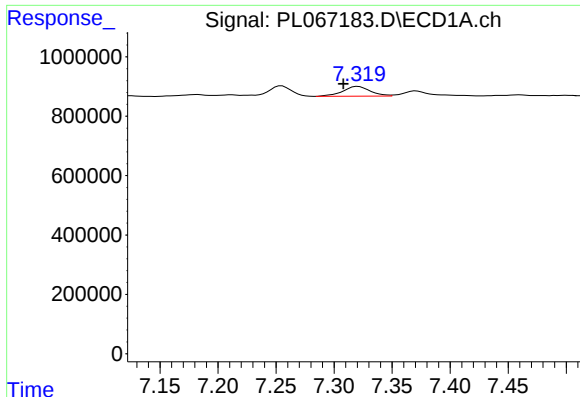

#9 Endosulfan I


R.T.: 7.321 min
Delta R.T.: 0.013 min
Response: 544625
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

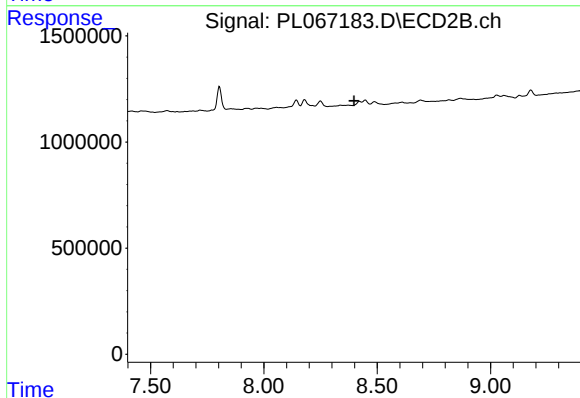


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.399 min
Response: 0
Conc: N.D.

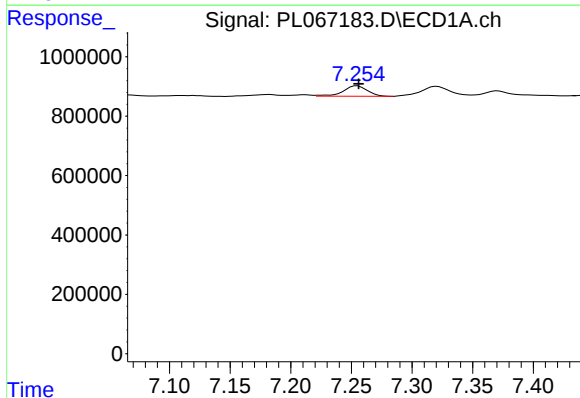


#11 alpha-Chlordane

R.T.: 7.255 min
Delta R.T.: -0.001 min
Response: 491482
Conc: 0.85 ng/ml

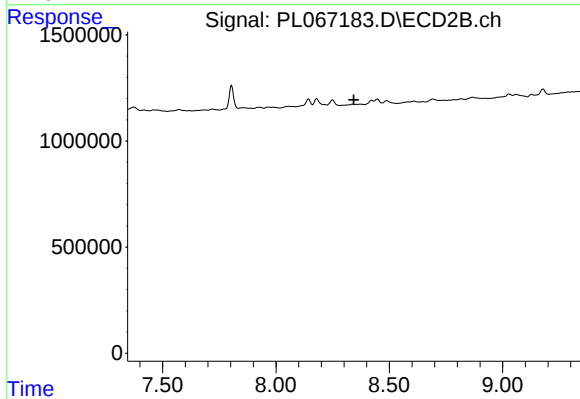

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.344 min
Response: 0
Conc: N.D.

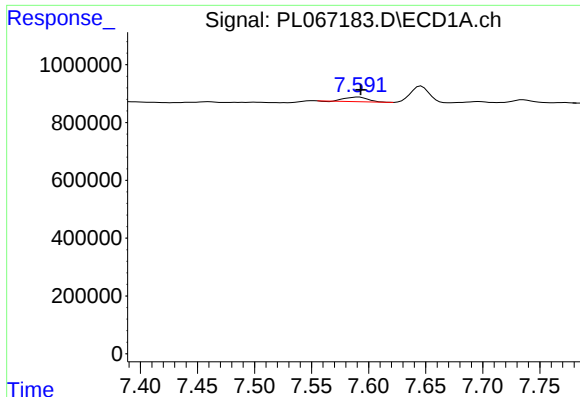

#13 Dieldrin


R.T.: 7.592 min
Delta R.T.: -0.002 min
Response: 225652
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

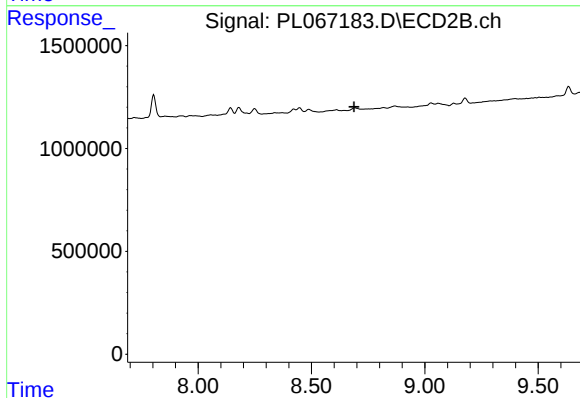


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.688 min
Response: 0
Conc: N.D.

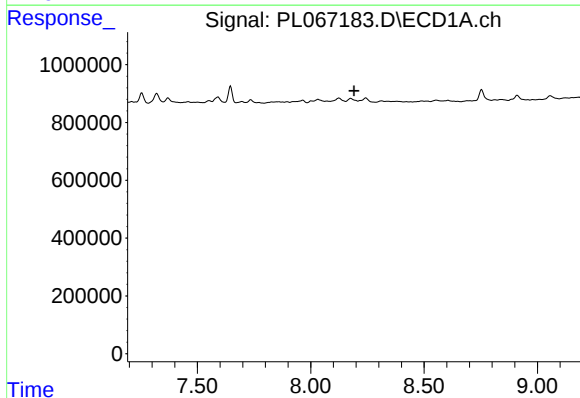


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

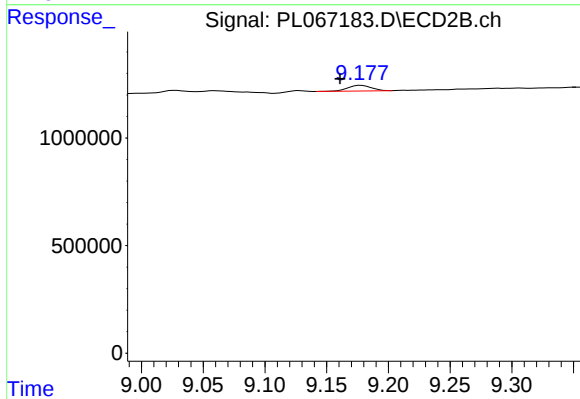

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 347426
Conc: 0.56 ng/ml

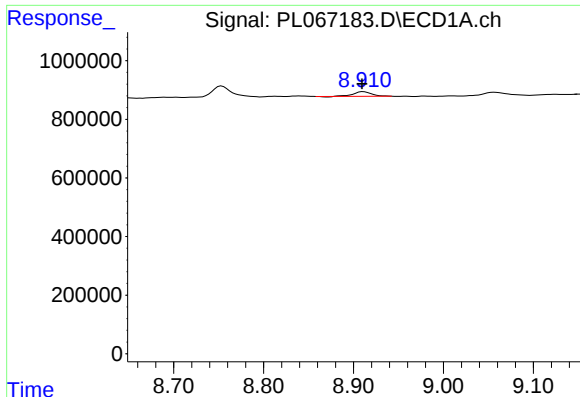

#20 Methoxychlor


R.T.: 8.911 min
Delta R.T.: 0.001 min
Response: 222574
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

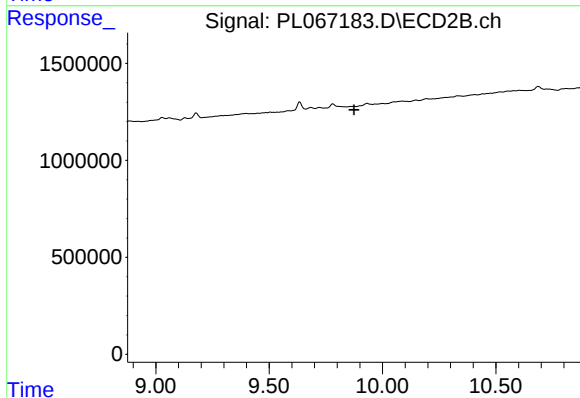


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.875 min
Response: 0
Conc: N.D.

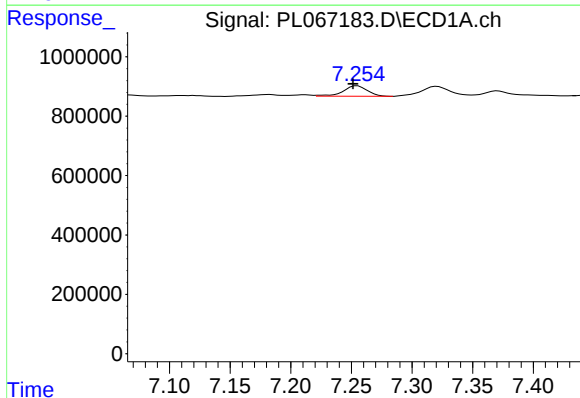


#26 Chlordane-4

R.T.: 7.255 min
Delta R.T.: 0.004 min
Response: 491482
Conc: 7.70 ng/ml

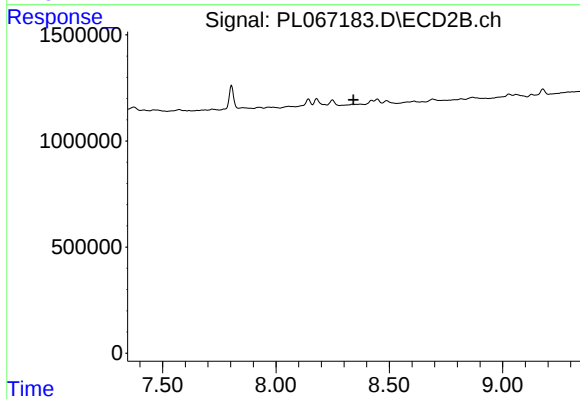

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

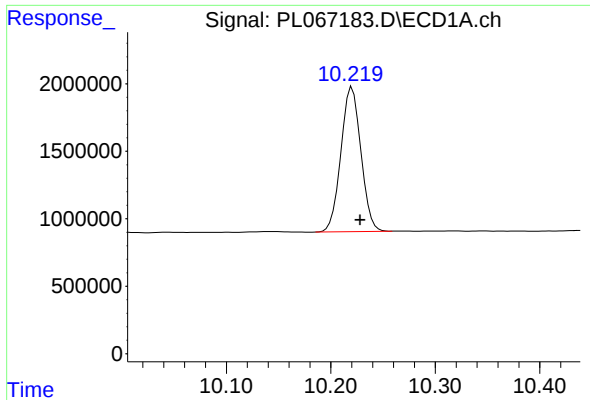

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.008 min
Response: 14218570
Conc: 21.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

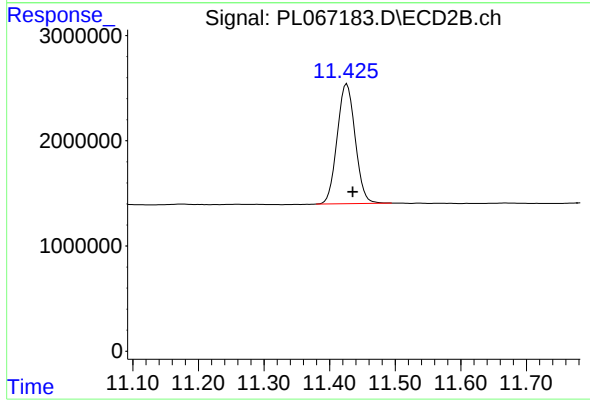

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.009 min
Response: 21740497
Conc: 26.06 ng/ml