

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
 Data File : PL067185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2021 12:49
 Operator : AR\AJ
 Sample : M2589-24
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 05:32:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	9341915	16646389	22.813	25.733
28)	SA Decachlor...	10.221	11.426	13416996	20385564	20.749	24.433
Target Compounds							
2)	A alpha-BHC	0.000	6.088f	0	301807	N.D.	0.382 #
3)	MA gamma-BHC...	5.588	0.000	161798	0	0.290	N.D. #
7)	B delta-BHC	0.000	7.003f	0	1362253	N.D.	1.794 #
11)	B alpha-Chl...	7.255	0.000	348531	0	0.606	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	496120	N.D.	0.804 #
26)	Chlordane-4	7.255	0.000	348531	0	5.460	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060821\
Data File : PL067185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2021 12:49
Operator : AR\AJ
Sample : M2589-24
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 05:32:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

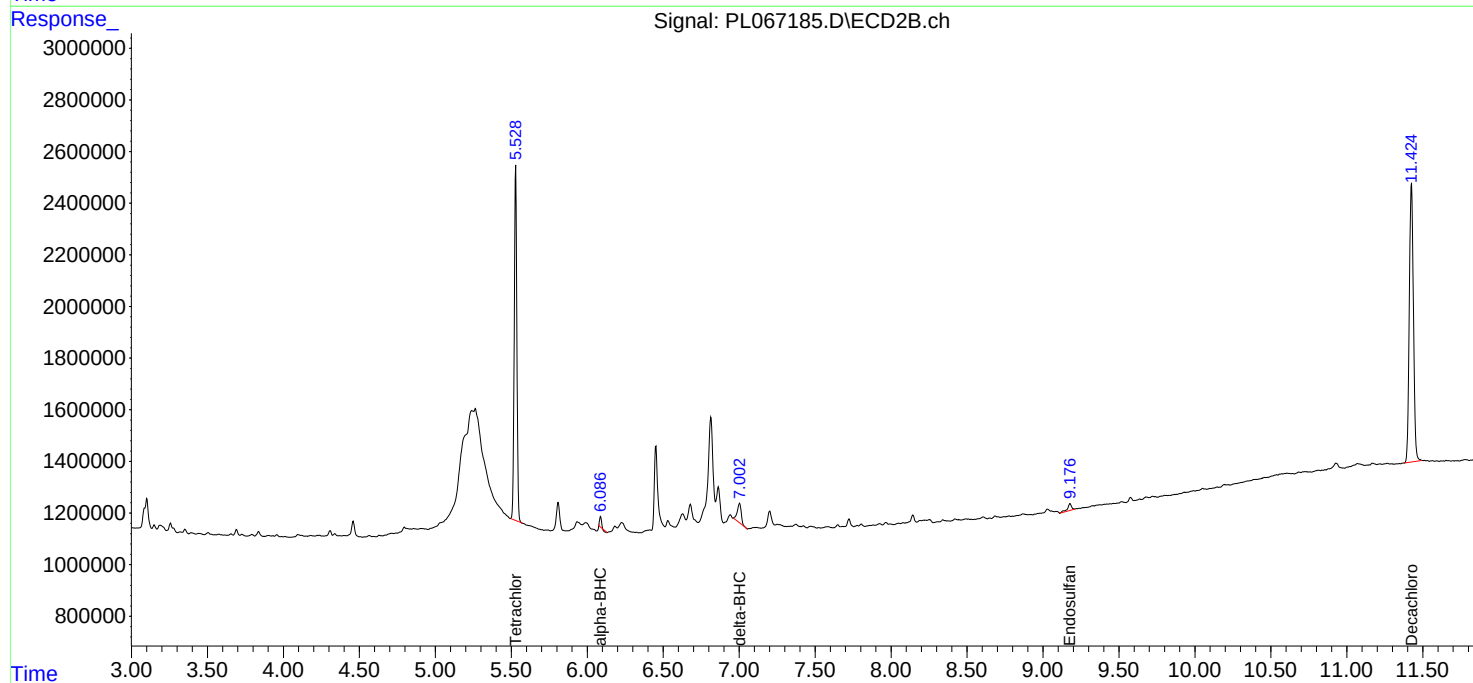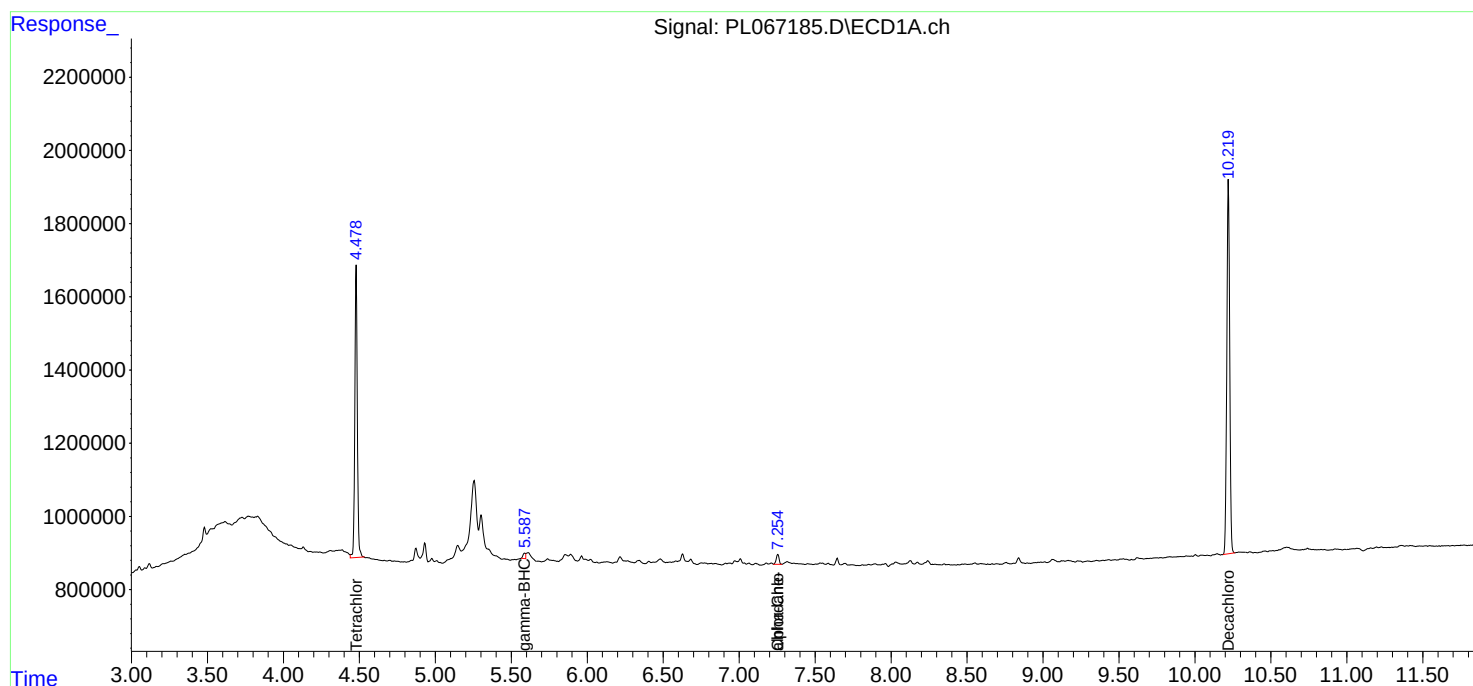


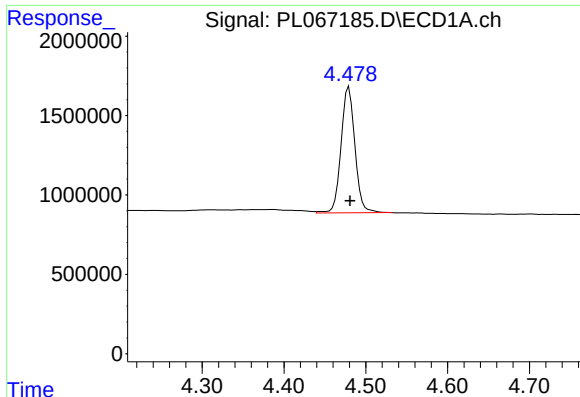

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 9341915
Conc: 22.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

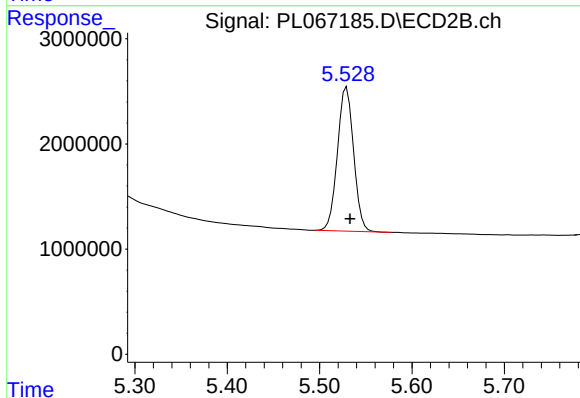


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 16646389
Conc: 25.73 ng/ml

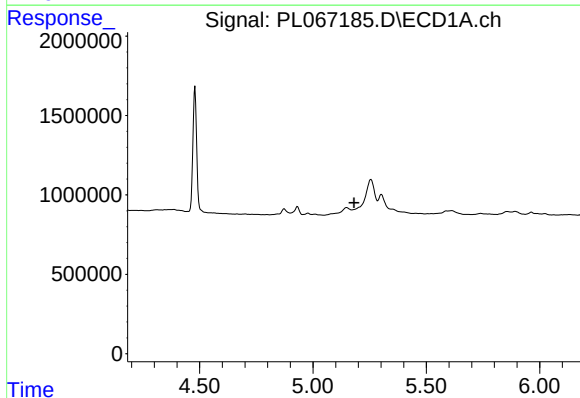


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.182 min
Response: 0
Conc: N.D.

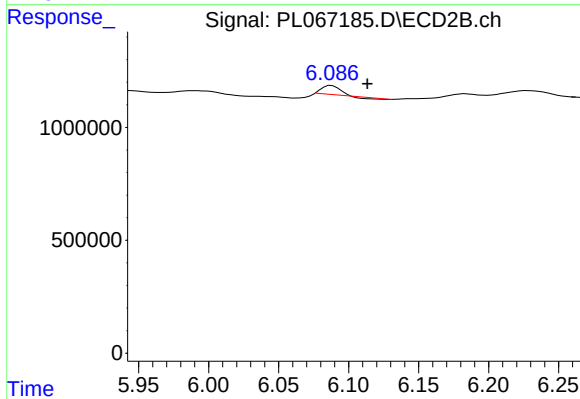

#2 alpha-BHC


R.T.: 6.088 min
Delta R.T.: -0.026 min
Response: 301807
Conc: 0.38 ng/ml

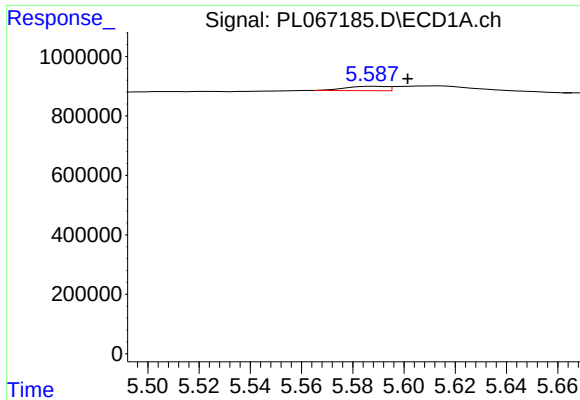

#3 gamma-BHC (Lindane)


R.T.: 5.588 min
Delta R.T.: -0.013 min
Response: 161798
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

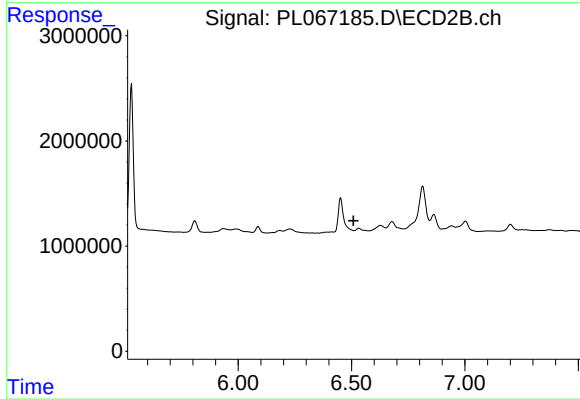


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

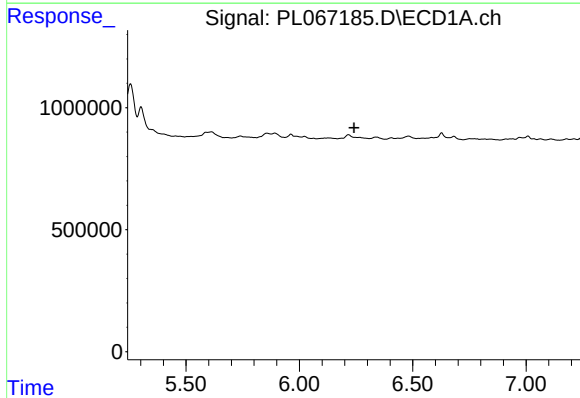


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

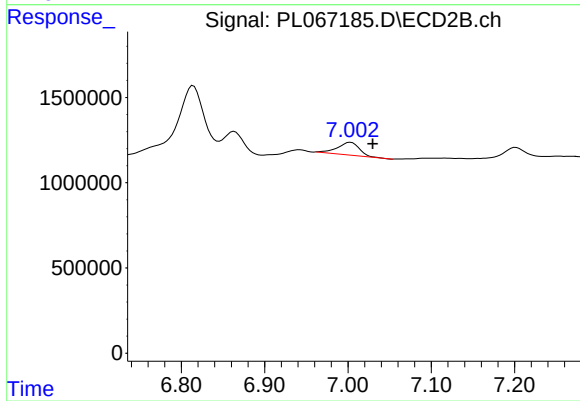

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.026 min
Response: 1362253
Conc: 1.79 ng/ml

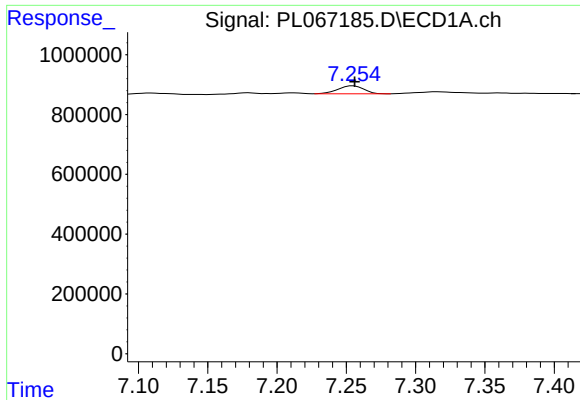

#11 alpha-Chlordane


R.T.: 7.255 min
Delta R.T.: -0.001 min
Response: 348531
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

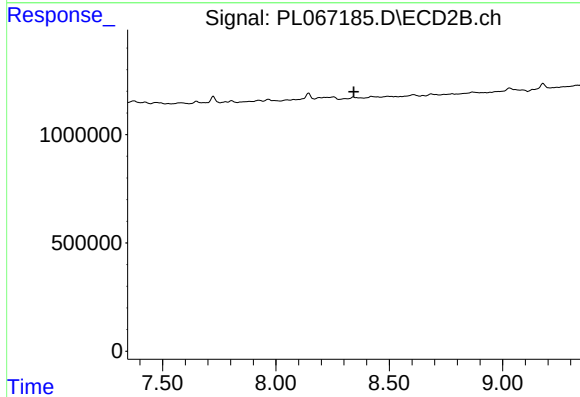


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.344 min
Response: 0
Conc: N.D.

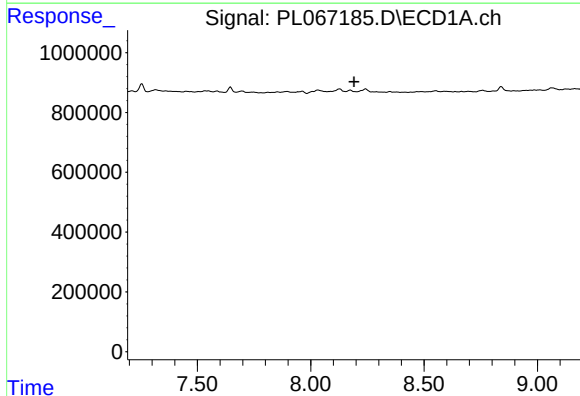


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.191 min
Response: 0
Conc: N.D.

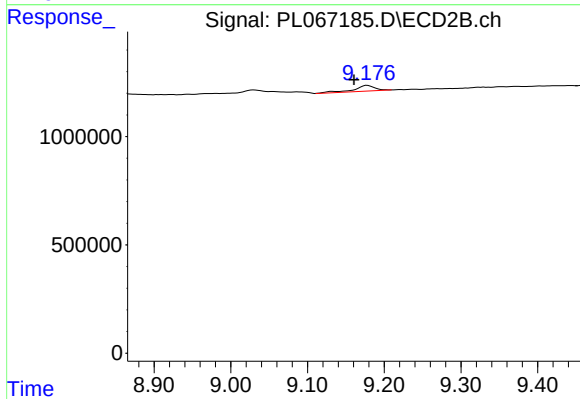

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.017 min
Response: 496120
Conc: 0.80 ng/ml

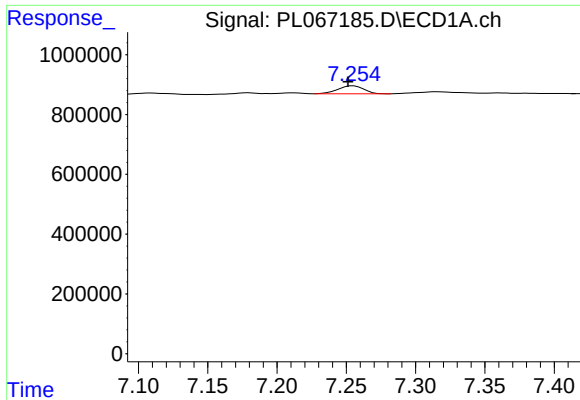

#26 Chlordane-4


R.T.: 7.255 min
Delta R.T.: 0.004 min
Response: 348531
Conc: 5.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

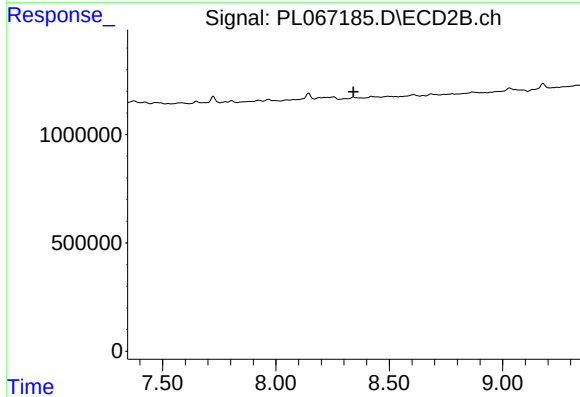


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

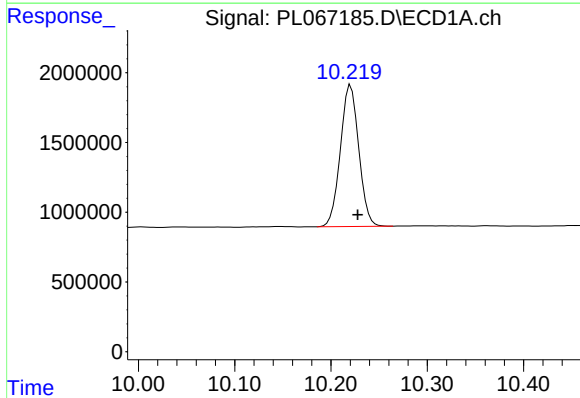

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.007 min
Response: 13416996
Conc: 20.75 ng/ml

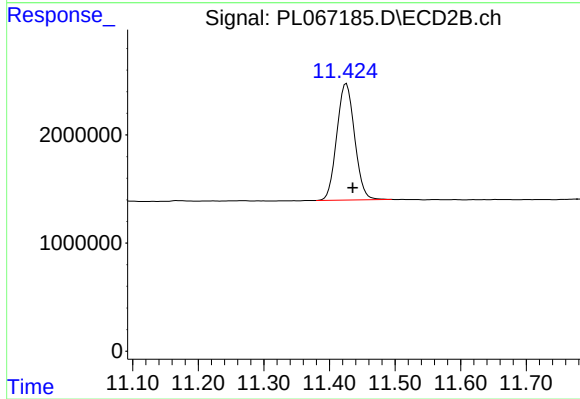

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.009 min
Response: 20385564
Conc: 24.43 ng/ml