

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060822\
 Data File : PL075641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 14:24
 Operator : AR\AJ
 Sample : PB145401BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 23:33:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.636	14031891	31223743	20.792	18.606
28)	SA Decachlor...	11.636	10.381	14254480	28568080	23.283	20.276
Target Compounds							
4)	MA Heptachlor	7.306f	0.000	554701	0	0.603	N.D. #
7)	B delta-BHC	0.000	6.404	0	227341	N.D.	0.106 #
10)	B gamma-Chl...	8.383	0.000	1643979	0	2.117	N.D. #
11)	B alpha-Chl...	8.459	0.000	148759	0	0.195	N.D. #
14)	MA Endrin	0.000	8.066f	0	549602	N.D.	0.402 #
15)	B Endosulfa...	9.300	0.000	973521	0	1.564	N.D. #
18)	B Endrin al...	9.440	0.000	378755	0	0.740	N.D. #
21)	B Endrin ke...	10.185f	0.000	475704	0	0.676	N.D. #
25)	Chlordane-3	8.383	0.000	1643979	0	15.922	N.D. #
26)	Chlordane-4	8.459	0.000	148759	0	1.175	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060822\
Data File : PL075641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 14:24
Operator : AR\AJ
Sample : PB145401BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 23:33:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

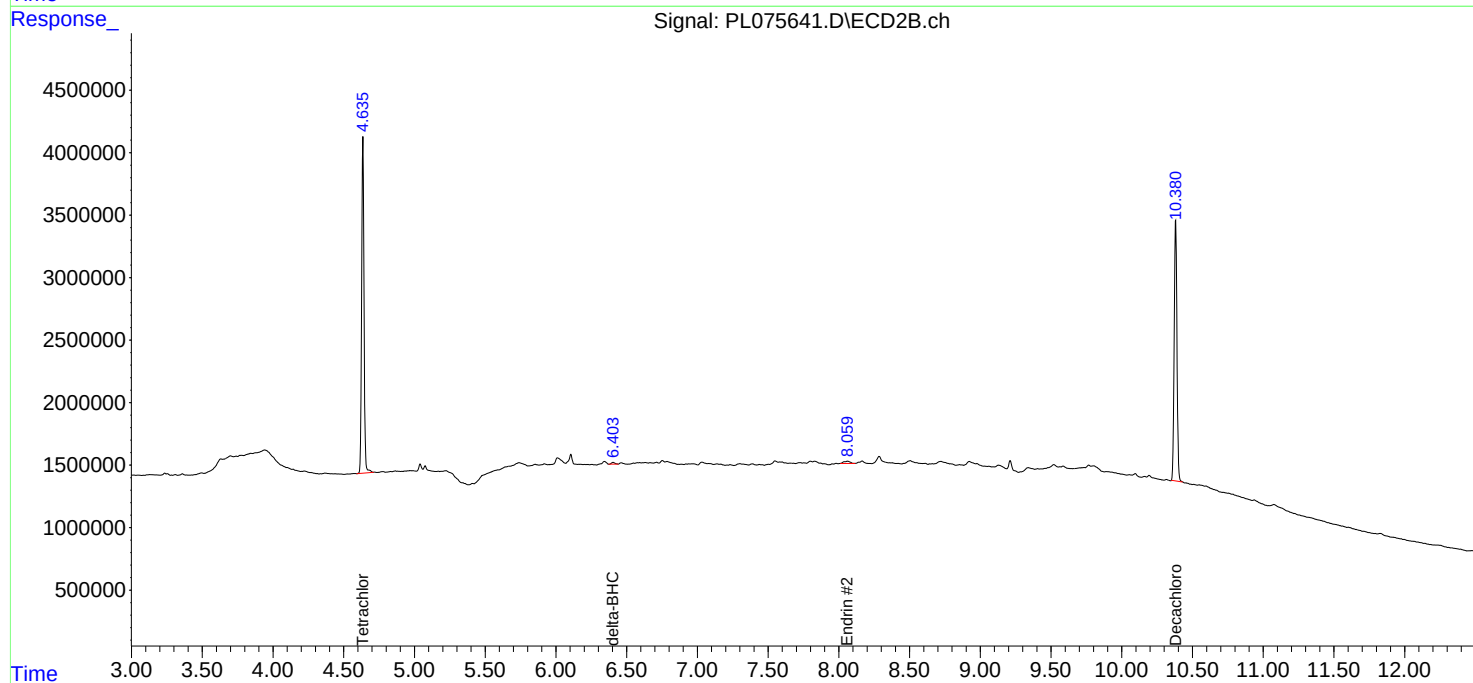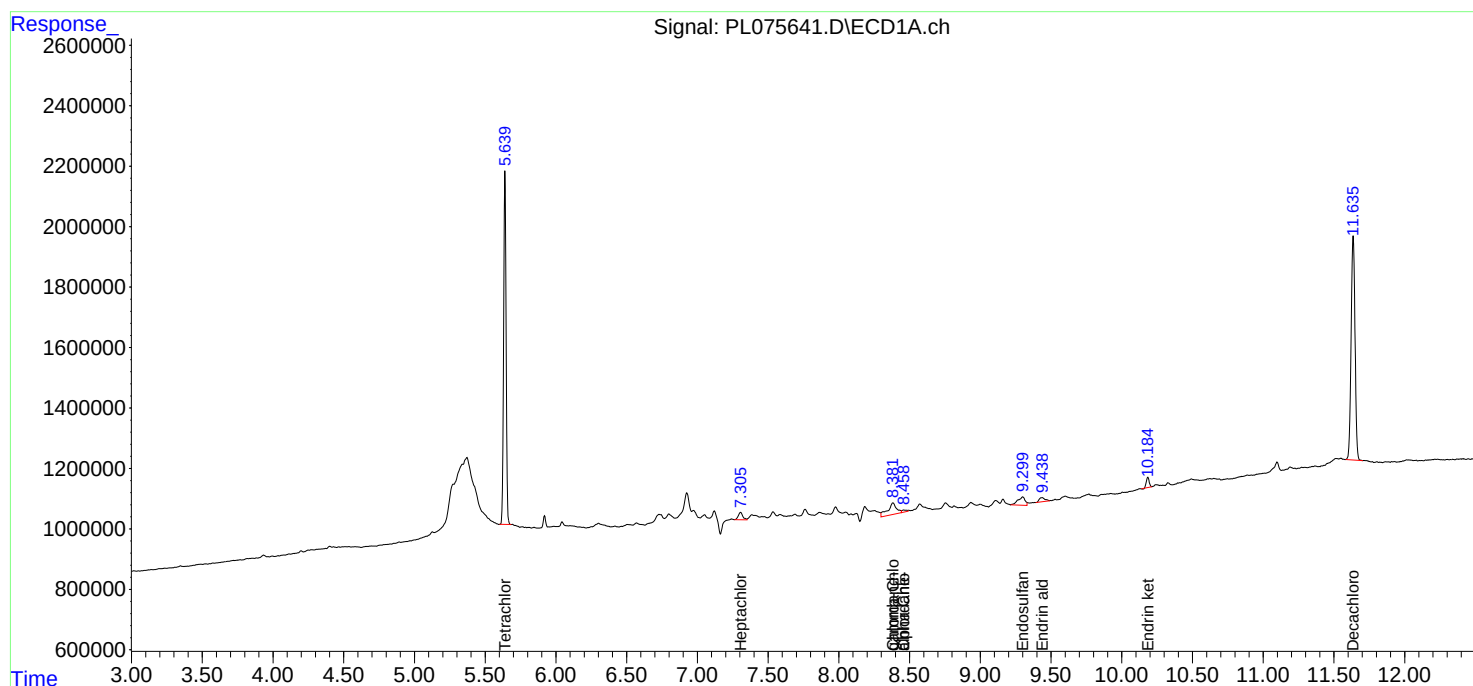


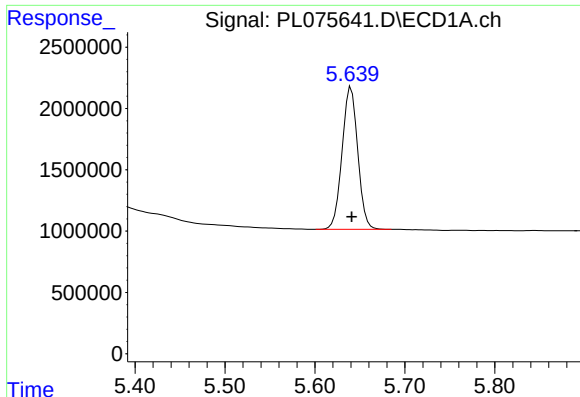

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 14031891
Conc: 20.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

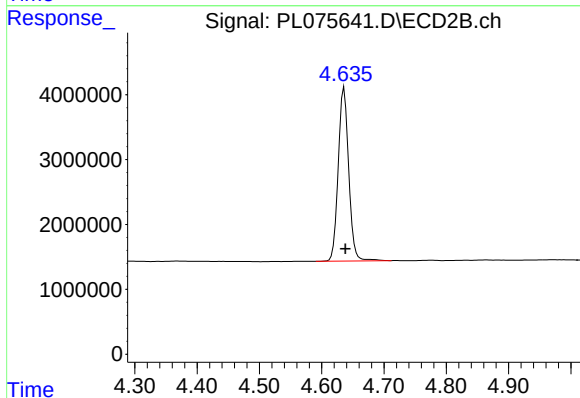


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 31223743
Conc: 18.61 ng/ml

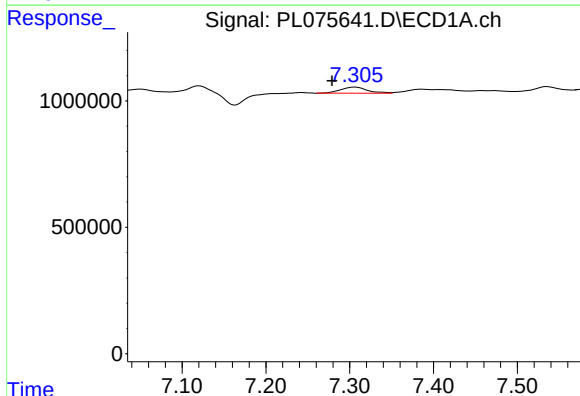


#4 Heptachlor

R.T.: 7.306 min
Delta R.T.: 0.027 min
Response: 554701
Conc: 0.60 ng/ml

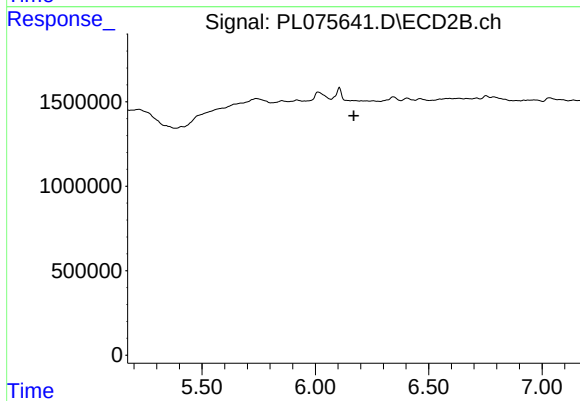

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.169 min
Response: 0
Conc: N.D.

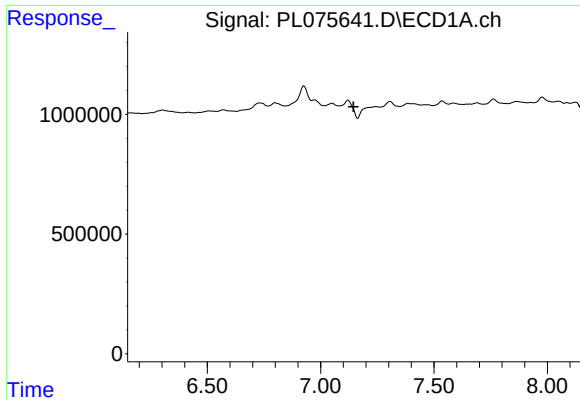

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

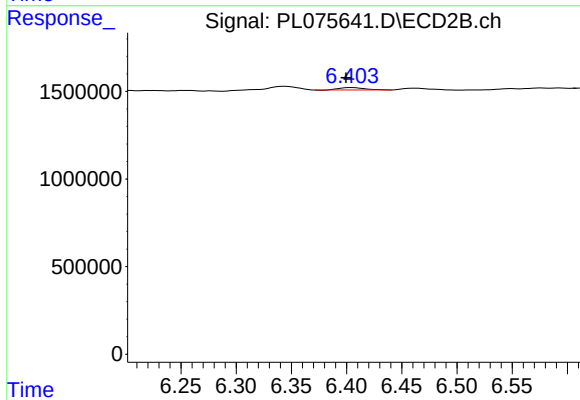


#7 delta-BHC

R.T.: 6.404 min
Delta R.T.: 0.005 min
Response: 227341
Conc: 0.11 ng/ml

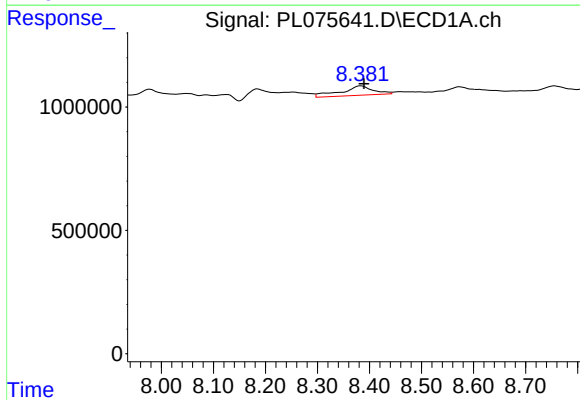


#10 gamma-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1643979
Conc: 2.12 ng/ml

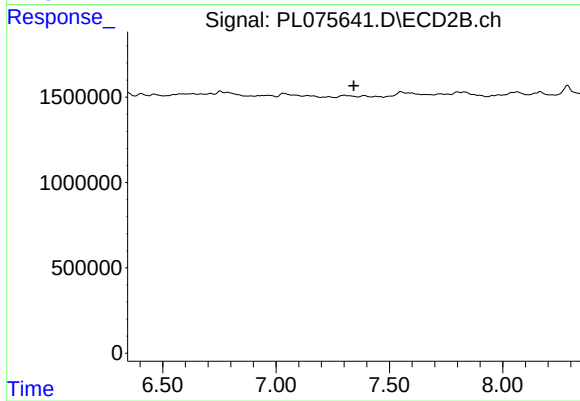

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.344 min
Response: 0
Conc: N.D.

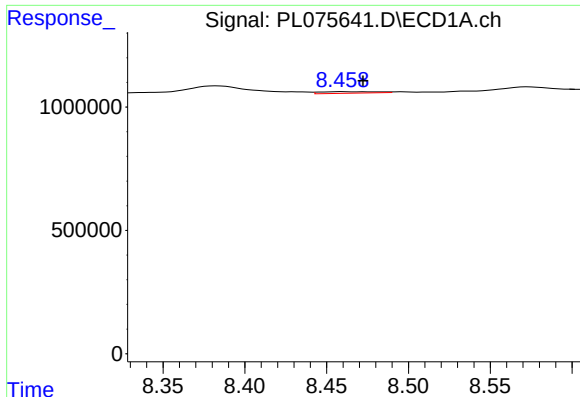

#11 alpha-Chlordane


R.T.: 8.459 min
Delta R.T.: -0.013 min
Response: 148759
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

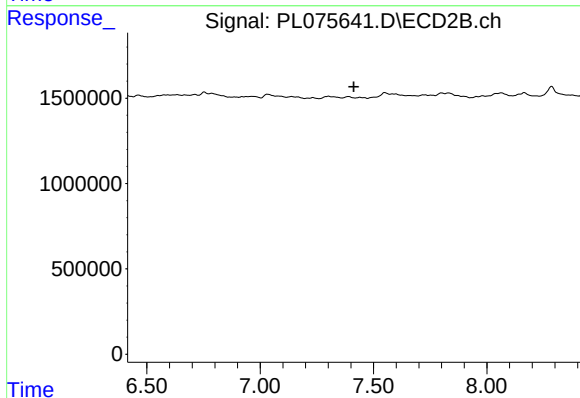


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

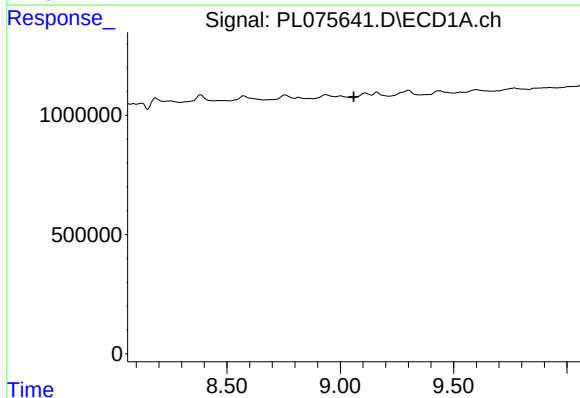


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

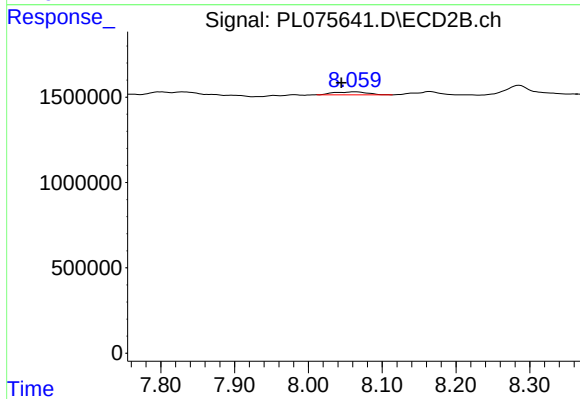

#14 Endrin


R.T.: 8.066 min
Delta R.T.: 0.021 min
Response: 549602
Conc: 0.40 ng/ml

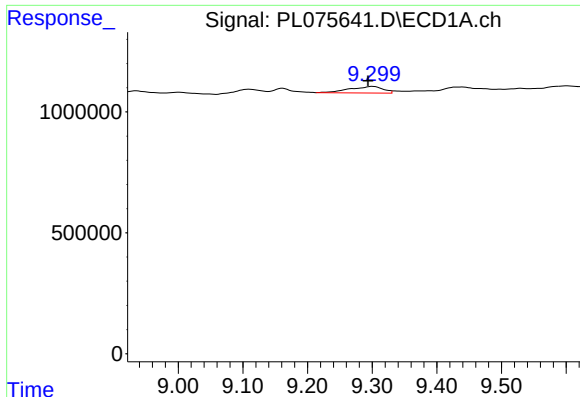

#15 Endosulfan II


R.T.: 9.300 min
Delta R.T.: 0.007 min
Response: 973521
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

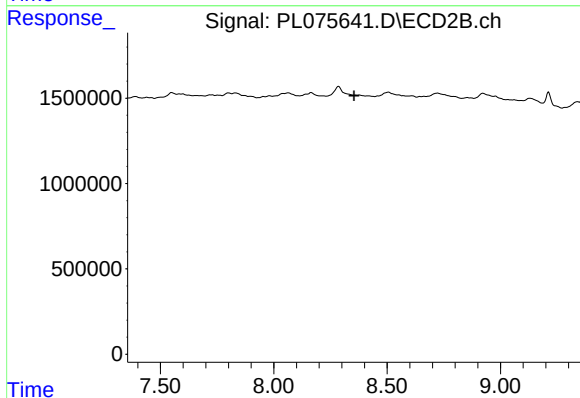


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

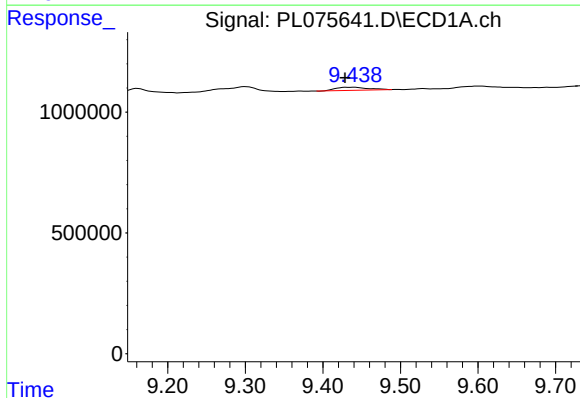


#18 Endrin aldehyde

R.T.: 9.440 min
Delta R.T.: 0.011 min
Response: 378755
Conc: 0.74 ng/ml

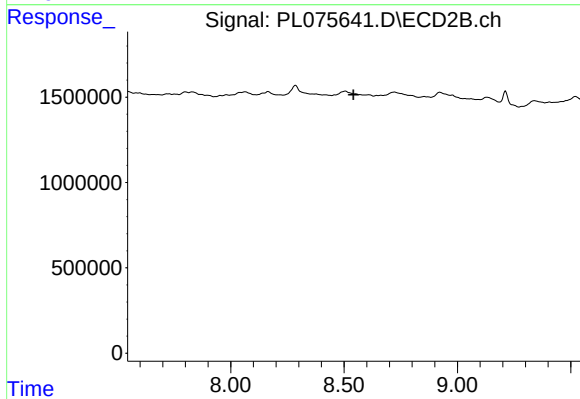

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.542 min
Response: 0
Conc: N.D.

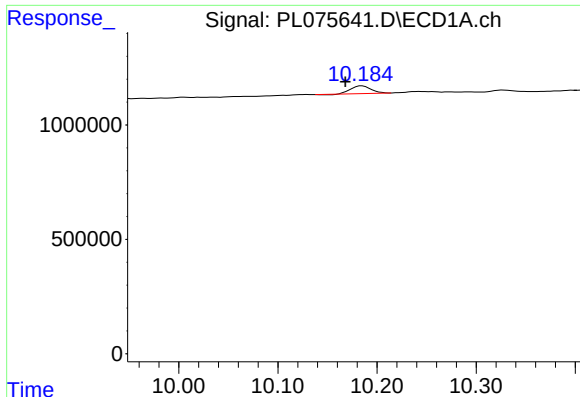

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 475704
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

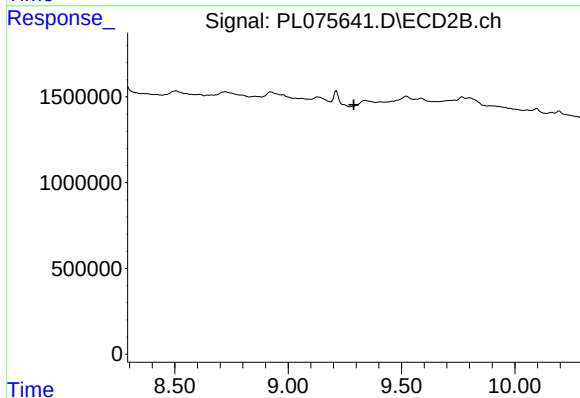


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

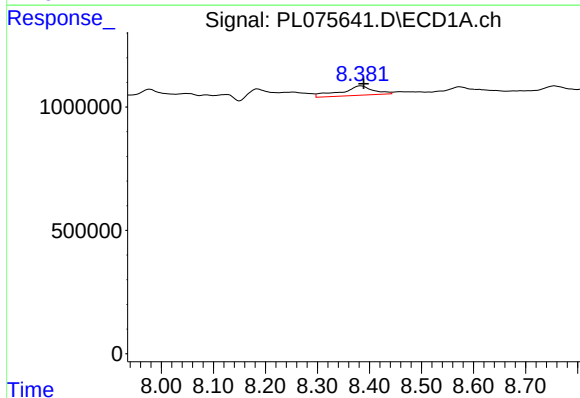


#25 Chlordane-3

R.T.: 8.383 min
Delta R.T.: -0.007 min
Response: 1643979
Conc: 15.92 ng/ml

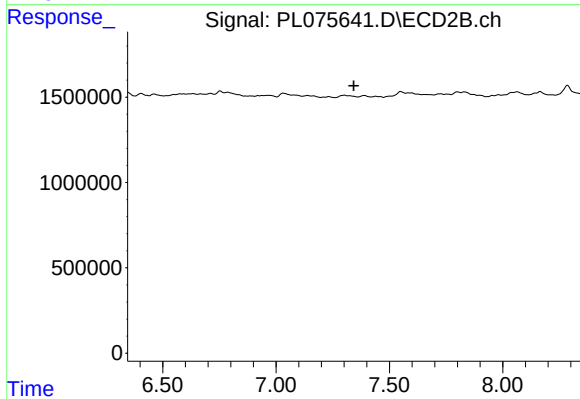

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

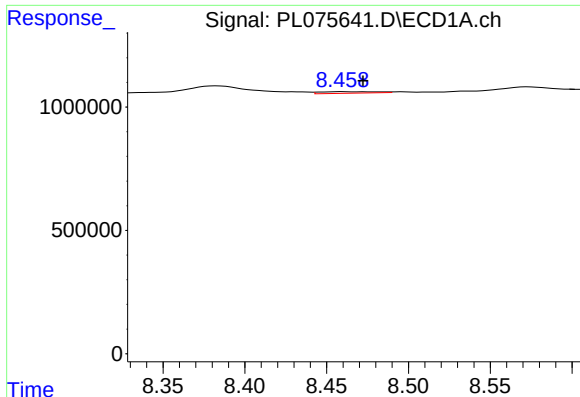

#26 Chlordane-4


R.T.: 8.459 min
Delta R.T.: -0.013 min
Response: 148759
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

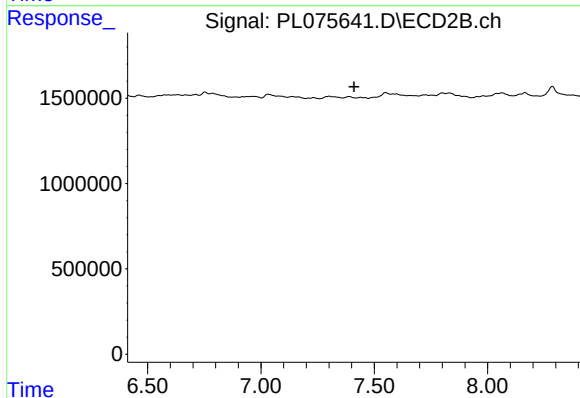


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

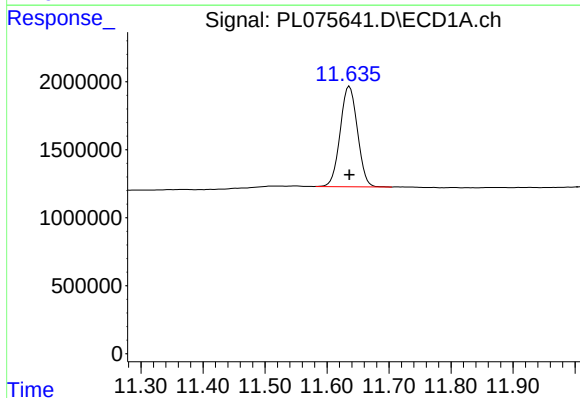

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 14254480
Conc: 23.28 ng/ml

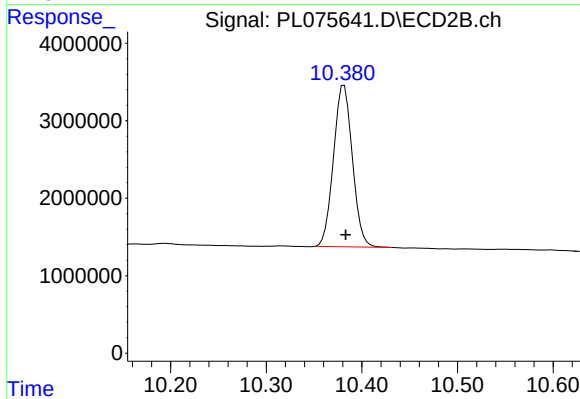

#28 Decachlorobiphenyl

R.T.: 10.381 min
Delta R.T.: -0.002 min
Response: 28568080
Conc: 20.28 ng/ml