

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060822\
 Data File : PL075654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 18:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 23:43:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.635	13651551	30624824	20.228	18.249
28)	SA Decachlor...	11.637	10.381	13534251	28228978	22.107	20.035
Target Compounds							
7)	B delta-BHC	0.000	6.401	0	317211	N.D.	0.148 #
8)	B Heptachlo...	8.125	0.000	293896	0	0.380	N.D. #
10)	B gamma-Chl...	8.379	0.000	330378	0	0.425	N.D. #
11)	B alpha-Chl...	0.000	7.388f	0	190936	N.D.	0.105 #
14)	MA Endrin	0.000	8.065f	0	254852	N.D.	0.186 #
15)	B Endosulfa...	9.303	0.000	220291	0	0.354	N.D. #
21)	B Endrin ke...	10.185f	0.000	461501	0	0.656	N.D. #
25)	Chlordane-3	8.379	0.000	330378	0	3.200	N.D. #
26)	Chlordane-4	0.000	7.388f	0	190936	N.D.	1.037 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060822\
Data File : PL075654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 18:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 23:43:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

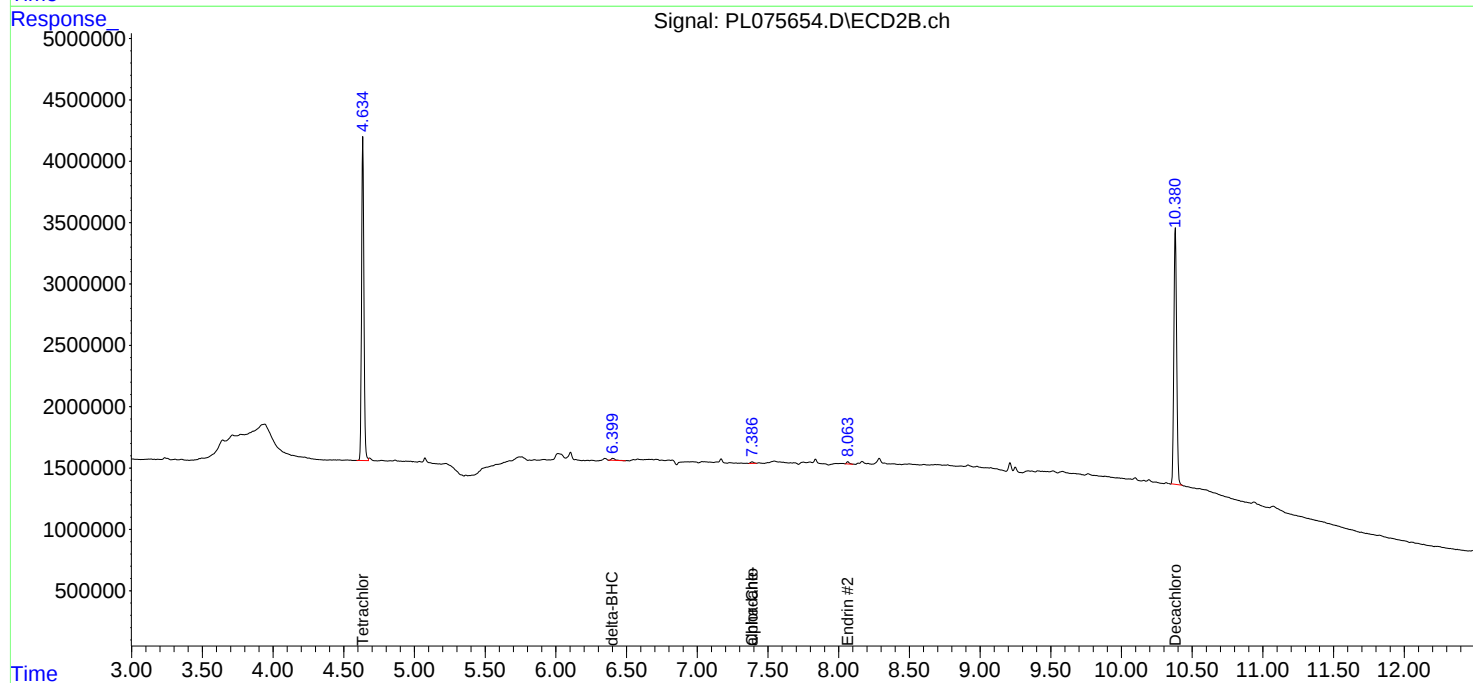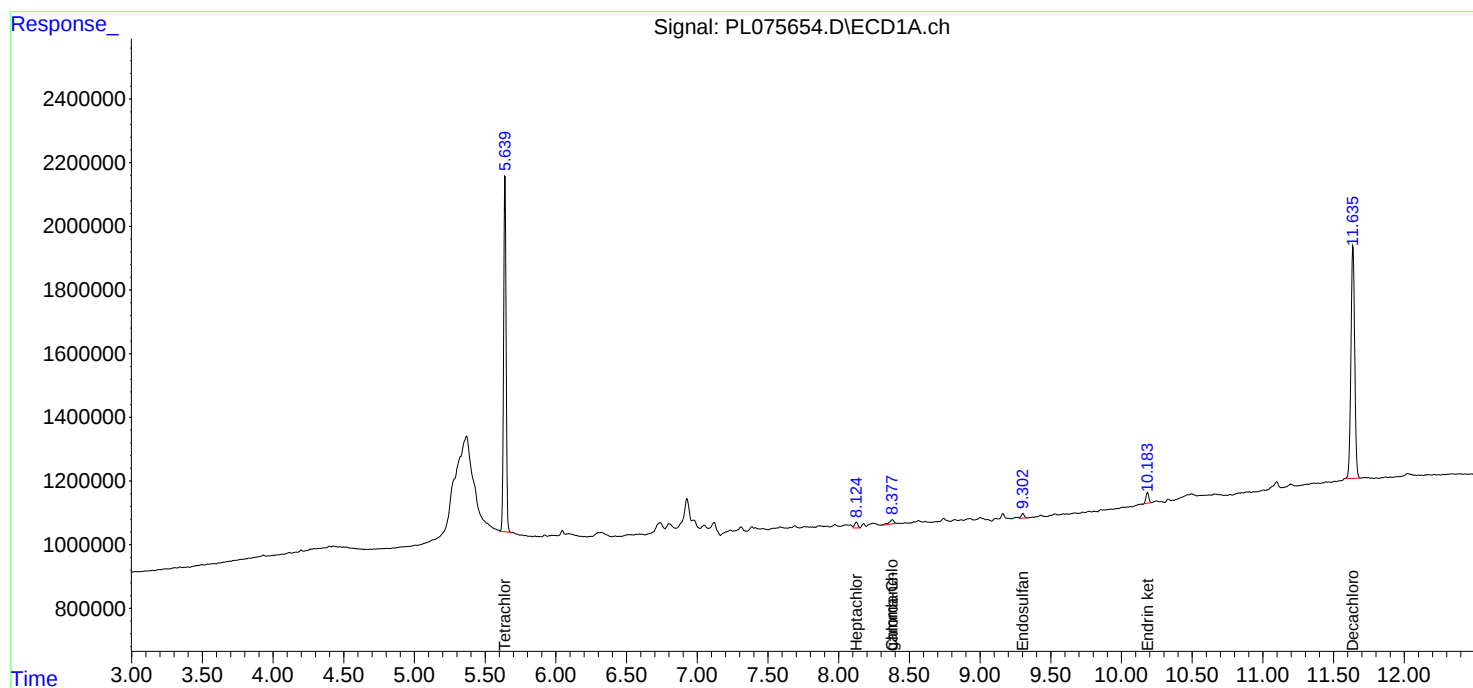


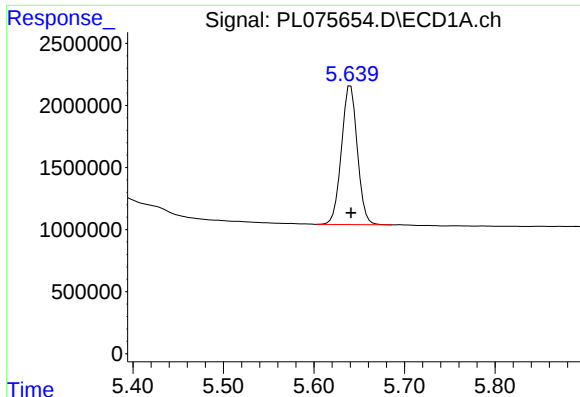

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 13651551
Conc: 20.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

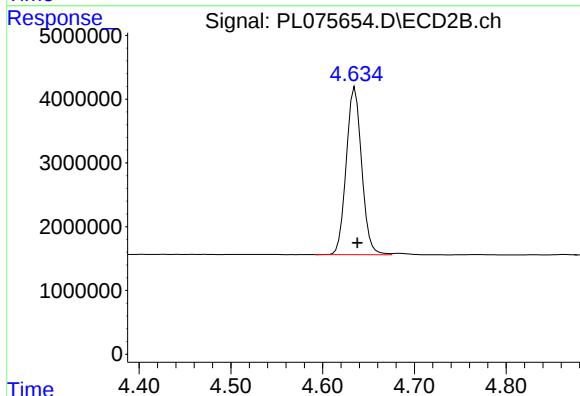


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 30624824
Conc: 18.25 ng/ml

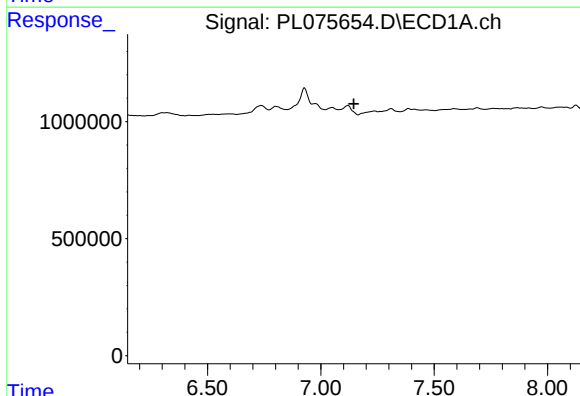


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

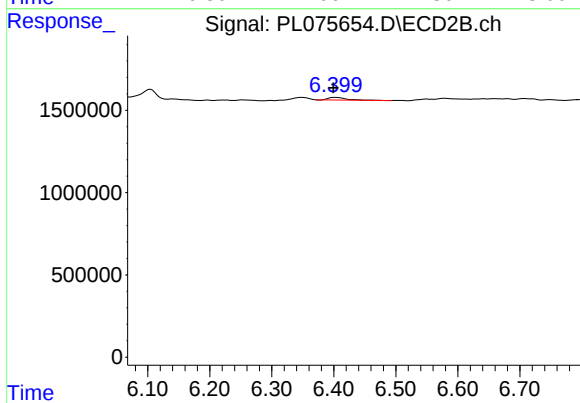

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: 0.001 min
Response: 317211
Conc: 0.15 ng/ml

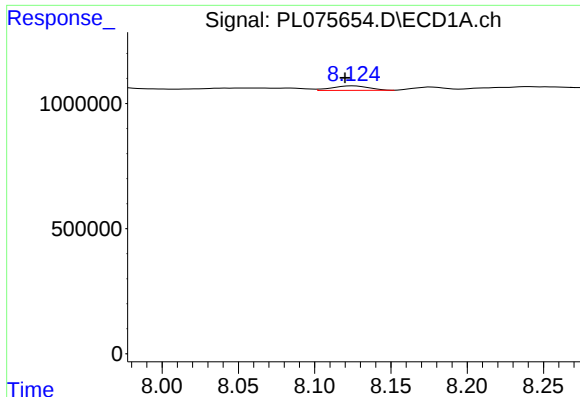

#8 Heptachlor epoxide


R.T.: 8.125 min
Delta R.T.: 0.005 min
Response: 293896
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

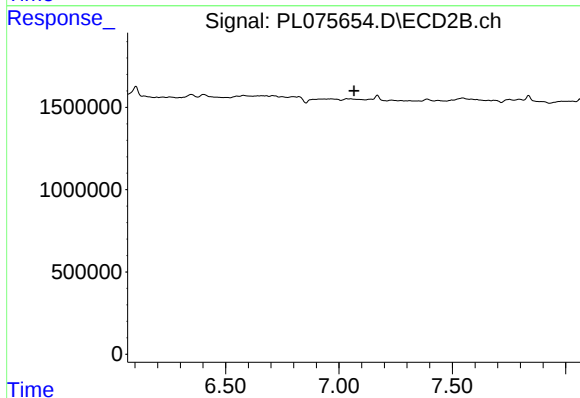


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

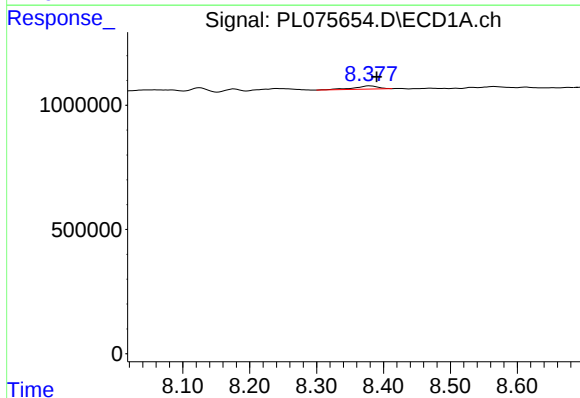


#10 gamma-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 330378
Conc: 0.43 ng/ml

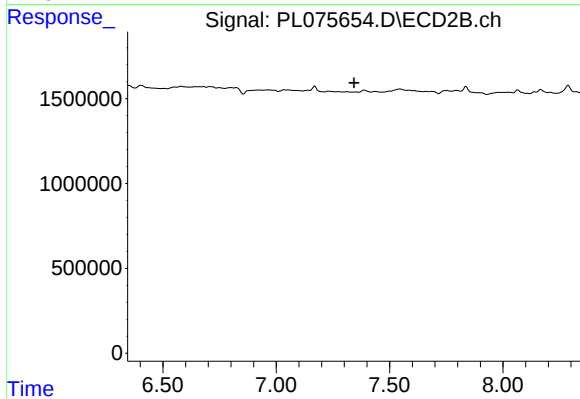

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

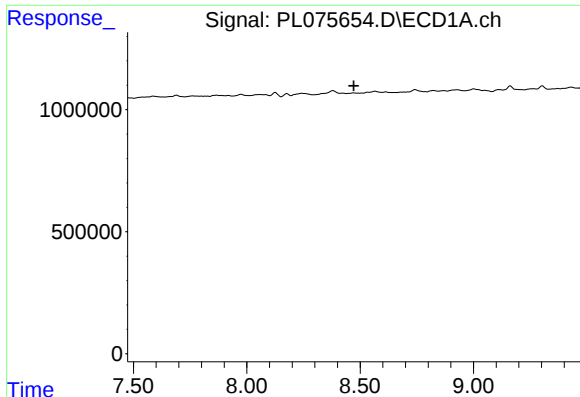

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

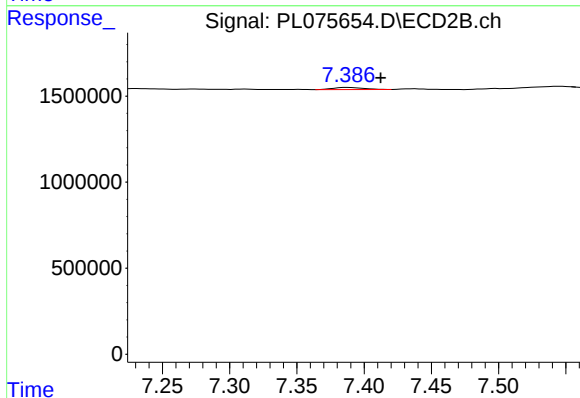


#11 alpha-Chlordane

R.T.: 7.388 min
Delta R.T.: -0.025 min
Response: 190936
Conc: 0.10 ng/ml

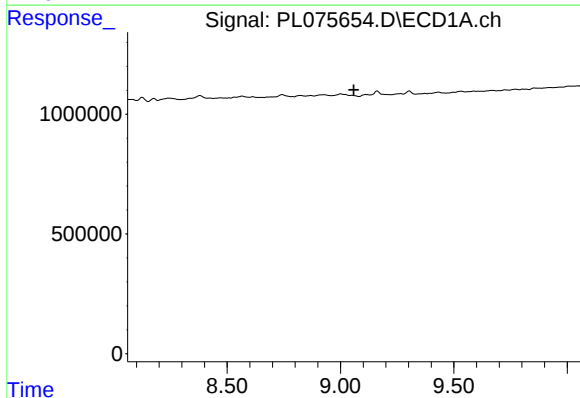


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

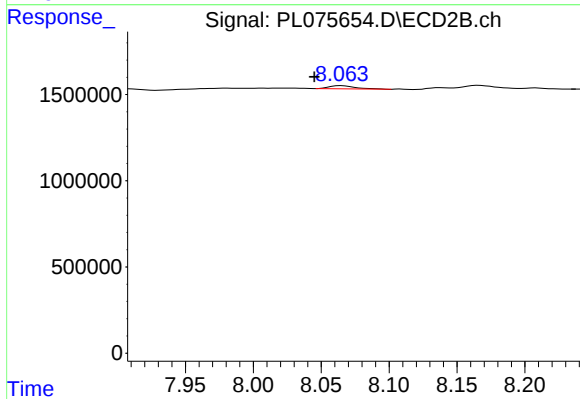

#14 Endrin


R.T.: 8.065 min
Delta R.T.: 0.020 min
Response: 254852
Conc: 0.19 ng/ml

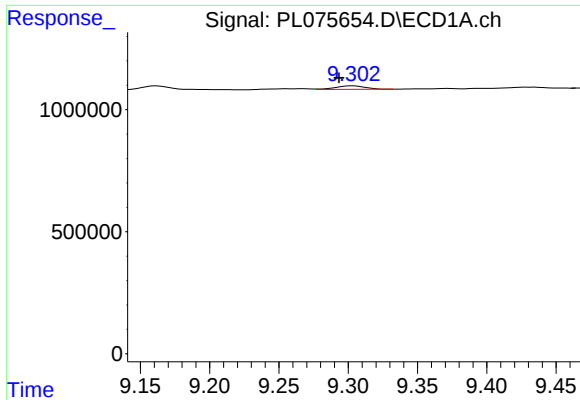

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 220291
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

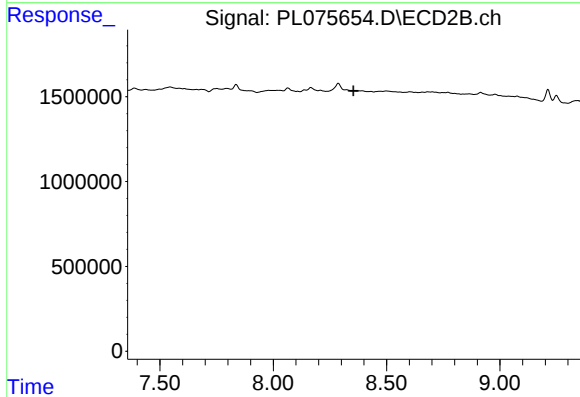


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

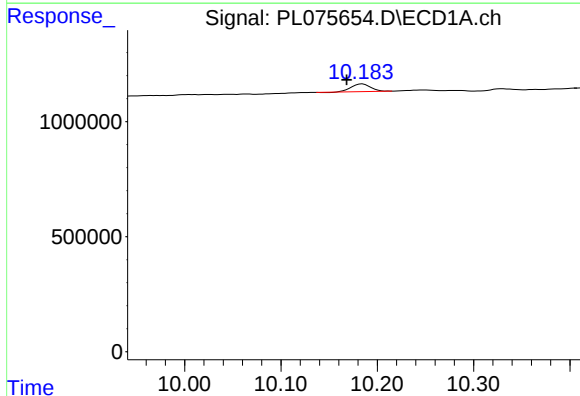


#21 Endrin ketone

R.T.: 10.185 min
Delta R.T.: 0.016 min
Response: 461501
Conc: 0.66 ng/ml

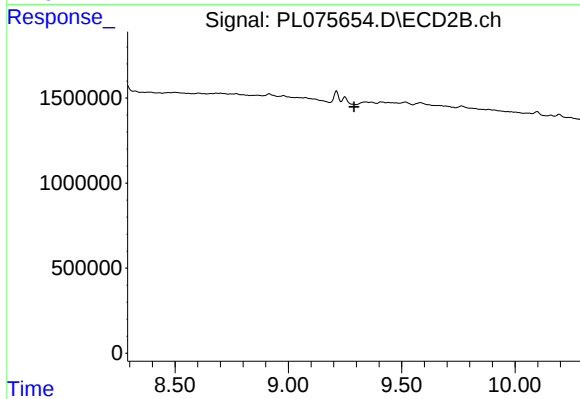

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

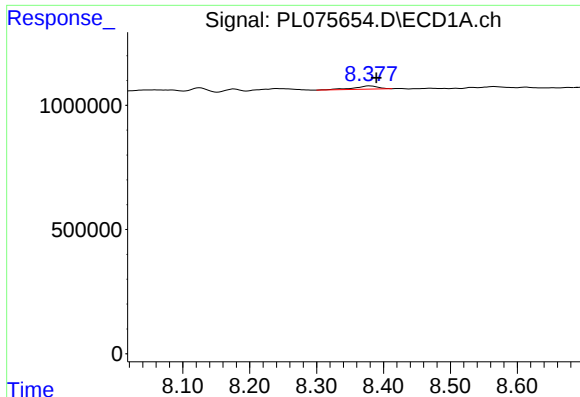

#25 Chlordane-3


R.T.: 8.379 min
Delta R.T.: -0.010 min
Response: 330378
Conc: 3.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

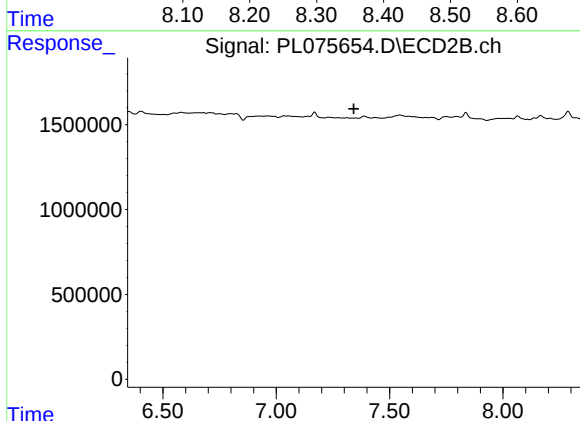


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

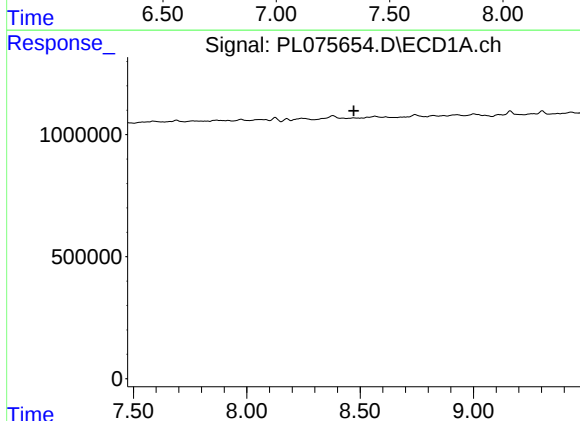


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.472 min
Response: 0
Conc: N.D.

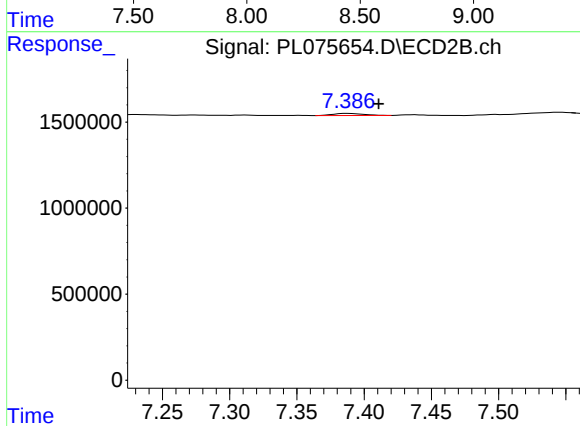

#26 Chlordane-4


R.T.: 7.388 min
Delta R.T.: -0.023 min
Response: 190936
Conc: 1.04 ng/ml

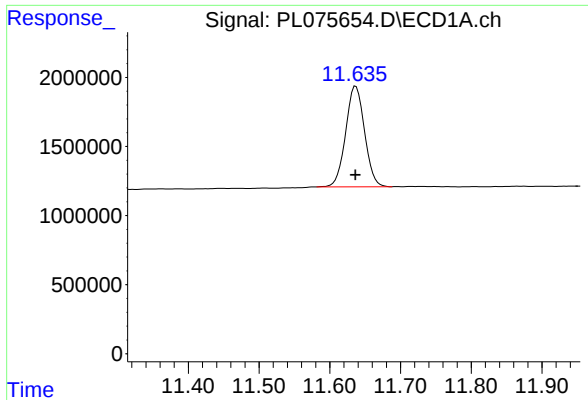

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.000 min
Response: 13534251
Conc: 22.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

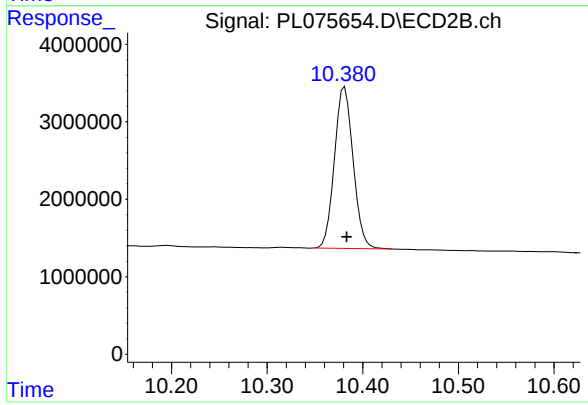

#28 Decachlorobiphenyl

R.T.: 10.381 min
Delta R.T.: -0.002 min
Response: 28228978
Conc: 20.04 ng/ml