

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060921\
 Data File : PL067206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 08:56
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 06:07:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
4) MA	Heptachlor	5.993f	0.000	864344	0	1.645	N.D. #
6) B	beta-BHC	5.993	0.000	864344	0	3.245	N.D. #
15) B	Endosulfa...	8.174f	0.000	986596	0	1.904	N.D. #
22)	Mirex	9.310	0.000	385580	0	0.667	N.D. #
24)	Chlordane-2	6.492	0.000	1200765	0	54.949	N.D. #
27)	Chlordane-5	8.174f	0.000	986596	0	52.287	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060921\
Data File : PL067206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 08:56
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 06:07:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

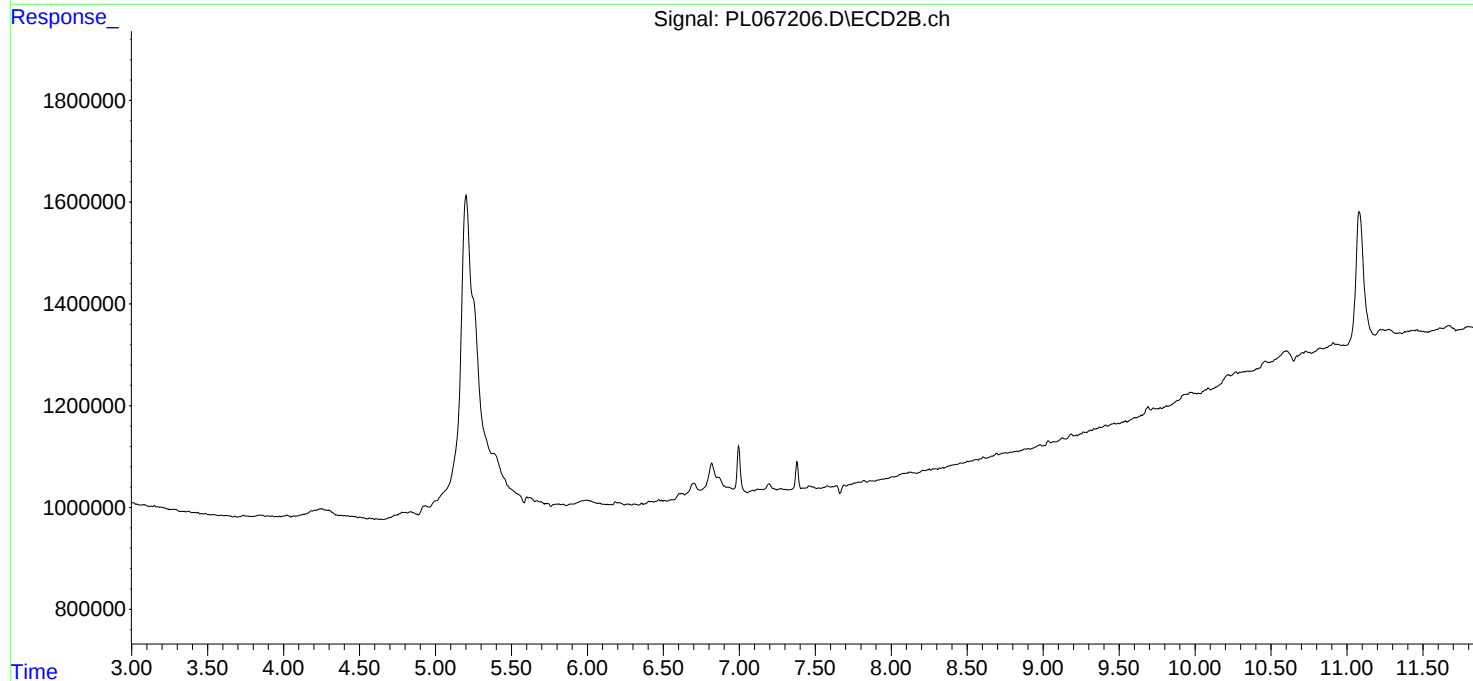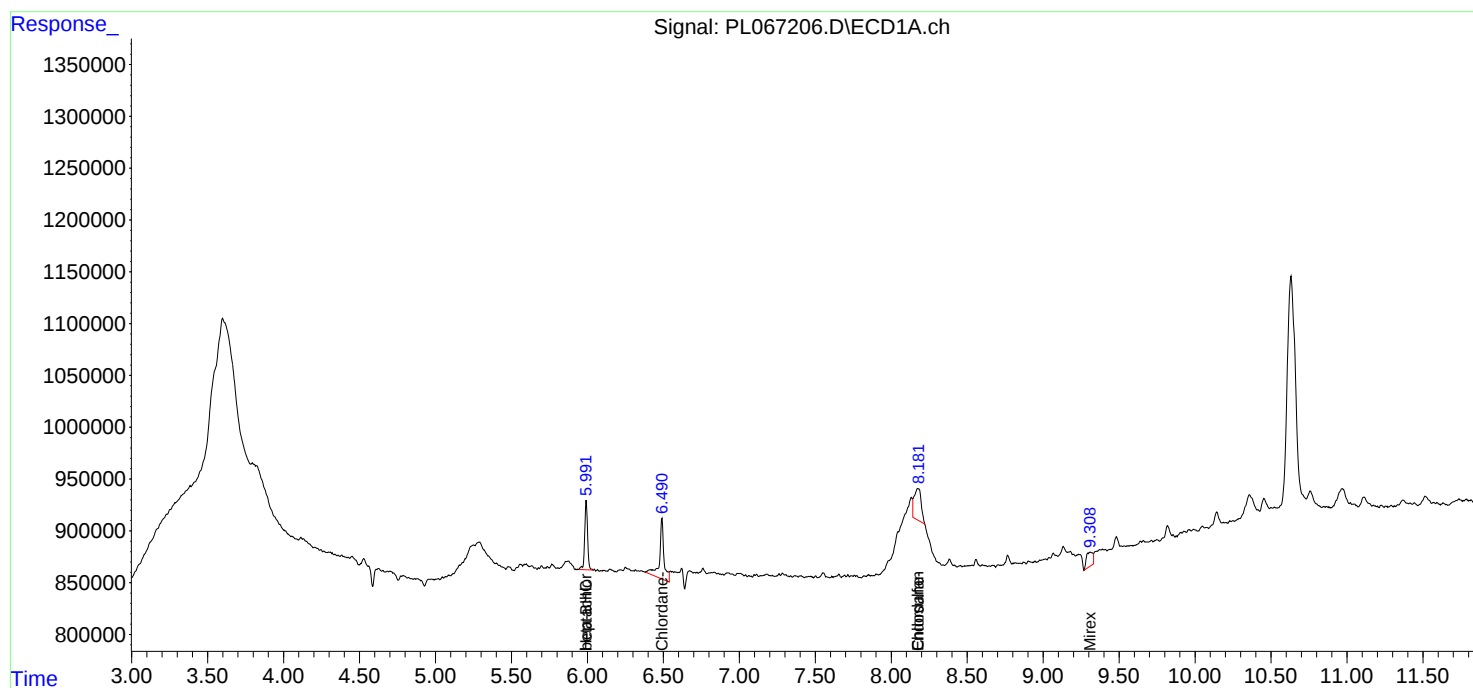


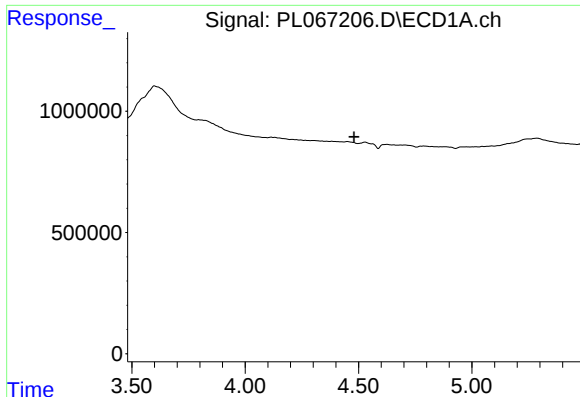

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

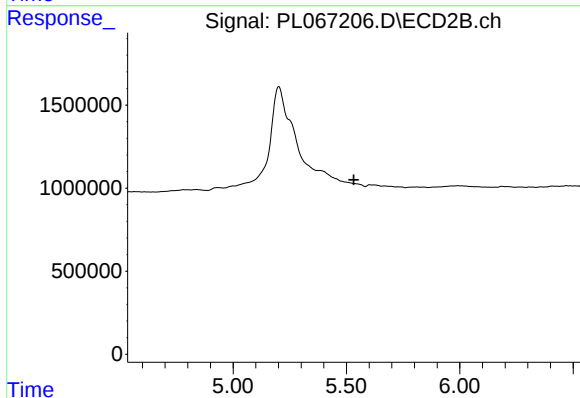


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

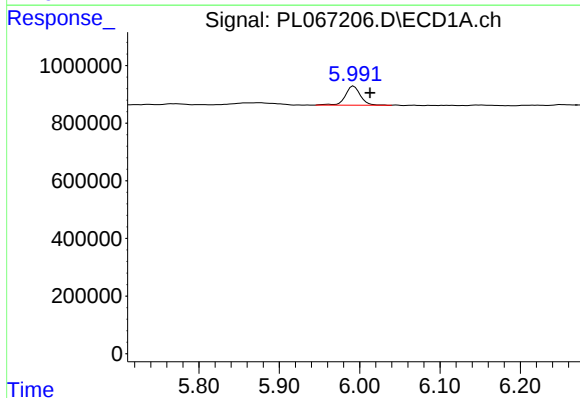


#4 Heptachlor

R.T.: 5.993 min
Delta R.T.: -0.021 min
Response: 864344
Conc: 1.65 ng/ml

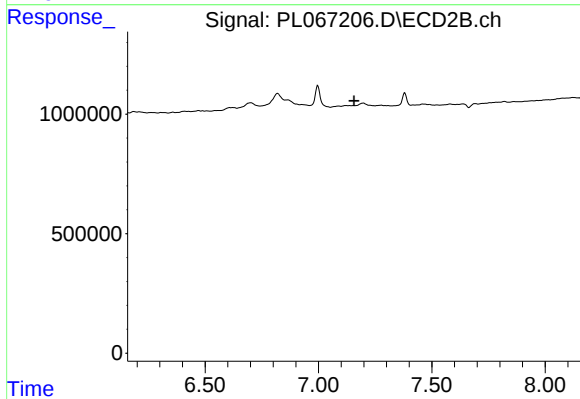

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

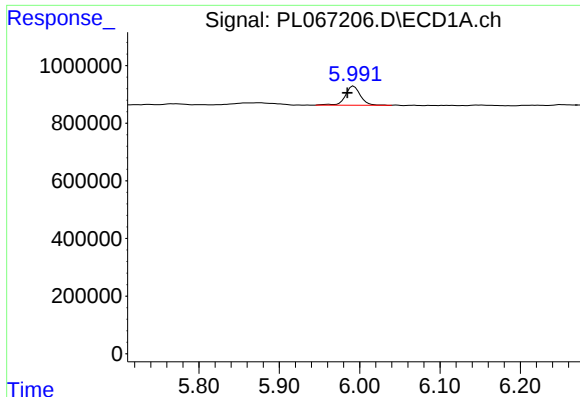

#6 beta-BHC


R.T.: 5.993 min
Delta R.T.: 0.008 min
Response: 864344
Conc: 3.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

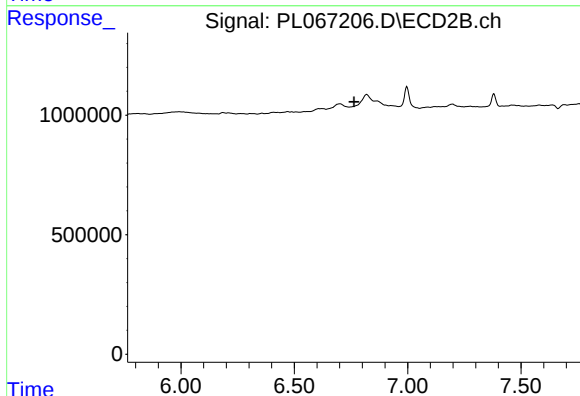


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

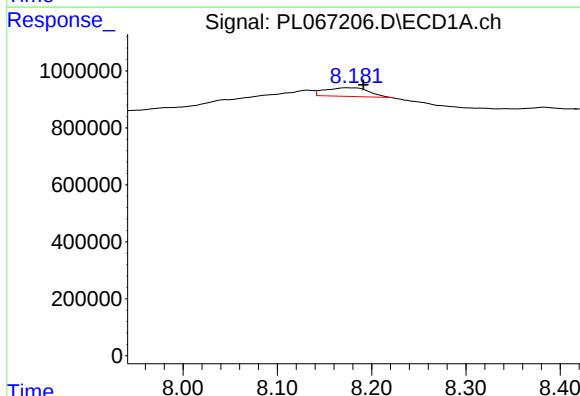


#15 Endosulfan II

R.T.: 8.174 min
Delta R.T.: -0.017 min
Response: 986596
Conc: 1.90 ng/ml

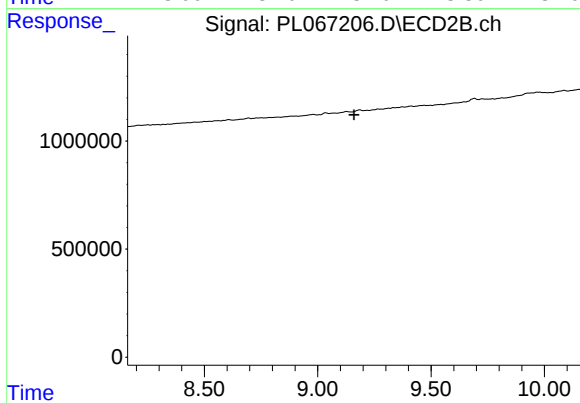

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.161 min
Response: 0
Conc: N.D.

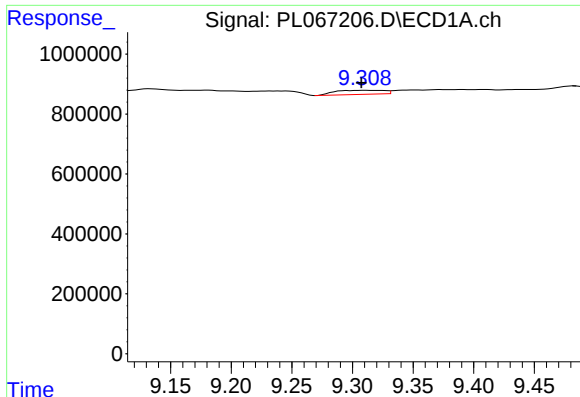

#22 Mirex


R.T.: 9.310 min

Delta R.T.: 0.003 min

Response: 385580

Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

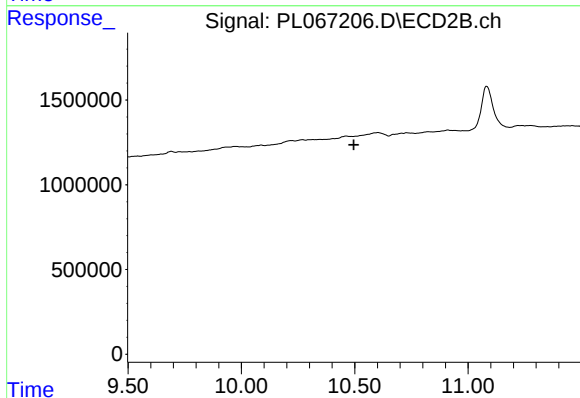


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 10.496 min

Response: 0

Conc: N.D.

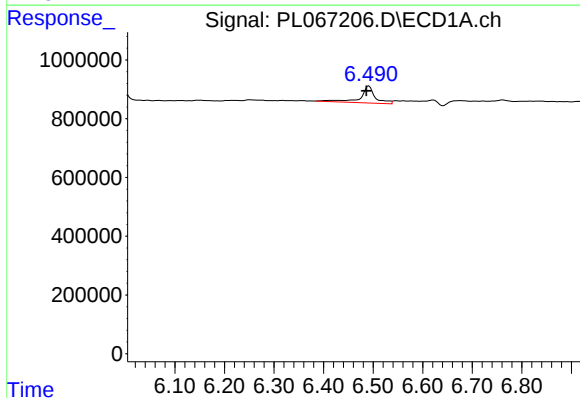


#24 Chlordane-2

R.T.: 6.492 min

Delta R.T.: 0.005 min

Response: 1200765

Conc: 54.95 ng/ml

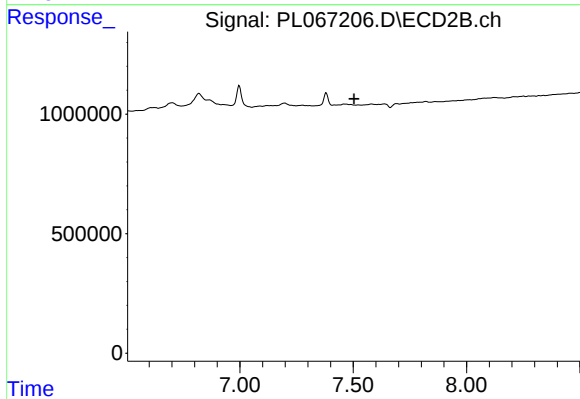


#24 Chlordane-2

R.T.: 0.000 min

Exp R.T. : 7.503 min

Response: 0


Conc: N.D.

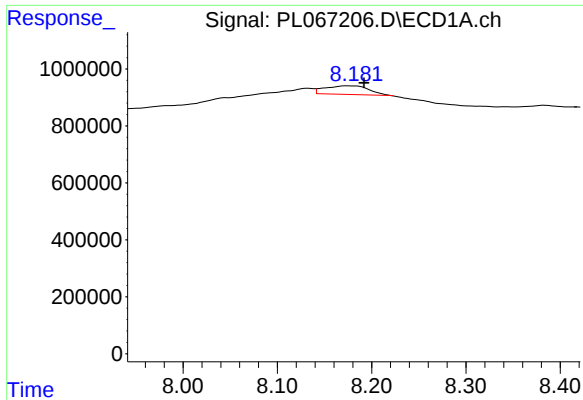

#27 Chlordane-5


R.T.: 8.174 min
Delta R.T.: -0.017 min
Response: 986596
Conc: 52.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

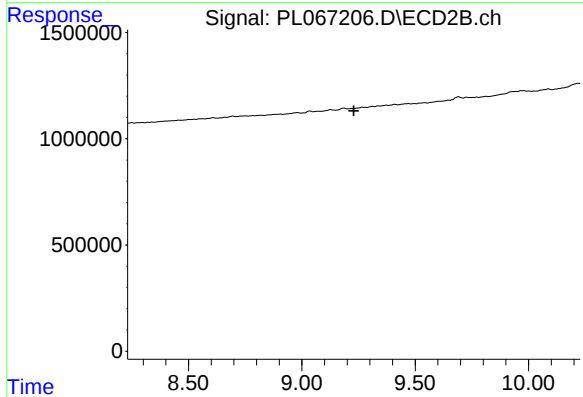


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.229 min
Response: 0
Conc: N.D.

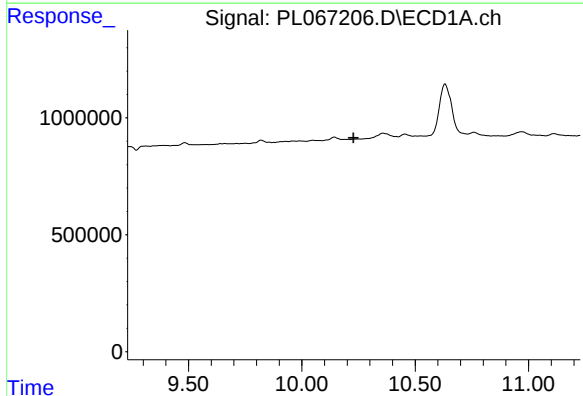

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.228 min
Response: 0
Conc: N.D.

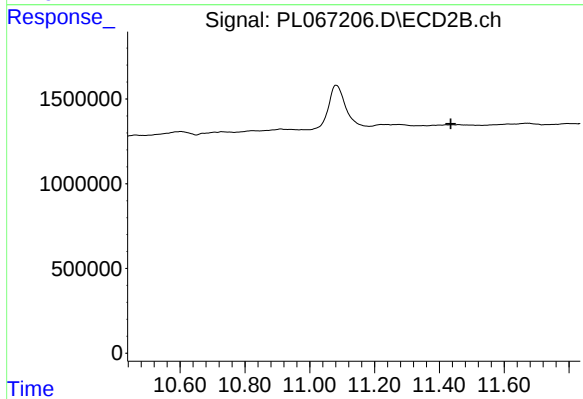

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.435 min
Response: 0
Conc: N.D.