

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060921\
 Data File : PL067207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2021 09:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 06:08:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 02 14:20:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.530	8044562	13455449	19.645	20.800
28)	SA Decachlor...	10.222	11.427	12481856	17427331	19.303	20.887
Target Compounds							
3)	MA gamma-BHC...	5.606	0.000	1456551	0	2.615	N.D. #
4)	MA Heptachlor	5.990f	0.000	536197	0	1.021	N.D. #
6)	B beta-BHC	5.990	0.000	536197	0	2.013	N.D. #
7)	B delta-BHC	6.215f	0.000	585761	0	1.104	N.D. #
24)	Chlordane-2	6.488	0.000	300950	0	13.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060921\
Data File : PL067207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2021 09:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 06:08:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060121.M
Quant Title : GC Extractables
QLast Update : Wed Jun 02 14:20:39 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

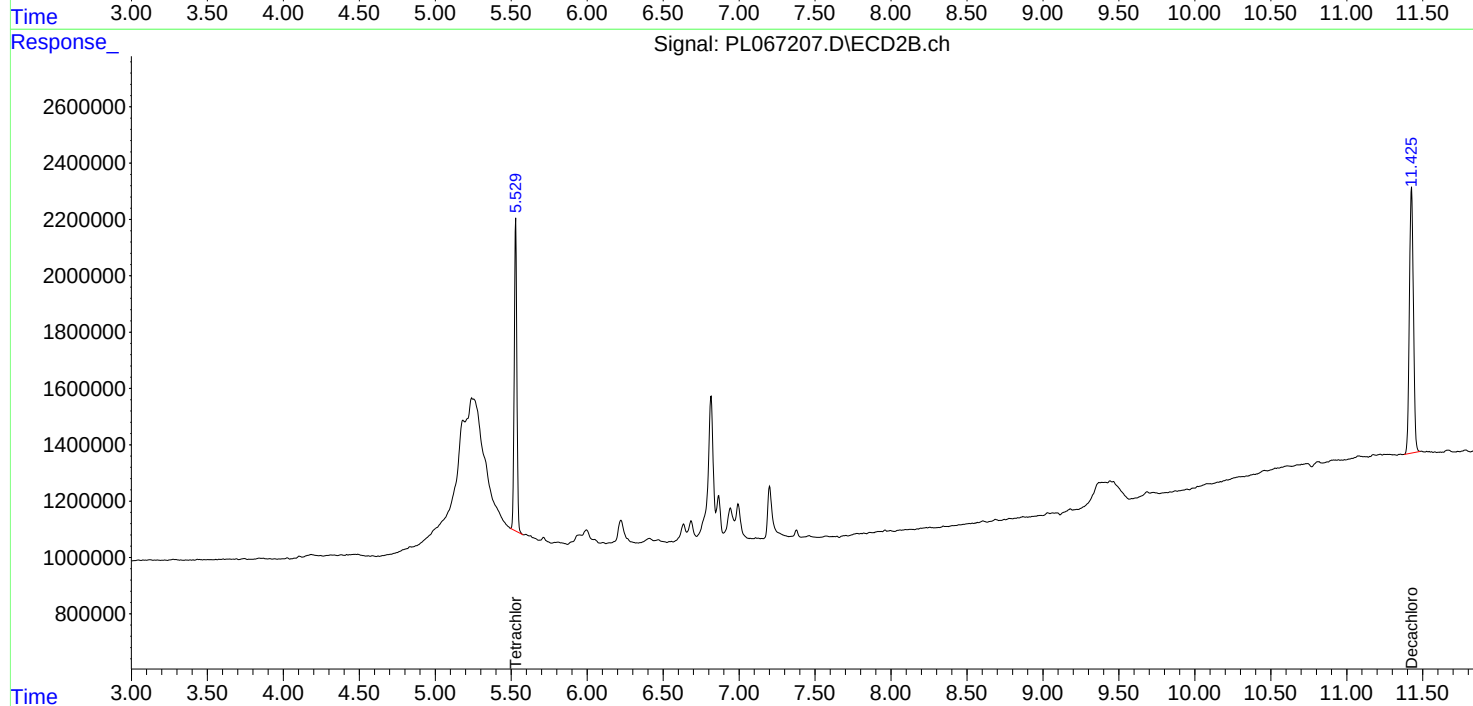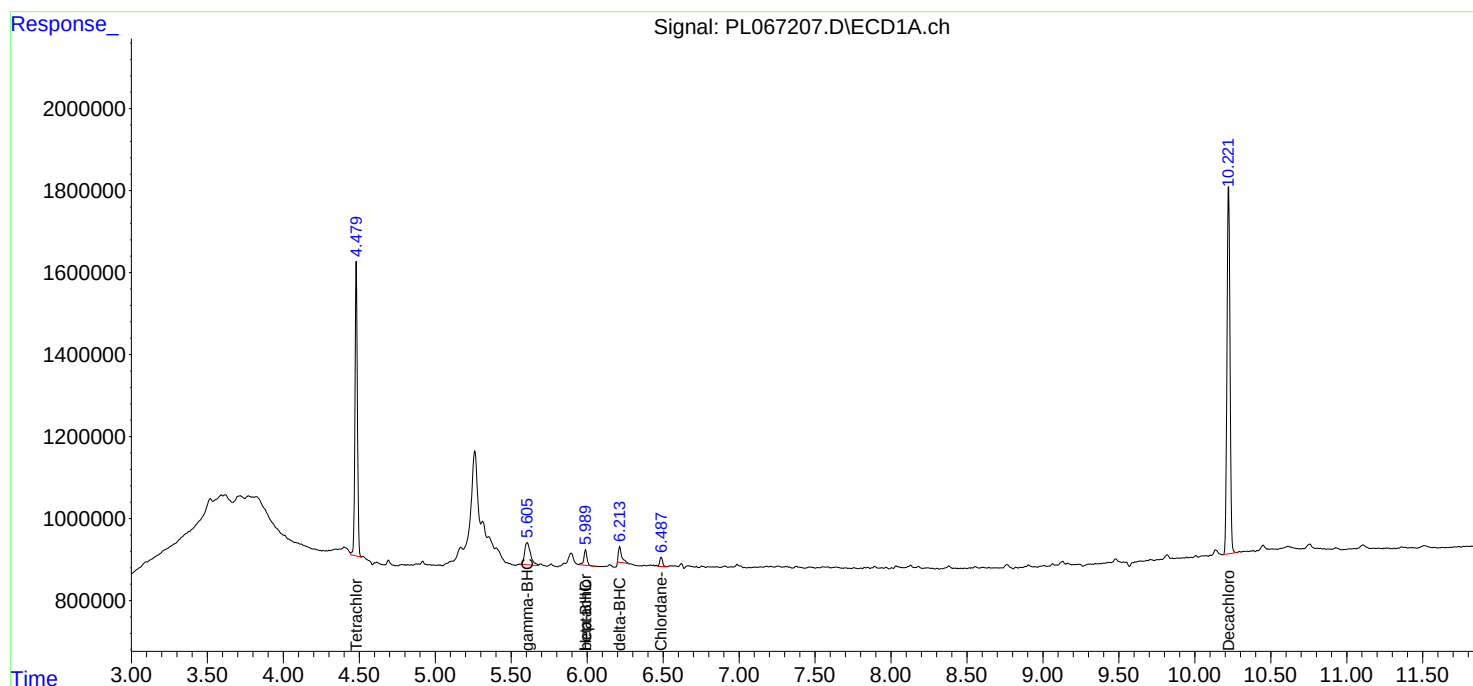


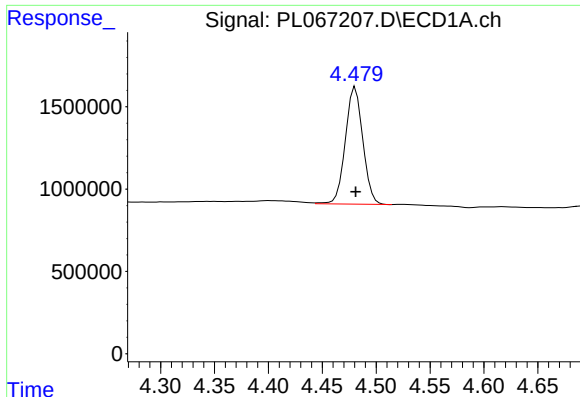

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 8044562
Conc: 19.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

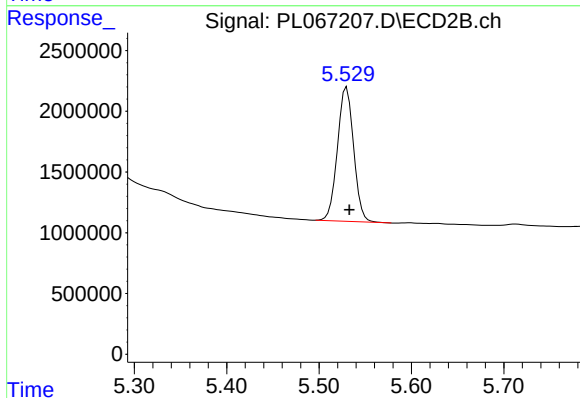


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.003 min
Response: 13455449
Conc: 20.80 ng/ml

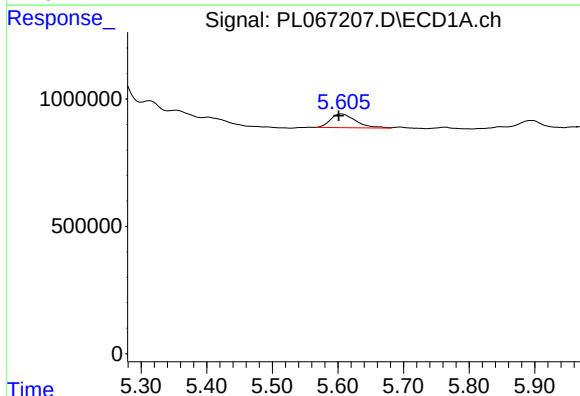


#3 gamma-BHC (Lindane)

R.T.: 5.606 min
Delta R.T.: 0.005 min
Response: 1456551
Conc: 2.62 ng/ml

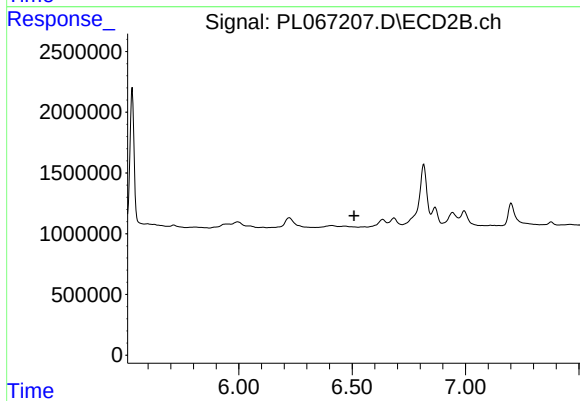

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.509 min
Response: 0
Conc: N.D.

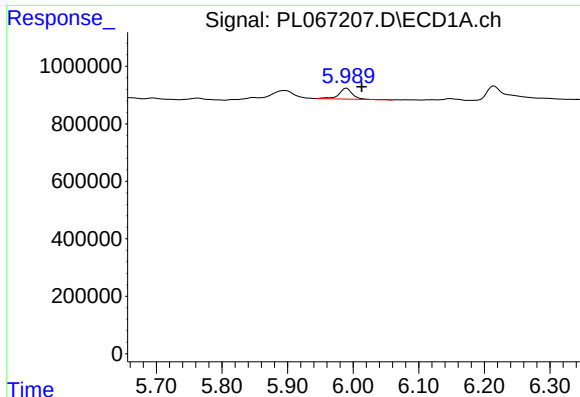

#4 Heptachlor


R.T.: 5.990 min
Delta R.T.: -0.023 min
Response: 536197
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

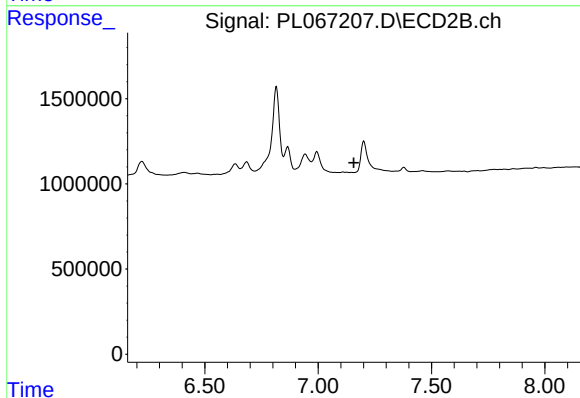


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.157 min
Response: 0
Conc: N.D.

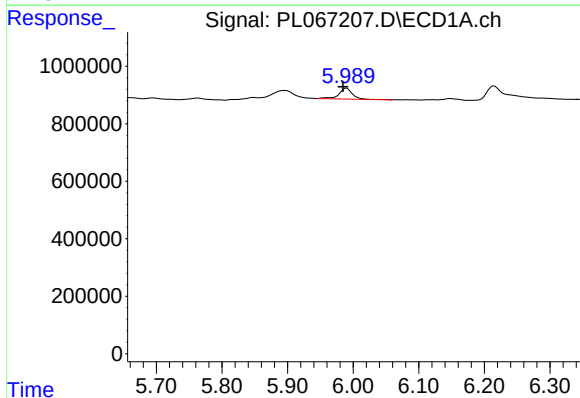


#6 beta-BHC

R.T.: 5.990 min
Delta R.T.: 0.005 min
Response: 536197
Conc: 2.01 ng/ml

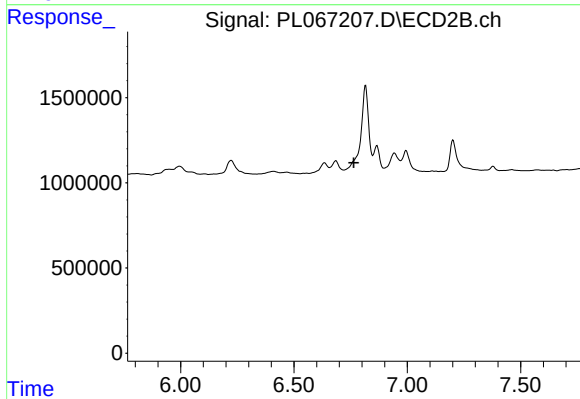

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

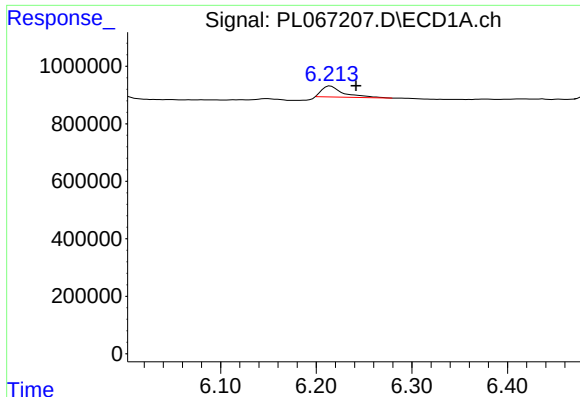

#7 delta-BHC


R.T.: 6.215 min
Delta R.T.: -0.027 min
Response: 585761
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

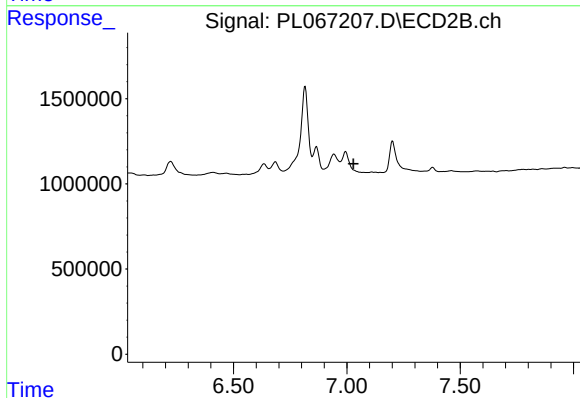


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.030 min
Response: 0
Conc: N.D.

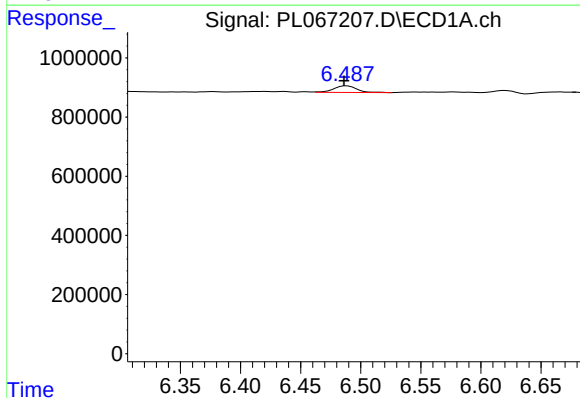


#24 Chlordane-2

R.T.: 6.488 min
Delta R.T.: 0.002 min
Response: 300950
Conc: 13.77 ng/ml

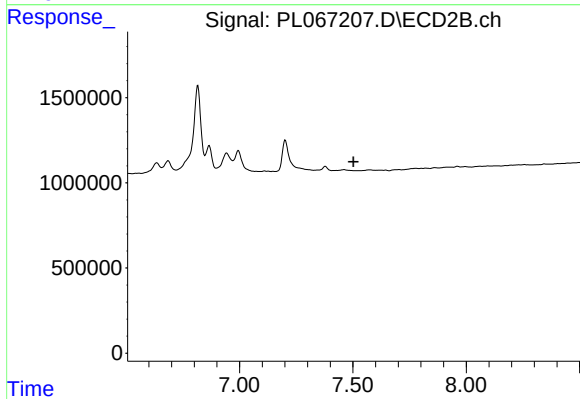

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

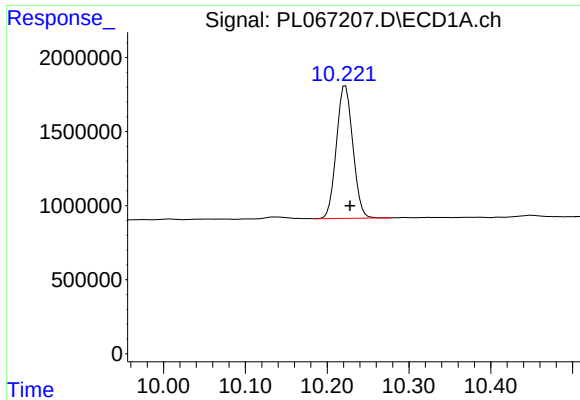

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.005 min
Response: 12481856
Conc: 19.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

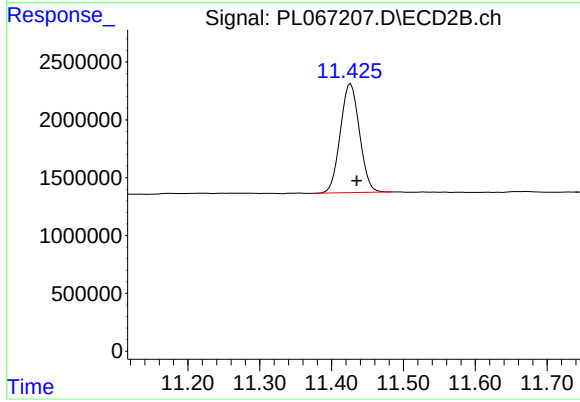

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.008 min
Response: 17427331
Conc: 20.89 ng/ml