

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060922\
 Data File : PL075657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 09:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 23:44:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.638	14161963	32592928	20.984	19.421
28)	SA Decachlor...	11.641	10.386	13874488	27167053	22.662	19.282
Target Compounds							
7)	B delta-BHC	0.000	6.401	0	403227	N.D.	0.188 #
10)	B gamma-Chl...	8.384	0.000	1151189	0	1.482	N.D. #
11)	B alpha-Chl...	8.466	7.389f	55841	220744	0.073	0.121 #
14)	MA Endrin	0.000	8.069f	0	372289	N.D.	0.272 #
15)	B Endosulfa...	9.306	0.000	299928	0	0.482	N.D. #
21)	B Endrin ke...	10.188f	0.000	524233	0	0.745	N.D. #
23)	Chlordane-1	0.000	5.978f	0	754664	N.D.	13.729 #
25)	Chlordane-3	8.384	0.000	1151189	0	11.149	N.D. #
26)	Chlordane-4	8.466	7.389f	55841	220744	0.441	1.199 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060922\
Data File : PL075657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 09:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 23:44:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

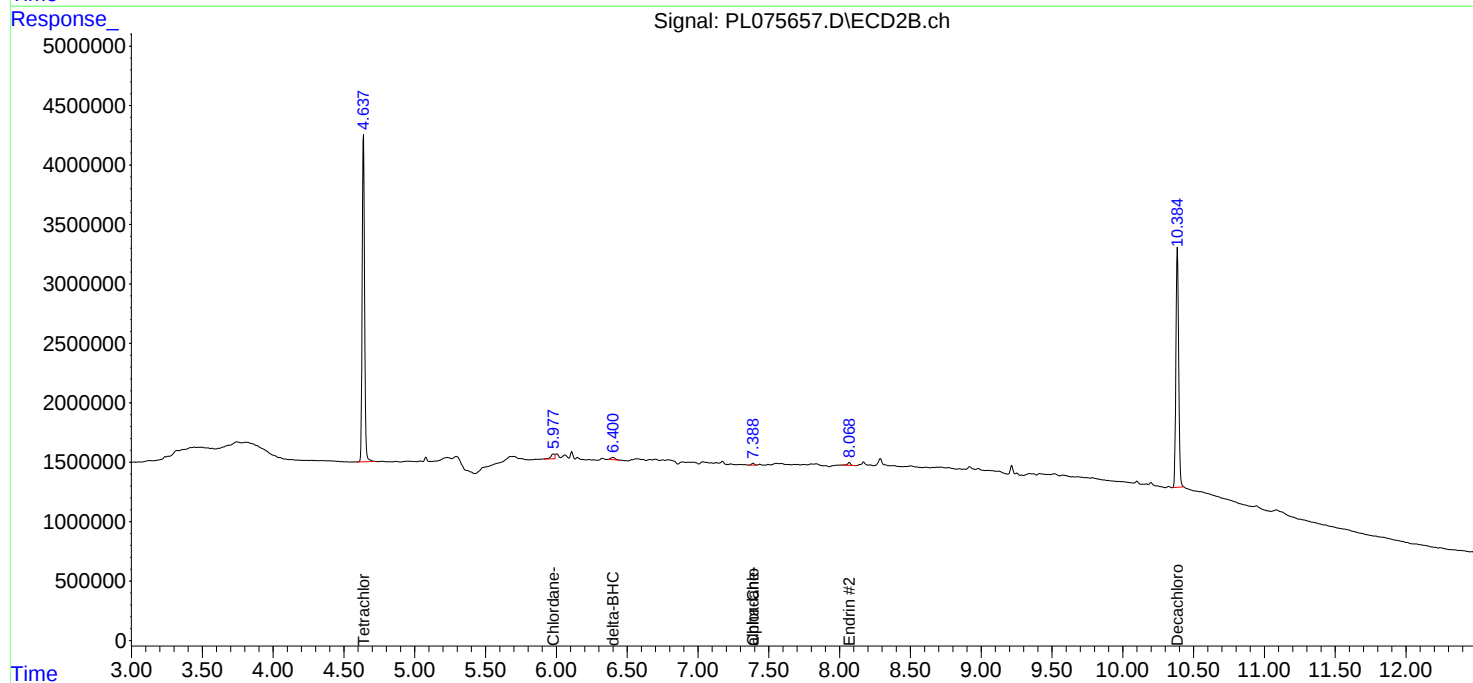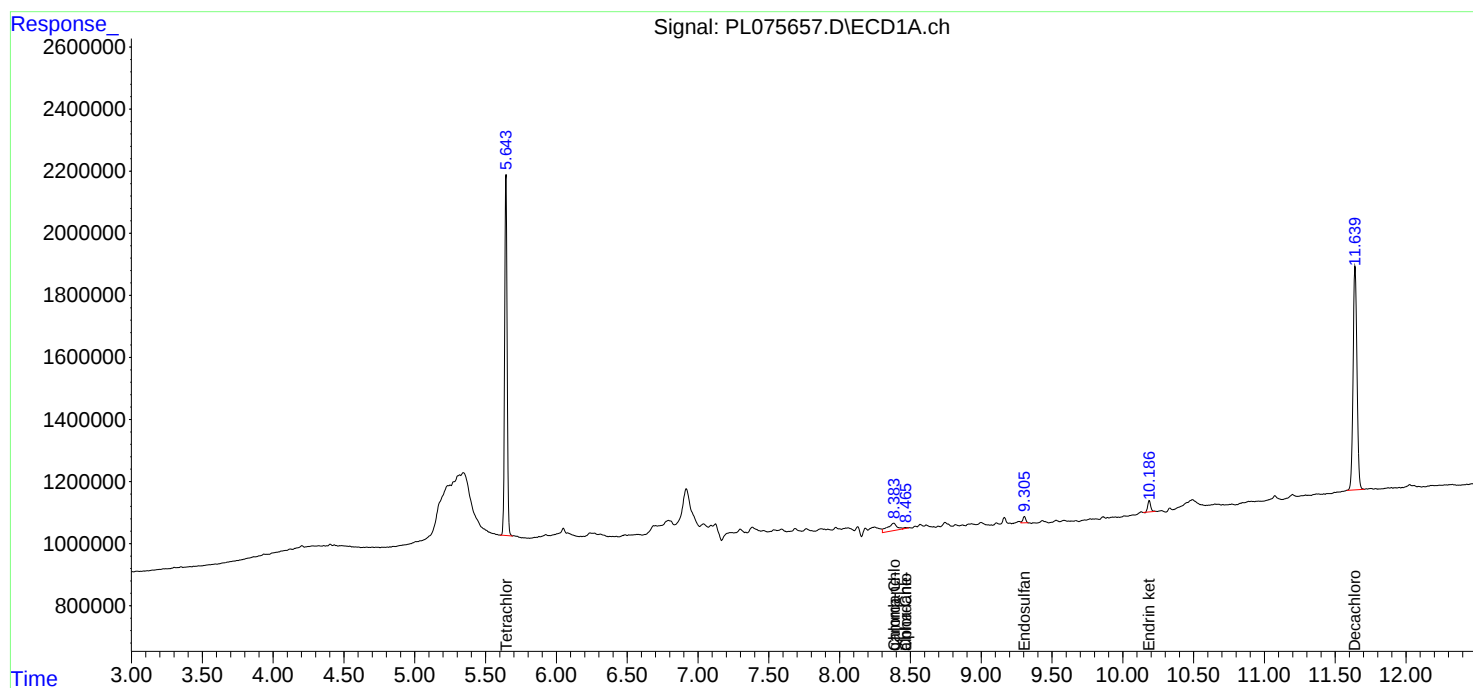


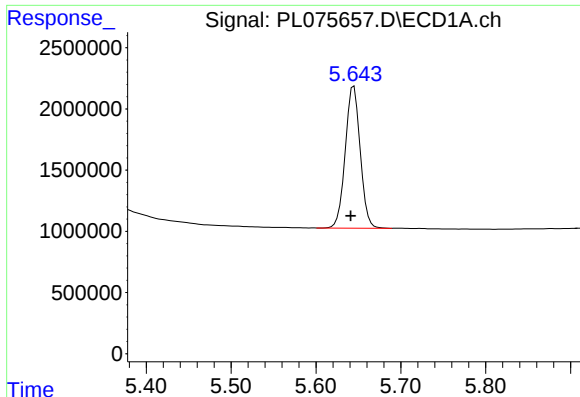

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: 0.004 min
Response: 14161963
Conc: 20.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

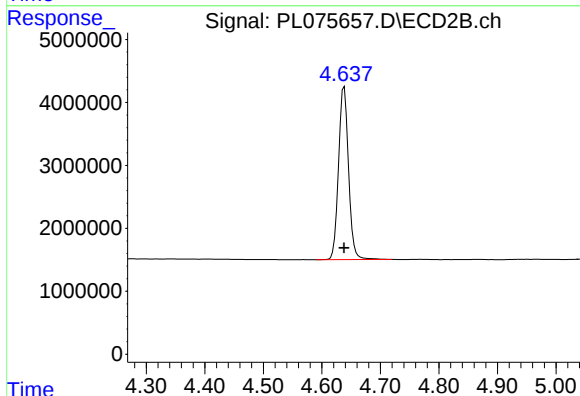


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 32592928
Conc: 19.42 ng/ml

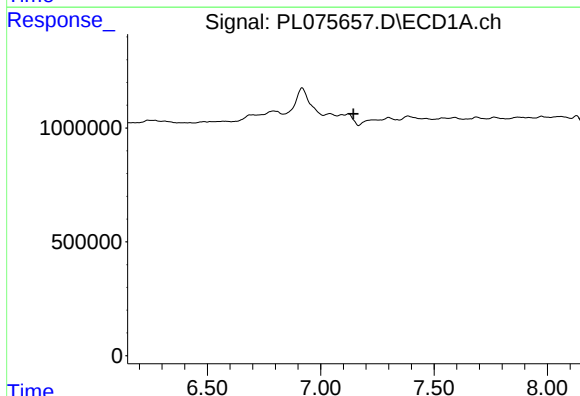


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

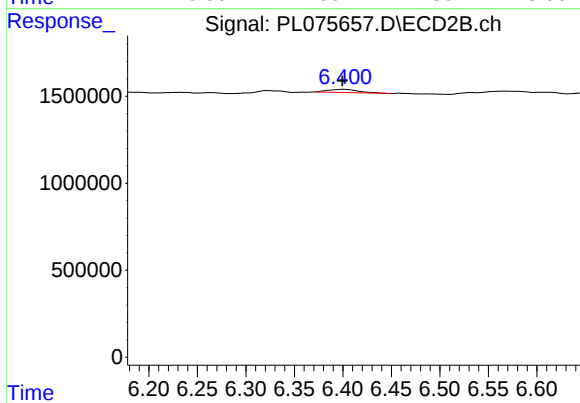

#7 delta-BHC


R.T.: 6.401 min
Delta R.T.: 0.001 min
Response: 403227
Conc: 0.19 ng/ml

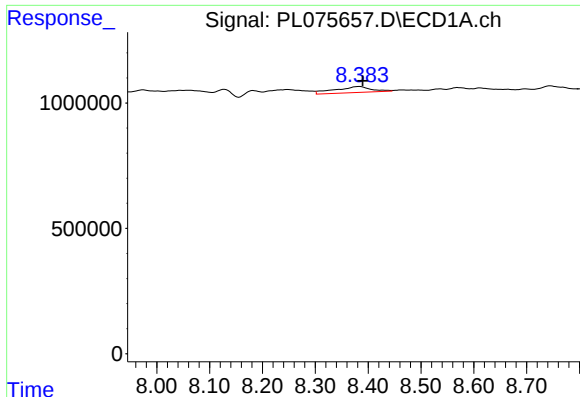

#10 gamma-Chlordane


R.T.: 8.384 min
Delta R.T.: -0.006 min
Response: 1151189
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

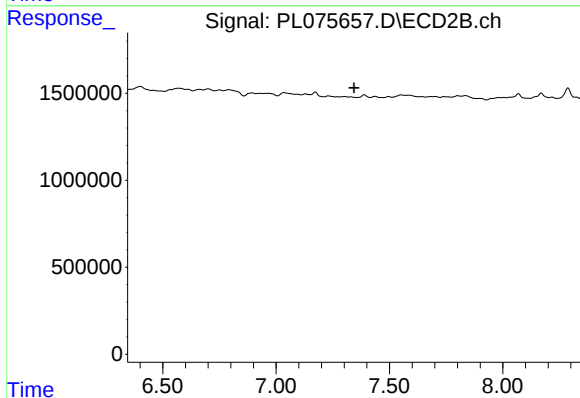


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

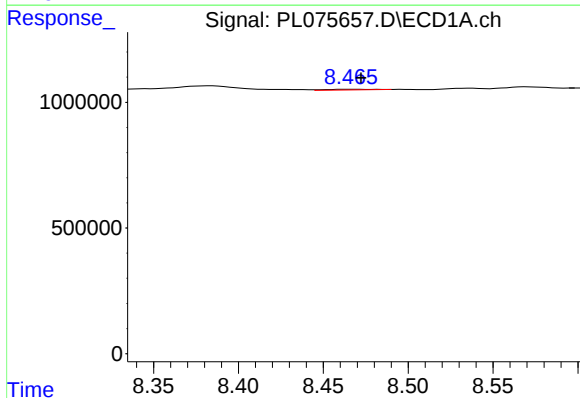


#11 alpha-Chlordane

R.T.: 8.466 min
Delta R.T.: -0.006 min
Response: 55841
Conc: 0.07 ng/ml

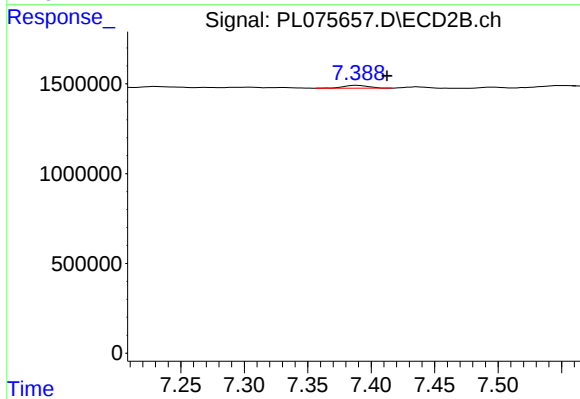

#11 alpha-Chlordane


R.T.: 7.389 min
Delta R.T.: -0.023 min
Response: 220744
Conc: 0.12 ng/ml

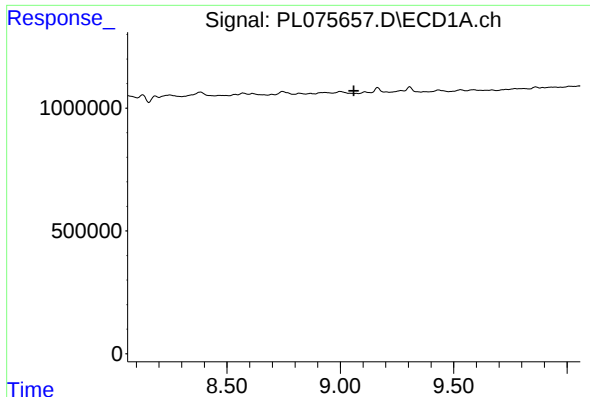

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

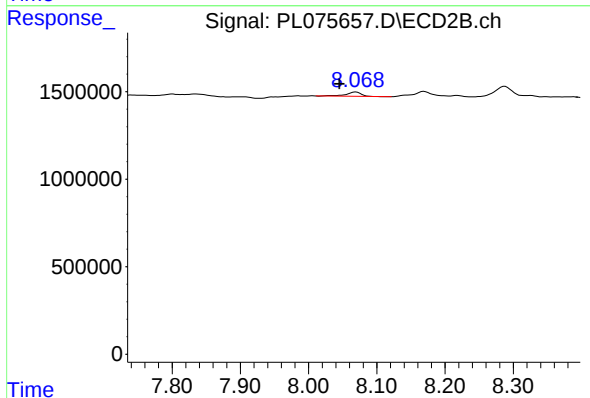


#14 Endrin

R.T.: 8.069 min
Delta R.T.: 0.024 min
Response: 372289
Conc: 0.27 ng/ml

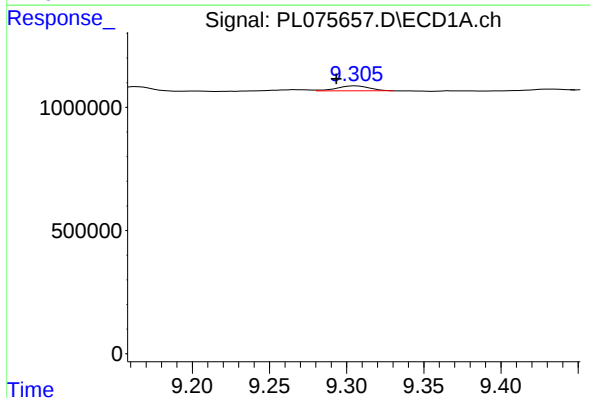


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.013 min
Response: 299928
Conc: 0.48 ng/ml

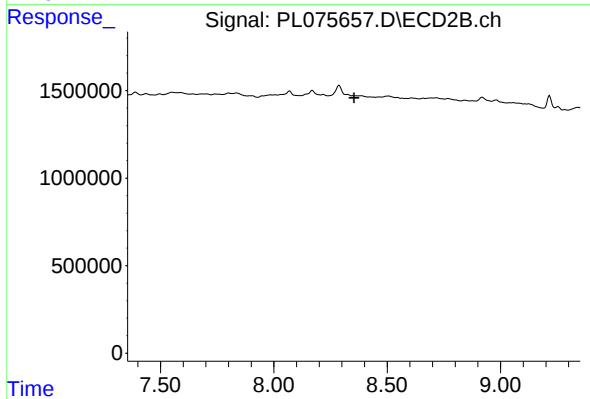

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

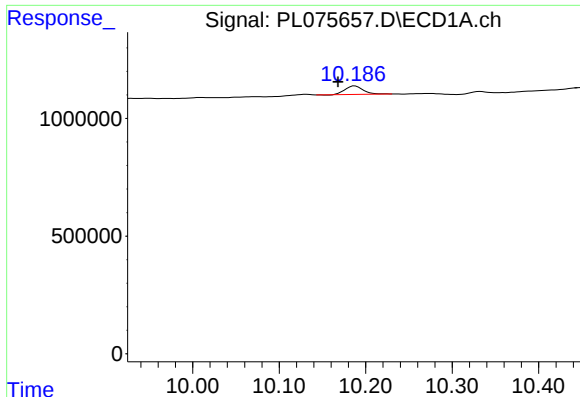

#21 Endrin ketone


R.T.: 10.188 min
Delta R.T.: 0.019 min
Response: 524233
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

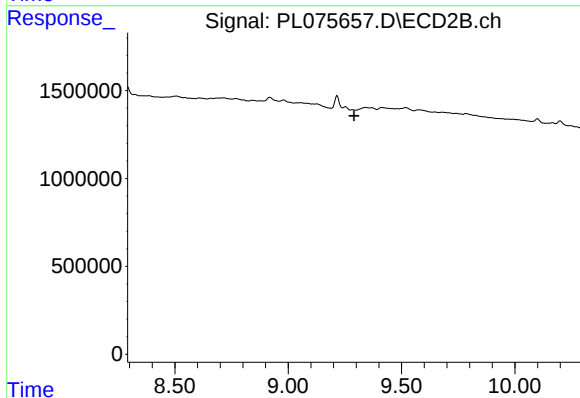


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

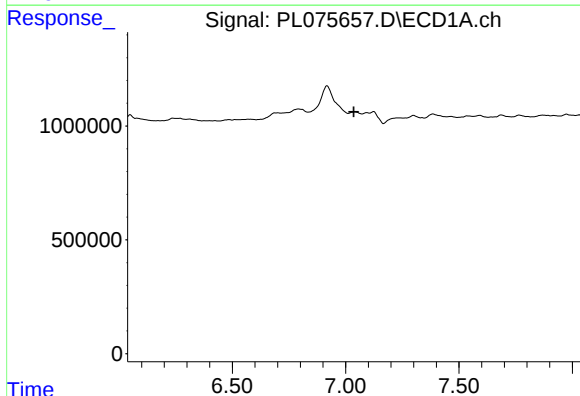


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.036 min
Response: 0
Conc: N.D.

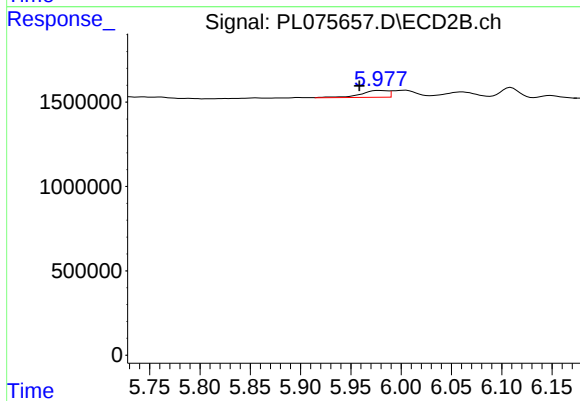

#23 Chlordane-1


R.T.: 5.978 min
Delta R.T.: 0.020 min
Response: 754664
Conc: 13.73 ng/ml

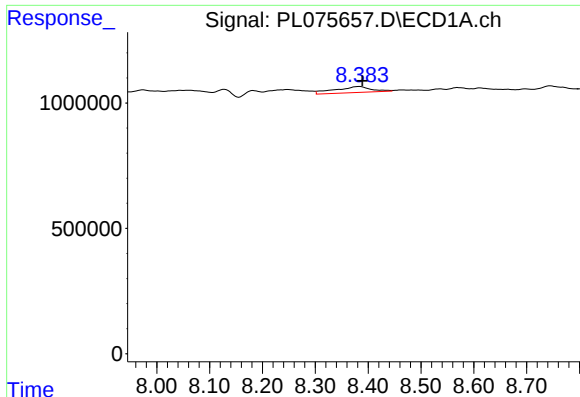

#25 Chlordane-3


R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 1151189
Conc: 11.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

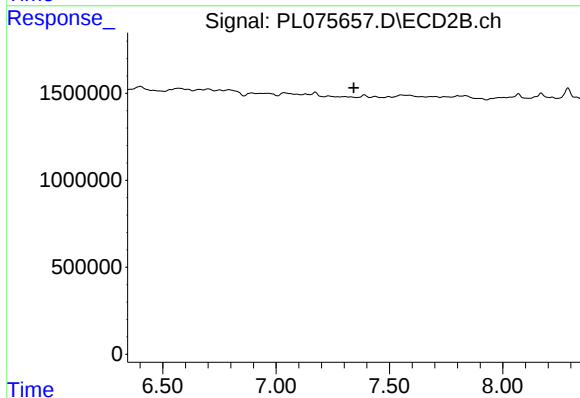


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

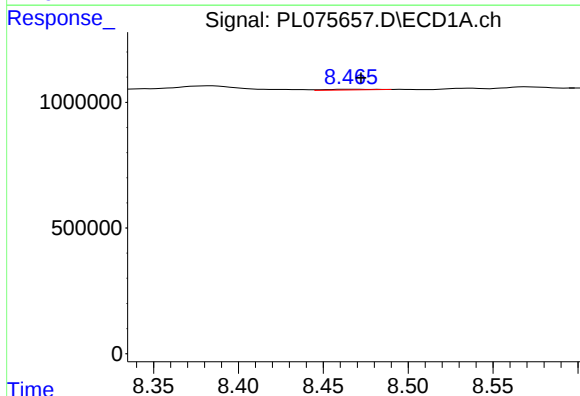


#26 Chlordane-4

R.T.: 8.466 min
Delta R.T.: -0.006 min
Response: 55841
Conc: 0.44 ng/ml

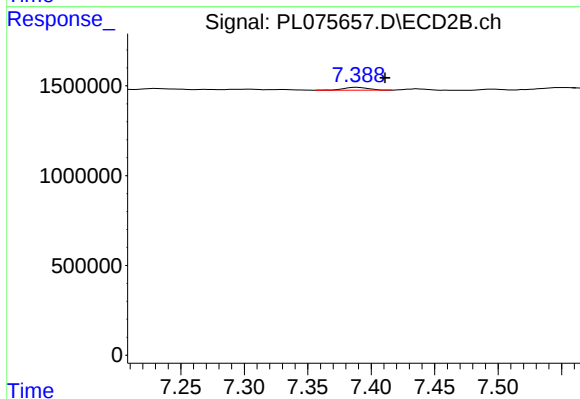

#26 Chlordane-4


R.T.: 7.389 min
Delta R.T.: -0.022 min
Response: 220744
Conc: 1.20 ng/ml

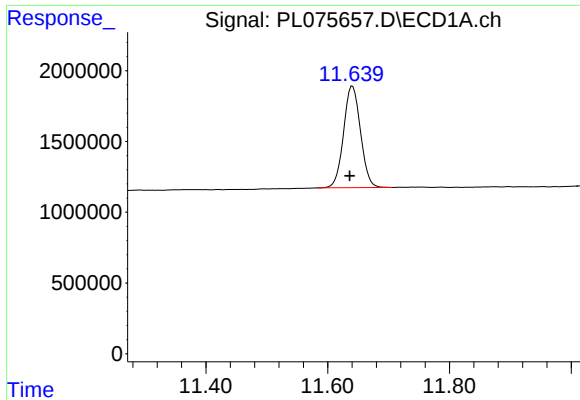

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.005 min
Response: 13874488
Conc: 22.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

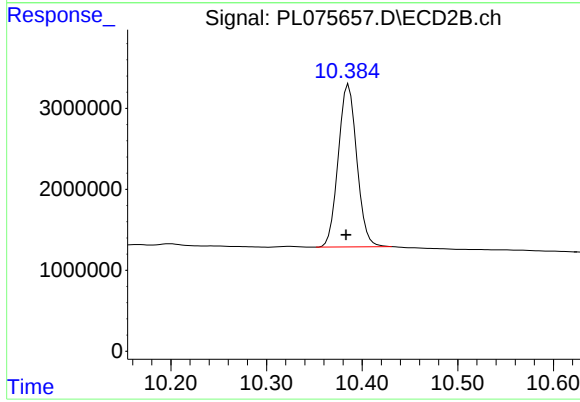

#28 Decachlorobiphenyl

R.T.: 10.386 min
Delta R.T.: 0.003 min
Response: 27167053
Conc: 19.28 ng/ml