

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060922\
 Data File : PL075669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2022 15:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 23:48:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.636	13625359	30773694	20.189	18.337
28)	SA Decachlor...	11.639	10.383	12442957	22673598	20.324	16.093
Target Compounds							
4)	MA Heptachlor	7.305f	6.167	889913	-83390	0.968	N.D. #
5)	MB Aldrin	0.000	6.468f	0	928976	N.D.	0.473 #
7)	B delta-BHC	0.000	6.405	0	241410	N.D.	0.113 #
10)	B gamma-Chl...	8.382	0.000	1416480	0	1.824	N.D. #
14)	MA Endrin	0.000	8.067f	0	1181467	N.D.	0.864 #
15)	B Endosulfa...	9.305	0.000	197149	0	0.317	N.D. #
21)	B Endrin ke...	10.186f	0.000	430935	0	0.613	N.D. #
23)	Chlordane-1	7.051f	0.000	314065	0	12.511	N.D. #
24)	Chlordane-2	0.000	6.656	0	191154	N.D.	2.859 #
25)	Chlordane-3	8.382	0.000	1416480	0	13.719	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060922\
Data File : PL075669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2022 15:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 23:48:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

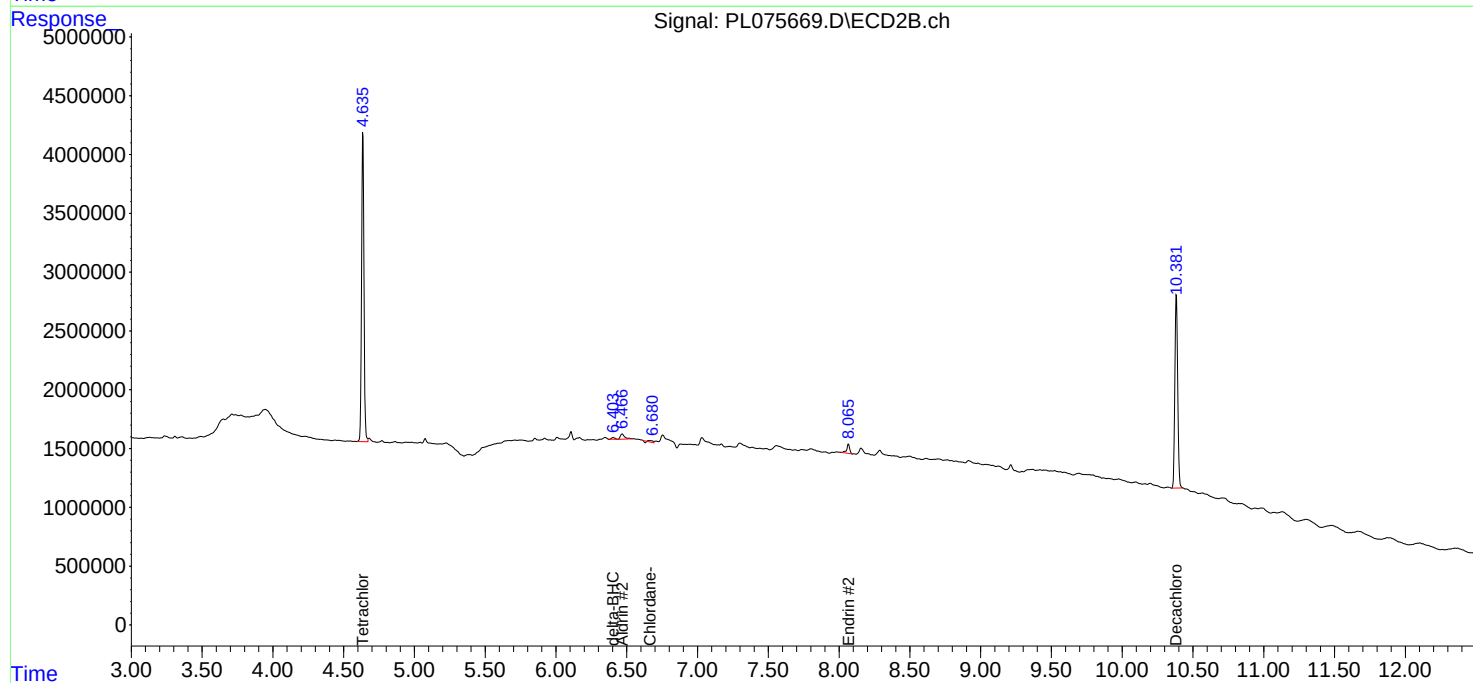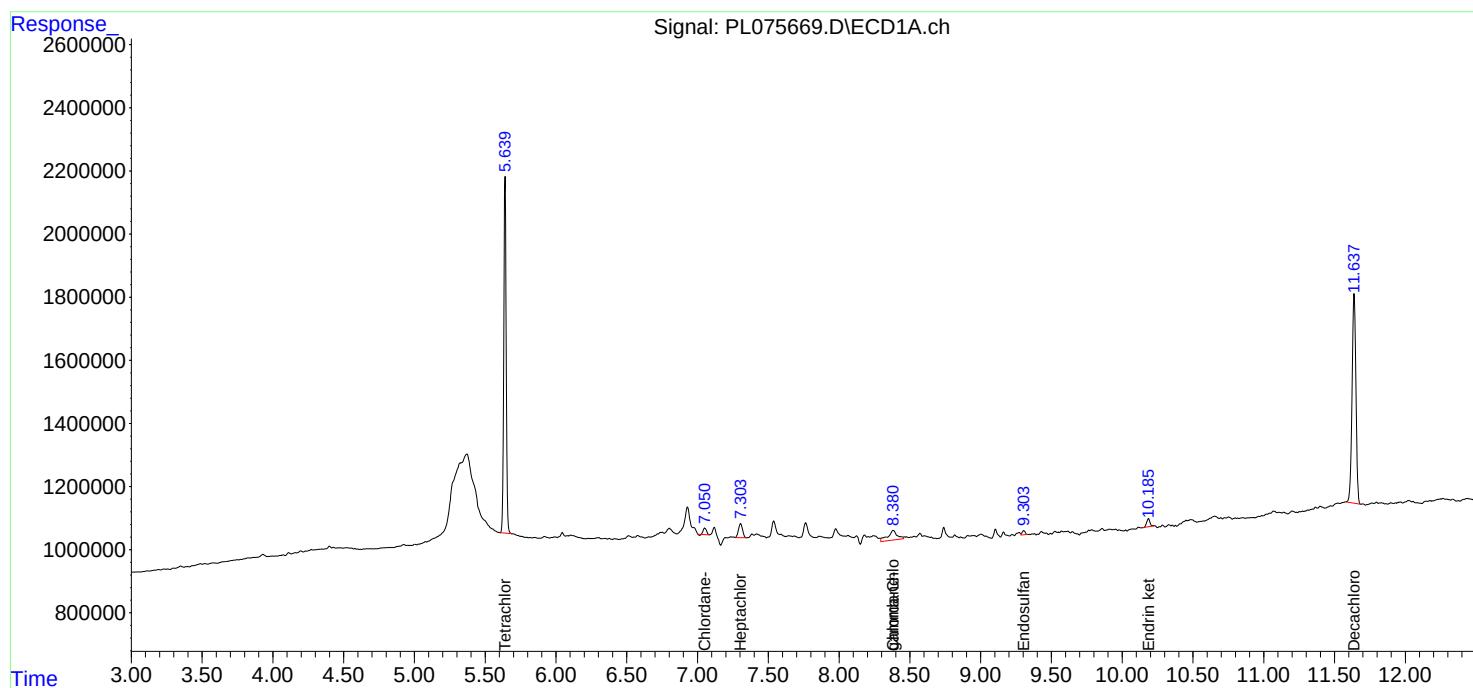


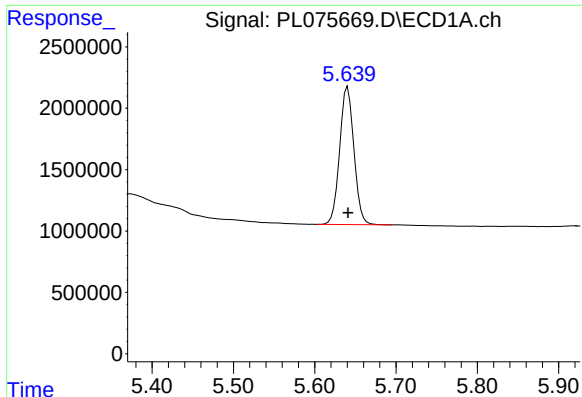

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13625359
Conc: 20.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

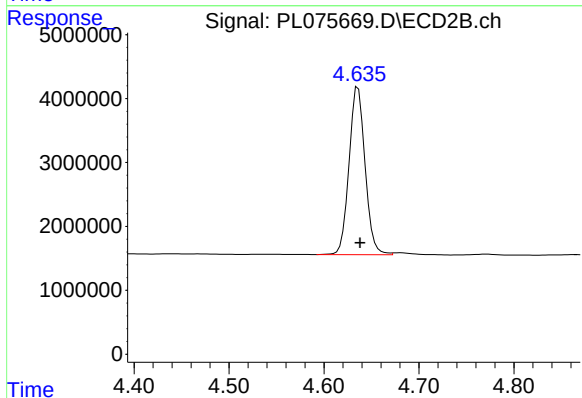


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 30773694
Conc: 18.34 ng/ml

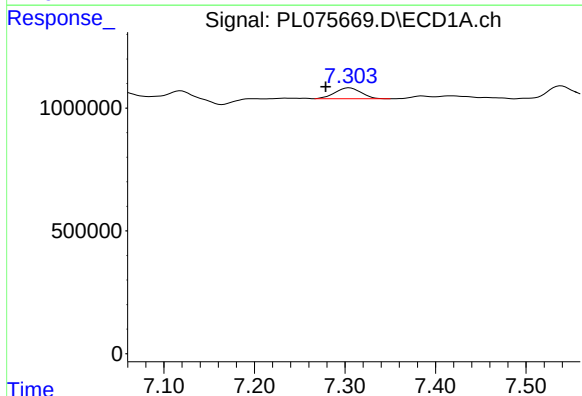


#4 Heptachlor

R.T.: 7.305 min
Delta R.T.: 0.026 min
Response: 889913
Conc: 0.97 ng/ml

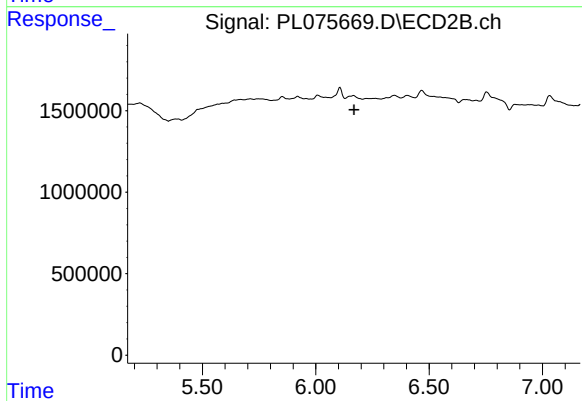

#4 Heptachlor


R.T.: 6.167 min
Delta R.T.: -0.002 min
Response: -83390
Conc: N.D.

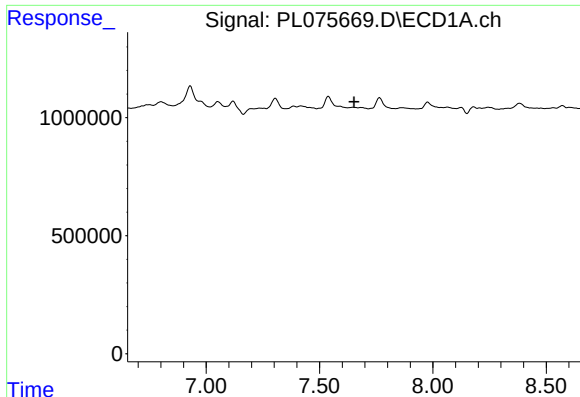

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

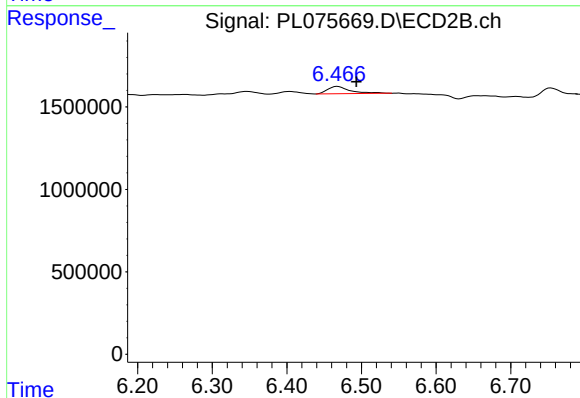


#5 Aldrin

R.T.: 6.468 min
Delta R.T.: -0.026 min
Response: 928976
Conc: 0.47 ng/ml

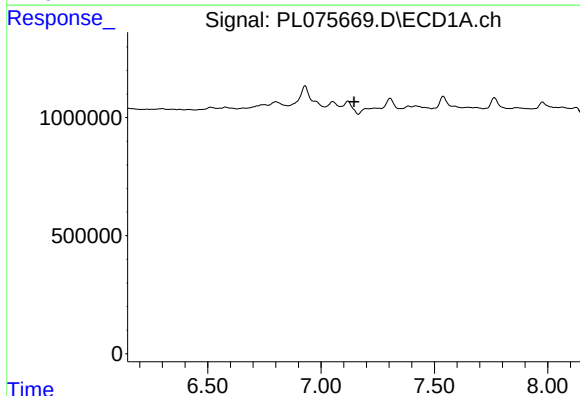


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

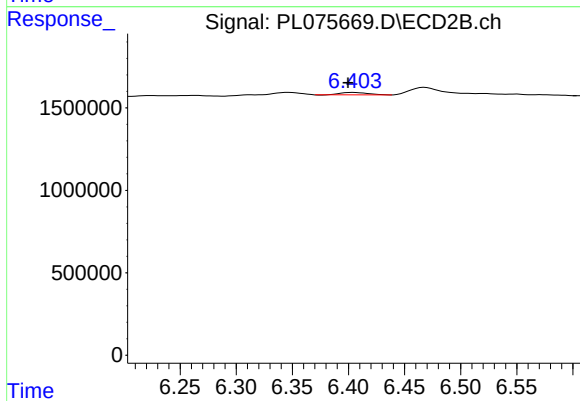

#7 delta-BHC


R.T.: 6.405 min
Delta R.T.: 0.005 min
Response: 241410
Conc: 0.11 ng/ml

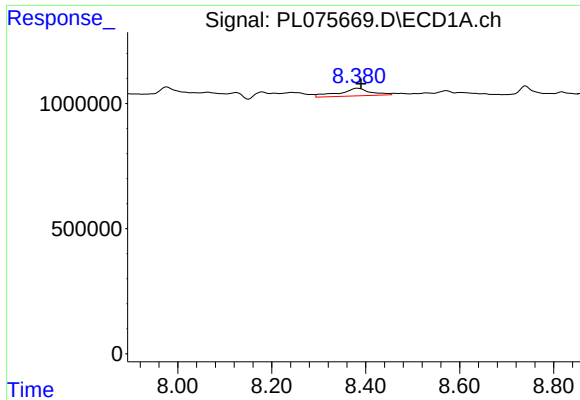

#10 gamma-Chlordane


R.T.: 8.382 min
Delta R.T.: -0.008 min
Response: 1416480
Conc: 1.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

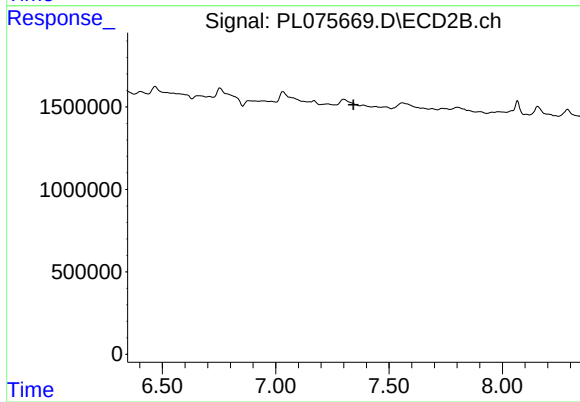


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

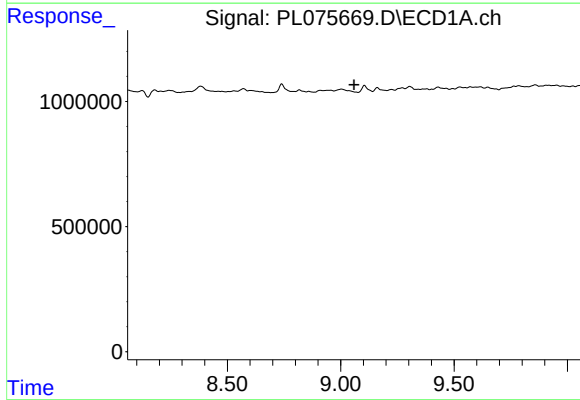


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

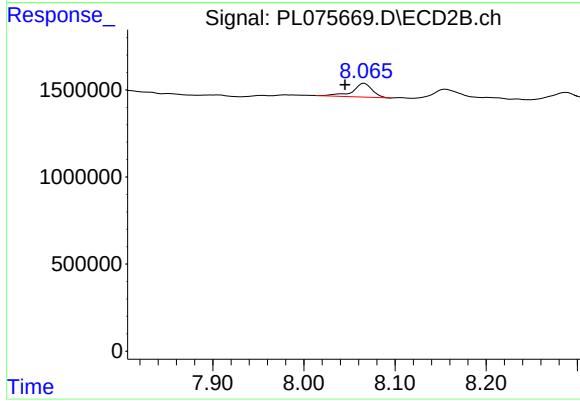

#14 Endrin


R.T.: 8.067 min
Delta R.T.: 0.022 min
Response: 1181467
Conc: 0.86 ng/ml

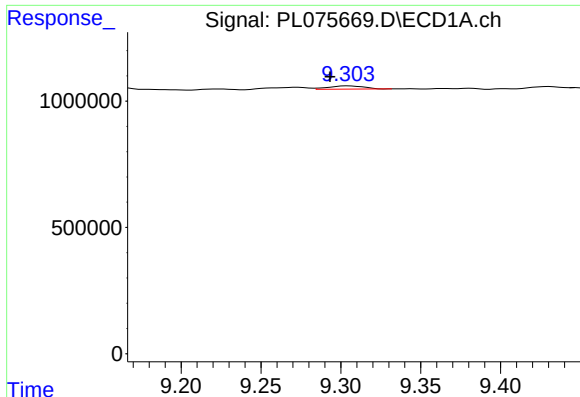

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.011 min
Response: 197149
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

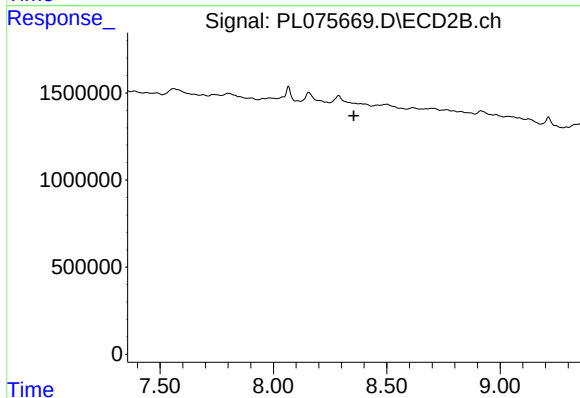


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

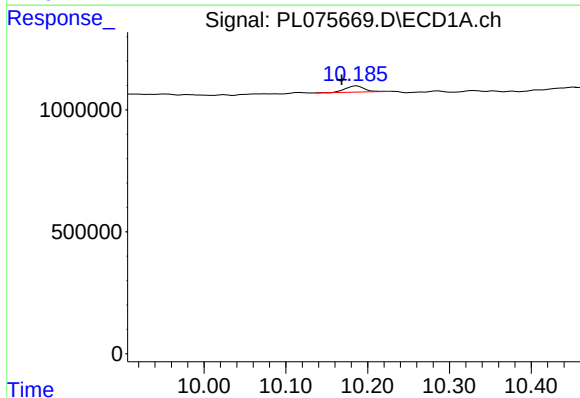


#21 Endrin ketone

R.T.: 10.186 min
Delta R.T.: 0.018 min
Response: 430935
Conc: 0.61 ng/ml

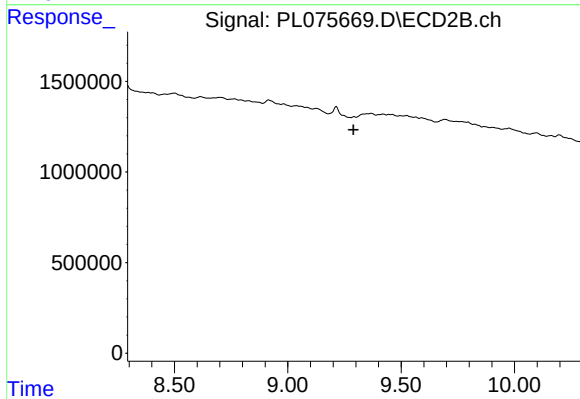

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

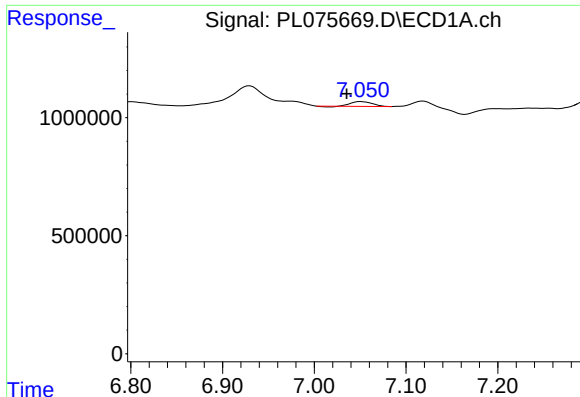

#23 Chlordane-1


R.T.: 7.051 min
Delta R.T.: 0.016 min
Response: 314065
Conc: 12.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

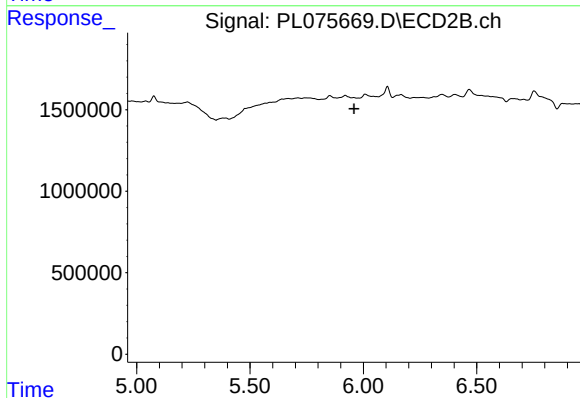


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.959 min
Response: 0
Conc: N.D.

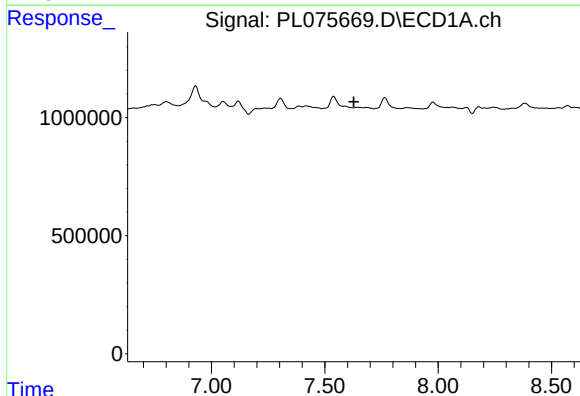


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.628 min
Response: 0
Conc: N.D.

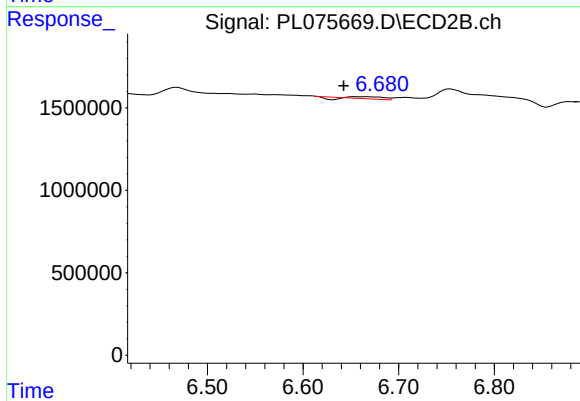

#24 Chlordane-2


R.T.: 6.656 min
Delta R.T.: 0.014 min
Response: 191154
Conc: 2.86 ng/ml

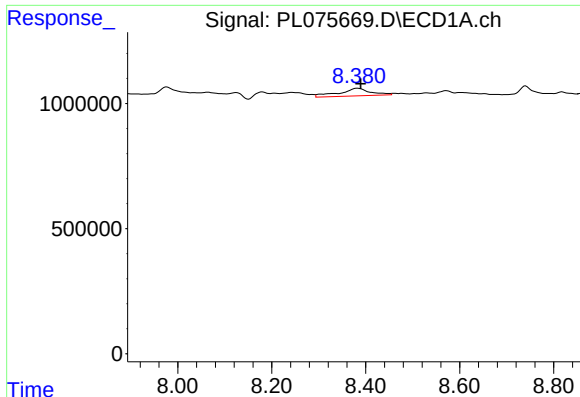

#25 Chlordane-3


R.T.: 8.382 min
Delta R.T.: -0.007 min
Response: 1416480
Conc: 13.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

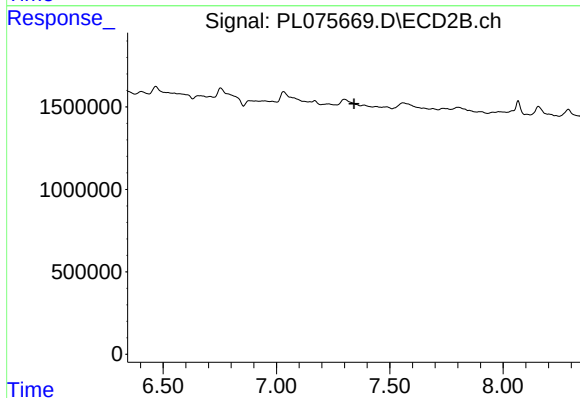


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

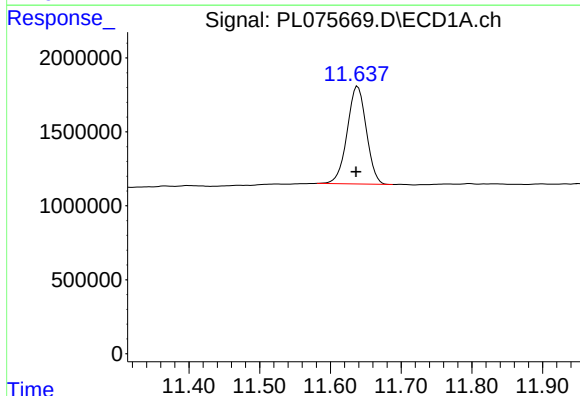

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: 0.002 min
Response: 12442957
Conc: 20.32 ng/ml

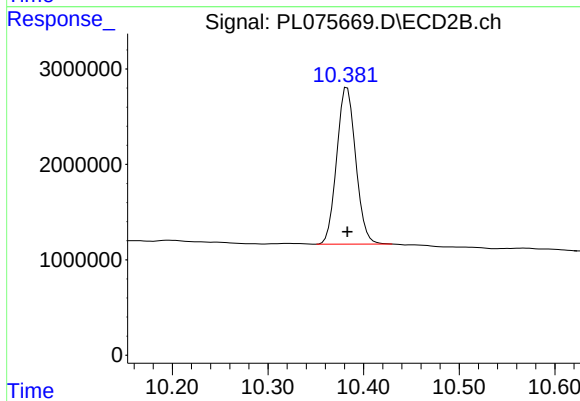

#28 Decachlorobiphenyl

R.T.: 10.383 min
Delta R.T.: 0.000 min
Response: 22673598
Conc: 16.09 ng/ml