

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061020\
 Data File : PL059231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2020 15:53
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 17:26:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.521	4.072	38891506	53883055	22.522	20.709
28)	SA Decachlor...	8.293	9.181	28411885	43665740	17.278	18.420
Target Compounds							
2)	A alpha-BHC	3.969	0.000	978460	0	0.391	N.D. #
4)	MA Heptachlor	0.000	5.258	0	572930	N.D.	0.166 #
7)	B delta-BHC	0.000	5.111f	0	1372332	N.D.	0.489 #
8)	B Heptachlo...	5.259	5.951	845366	6591154	0.495	2.379 #
10)	B gamma-Chl...	0.000	6.195	0	512992	N.D.	0.171 #
14)	MA Endrin	6.089	0.000	325862	0	0.215	N.D. #
15)	B Endosulfa...	0.000	7.008	0	871255	N.D.	0.334 #
17)	MA 4,4'-DDT	0.000	7.217	0	271629	N.D.	0.119 #
23)	Chlordane-1	4.398	0.000	184573	0	3.669	N.D. #
25)	Chlordane-3	0.000	6.195	0	512992	N.D.	1.368 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061020\
Data File : PL059231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2020 15:53
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 17:26:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

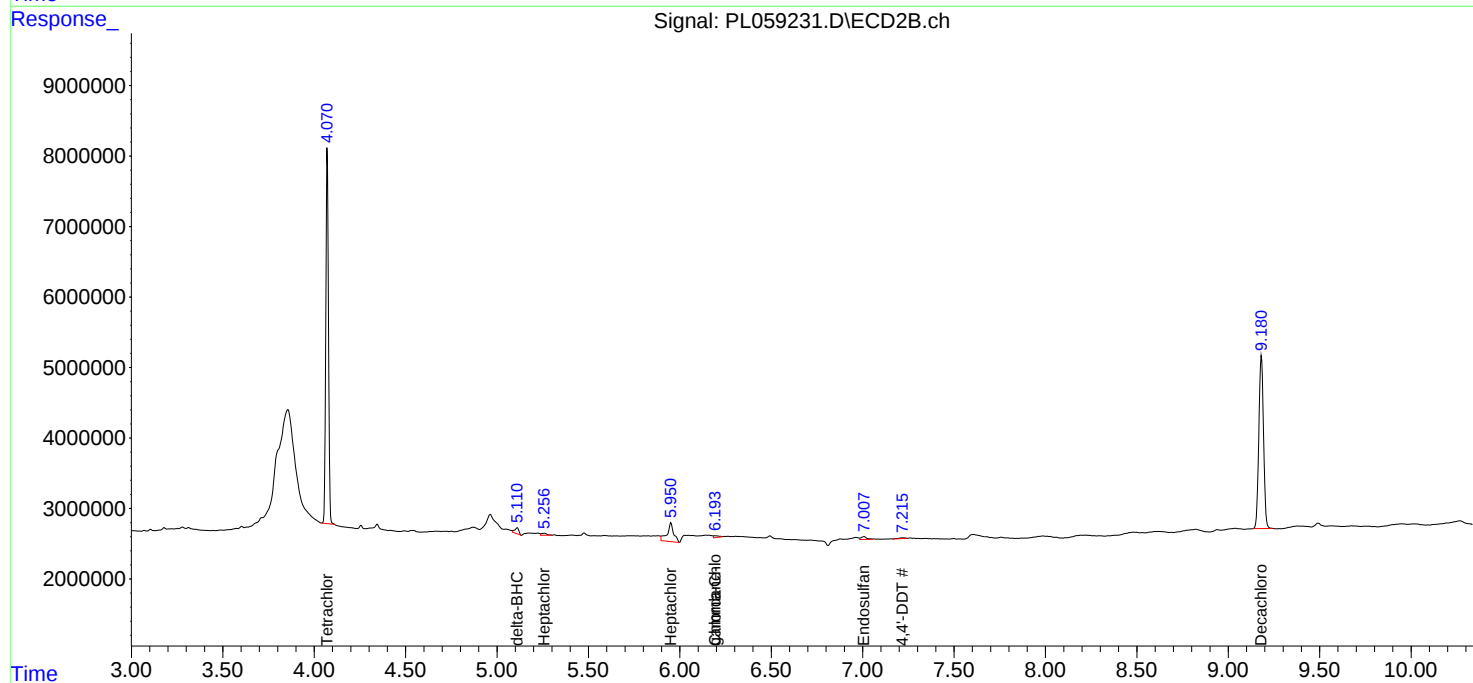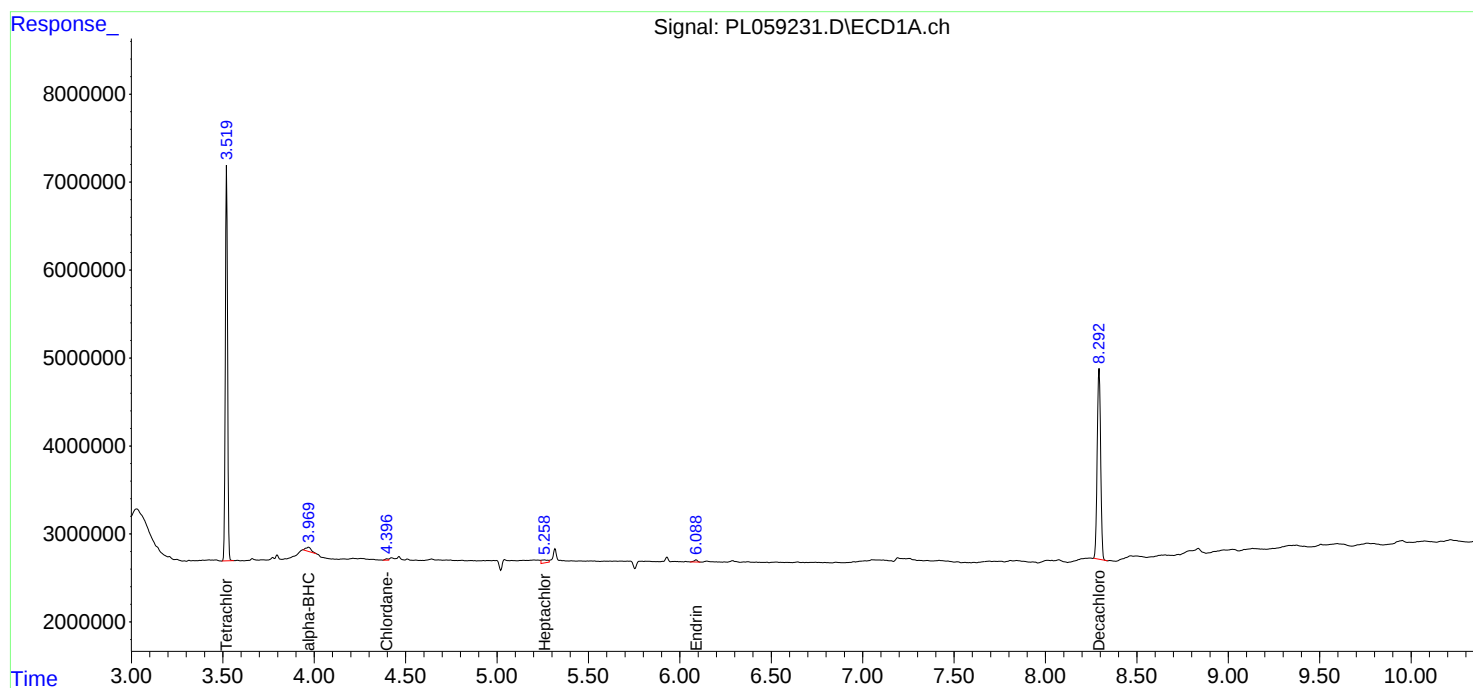


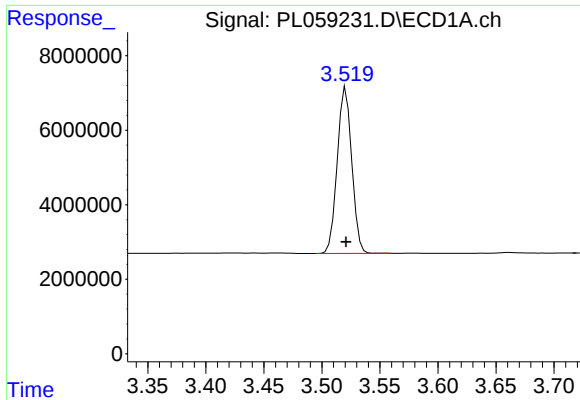

#1 Tetrachloro-m-xylene


R.T.: 3.521 min
Delta R.T.: 0.000 min
Response: 38891506
Conc: 22.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

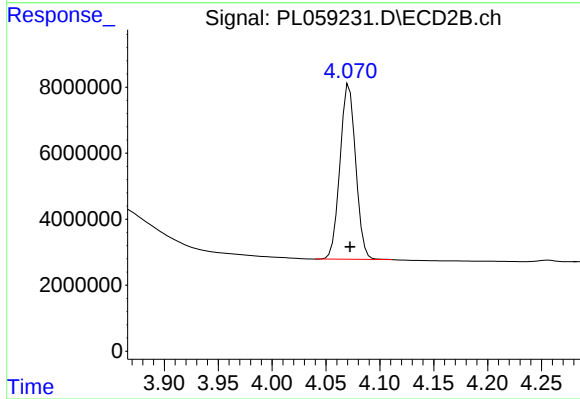


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 53883055
Conc: 20.71 ng/ml

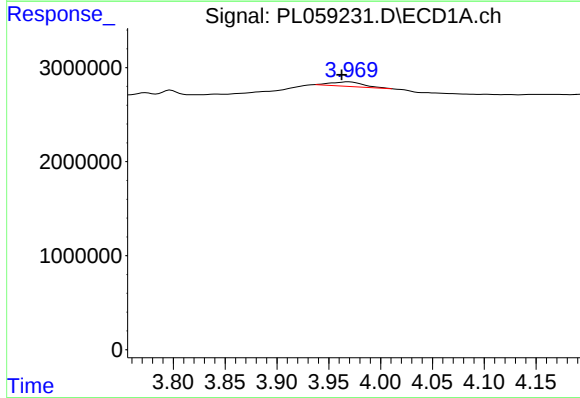


#2 alpha-BHC

R.T.: 3.969 min
Delta R.T.: 0.007 min
Response: 978460
Conc: 0.39 ng/ml

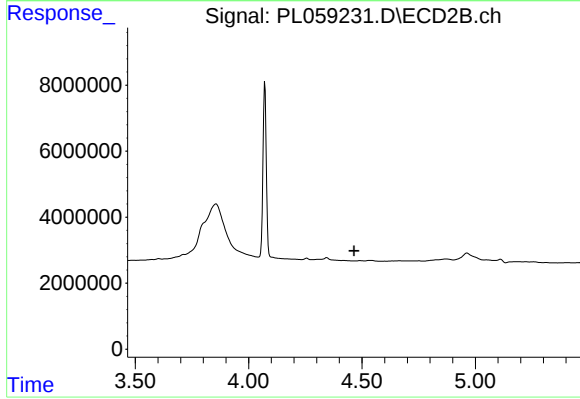

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.465 min
Response: 0
Conc: N.D.

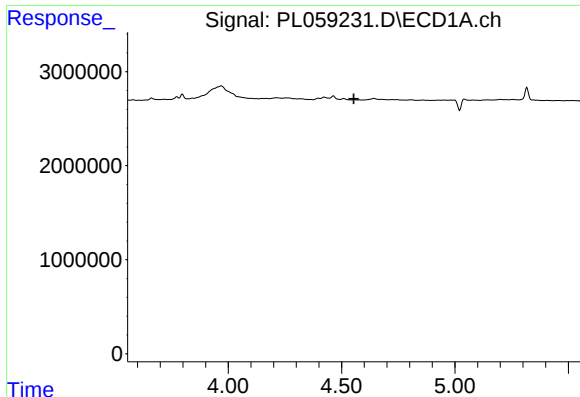

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

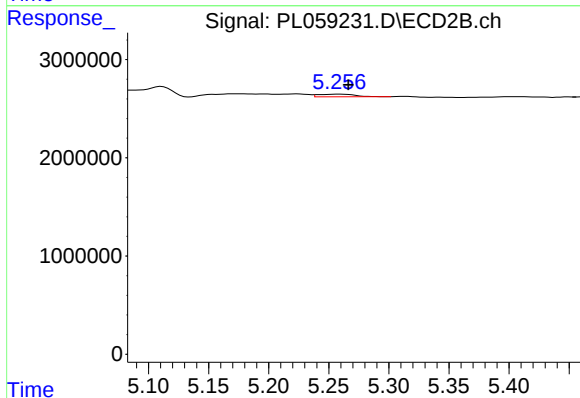


#4 Heptachlor

R.T.: 5.258 min
Delta R.T.: -0.008 min
Response: 572930
Conc: 0.17 ng/ml

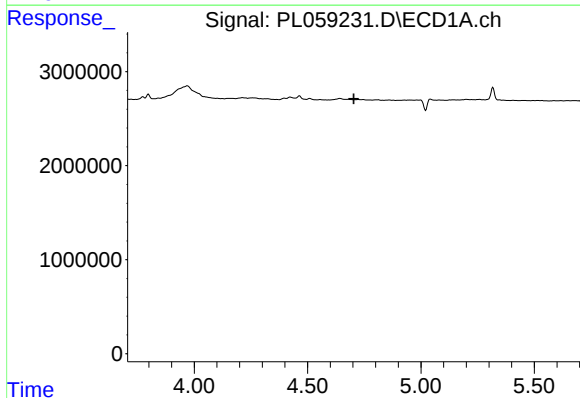


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

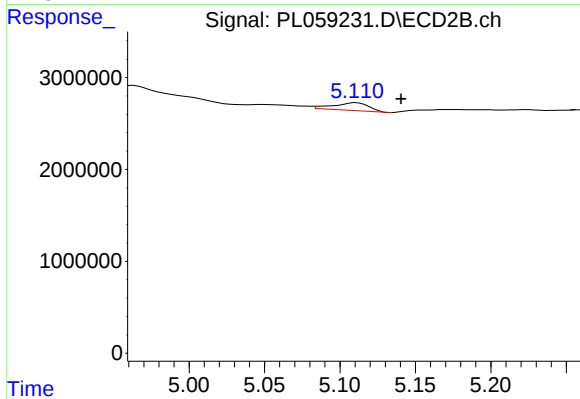

#7 delta-BHC


R.T.: 5.111 min
Delta R.T.: -0.030 min
Response: 1372332
Conc: 0.49 ng/ml

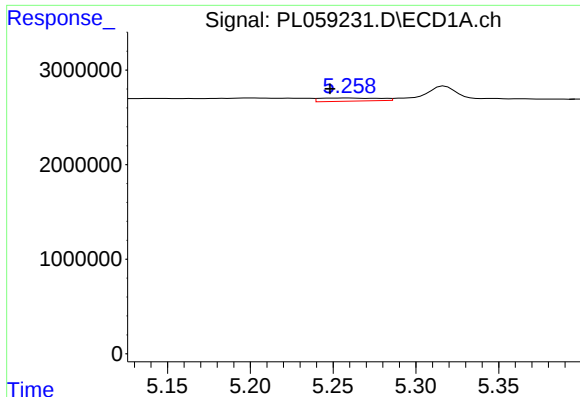

#8 Heptachlor epoxide


R.T.: 5.259 min
Delta R.T.: 0.011 min
Response: 845366
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

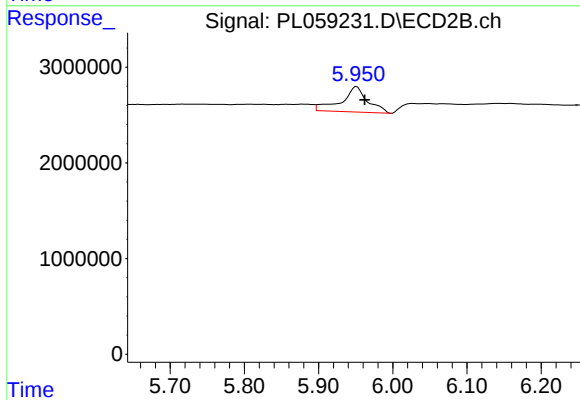


#8 Heptachlor epoxide

R.T.: 5.951 min
Delta R.T.: -0.011 min
Response: 6591154
Conc: 2.38 ng/ml

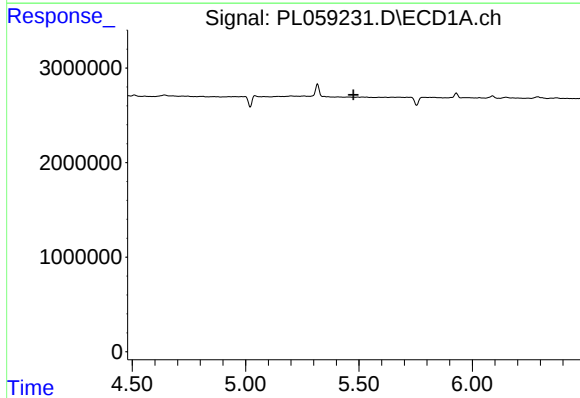


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

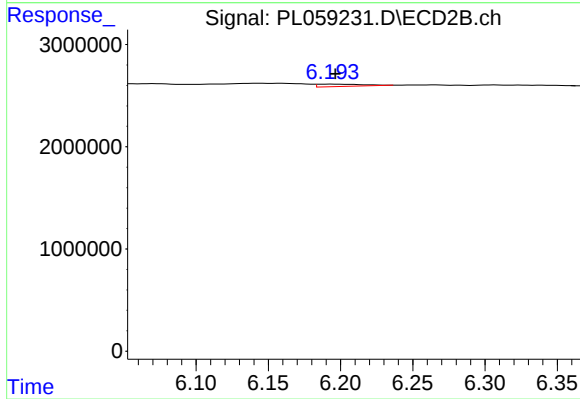

#10 gamma-Chlordane


R.T.: 6.195 min
Delta R.T.: -0.002 min
Response: 512992
Conc: 0.17 ng/ml

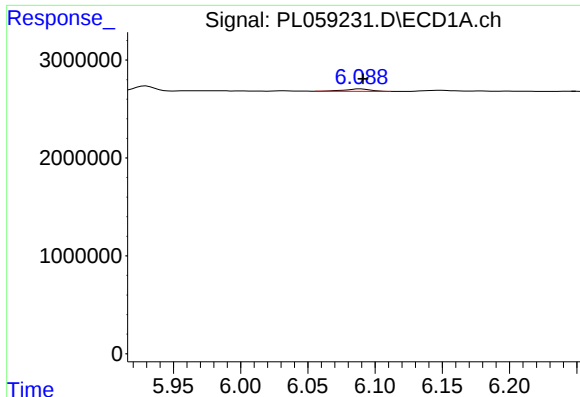

#14 Endrin


R.T.: 6.089 min
Delta R.T.: -0.002 min
Response: 325862
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

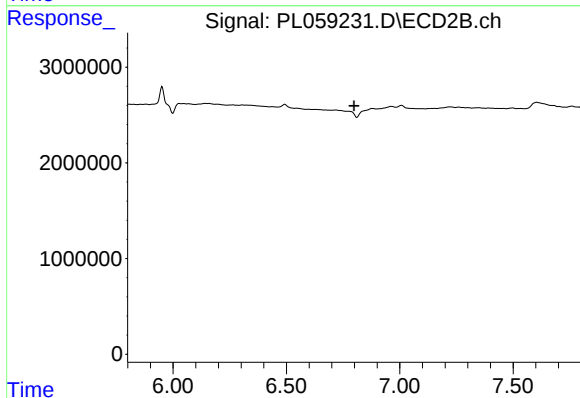


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

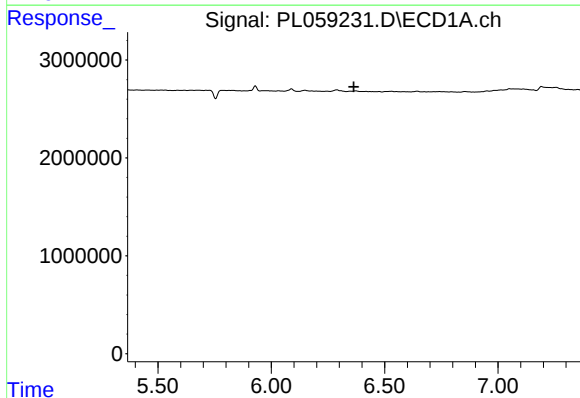


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

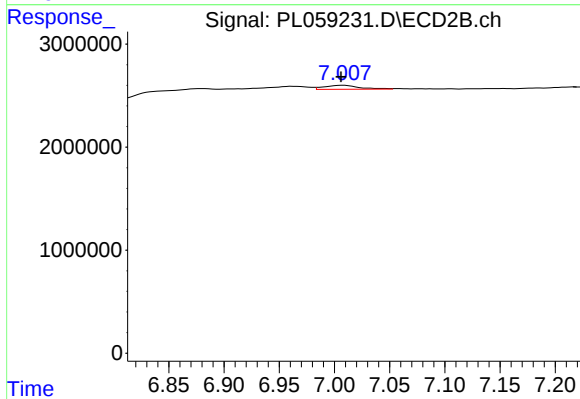

#15 Endosulfan II


R.T.: 7.008 min
Delta R.T.: 0.002 min
Response: 871255
Conc: 0.33 ng/ml

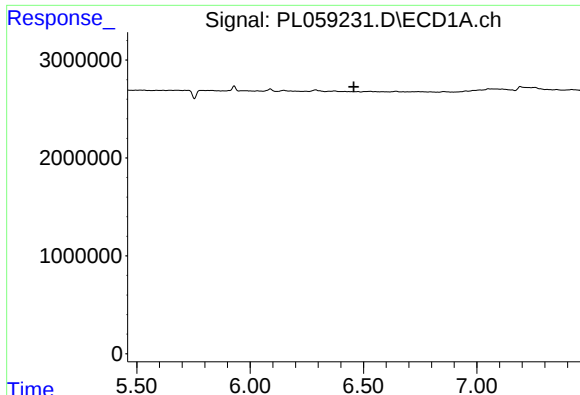

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

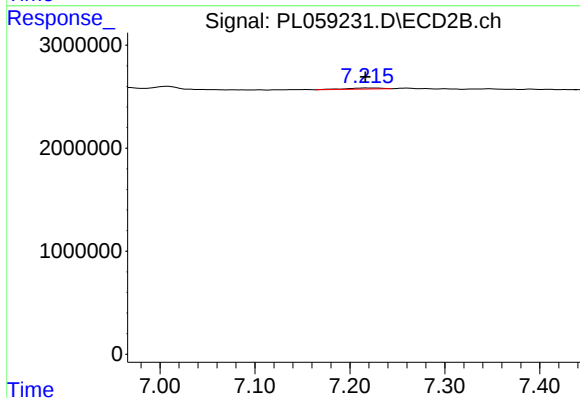


#17 4,4'-DDT

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 271629
Conc: 0.12 ng/ml

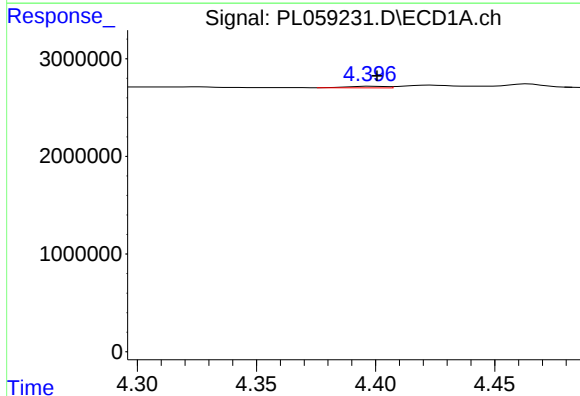


#23 Chlordane-1

R.T.: 4.398 min
Delta R.T.: -0.003 min
Response: 184573
Conc: 3.67 ng/ml

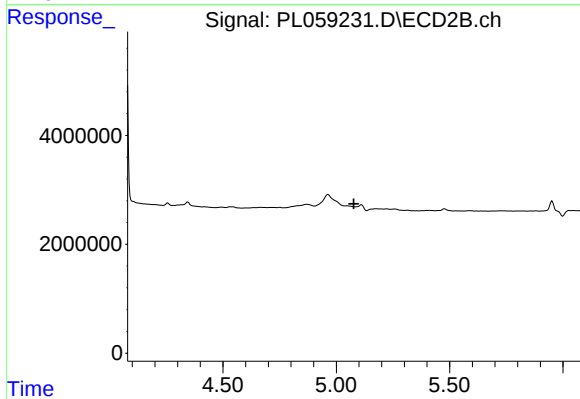

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

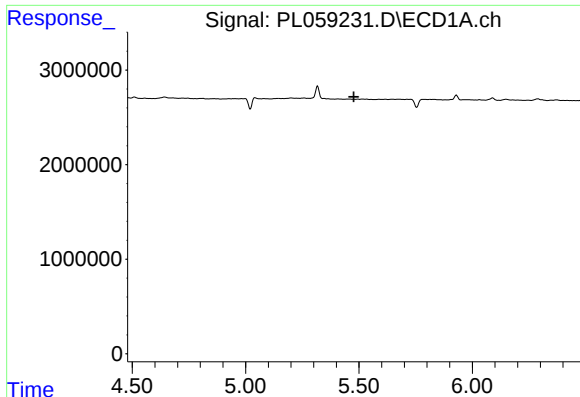

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

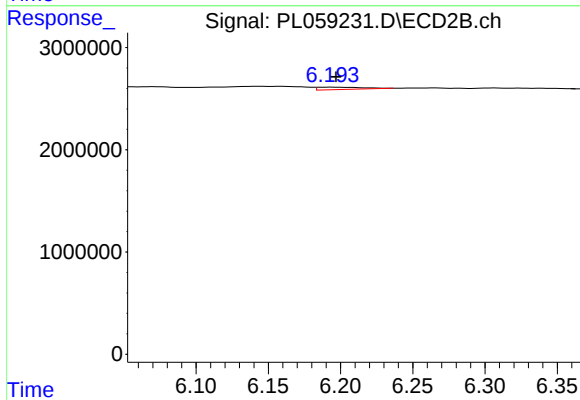


#25 Chlordane-3

R.T.: 6.195 min
Delta R.T.: -0.002 min
Response: 512992
Conc: 1.37 ng/ml

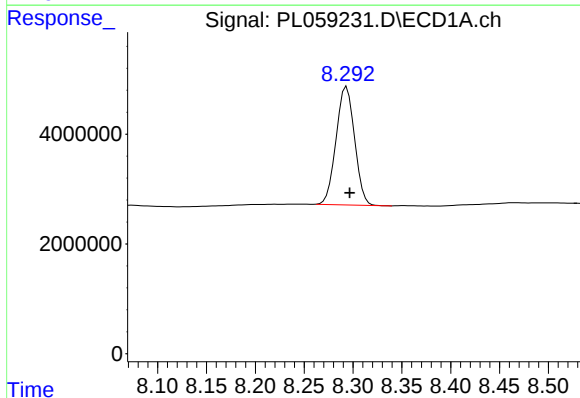

#28 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: -0.003 min
Response: 28411885
Conc: 17.28 ng/ml

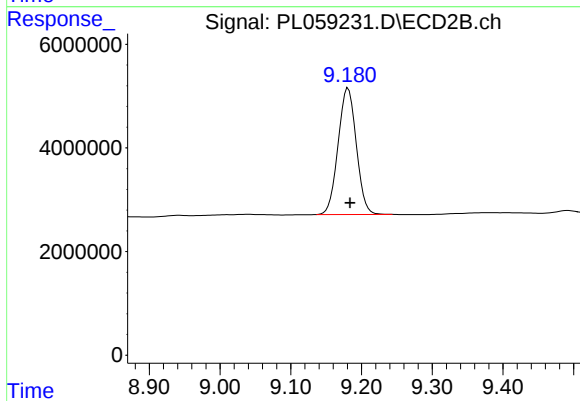

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 43665740
Conc: 18.42 ng/ml