

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 09:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:09:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.482	5.531	10093720	16776898	18.359	17.796
28)	SA Decachlor...	10.223	11.428	13296326	18726499	18.762	18.801
Target Compounds							
2)	A alpha-BHC	5.174	0.000	322176	0	0.438	N.D. #
4)	MA Heptachlor	5.991f	0.000	494110	0	0.655	N.D. #
6)	B beta-BHC	5.991	0.000	494110	0	1.381	N.D. #
7)	B delta-BHC	0.000	6.999f	0	1415183	N.D.	1.204 #
17)	MA 4,4'-DDT	0.000	9.366f	0	764038	N.D.	1.042 #
18)	B Endrin al...	8.379	0.000	254166	0	0.502	N.D. #
21)	B Endrin ke...	9.130	0.000	229059	0	0.301	N.D. #
23)	Chlordane-1	0.000	6.938f	0	632254	N.D.	22.390 #
24)	Chlordane-2	6.489	0.000	258638	0	9.659	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 09:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:09:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

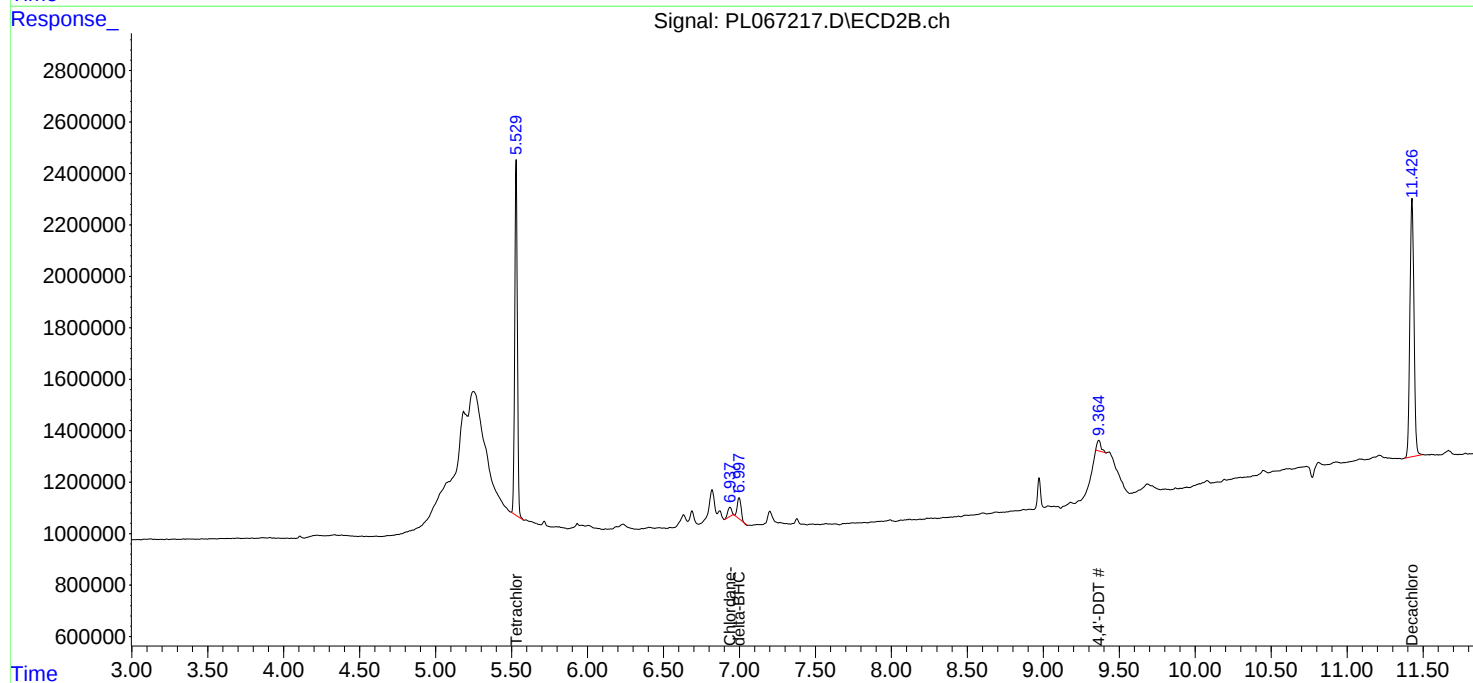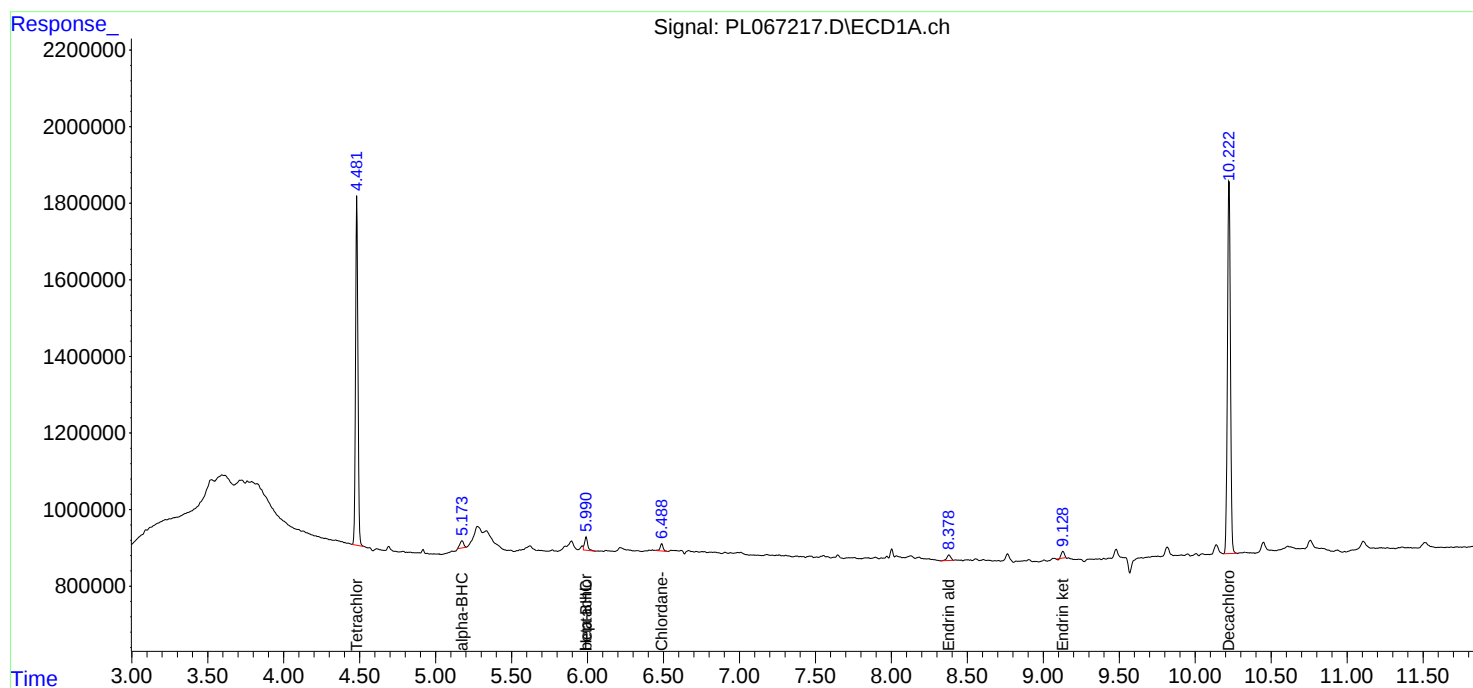


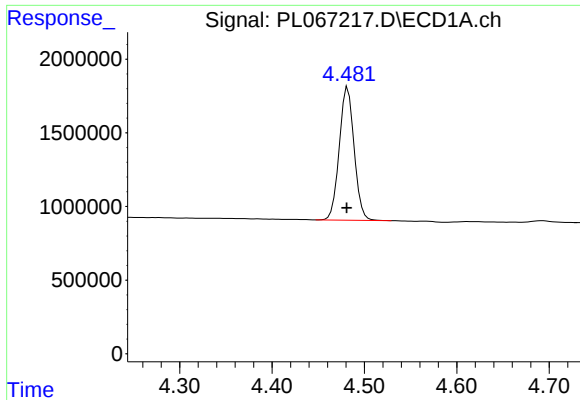

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: 0.001 min
Response: 10093720
Conc: 18.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

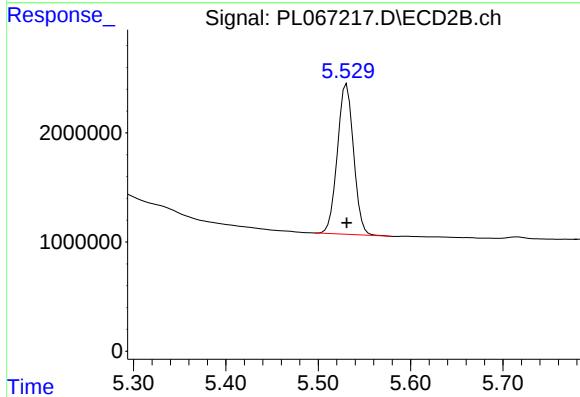


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 16776898
Conc: 17.80 ng/ml

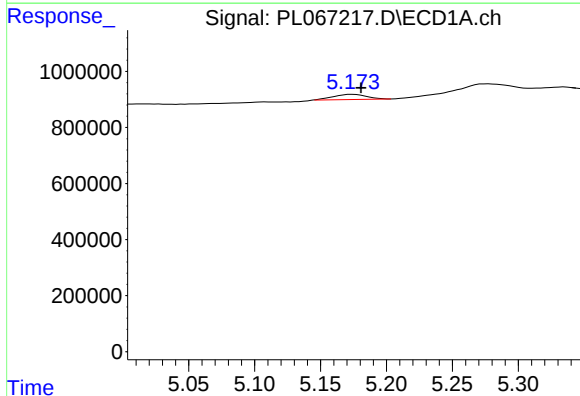


#2 alpha-BHC

R.T.: 5.174 min
Delta R.T.: -0.006 min
Response: 322176
Conc: 0.44 ng/ml

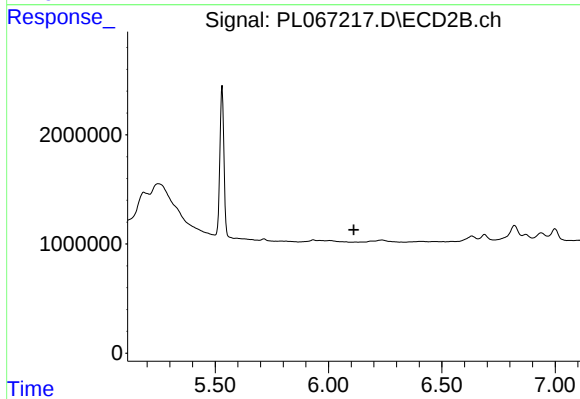

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

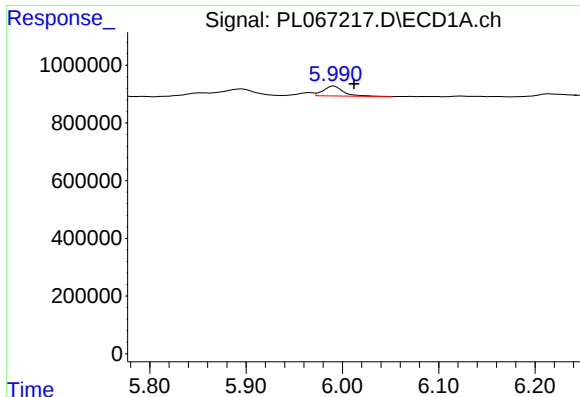

#4 Heptachlor


R.T.: 5.991 min
Delta R.T.: -0.021 min
Response: 494110
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

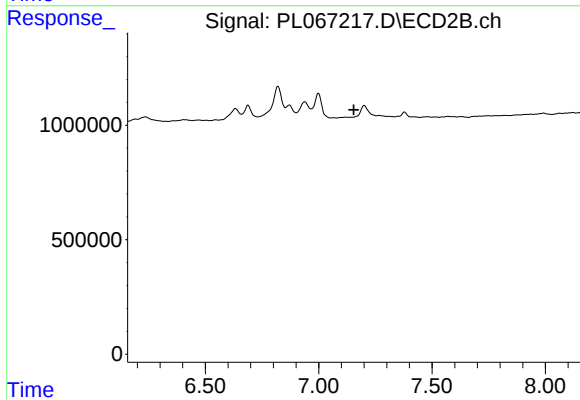


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

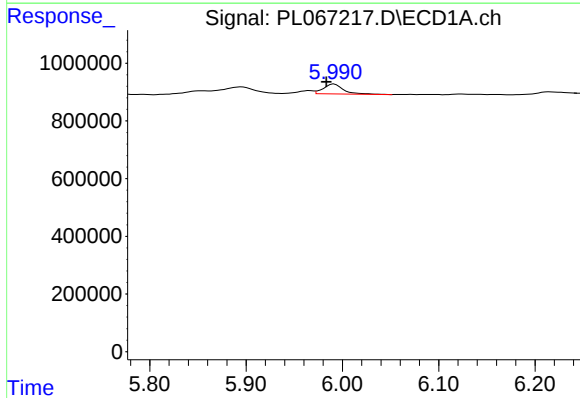


#6 beta-BHC

R.T.: 5.991 min
Delta R.T.: 0.008 min
Response: 494110
Conc: 1.38 ng/ml

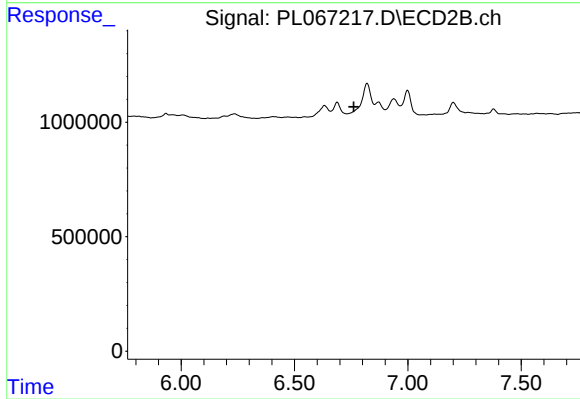

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

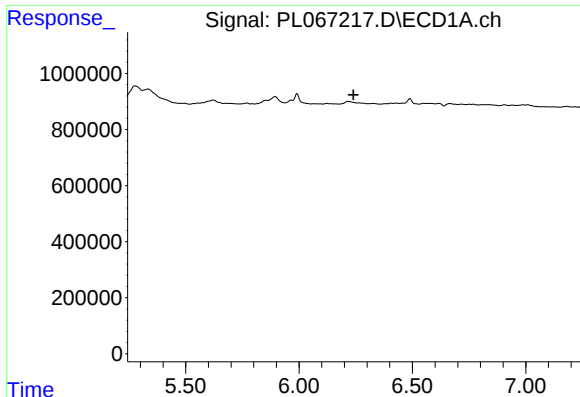

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

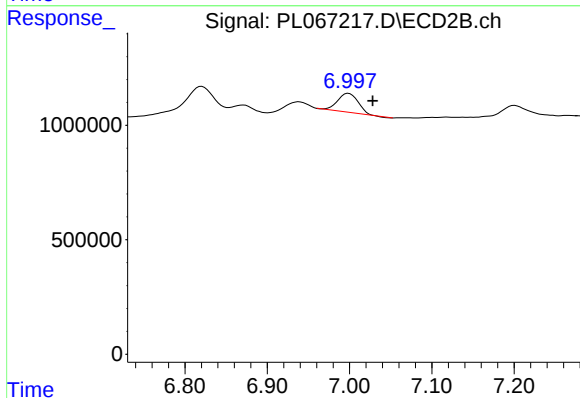


#7 delta-BHC

R.T.: 6.999 min
Delta R.T.: -0.029 min
Response: 1415183
Conc: 1.20 ng/ml

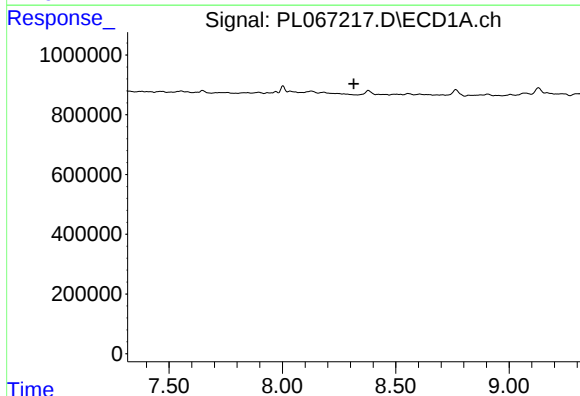


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.314 min
Response: 0
Conc: N.D.

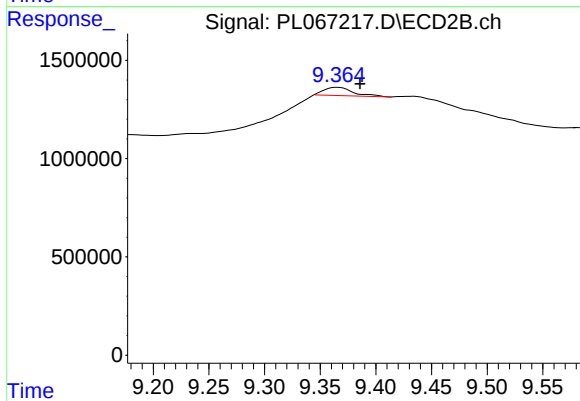

#17 4,4'-DDT


R.T.: 9.366 min
Delta R.T.: -0.020 min
Response: 764038
Conc: 1.04 ng/ml

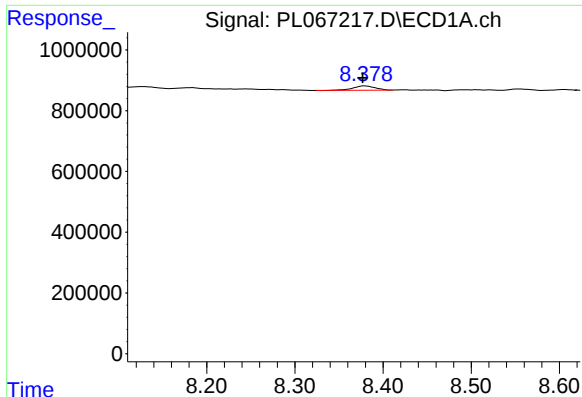

#18 Endrin aldehyde


R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 254166
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

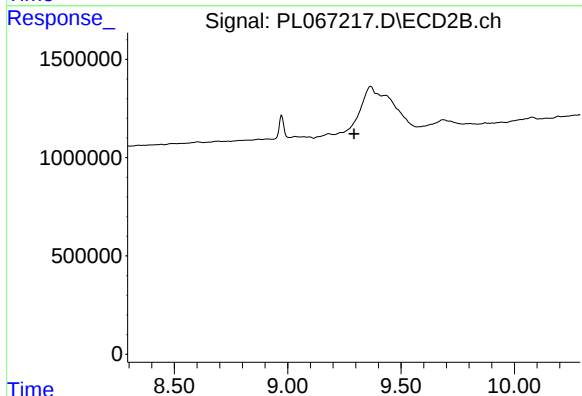


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

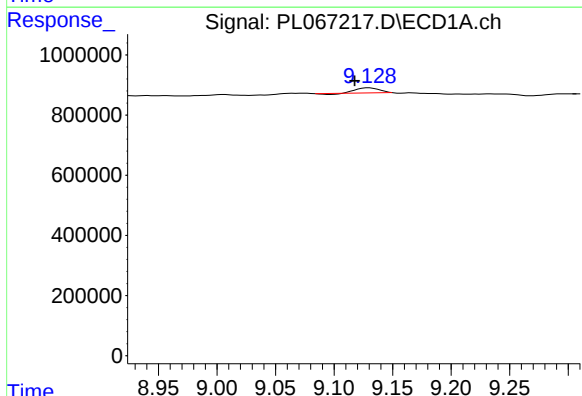


#21 Endrin ketone

R.T.: 9.130 min
Delta R.T.: 0.012 min
Response: 229059
Conc: 0.30 ng/ml

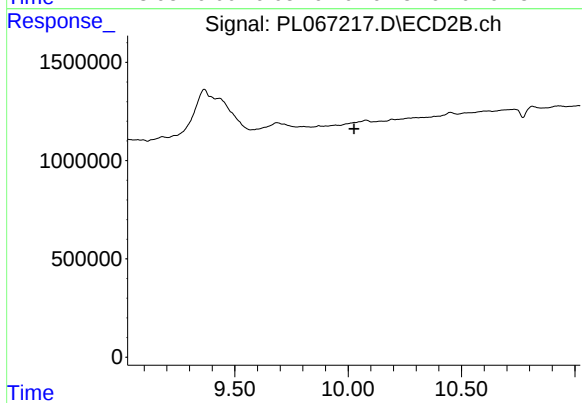

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

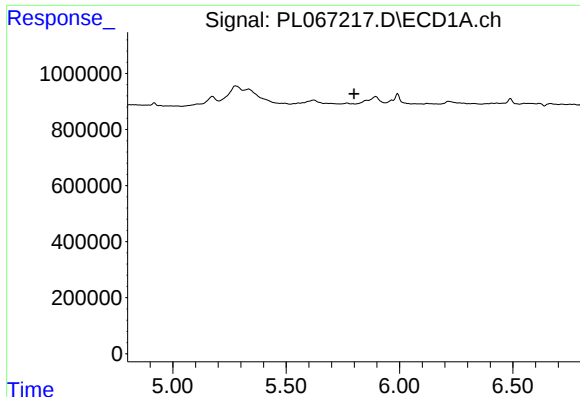

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

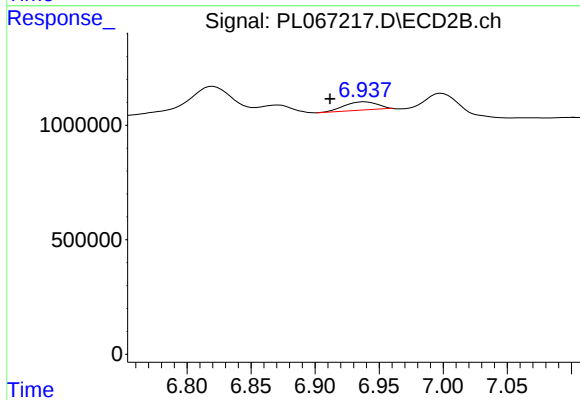


#23 Chlordane-1

R.T.: 6.938 min
Delta R.T.: 0.027 min
Response: 632254
Conc: 22.39 ng/ml

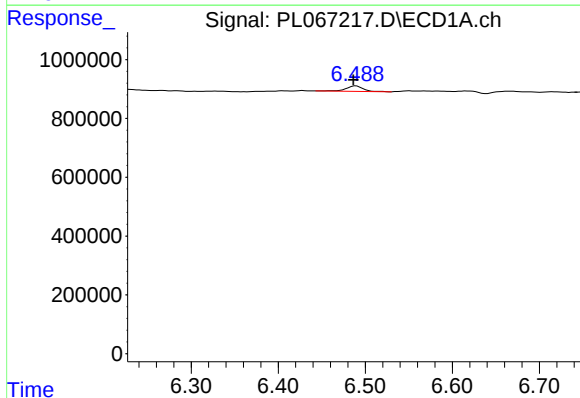


#24 Chlordane-2

R.T.: 6.489 min
Delta R.T.: 0.003 min
Response: 258638
Conc: 9.66 ng/ml

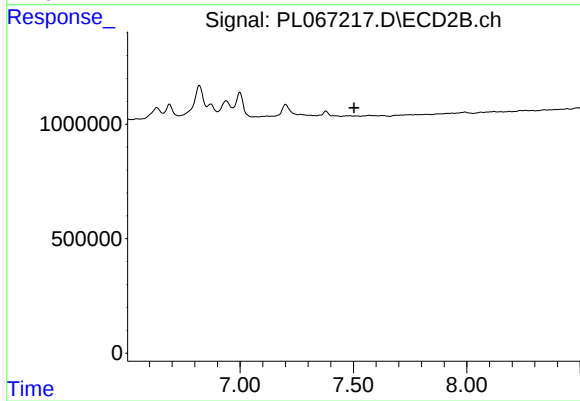

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

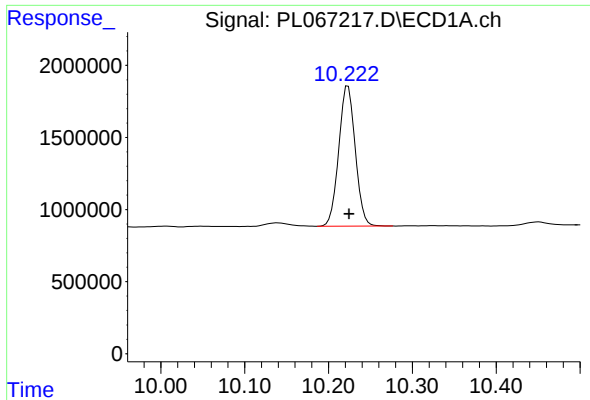

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.001 min
Response: 13296326
Conc: 18.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

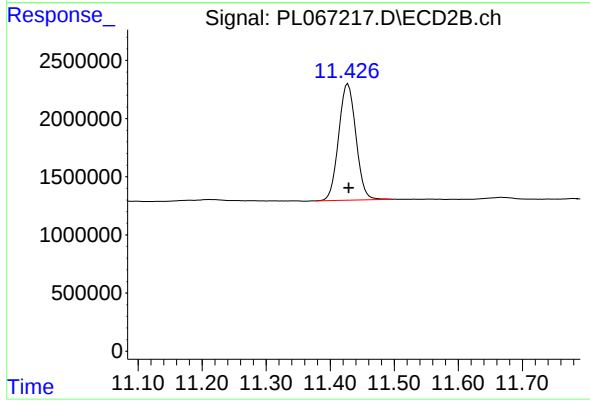

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 18726499
Conc: 18.80 ng/ml