

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 11:24
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:46:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 01:46:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	55544109	96280361	96.442	98.808
28)	SA Decachlor...	10.222	11.427	64049618	91039456	92.688	92.352
Target Compounds							
23)	Chlordane-1	5.799	6.911	18284044	31271422	979.876	1027.831
24)	Chlordane-2	6.485	7.502	24050342	35932688	925.737	950.940
25)	Chlordane-3	7.184	8.259	67685242	141.1E6	993.164	1021.219
26)	Chlordane-4	7.250	8.341	73552544	167.3E6	995.616	1001.651
27)	Chlordane-5	8.190	9.226	21683277	29721433	965.171	983.746



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 11:24
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:46:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 01:46:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

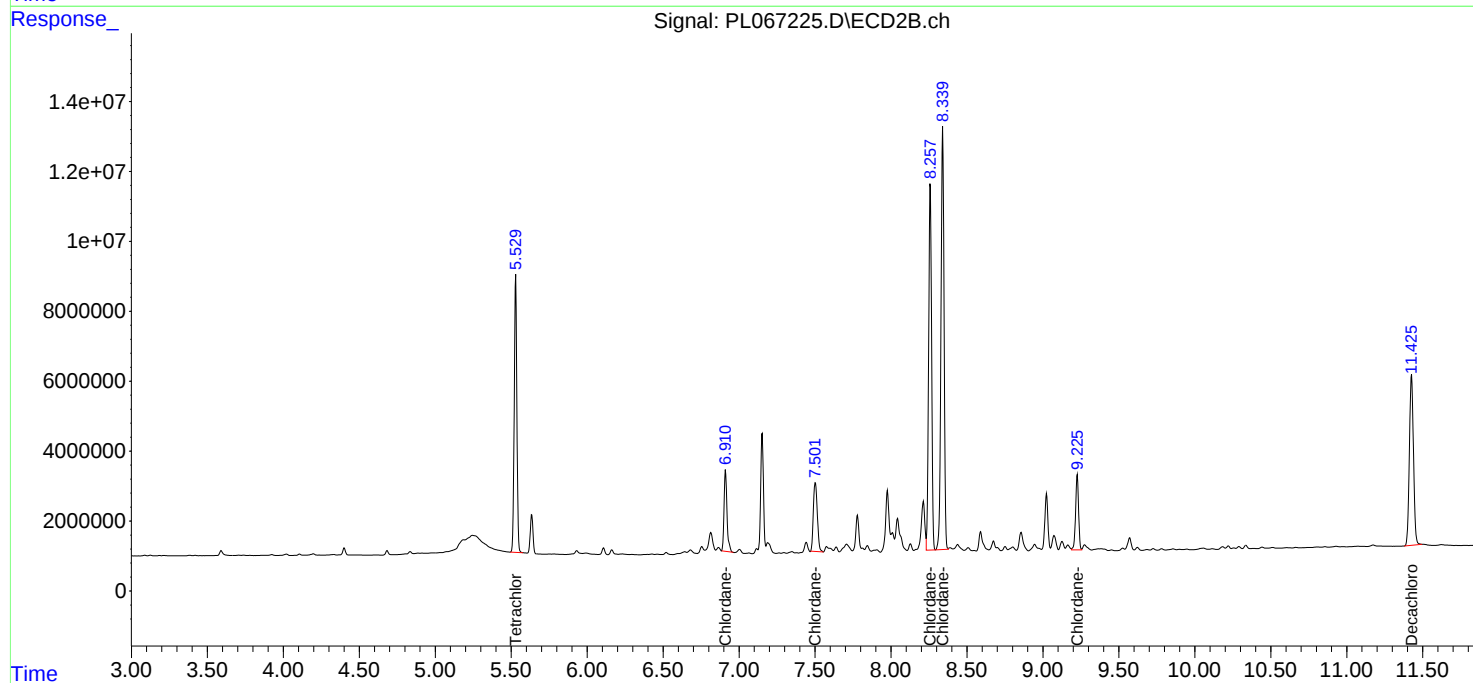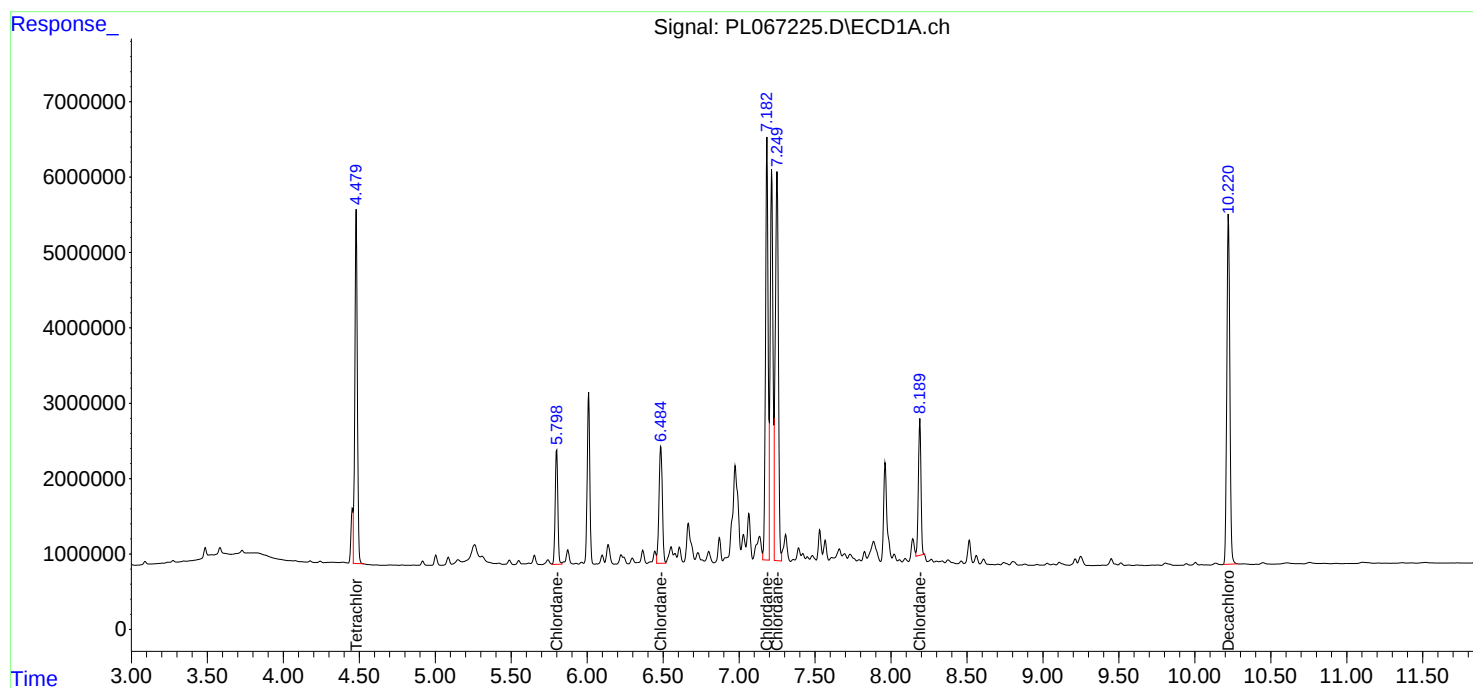


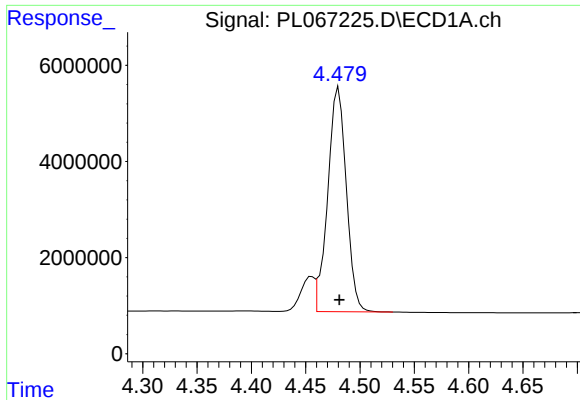

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 55544109
Conc: 96.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

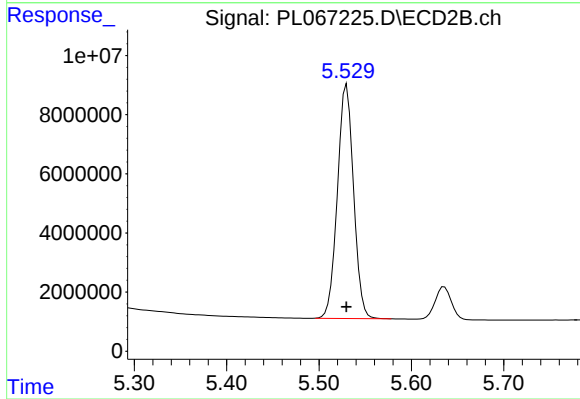


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 96280361
Conc: 98.81 ng/ml

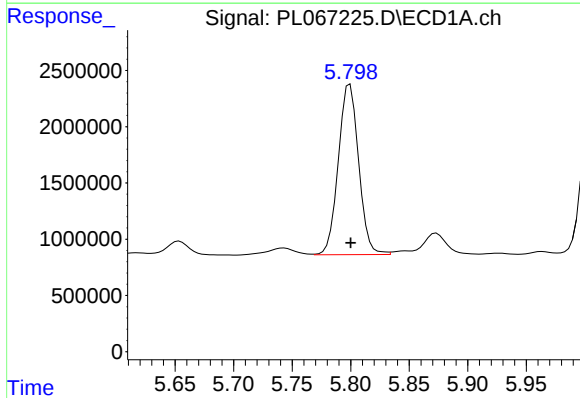


#23 Chlordane-1

R.T.: 5.799 min
Delta R.T.: 0.000 min
Response: 18284044
Conc: 979.88 ng/ml

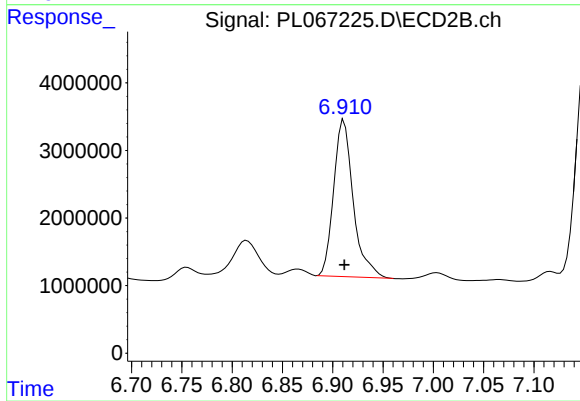

#23 Chlordane-1


R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 31271422
Conc: 1027.83 ng/ml

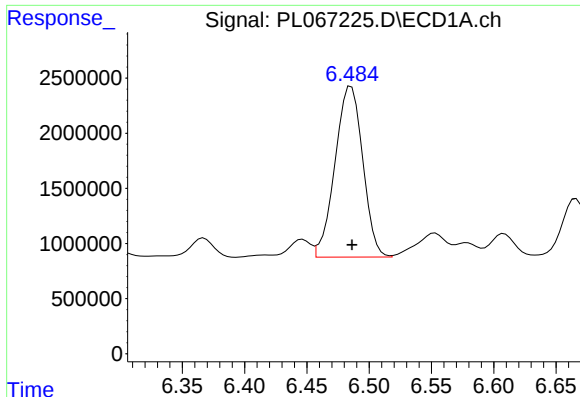

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 24050342
Conc: 925.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

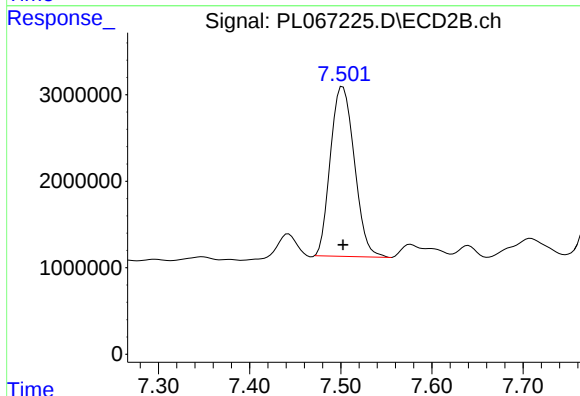


#24 Chlordane-2

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 35932688
Conc: 950.94 ng/ml

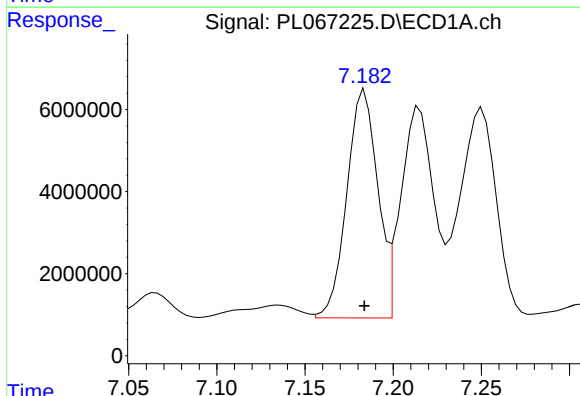


#25 Chlordane-3

R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 67685242
Conc: 993.16 ng/ml

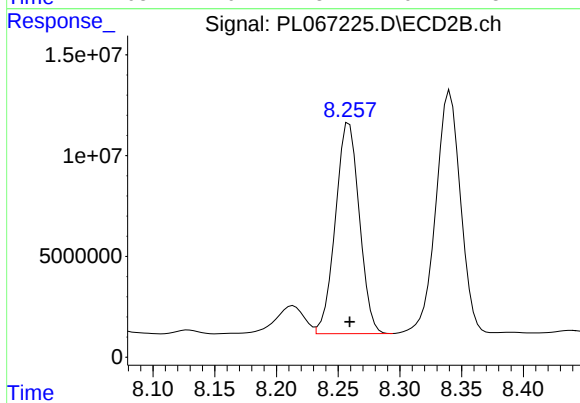

#25 Chlordane-3


R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 141067795
Conc: 1021.22 ng/ml

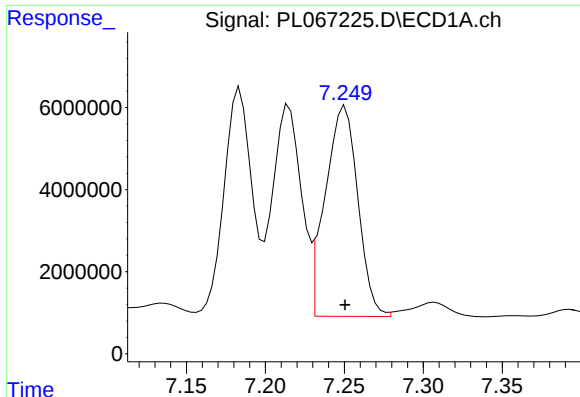

#26 Chlordane-4


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 73552544
Conc: 995.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

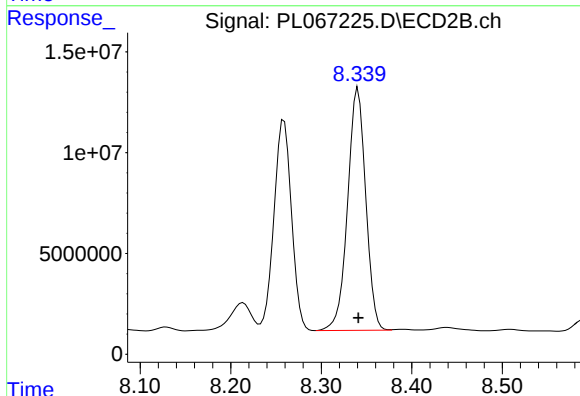


#26 Chlordane-4

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 167280264
Conc: 1001.65 ng/ml

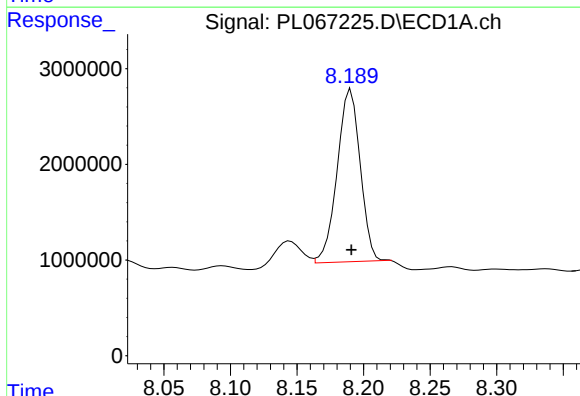


#27 Chlordane-5

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 21683277
Conc: 965.17 ng/ml

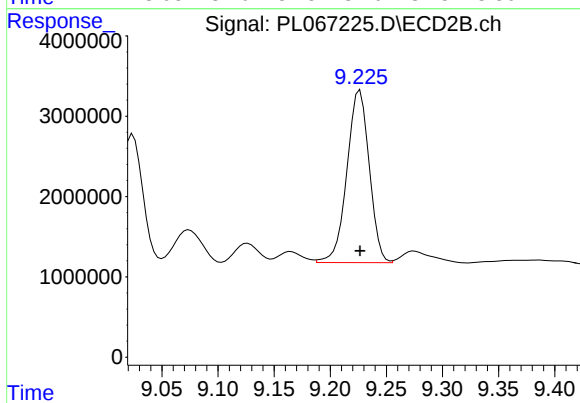

#27 Chlordane-5


R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 29721433
Conc: 983.75 ng/ml

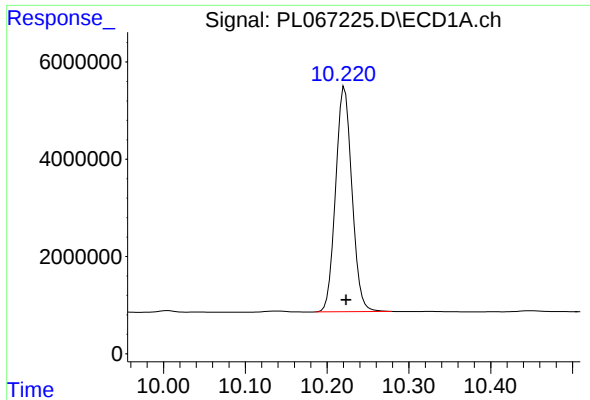

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.001 min
Response: 64049618
Conc: 92.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

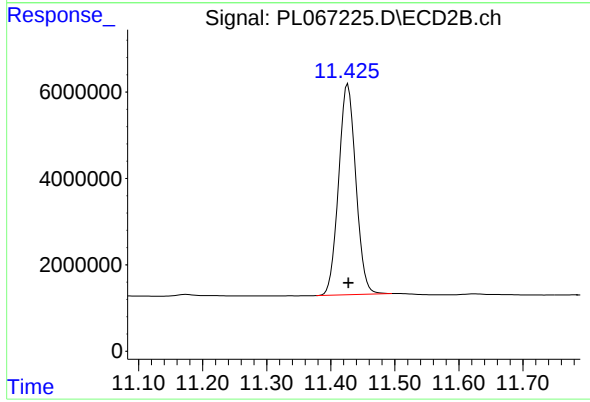

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: 0.000 min
Response: 91039456
Conc: 92.35 ng/ml