

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 11:40
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:46:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 01:46:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	42714386	73382690	74.166	75.309
28)	SA Decachlor...	10.222	11.428	49764273	70959467	72.016	71.982
Target Compounds							
23)	Chlordane-1	5.800	6.912	14036199	23763707	752.226	781.067
24)	Chlordane-2	6.486	7.503	18824150	27944954	724.572	739.549
25)	Chlordane-3	7.184	8.259	51239327	105.7E6	751.848	765.285
26)	Chlordane-4	7.251	8.342	55535271	126.3E6	751.732	756.369
27)	Chlordane-5	8.190	9.228	16735606	22545225	744.939	746.221



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 11:40
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:46:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 01:46:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

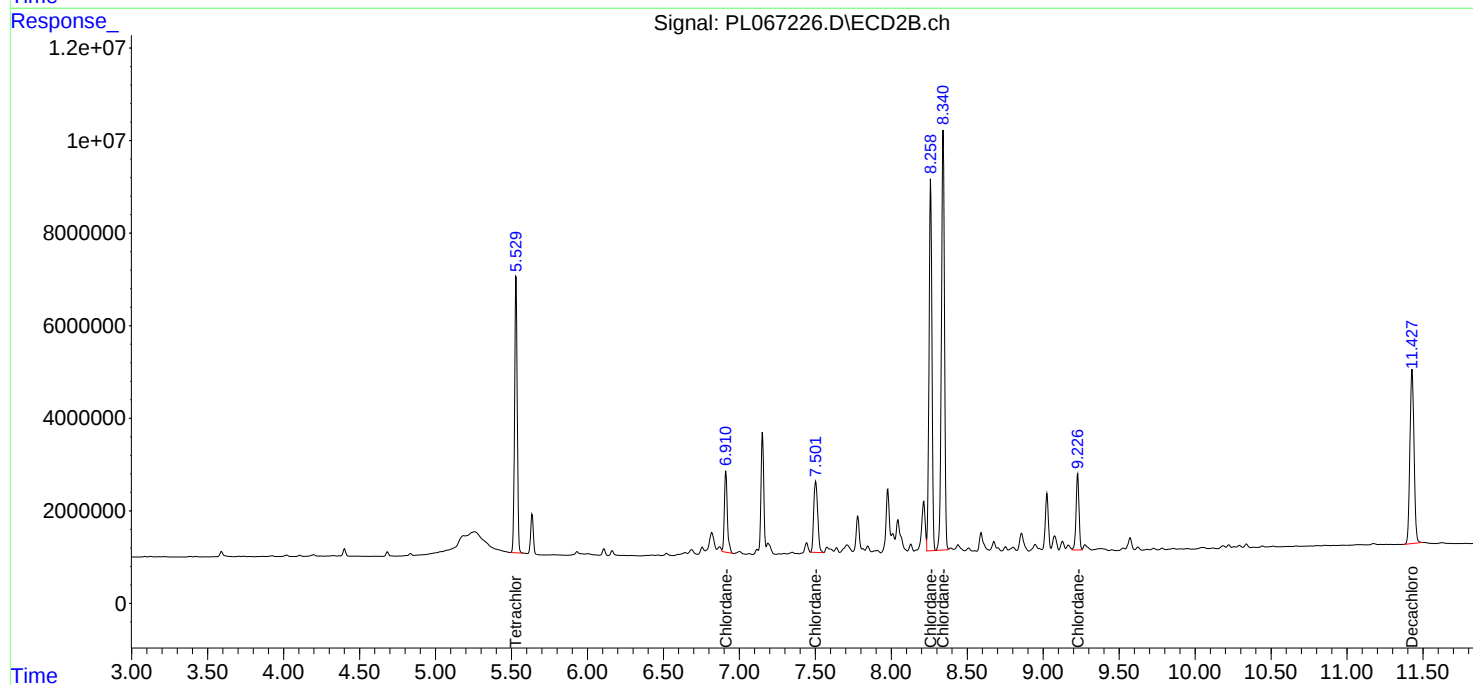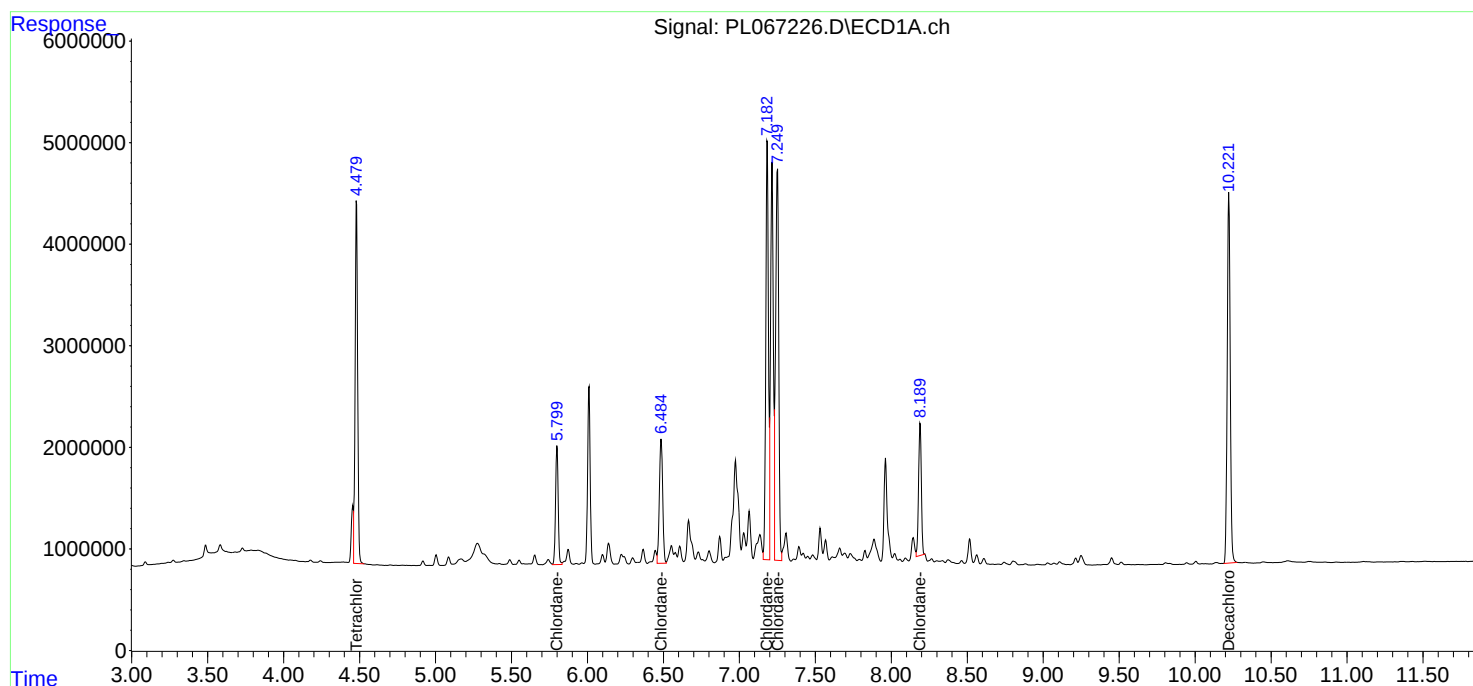


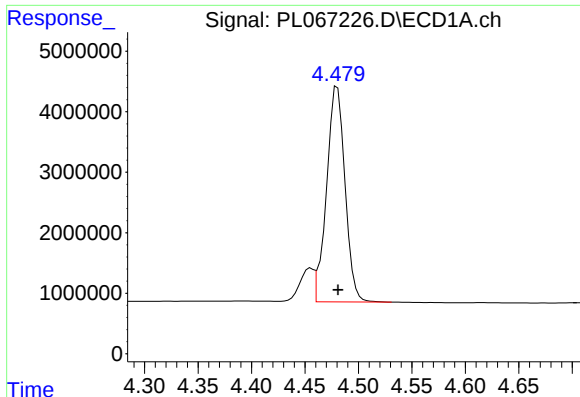

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 42714386
Conc: 74.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

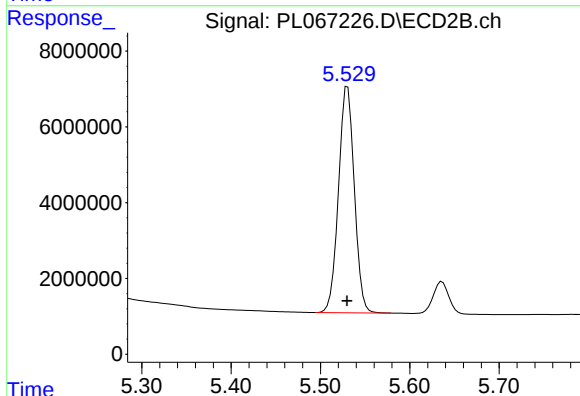


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 73382690
Conc: 75.31 ng/ml

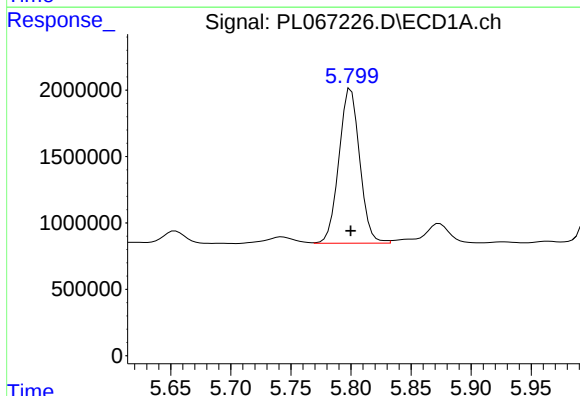


#23 Chlordane-1

R.T.: 5.800 min
Delta R.T.: 0.000 min
Response: 14036199
Conc: 752.23 ng/ml

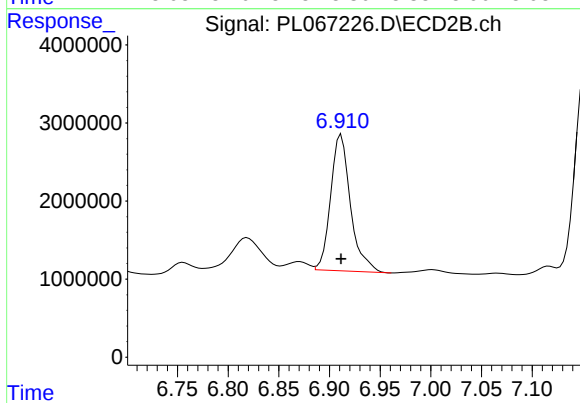

#23 Chlordane-1


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 23763707
Conc: 781.07 ng/ml

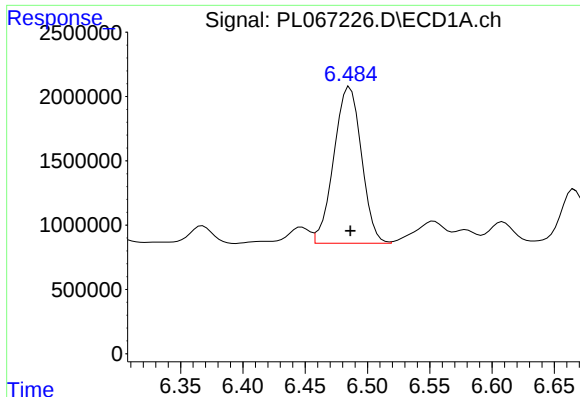

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 18824150
Conc: 724.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

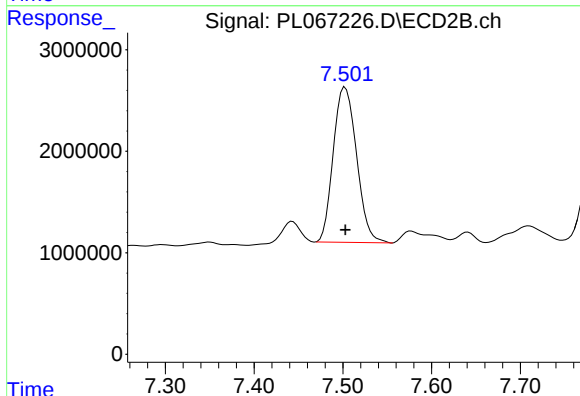


#24 Chlordane-2

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 27944954
Conc: 739.55 ng/ml

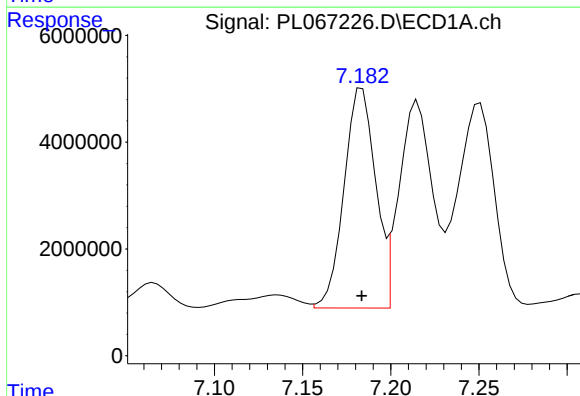


#25 Chlordane-3

R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 51239327
Conc: 751.85 ng/ml

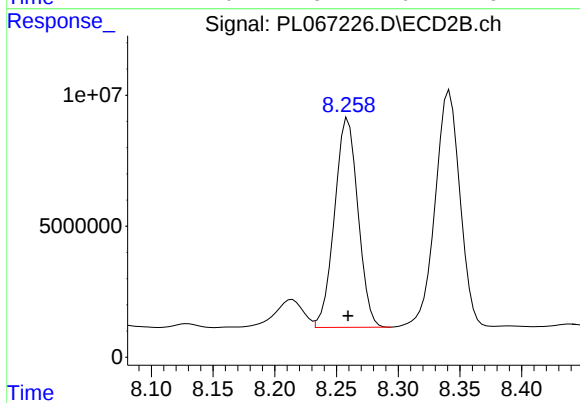

#25 Chlordane-3


R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 105713955
Conc: 765.29 ng/ml

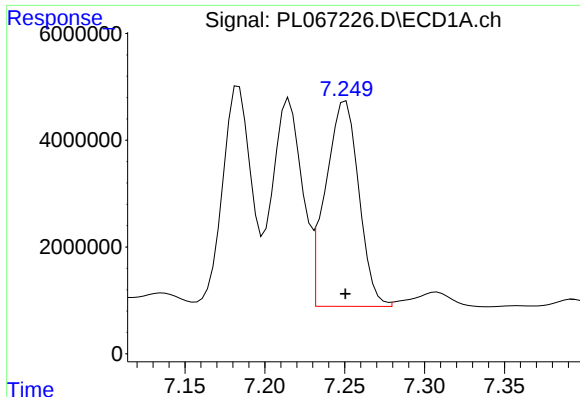

#26 Chlordane-4


R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 55535271
Conc: 751.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

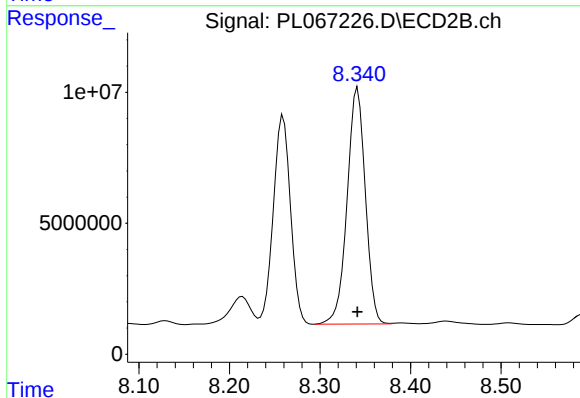


#26 Chlordane-4

R.T.: 8.342 min
Delta R.T.: 0.000 min
Response: 126317118
Conc: 756.37 ng/ml

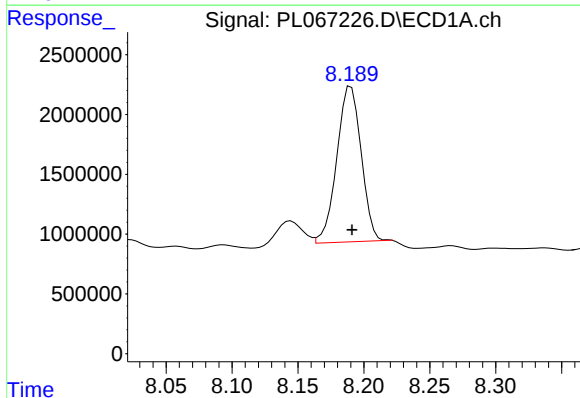


#27 Chlordane-5

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 16735606
Conc: 744.94 ng/ml

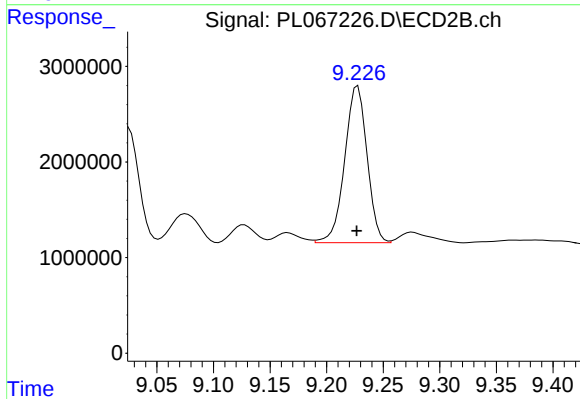

#27 Chlordane-5


R.T.: 9.228 min
Delta R.T.: 0.001 min
Response: 22545225
Conc: 746.22 ng/ml

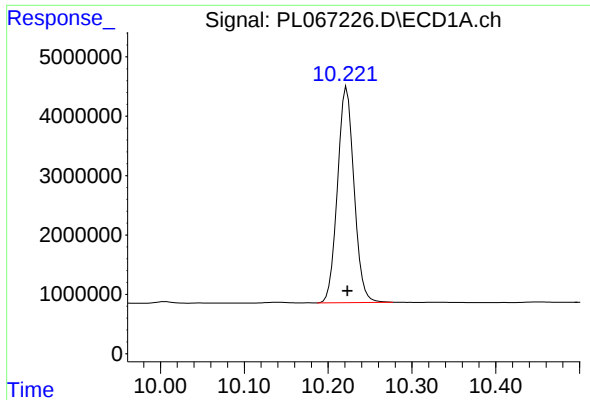

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: 0.000 min
Response: 49764273
Conc: 72.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

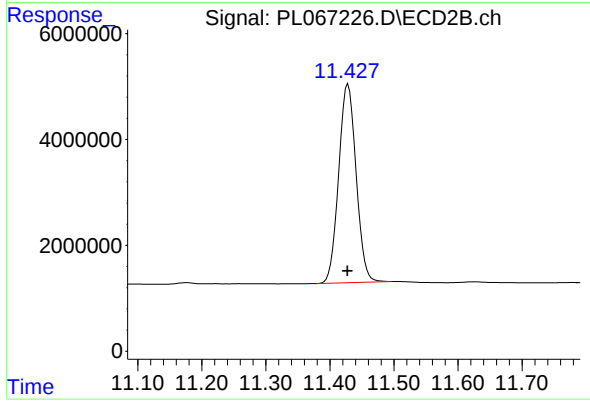

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 70959467
Conc: 71.98 ng/ml