

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 11:57
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 01:46:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.530	28796533	48720888	50.000	50.000
28)	SA Decachlor...	10.223	11.428	34551058	49289502	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.800	6.912	9329777	15212333	500.000	500.000
24)	Chlordane-2	6.486	7.503	12989836	18893251	500.000	500.000
25)	Chlordane-3	7.184	8.259	34075577	69068331	500.000	500.000
26)	Chlordane-4	7.250	8.341	36938215	83502288	500.000	500.000
27)	Chlordane-5	8.191	9.227	11232864	15106256	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 11:57
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 01:46:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

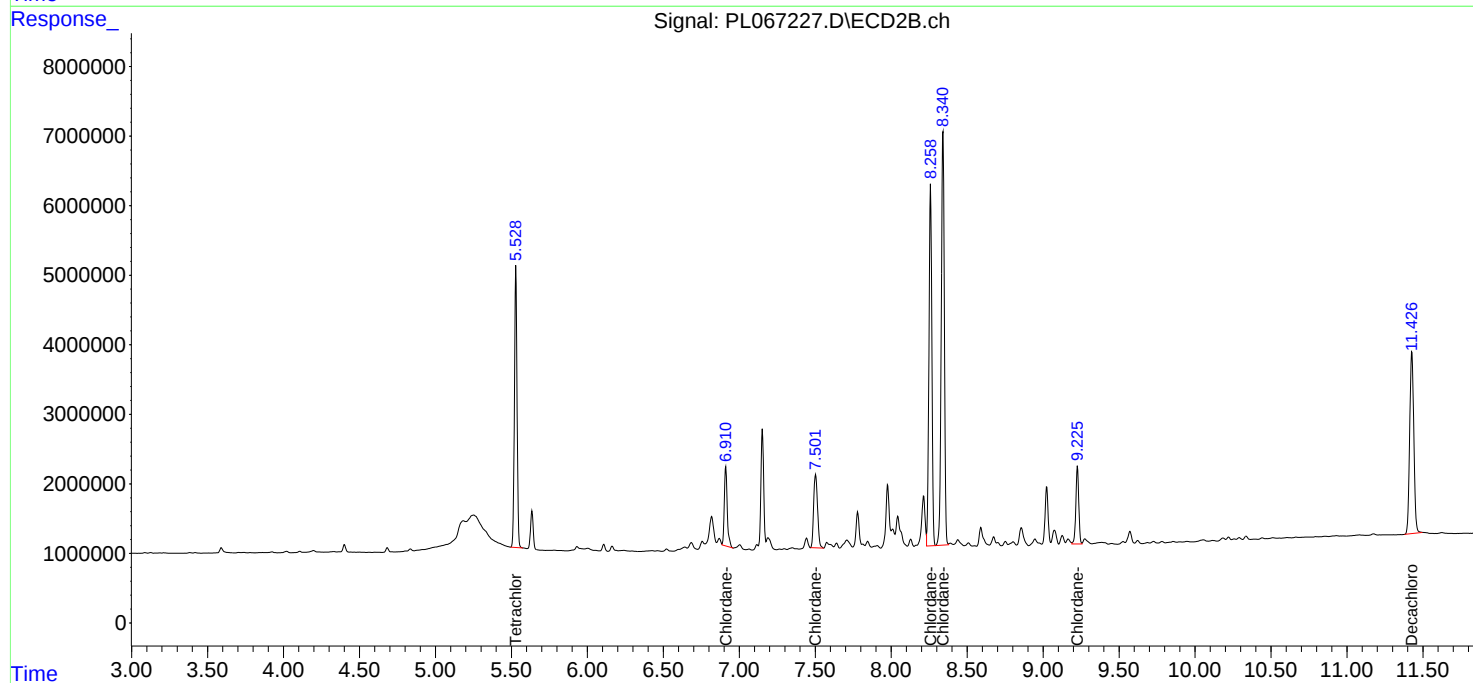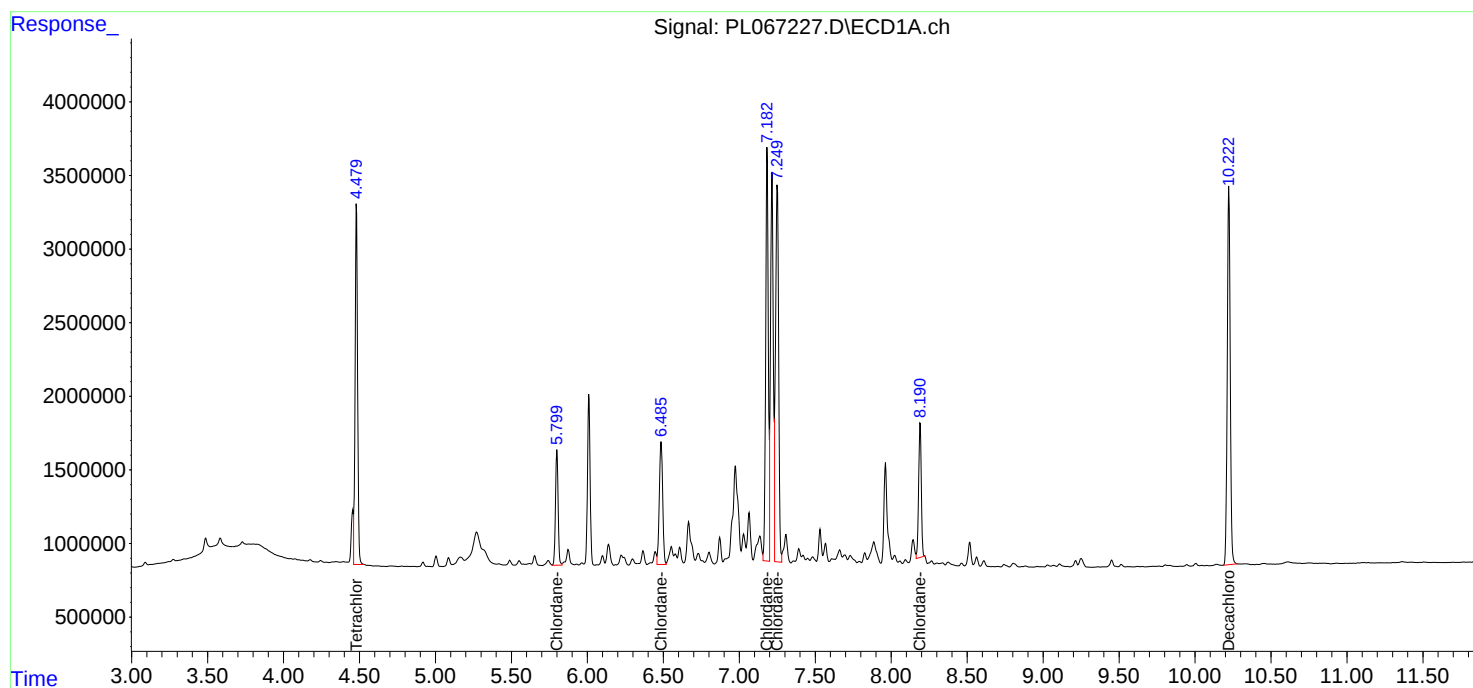


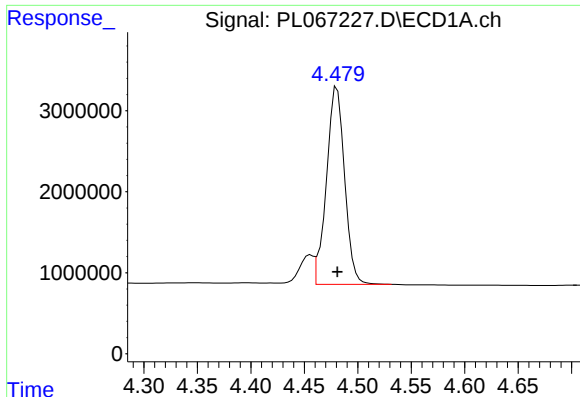

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 28796533
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

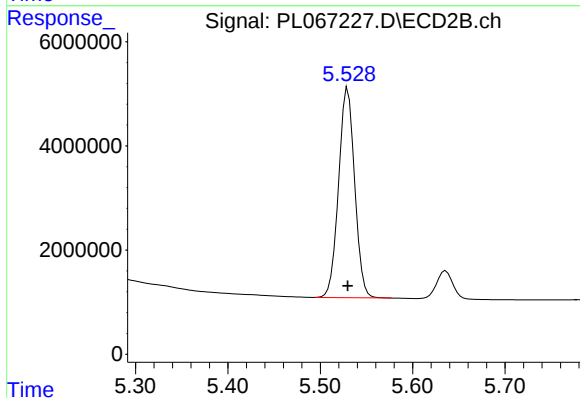


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 48720888
Conc: 50.00 ng/ml

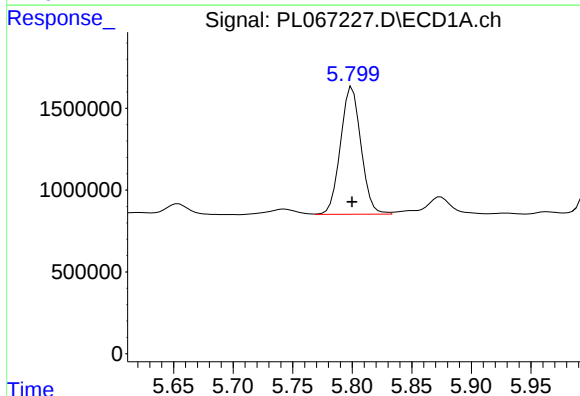


#23 Chlordane-1

R.T.: 5.800 min
Delta R.T.: 0.000 min
Response: 9329777
Conc: 500.00 ng/ml

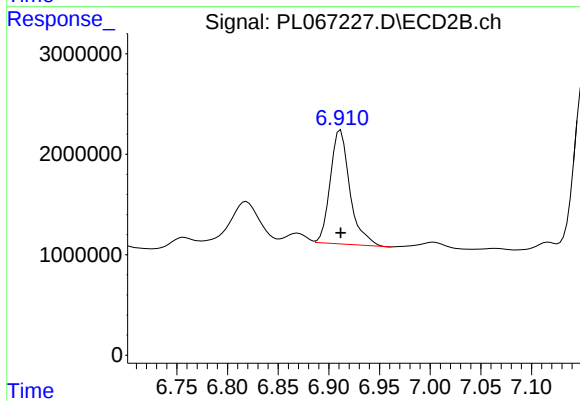

#23 Chlordane-1


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 15212333
Conc: 500.00 ng/ml

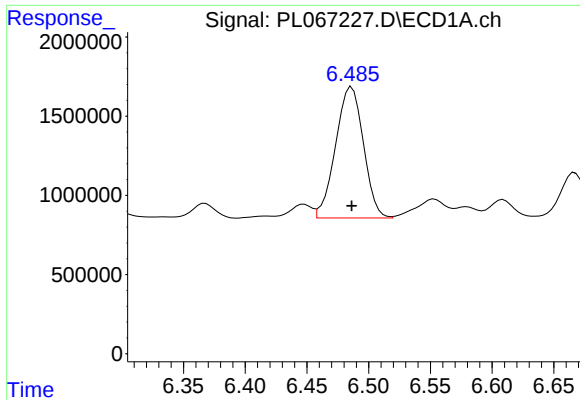

#24 Chlordane-2


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 12989836
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

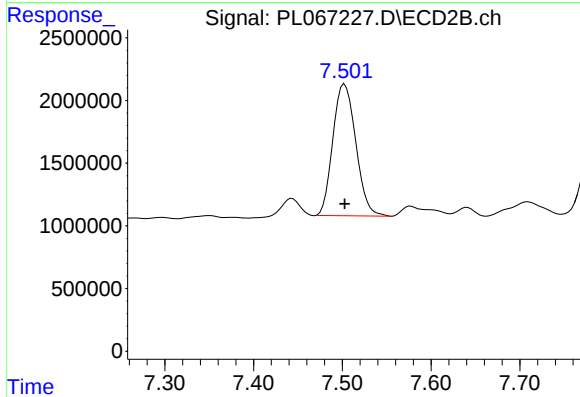


#24 Chlordane-2

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 18893251
Conc: 500.00 ng/ml

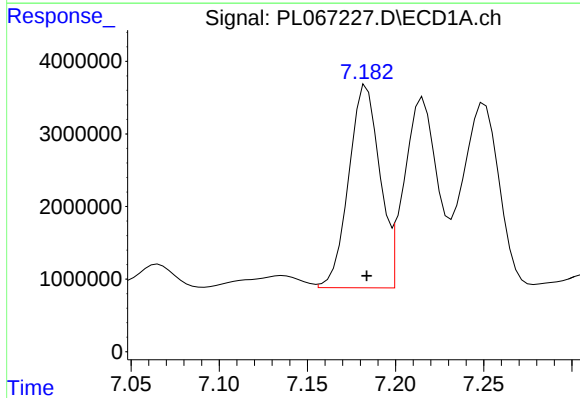


#25 Chlordane-3

R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 34075577
Conc: 500.00 ng/ml

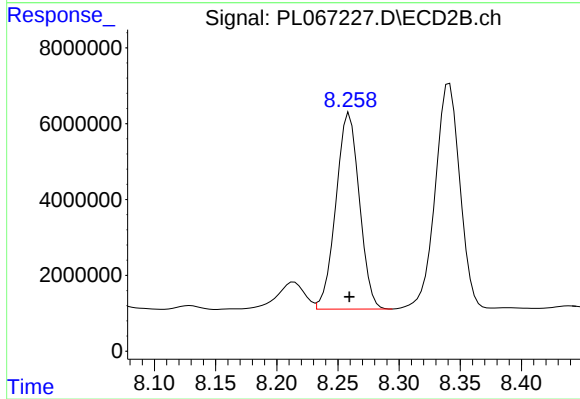

#25 Chlordane-3


R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 69068331
Conc: 500.00 ng/ml

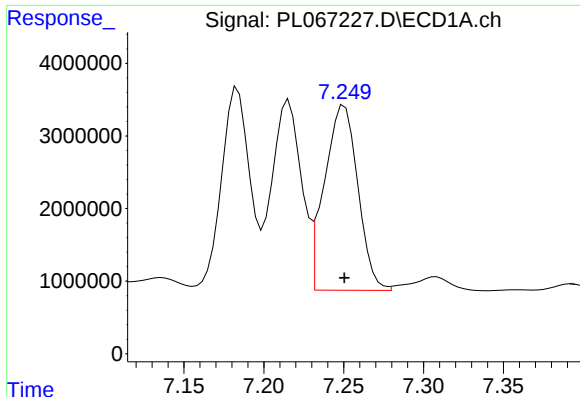

#26 Chlordane-4


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 36938215
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

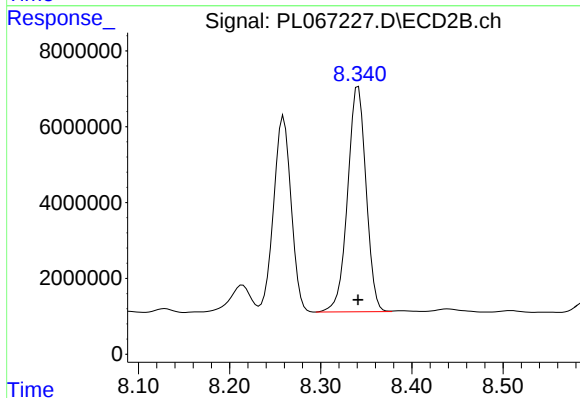


#26 Chlordane-4

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 83502288
Conc: 500.00 ng/ml

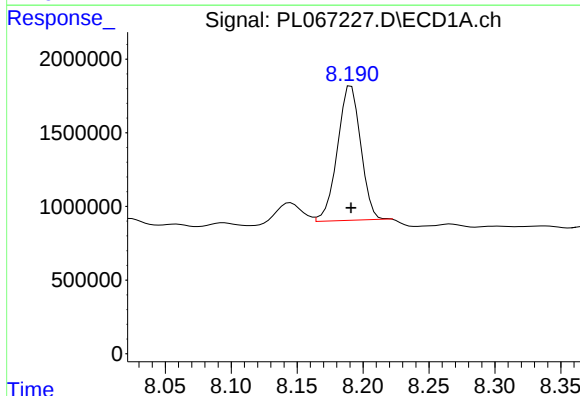


#27 Chlordane-5

R.T.: 8.191 min
Delta R.T.: 0.000 min
Response: 11232864
Conc: 500.00 ng/ml

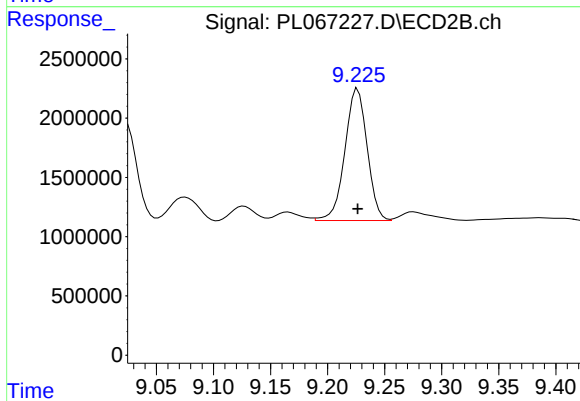

#27 Chlordane-5


R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 15106256
Conc: 500.00 ng/ml

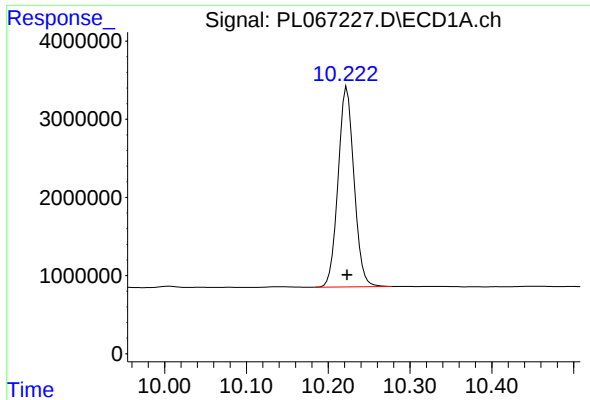

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: 0.000 min
Response: 34551058
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

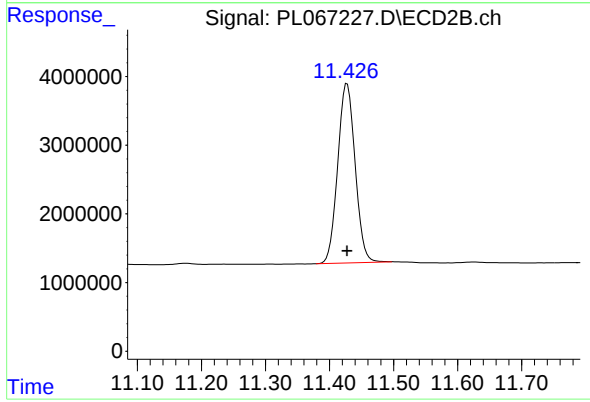

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 49289502
Conc: 50.00 ng/ml