

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 14:51
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL061021CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:55:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 01:54:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	28380965	46536408	50.299	49.384
28)	SA Decachlor...	10.222	11.427	34145371	48555789	48.780	49.277
Target Compounds							
23)	Chlordane-1	5.800	6.911	9433098	15449591	509.845	547.120
24)	Chlordane-2	6.485	7.502	12975682	18003616	484.561	493.978
25)	Chlordane-3	7.184	8.259	33822347	65981766	503.379	492.997
26)	Chlordane-4	7.250	8.341	36820612	79862791	503.849	492.675
27)	Chlordane-5	8.190	9.227	11193272	14611798	511.597	502.509



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 14:51
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL061021CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:55:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 01:54:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

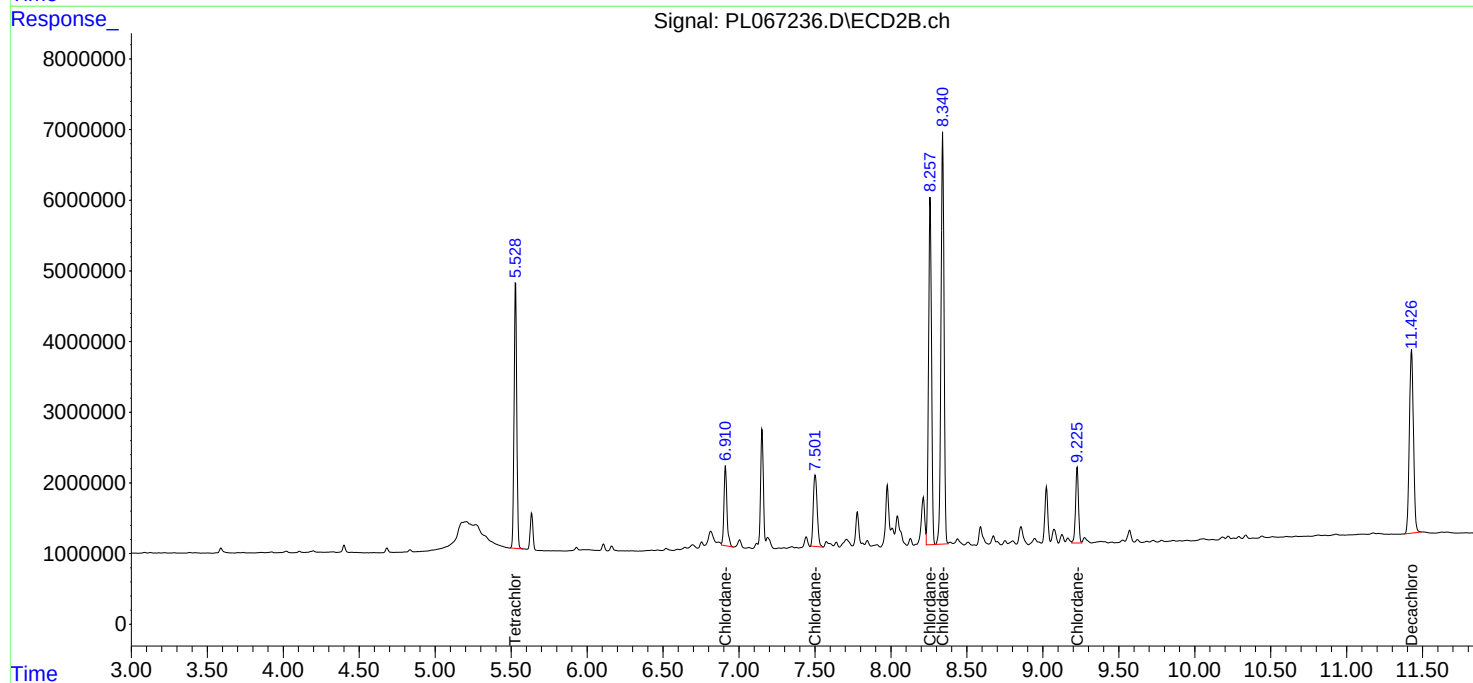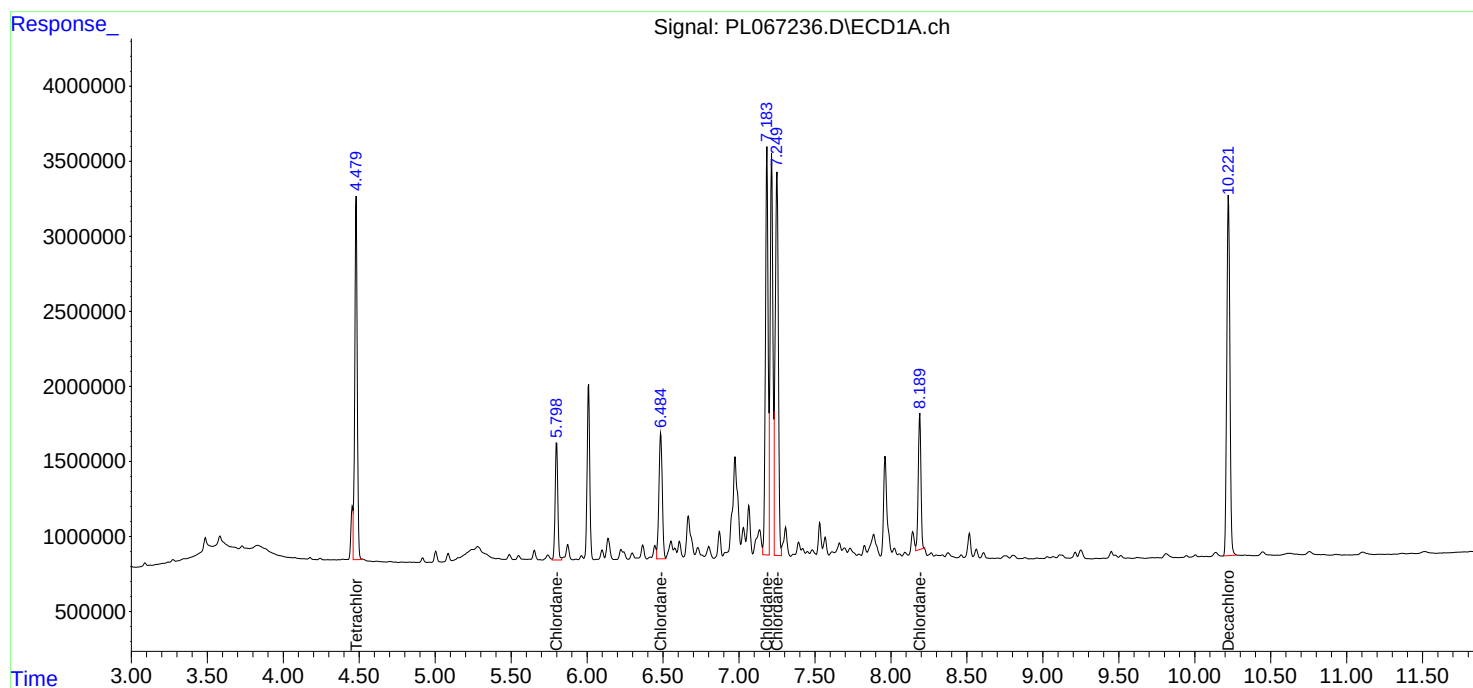


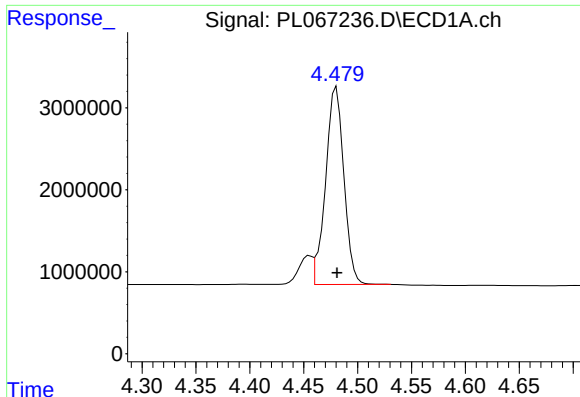

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 28380965
Conc: 50.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061021CHLOR

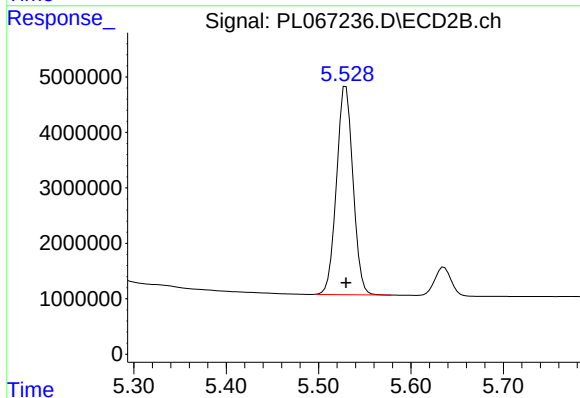


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 46536408
Conc: 49.38 ng/ml

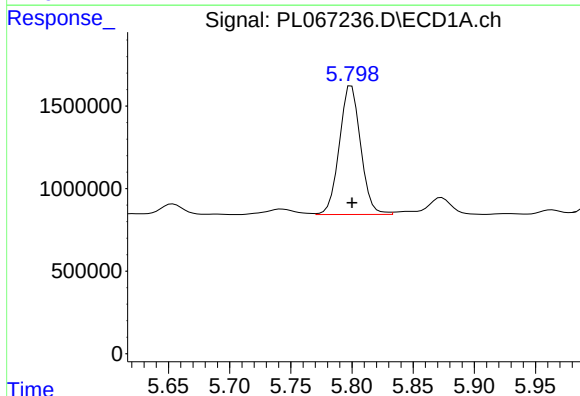


#23 Chlordane-1

R.T.: 5.800 min
Delta R.T.: 0.000 min
Response: 9433098
Conc: 509.85 ng/ml

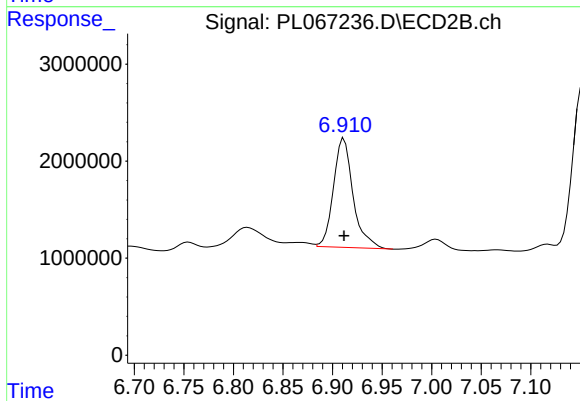

#23 Chlordane-1


R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 15449591
Conc: 547.12 ng/ml

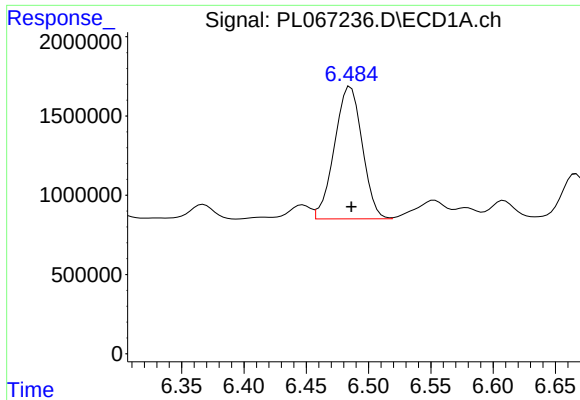

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 12975682
Conc: 484.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061021CHLOR

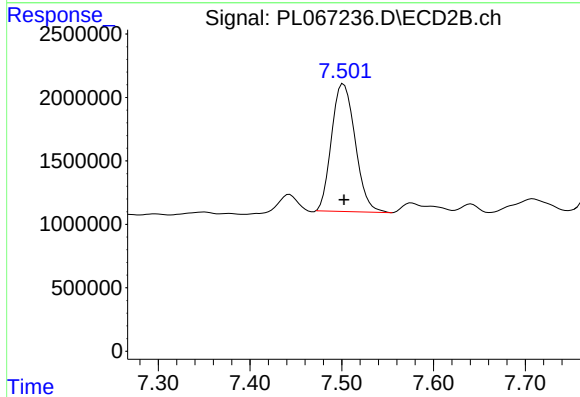


#24 Chlordane-2

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 18003616
Conc: 493.98 ng/ml

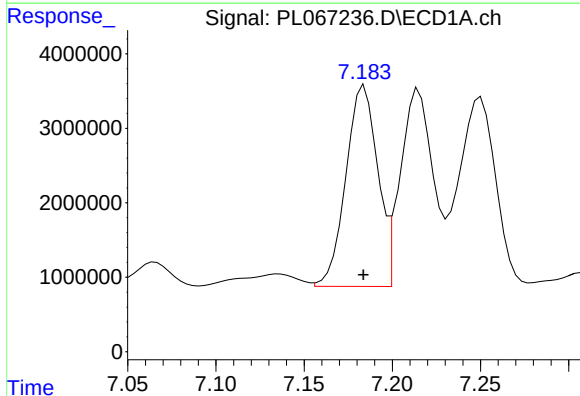


#25 Chlordane-3

R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 33822347
Conc: 503.38 ng/ml

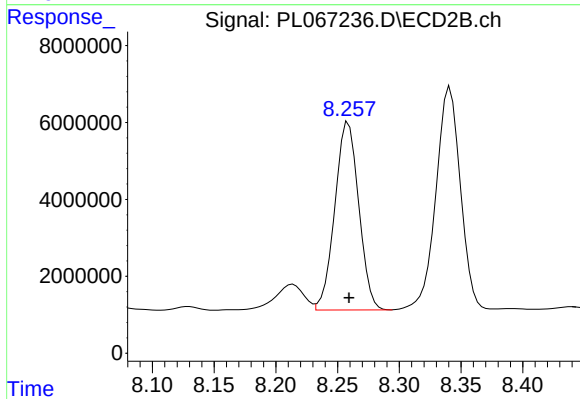

#25 Chlordane-3


R.T.: 8.259 min
Delta R.T.: 0.000 min
Response: 65981766
Conc: 493.00 ng/ml

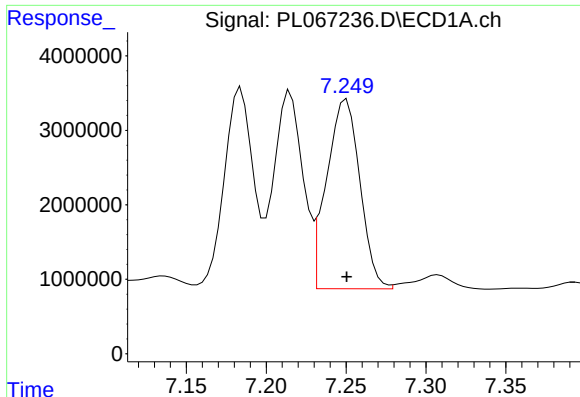

#26 Chlordane-4


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 36820612
Conc: 503.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061021CHLOR

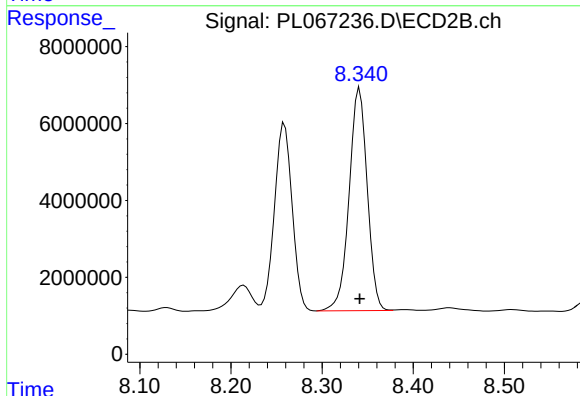


#26 Chlordane-4

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 79862791
Conc: 492.67 ng/ml

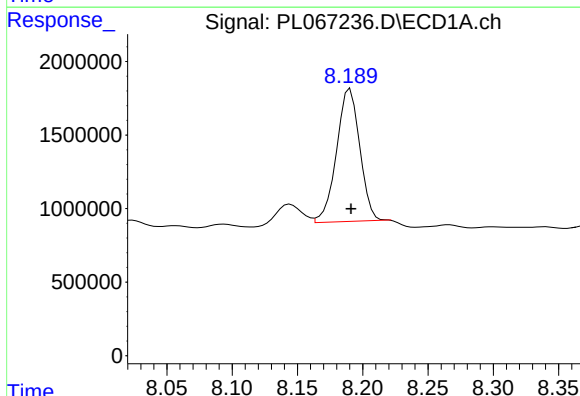


#27 Chlordane-5

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 11193272
Conc: 511.60 ng/ml

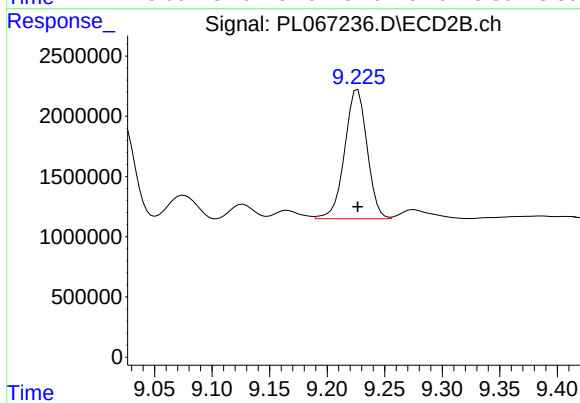

#27 Chlordane-5


R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 14611798
Conc: 502.51 ng/ml

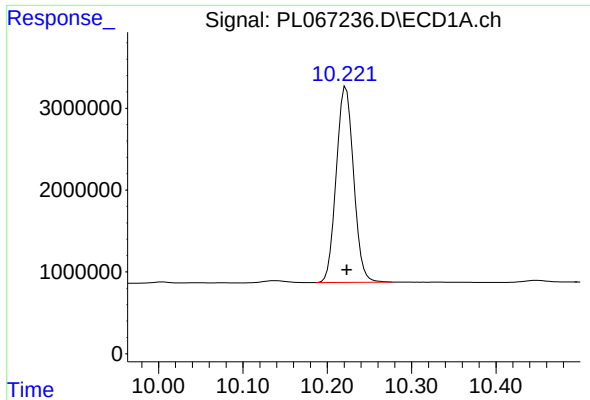

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: 0.000 min
Response: 34145371
Conc: 48.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061021CHLOR

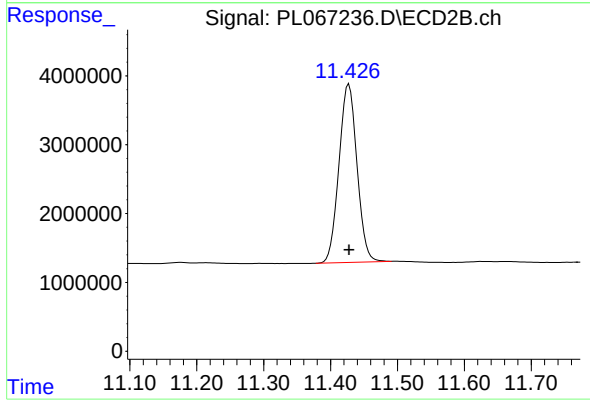

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: 0.000 min
Response: 48555789
Conc: 49.28 ng/ml