

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 16:16
 Operator : AR\AJ
 Sample : PB136983BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB136983BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:12:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.482	5.529	10714058	18475738	19.488	19.598
28)	SA Decachlor...	10.223	11.428	14332288	21014458	20.224	21.098
Target Compounds							
15)	B Endosulfa...	0.000	9.177f	0	726484	N.D.	0.911 #
23)	Chlordane-1	0.000	6.936f	0	342396	N.D.	12.125 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 16:16
Operator : AR\AJ
Sample : PB136983BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB136983BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:12:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

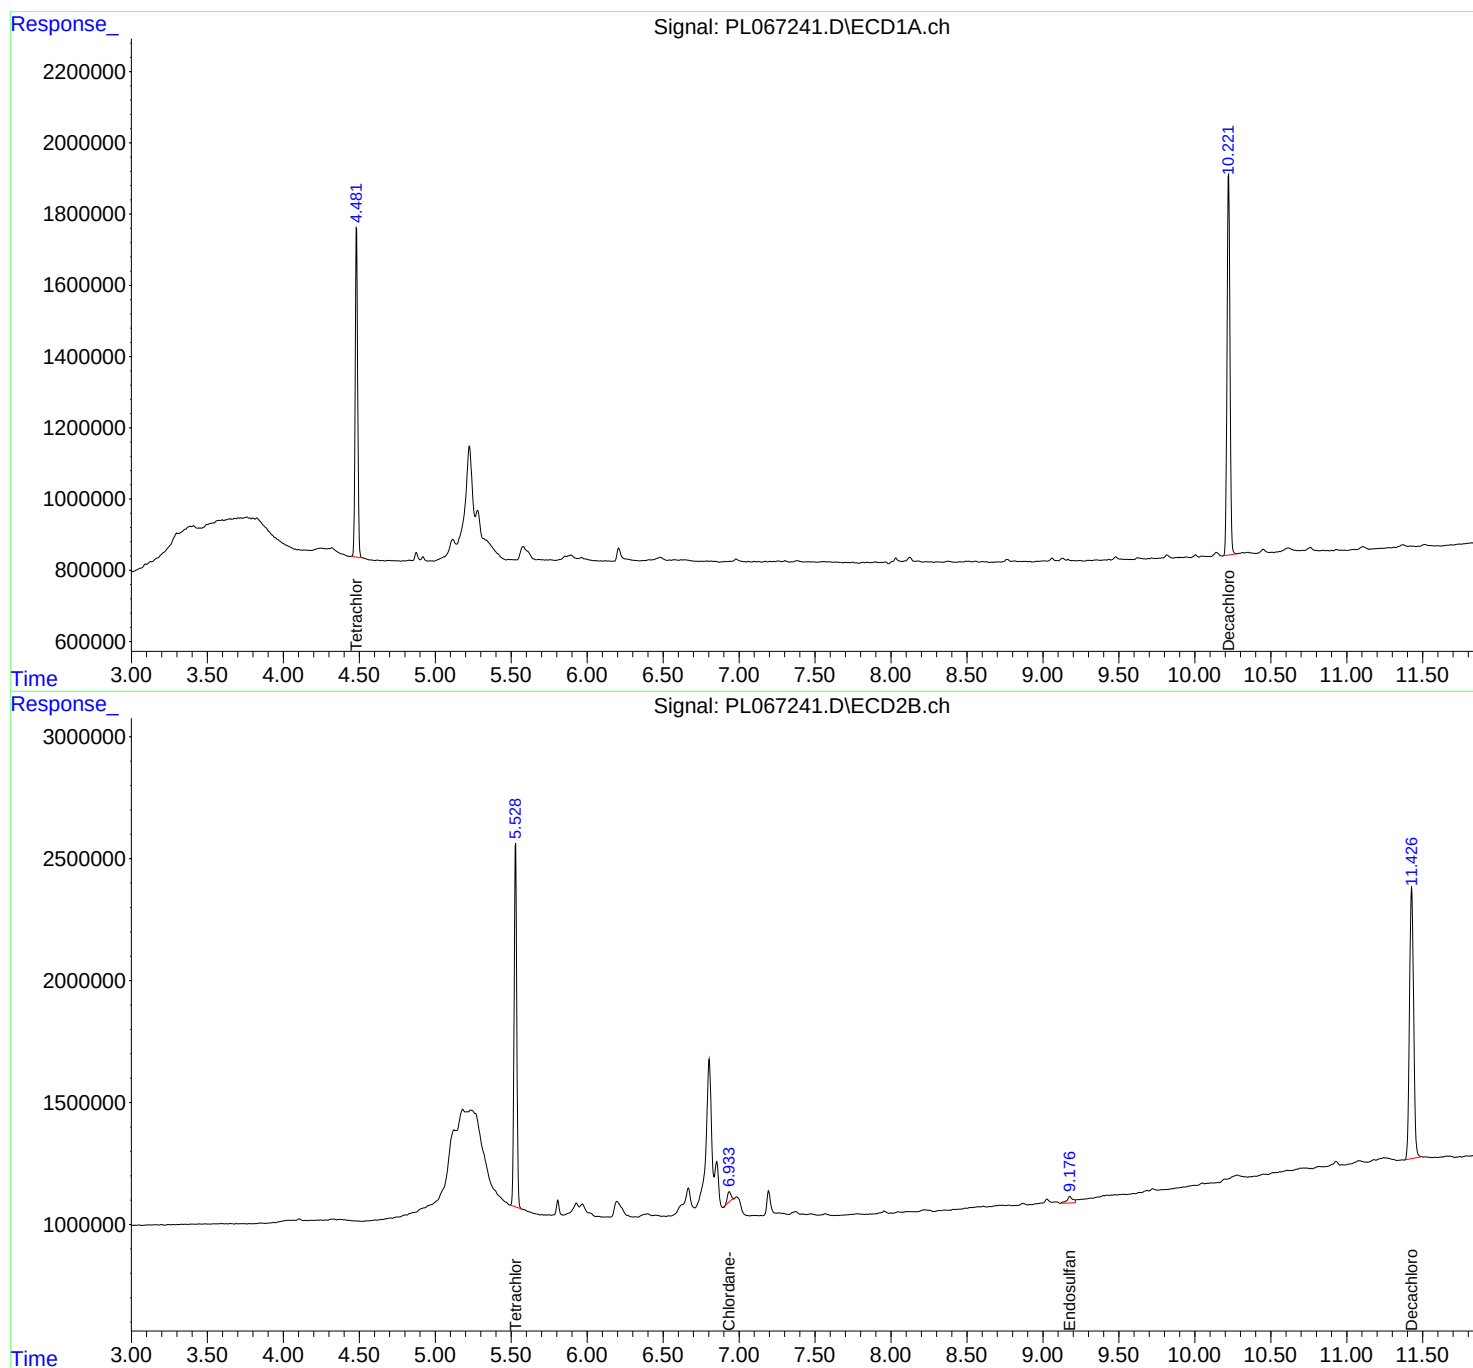


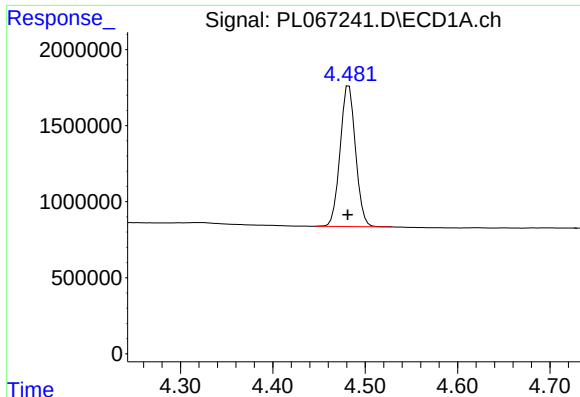

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: 0.001 min
Response: 10714058
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136983BL

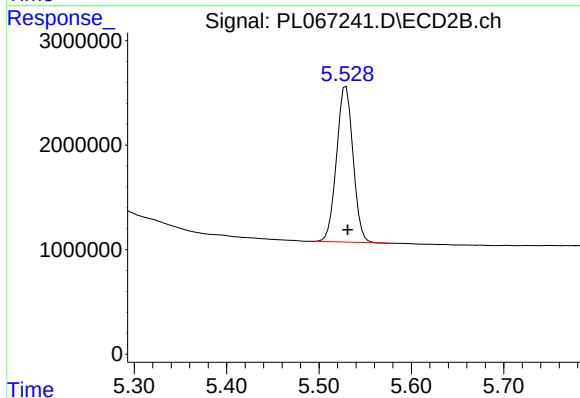


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 18475738
Conc: 19.60 ng/ml

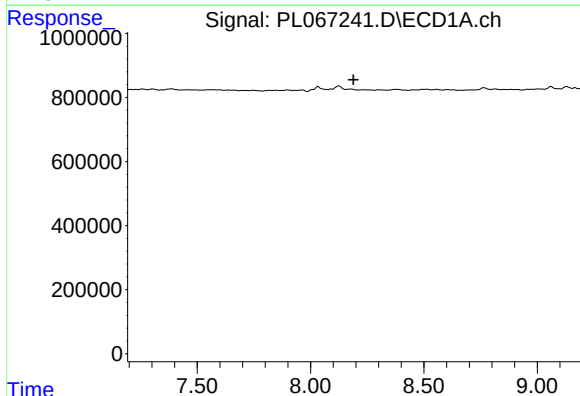


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

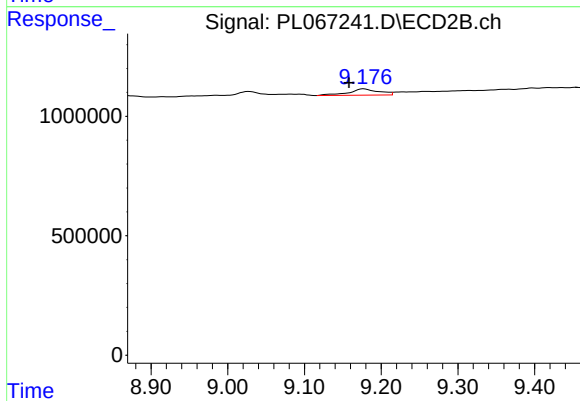

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 726484
Conc: 0.91 ng/ml

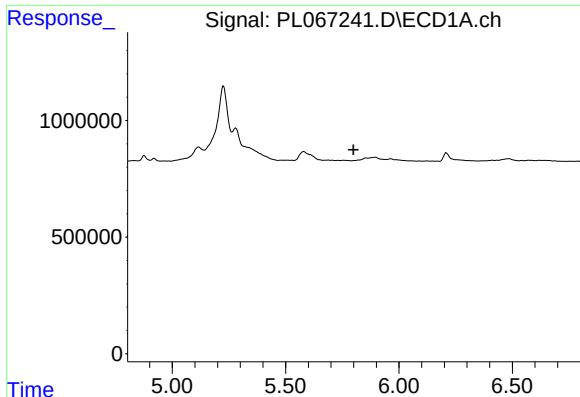

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB136983BL

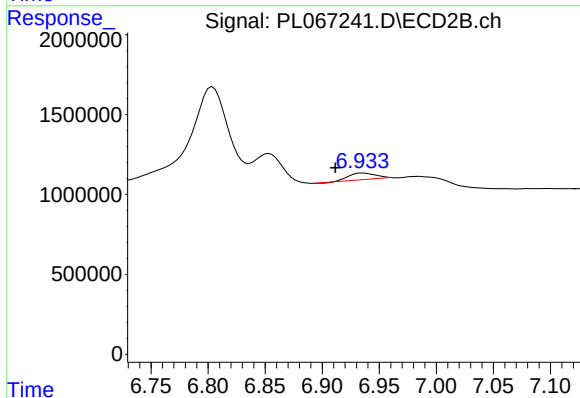


#23 Chlordane-1

R.T.: 6.936 min
Delta R.T.: 0.024 min
Response: 342396
Conc: 12.13 ng/ml

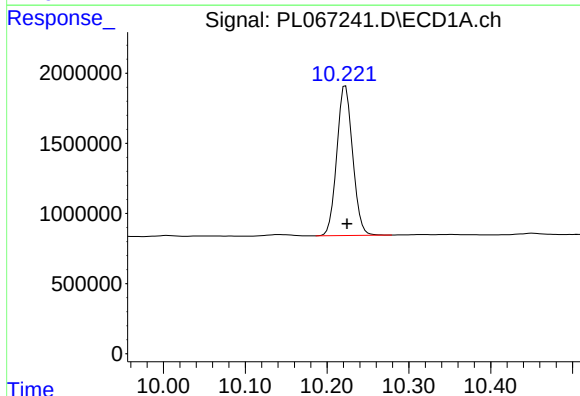

#28 Decachlorobiphenyl

R.T.: 10.223 min
Delta R.T.: -0.002 min
Response: 14332288
Conc: 20.22 ng/ml

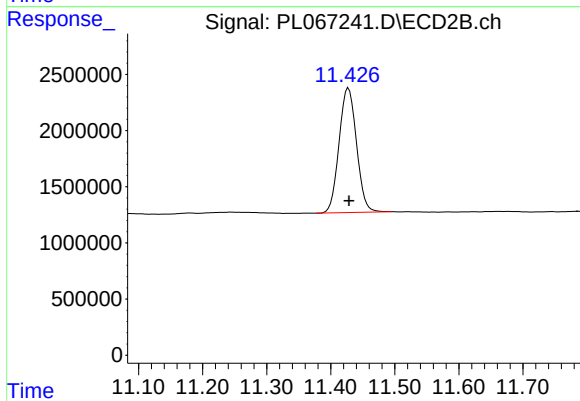

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 21014458
Conc: 21.10 ng/ml