

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 17:06
 Operator : AR\AJ
 Sample : M2612-21
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B12(6-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:12:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	11955245	20530395	21.745	21.778
28)	SA Decachlor...	10.222	11.428	14998389	23260941	21.164	23.353
Target Compounds							
3)	MA gamma-BHC...	5.615	0.000	474847	0	0.634	N.D. #
6)	B beta-BHC	5.964f	0.000	195329	0	0.546	N.D. #
7)	B delta-BHC	0.000	7.005f	0	1765792	N.D.	1.502 #
13)	MA Dieldrin	0.000	8.687	0	347814	N.D.	0.383 #
15)	B Endosulfa...	0.000	9.177f	0	1166792	N.D.	1.463 #
18)	B Endrin al...	8.380	0.000	1188808	0	2.348	N.D. #
21)	B Endrin ke...	9.130	0.000	900706	0	1.183	N.D. #
22)	Mirex	9.298	0.000	140476	0	0.223	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 17:06
Operator : AR\AJ
Sample : M2612-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:12:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

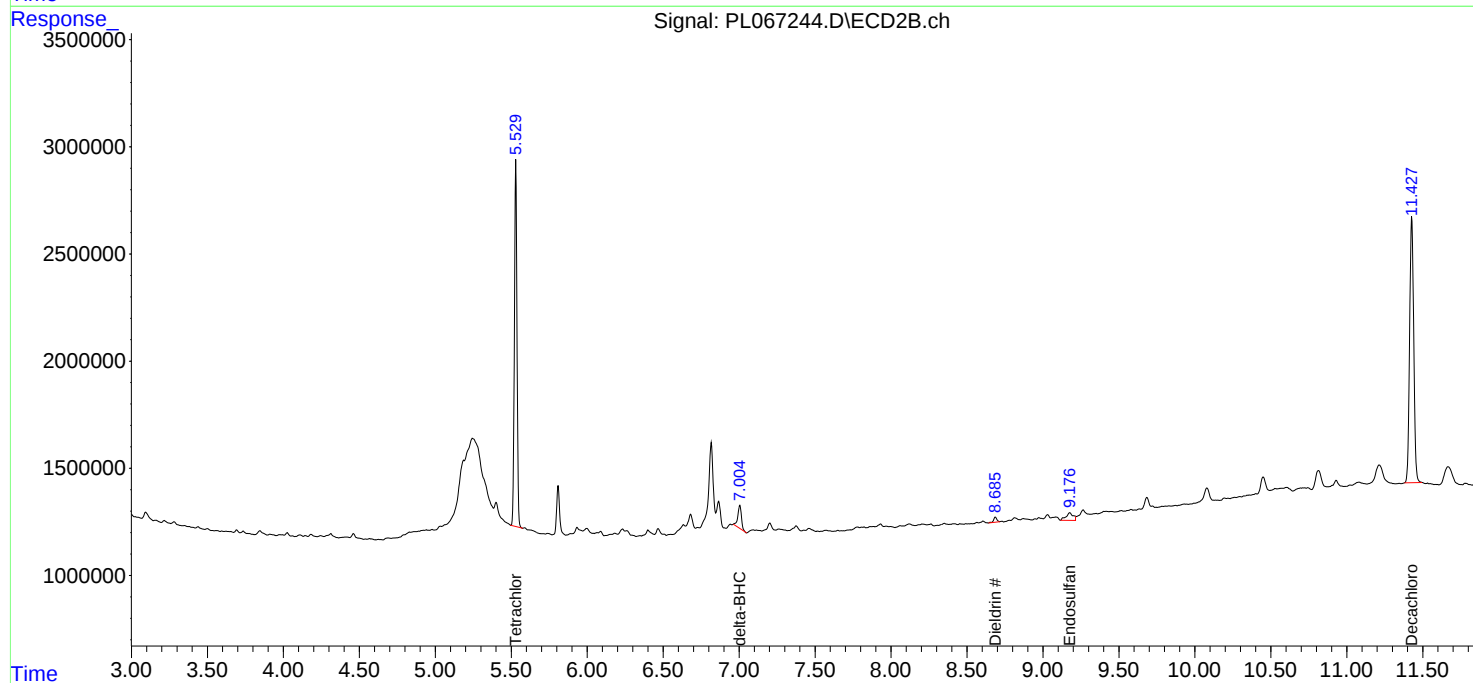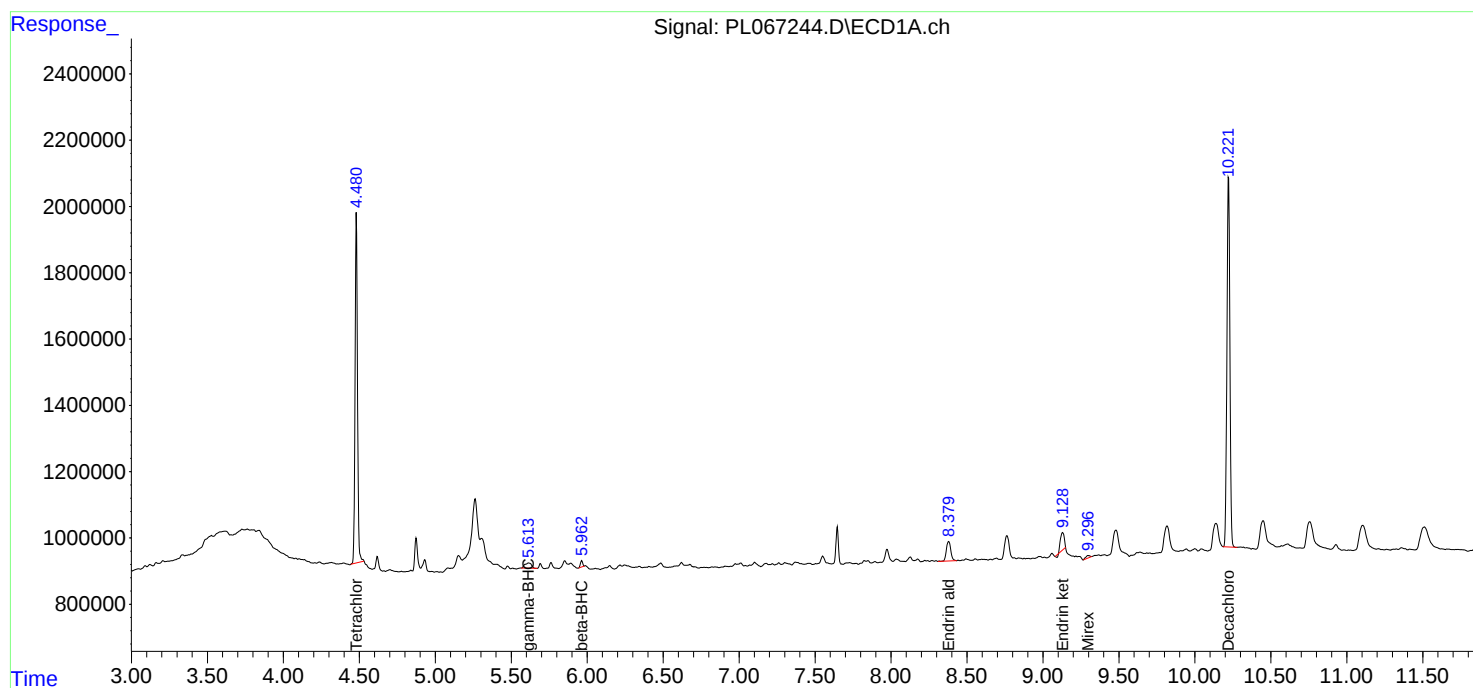


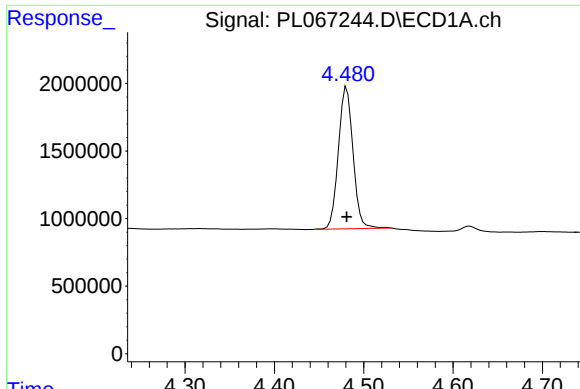

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 11955245
Conc: 21.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

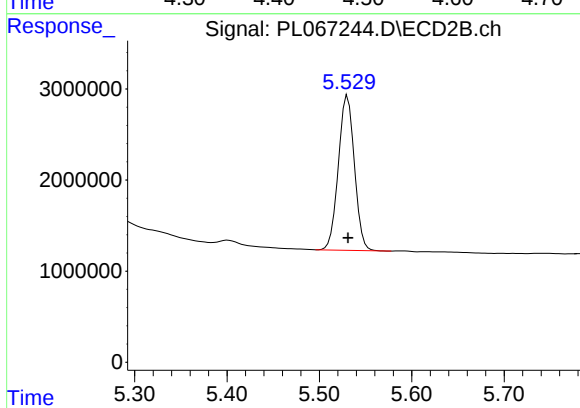


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 20530395
Conc: 21.78 ng/ml

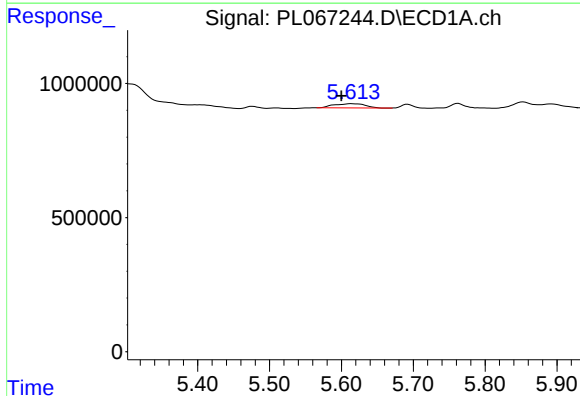


#3 gamma-BHC (Lindane)

R.T.: 5.615 min
Delta R.T.: 0.014 min
Response: 474847
Conc: 0.63 ng/ml

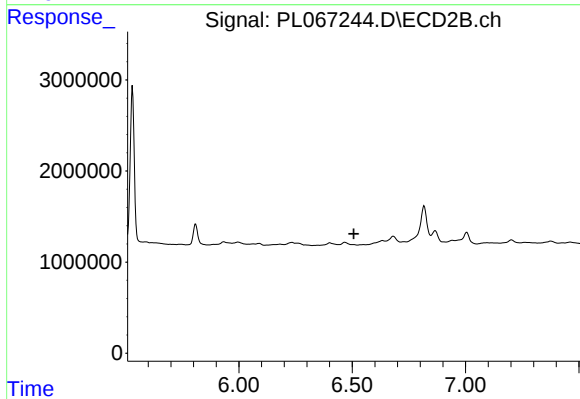

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

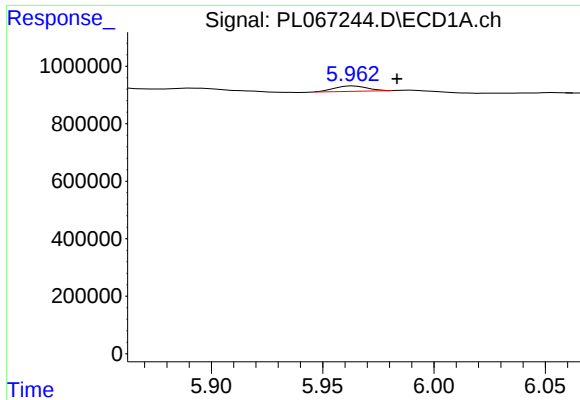

#6 beta-BHC


R.T.: 5.964 min
Delta R.T.: -0.019 min
Response: 195329
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

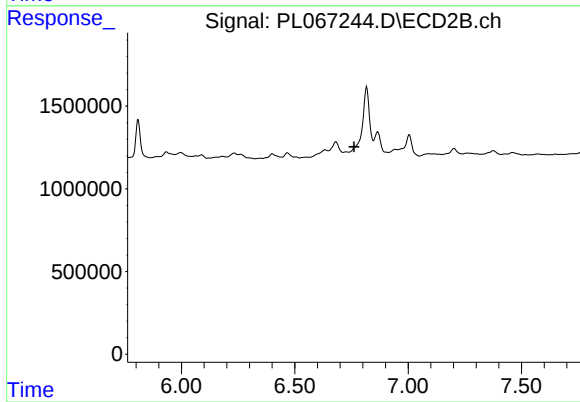


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

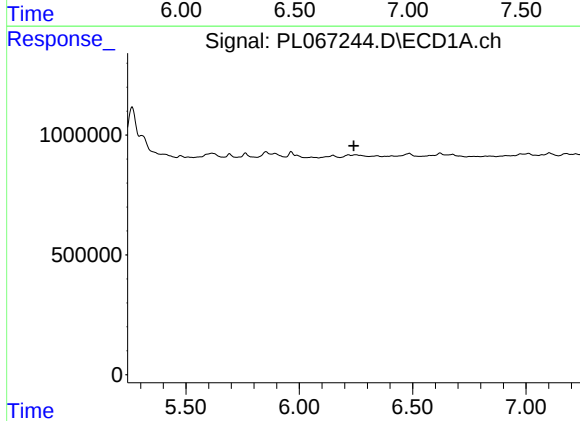


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

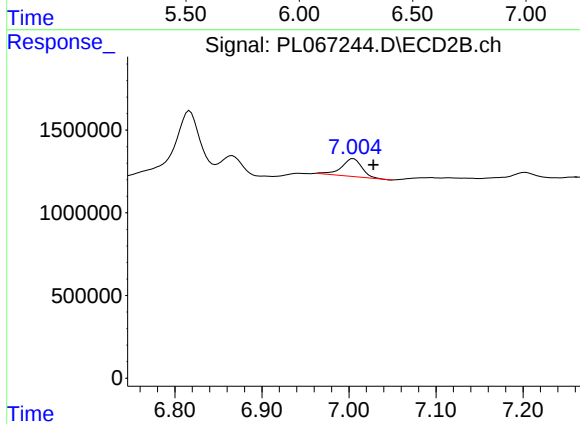

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 1765792
Conc: 1.50 ng/ml

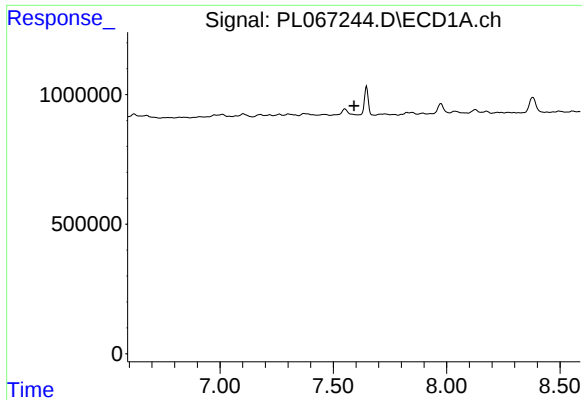

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

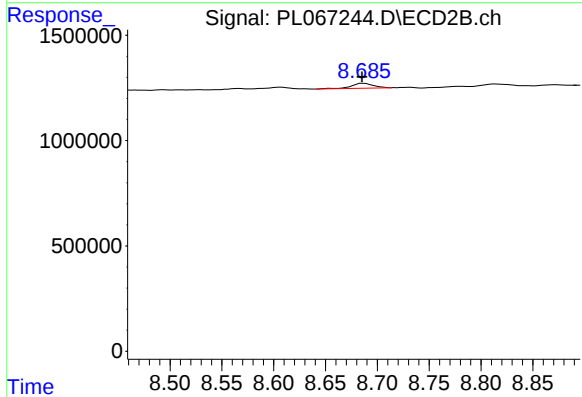


#13 Dieldrin

R.T.: 8.687 min
Delta R.T.: 0.001 min
Response: 347814
Conc: 0.38 ng/ml

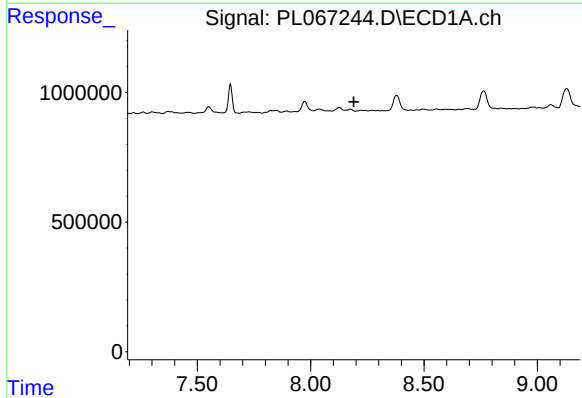


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

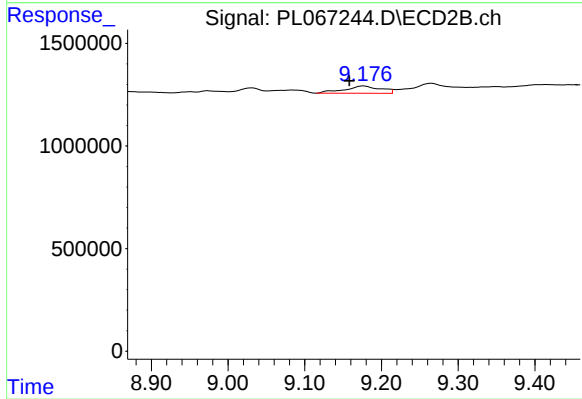

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 1166792
Conc: 1.46 ng/ml

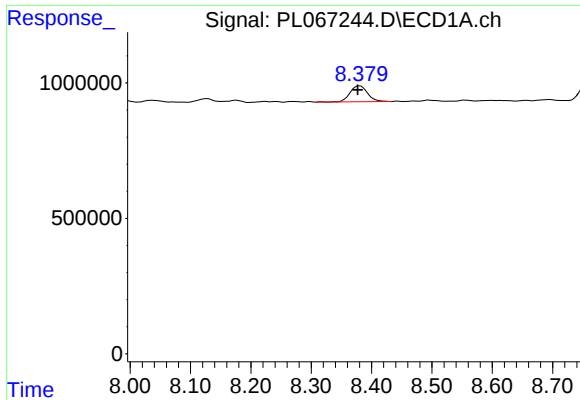

#18 Endrin aldehyde


R.T.: 8.380 min
Delta R.T.: 0.003 min
Response: 1188808
Conc: 2.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

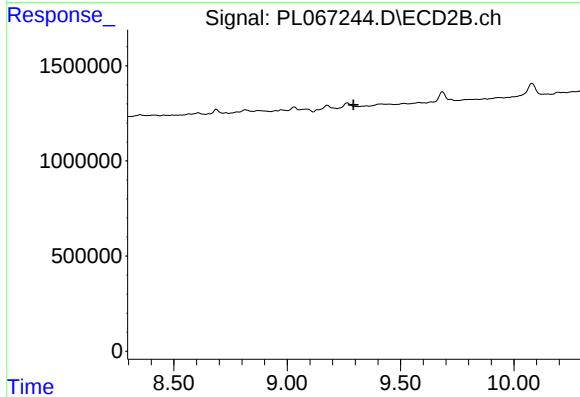


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

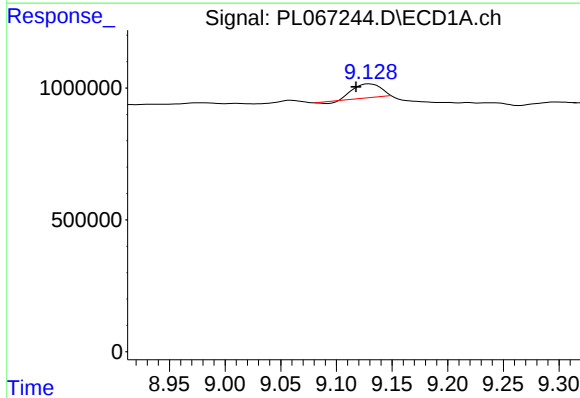


#21 Endrin ketone

R.T.: 9.130 min
Delta R.T.: 0.012 min
Response: 900706
Conc: 1.18 ng/ml

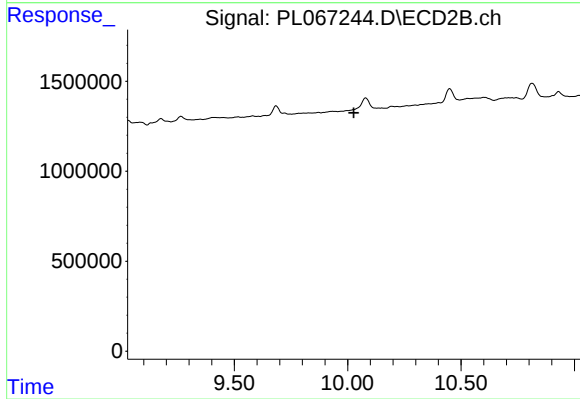

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

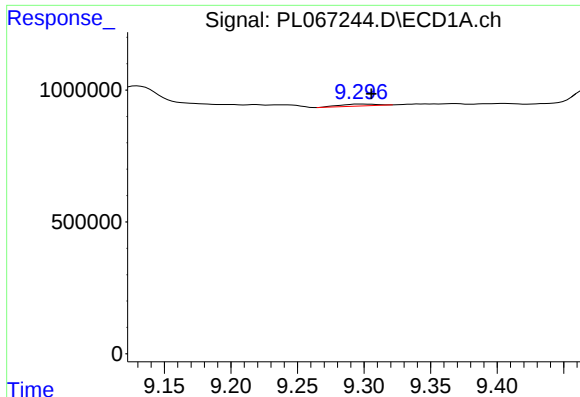

#22 Mirex


R.T.: 9.298 min
Delta R.T.: -0.008 min
Response: 140476
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(6-10)

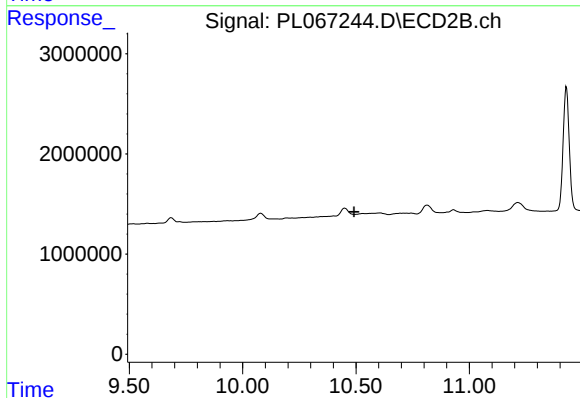


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 10.492 min
Response: 0
Conc: N.D.

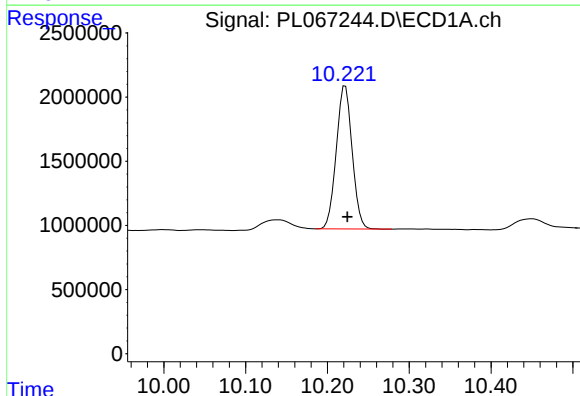

#28 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.002 min
Response: 14998389
Conc: 21.16 ng/ml

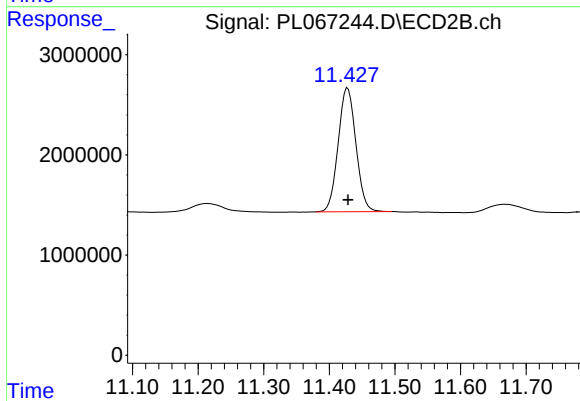

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 23260941
Conc: 23.35 ng/ml