

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 18:28
 Operator : AR\AJ
 Sample : M2612-24
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18-B12(18-22)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:14:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	11081336	18772269	20.156	19.913
28)	SA Decachlor...	10.221	11.427	12765123	19805226	18.012	19.884
Target Compounds							
2)	A alpha-BHC	5.169	0.000	282676	0	0.384	N.D. #
6)	B beta-BHC	5.963f	0.000	452863	0	1.266	N.D. #
7)	B delta-BHC	0.000	7.005f	0	2278837	N.D.	1.939 #
11)	B alpha-Chl...	7.256	0.000	2370305	0	3.238	N.D. #
15)	B Endosulfa...	0.000	9.178f	0	386056	N.D.	0.484 #
18)	B Endrin al...	8.379	0.000	868492	0	1.715	N.D. #
21)	B Endrin ke...	9.129	0.000	787266	0	1.034	N.D. #
26)	Chlordane-4	7.256	0.000	2370305	0	32.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 18:28
Operator : AR\AJ
Sample : M2612-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:14:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

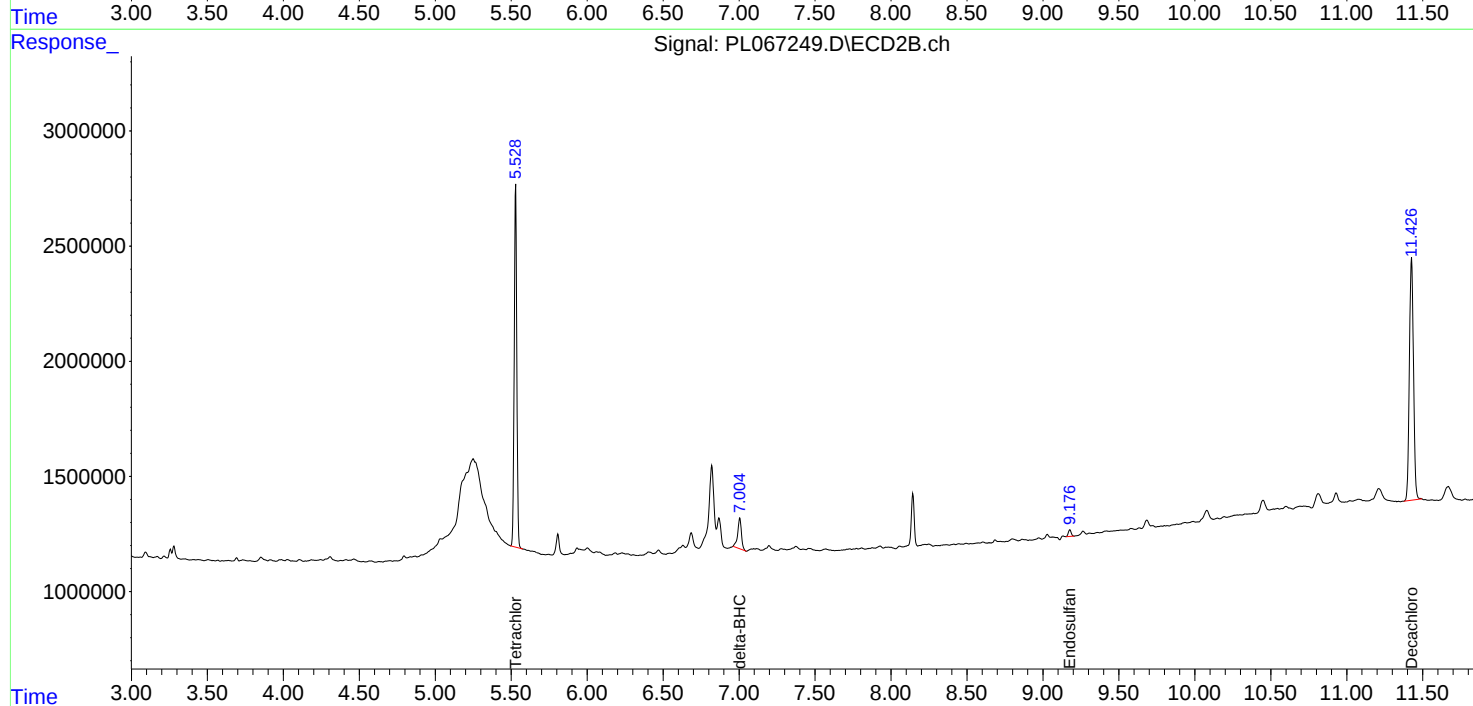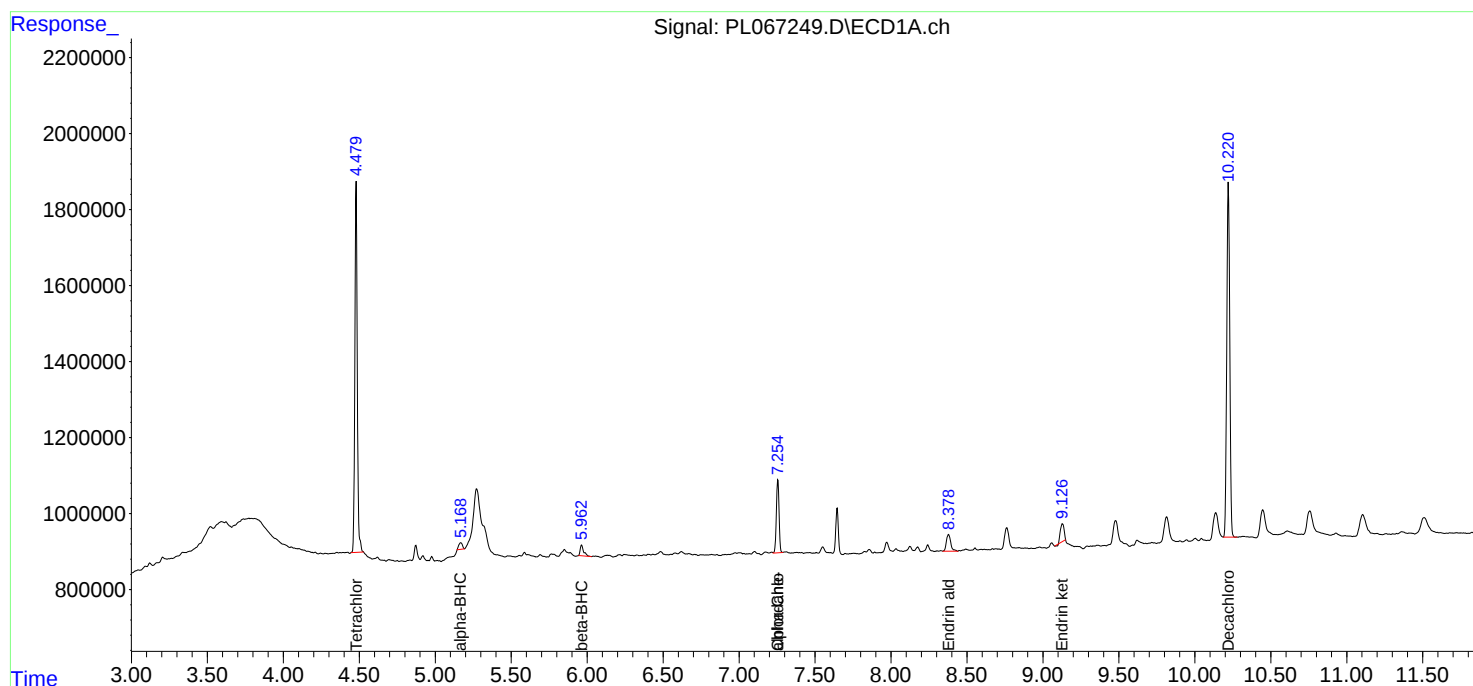


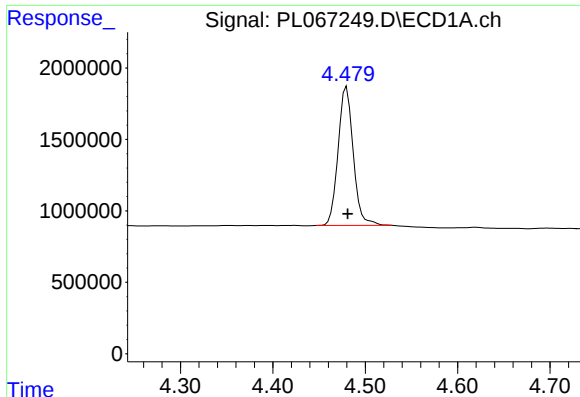

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.001 min
Response: 11081336
Conc: 20.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

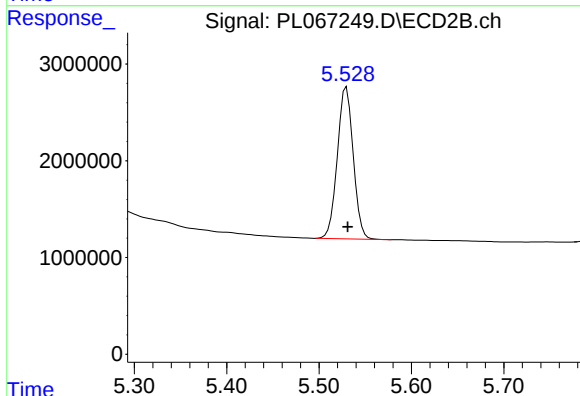


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 18772269
Conc: 19.91 ng/ml

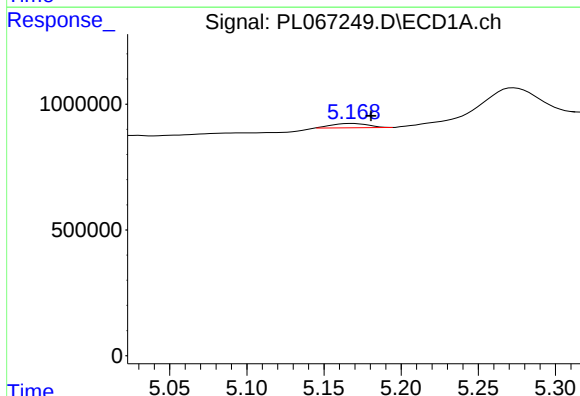


#2 alpha-BHC

R.T.: 5.169 min
Delta R.T.: -0.012 min
Response: 282676
Conc: 0.38 ng/ml

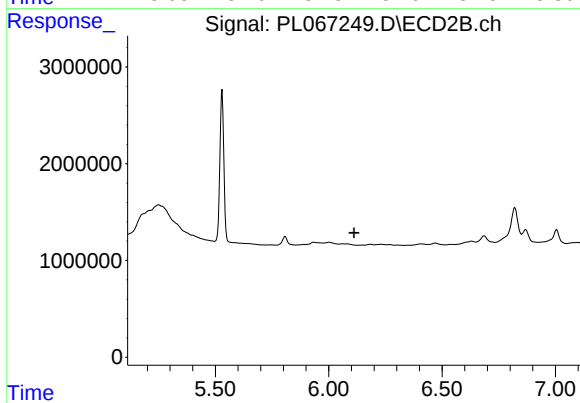

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

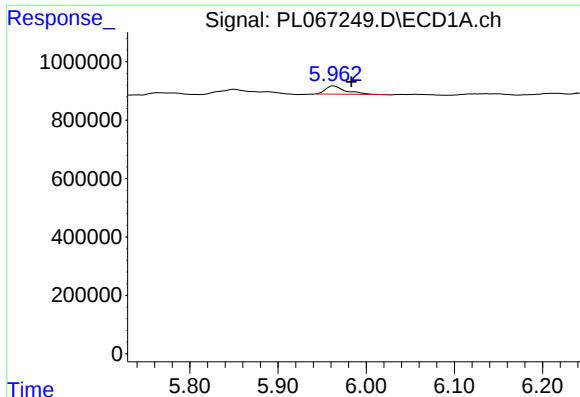

#6 beta-BHC


R.T.: 5.963 min
Delta R.T.: -0.020 min
Response: 452863
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

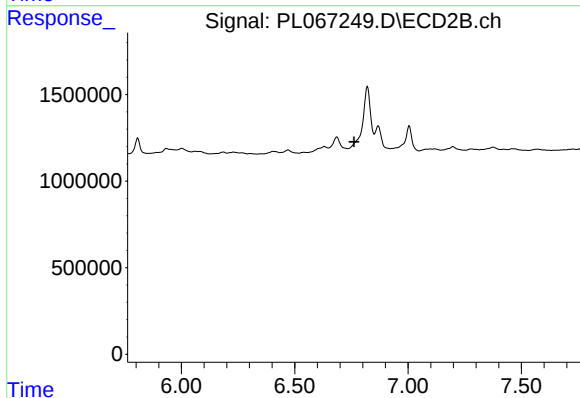


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

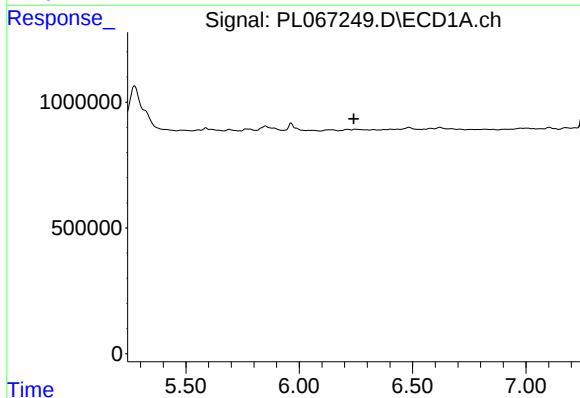


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

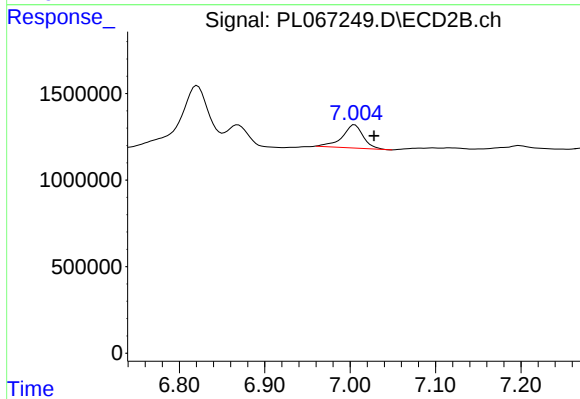

#7 delta-BHC


R.T.: 7.005 min
Delta R.T.: -0.023 min
Response: 2278837
Conc: 1.94 ng/ml

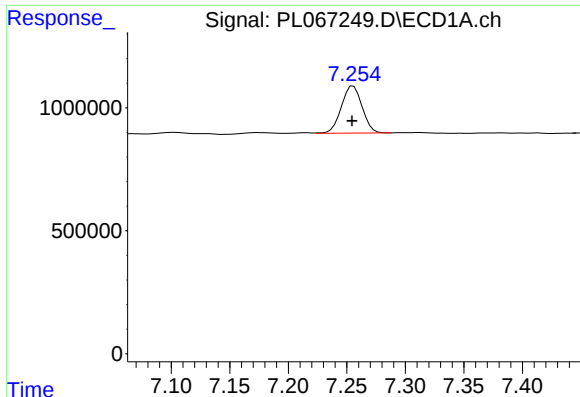

#11 alpha-Chlordane


R.T.: 7.256 min
Delta R.T.: 0.001 min
Response: 2370305
Conc: 3.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

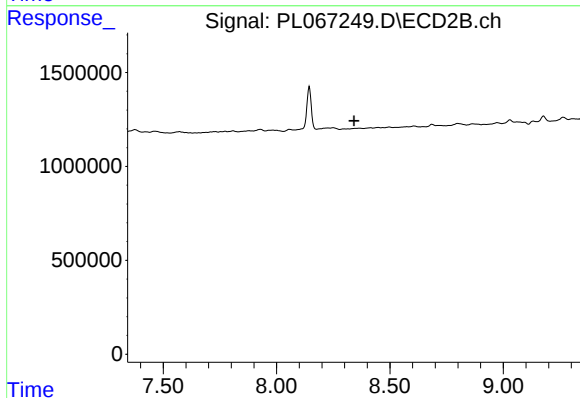


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

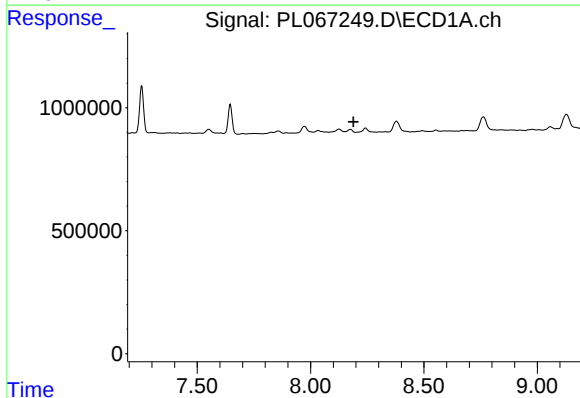


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.190 min
Response: 0
Conc: N.D.

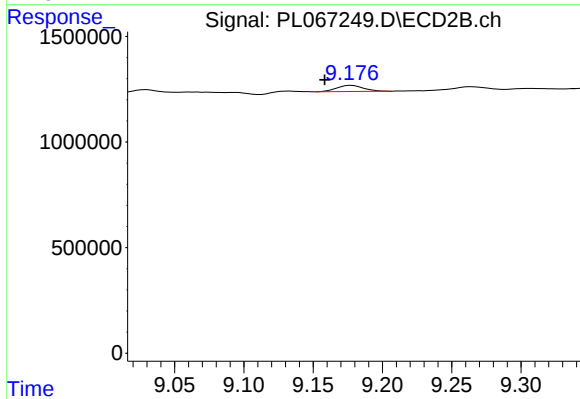

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 386056
Conc: 0.48 ng/ml

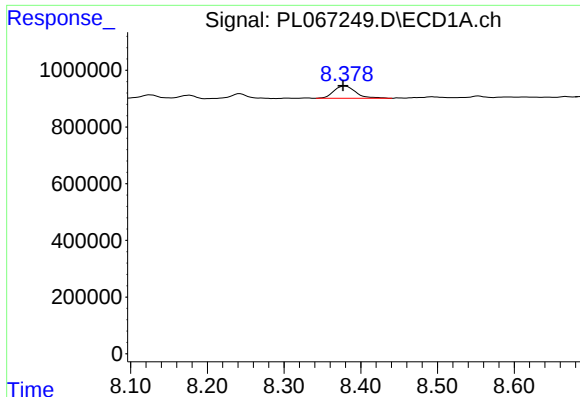

#18 Endrin aldehyde


R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 868492
Conc: 1.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

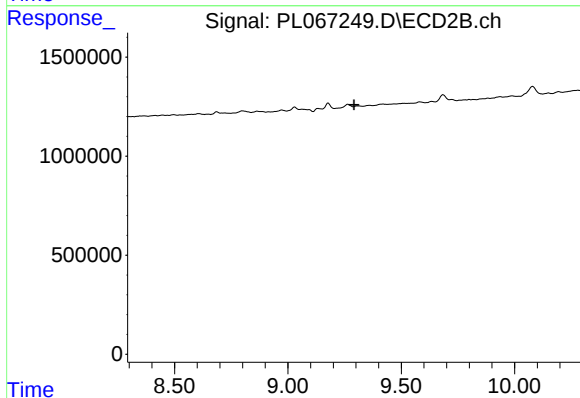


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

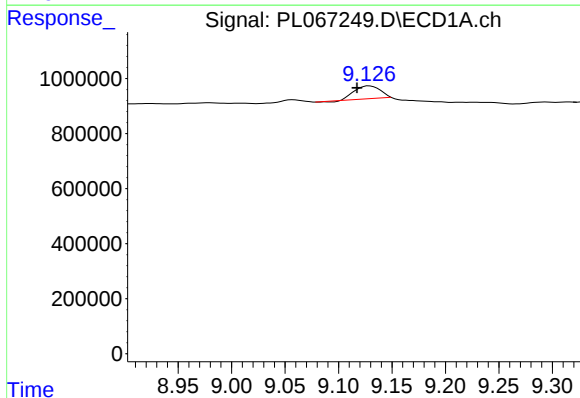


#21 Endrin ketone

R.T.: 9.129 min
Delta R.T.: 0.011 min
Response: 787266
Conc: 1.03 ng/ml

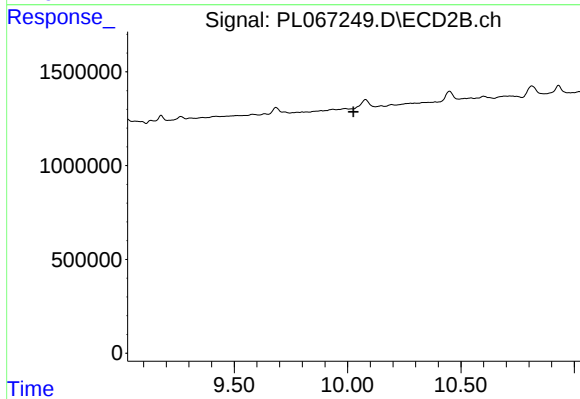

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 10.027 min
Response: 0
Conc: N.D.

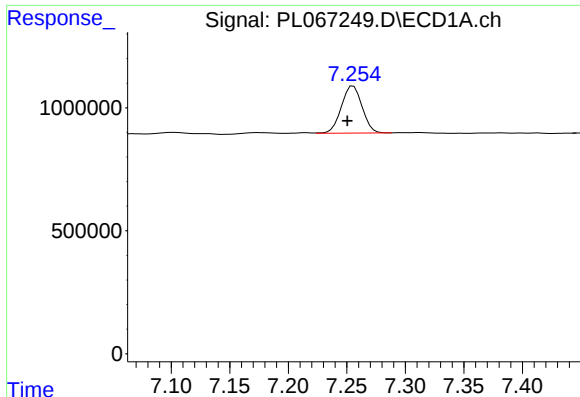

#26 Chlordane-4


R.T.: 7.256 min
Delta R.T.: 0.005 min
Response: 2370305
Conc: 32.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
18-B12(18-22)

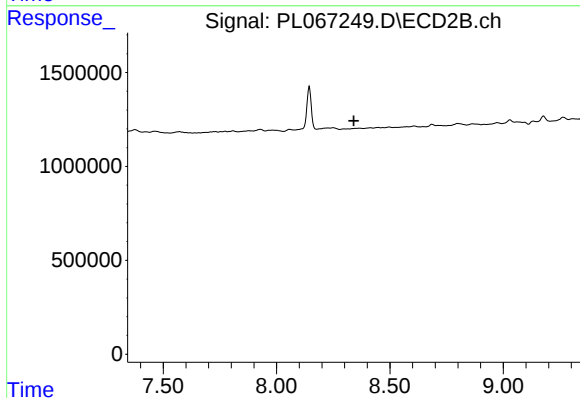


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

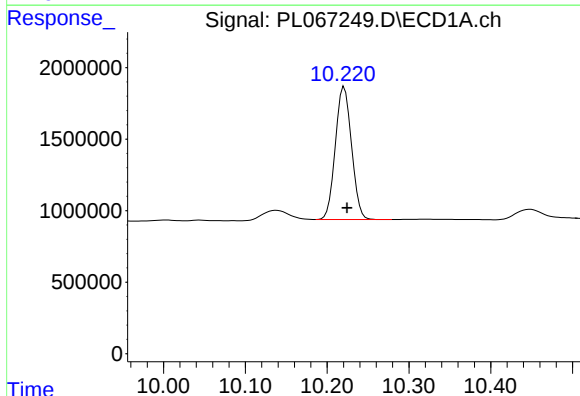

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.003 min
Response: 12765123
Conc: 18.01 ng/ml

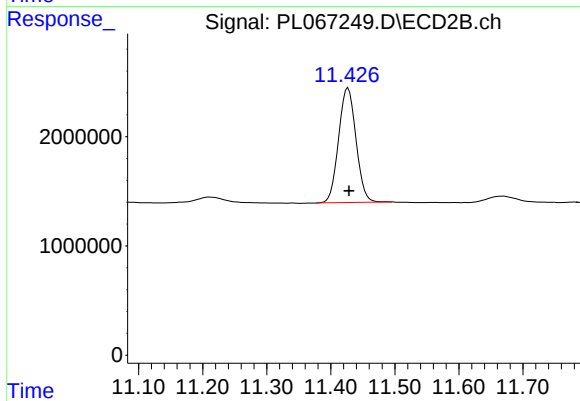

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 19805226
Conc: 19.88 ng/ml