

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
 Data File : PL067270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 01:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:19:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.530	10485797	17248226	19.073	18.296
28)	SA Decachlor...	10.221	11.427	13296820	19667811	18.763	19.746
Target Compounds							
2)	A alpha-BHC	5.171	0.000	385002	0	0.523	N.D. #
4)	MA Heptachlor	5.989f	0.000	465974	0	0.618	N.D. #
6)	B beta-BHC	5.989	0.000	465974	0	1.302	N.D. #
7)	B delta-BHC	0.000	7.000f	0	1603961	N.D.	1.364 #
8)	B Heptachlo...	0.000	7.996	0	516752	N.D.	0.516 #
24)	Chlordane-2	6.487	0.000	307004	0	11.465	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061021\
Data File : PL067270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 01:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:19:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

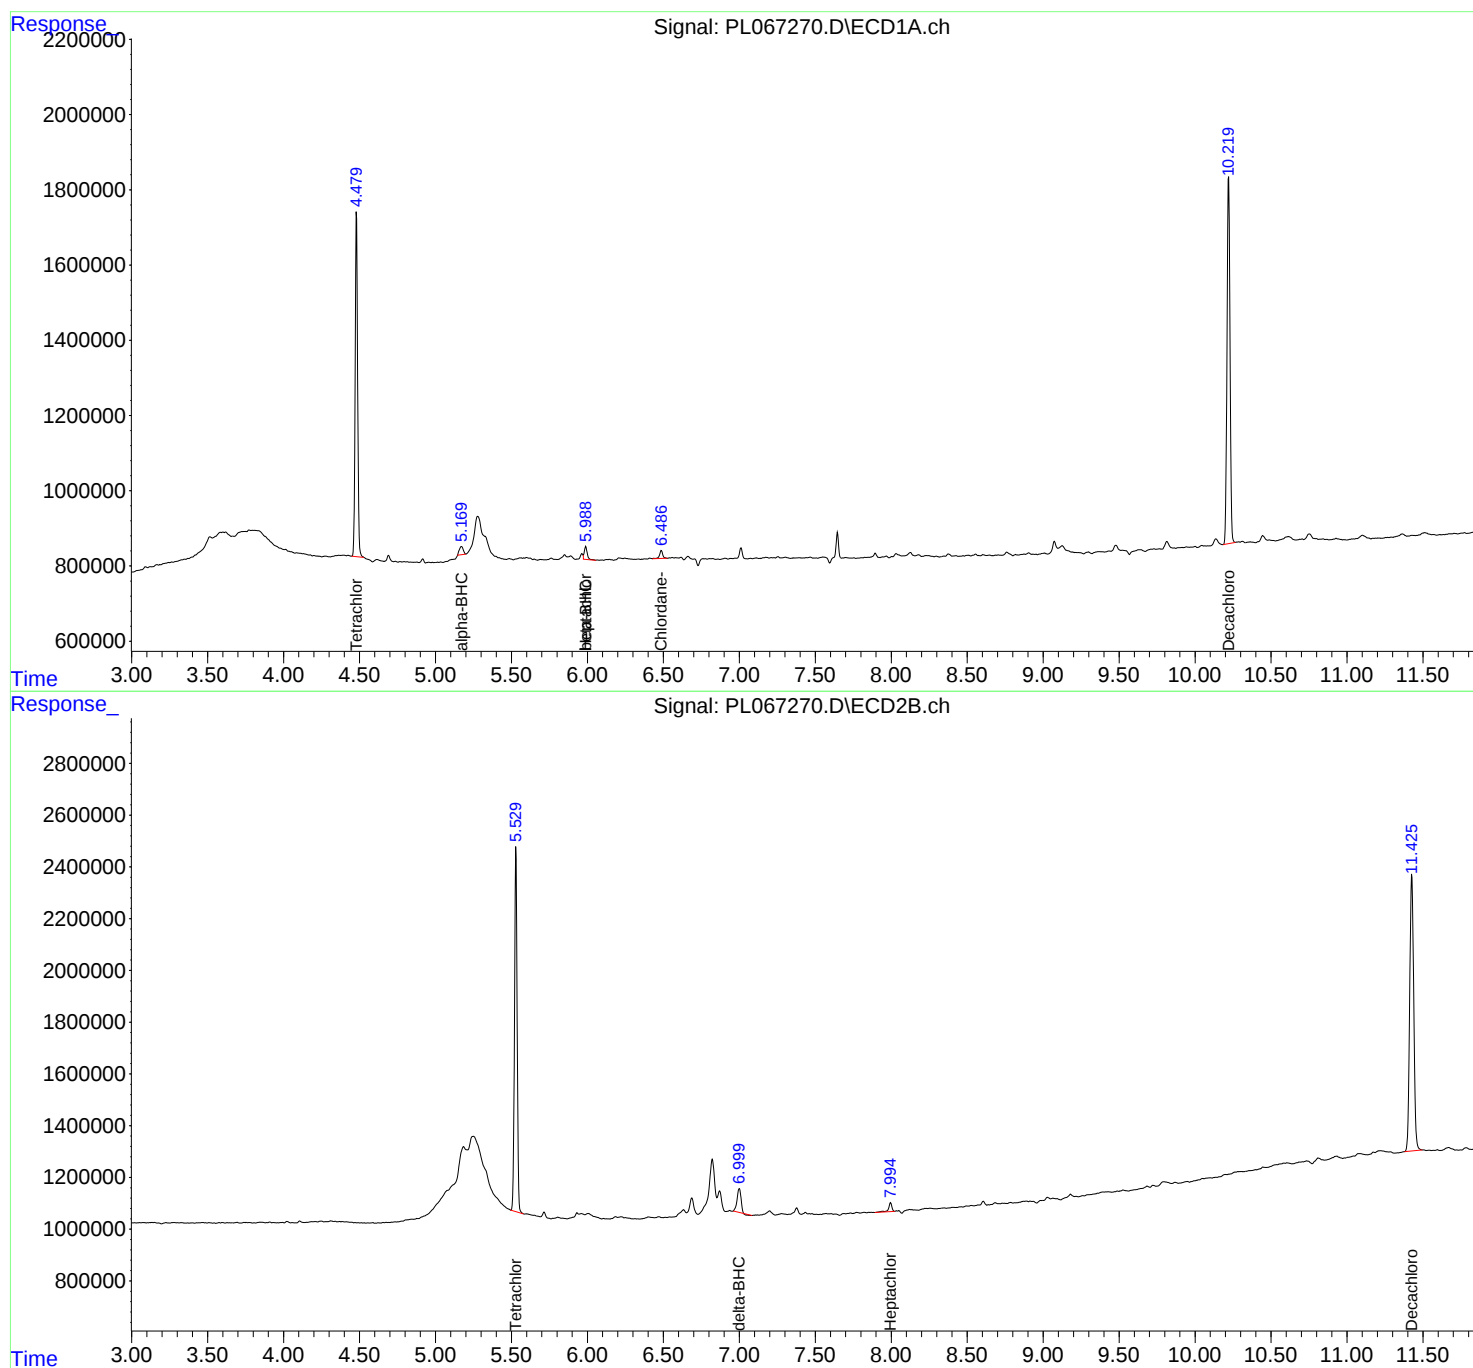


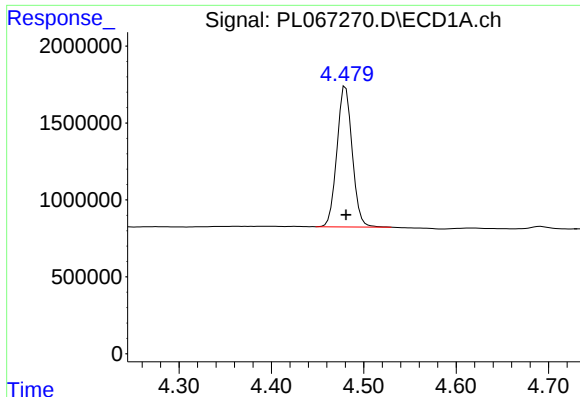

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 10485797
Conc: 19.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

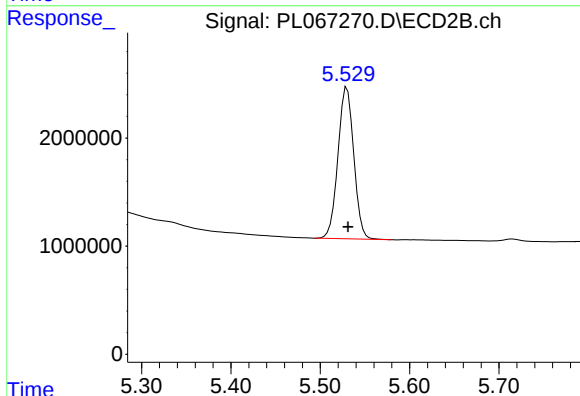


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 17248226
Conc: 18.30 ng/ml

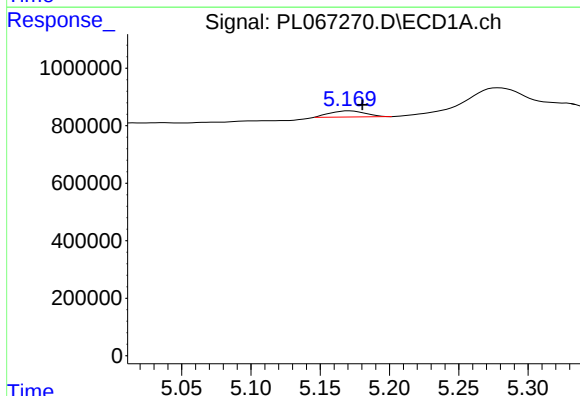


#2 alpha-BHC

R.T.: 5.171 min
Delta R.T.: -0.010 min
Response: 385002
Conc: 0.52 ng/ml

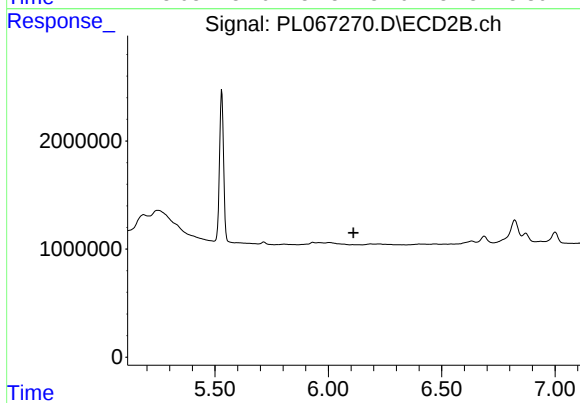

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

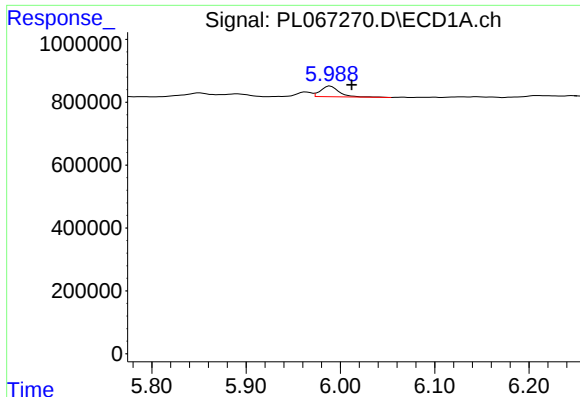

#4 Heptachlor


R.T.: 5.989 min
Delta R.T.: -0.023 min
Response: 465974
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

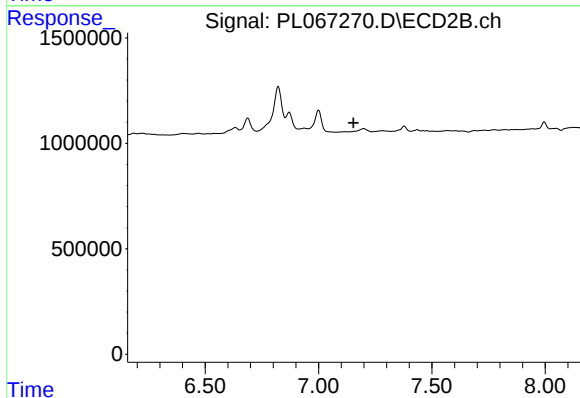


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

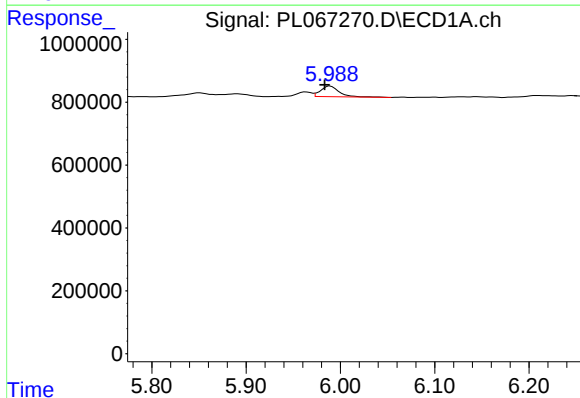


#6 beta-BHC

R.T.: 5.989 min
Delta R.T.: 0.006 min
Response: 465974
Conc: 1.30 ng/ml

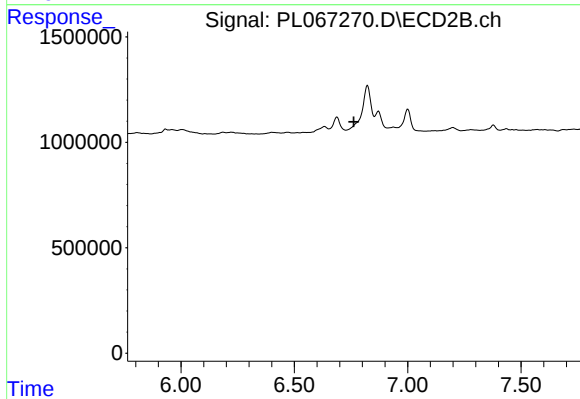

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

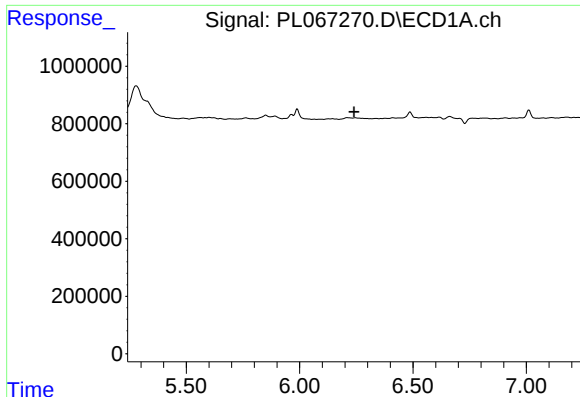

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

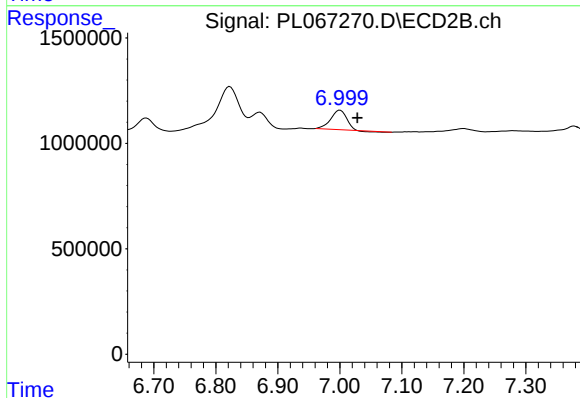


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 1603961
Conc: 1.36 ng/ml

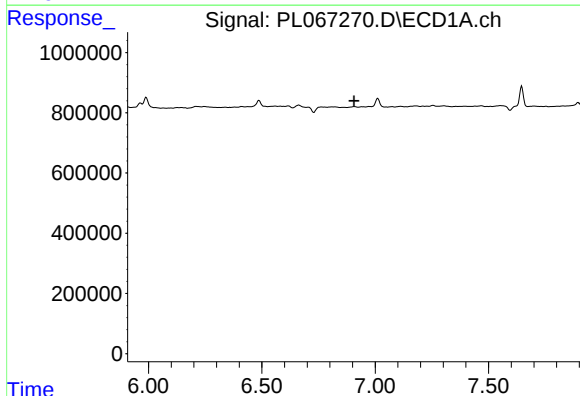


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

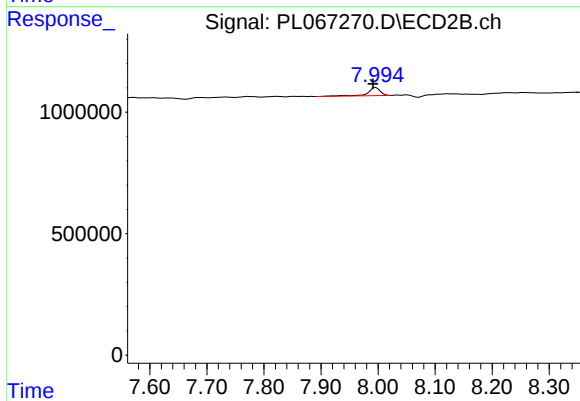

#8 Heptachlor epoxide


R.T.: 7.996 min
Delta R.T.: 0.004 min
Response: 516752
Conc: 0.52 ng/ml

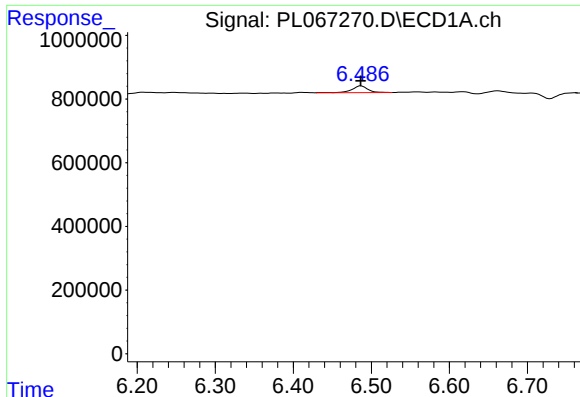

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 307004
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

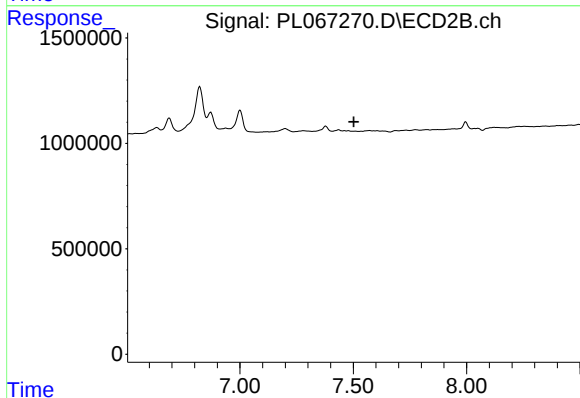


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

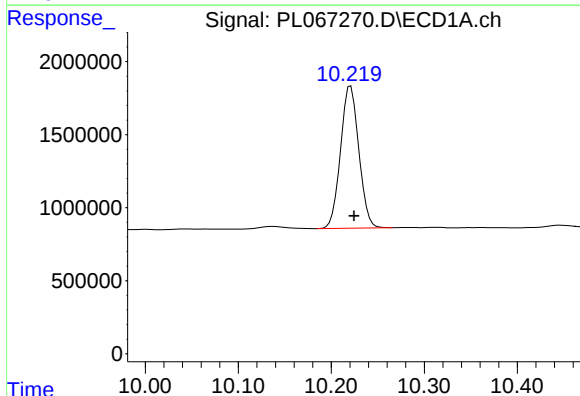

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.003 min
Response: 13296820
Conc: 18.76 ng/ml

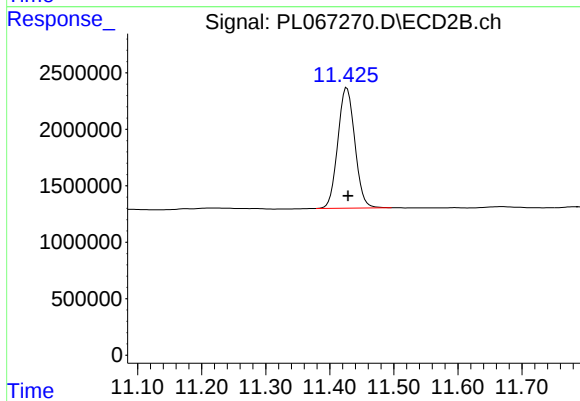

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 19667811
Conc: 19.75 ng/ml