

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061022\
 Data File : PL075683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2022 14:59
 Operator : AR\AJ
 Sample : N3296-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-060922

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/13/2022
 Supervised By : Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:29:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.649	4.639	7516628	15868321	11.138	9.456
28)	SA Decachlor...	11.645	10.385	6646158	12115699	10.856	8.599
Target Compounds							
10)	B gamma-Chl...	8.393	7.346	811471	942023	1.045m	0.514 #
11)	B alpha-Chl...	8.480	7.414	1423789	1951380	1.867m	1.069 #
12)	B 4,4'-DDE	8.664	7.625	956589	1915623	1.445m	1.198m
17)	MA 4,4'-DDT	9.524	8.470	807628	1338496	1.261m	0.952

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061022\
Data File : PL075683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2022 14:59
Operator : AR\AJ
Sample : N3296-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-060922


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:29:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

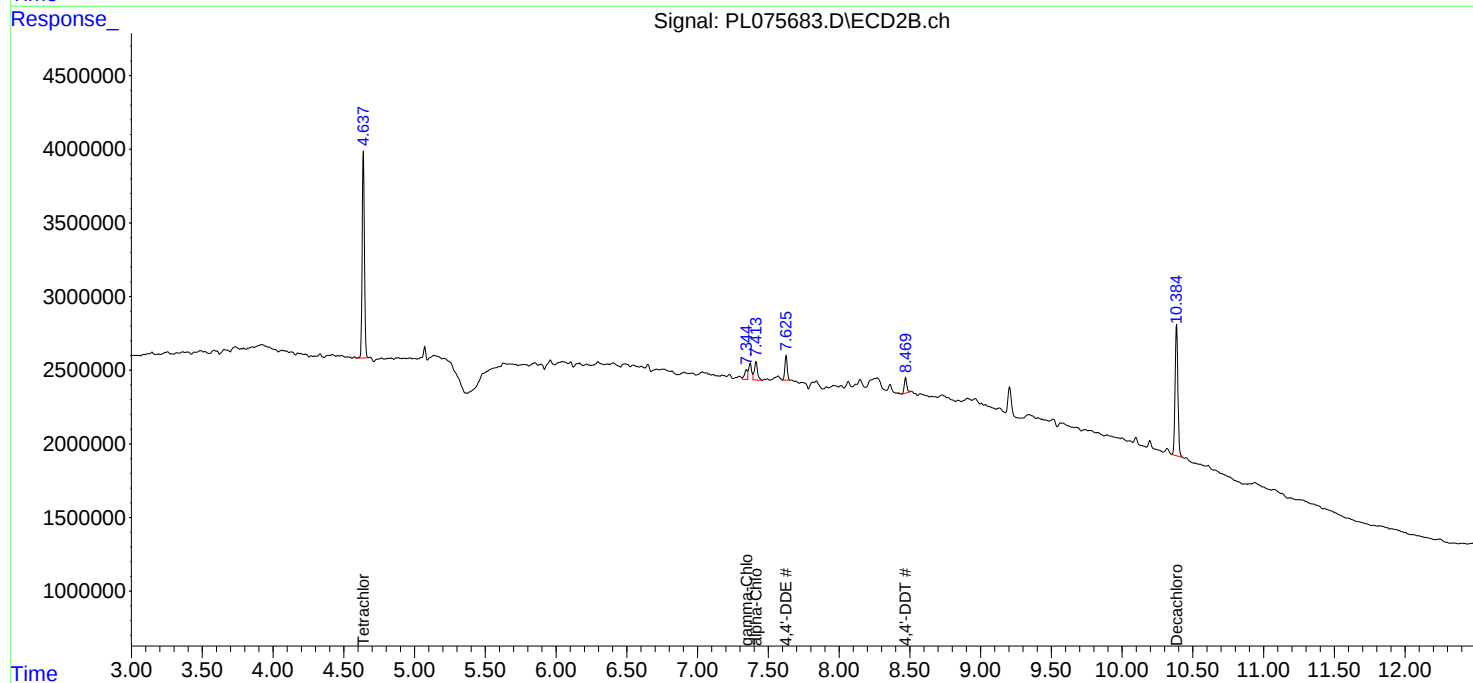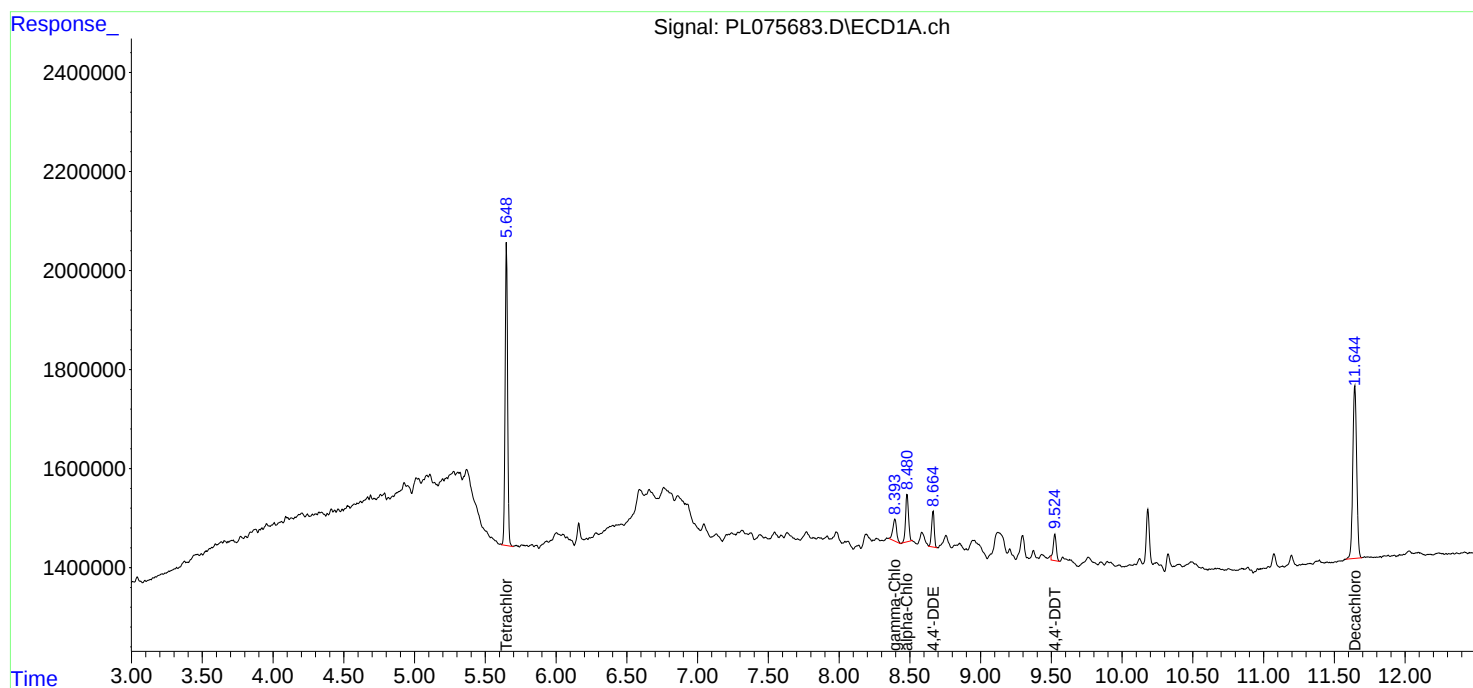

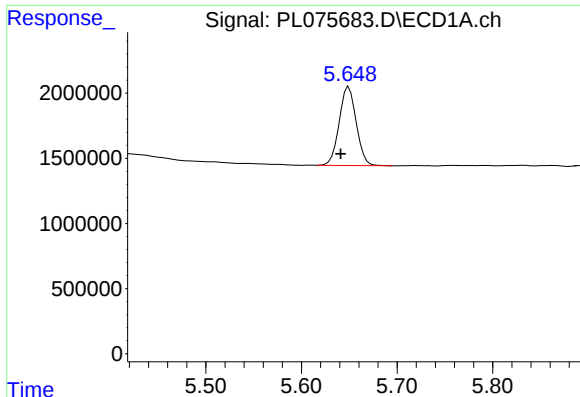


#1 Tetrachloro-m-xylene

R.T.: 5.649 min
Delta R.T.: 0.008 min
Response: 7516628
Conc: 11.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-060922


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

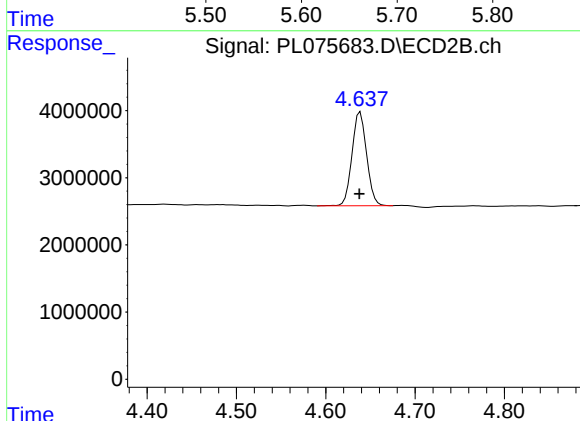


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 15868321
Conc: 9.46 ng/ml

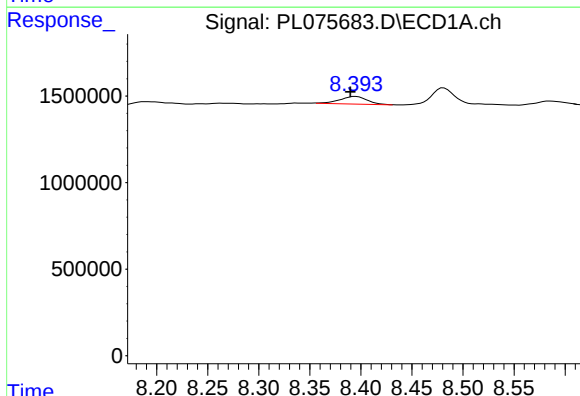


#10 gamma-Chlordane

R.T.: 8.393 min
Delta R.T.: 0.003 min
Response: 811471
Conc: 1.04 ng/ml m

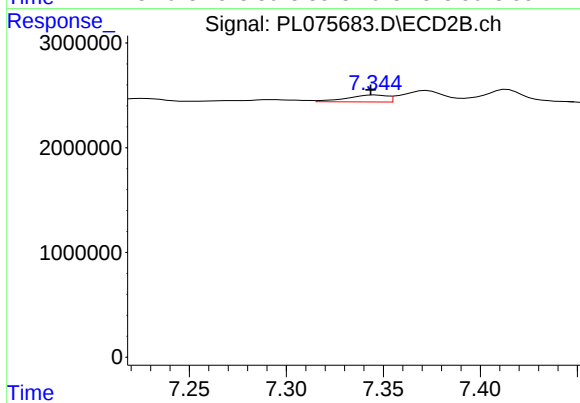

#10 gamma-Chlordane

R.T.: 7.346 min
Delta R.T.: 0.002 min
Response: 942023
Conc: 0.51 ng/ml

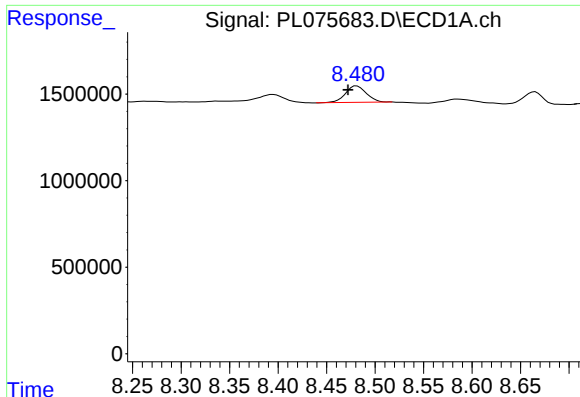


#11 alpha-Chlordane

R.T.: 8.480 min
Delta R.T.: 0.007 min
Response: 1423789
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-060922


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

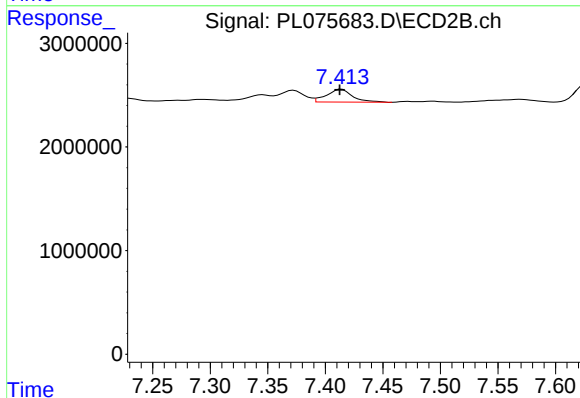


#11 alpha-Chlordane

R.T.: 7.414 min
Delta R.T.: 0.002 min
Response: 1951380
Conc: 1.07 ng/ml

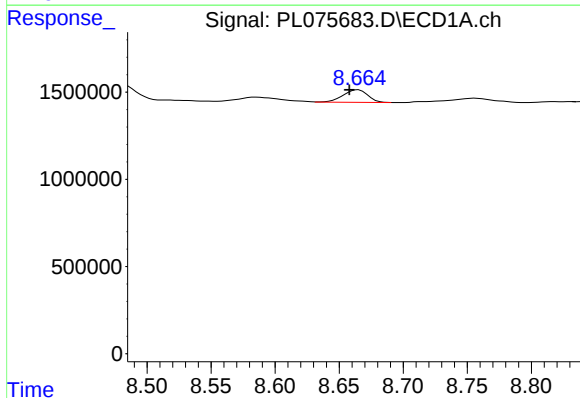


#12 4,4'-DDE

R.T.: 8.664 min
Delta R.T.: 0.006 min
Response: 956589
Conc: 1.45 ng/ml m

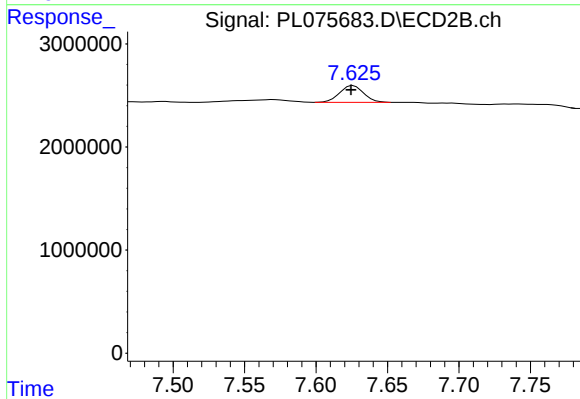

#12 4,4'-DDE

R.T.: 7.625 min
Delta R.T.: 0.000 min
Response: 1915623
Conc: 1.20 ng/ml m

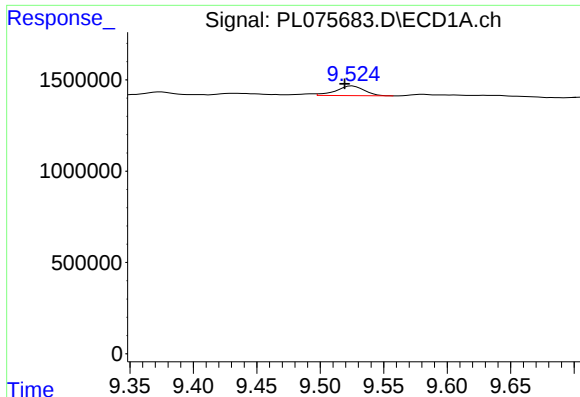


#17 4,4'-DDT

R.T.: 9.524 min
Delta R.T.: 0.005 min
Response: 807628
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-060922


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/13/2022
Supervised By :Ankita Jodhani 06/13/2022

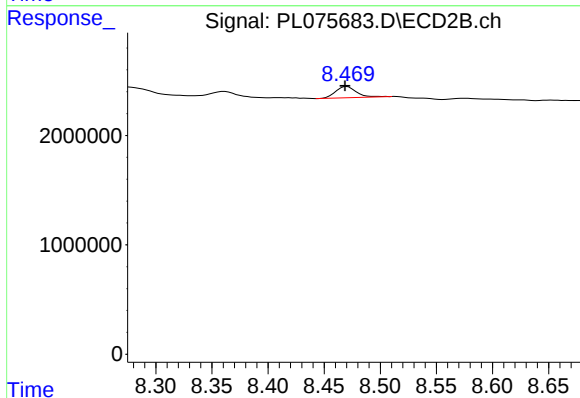


#17 4,4'-DDT

R.T.: 8.470 min
Delta R.T.: 0.002 min
Response: 1338496
Conc: 0.95 ng/ml

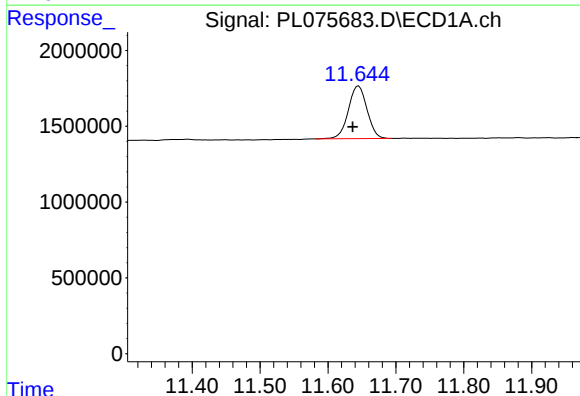

#28 Decachlorobiphenyl

R.T.: 11.645 min
Delta R.T.: 0.009 min
Response: 6646158
Conc: 10.86 ng/ml

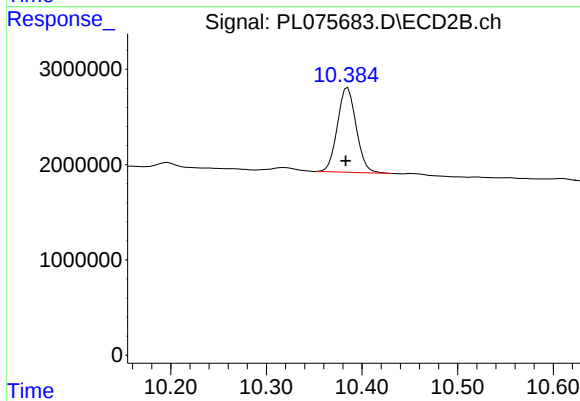

#28 Decachlorobiphenyl

R.T.: 10.385 min
Delta R.T.: 0.002 min
Response: 12115699
Conc: 8.60 ng/ml