

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061024\
 Data File : PL090099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2024 11:02
 Operator : AR\AJ
 Sample : P2756-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-06062024

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/11/2024
 Supervised By : Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 01:14:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.793	4794332	3277003	2.290m	2.285
2) SA Decachlor...	9.066	7.943	2829251	2533470	1.924	1.705

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061024\
Data File : PL090099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 11:02
Operator : AR\AJ
Sample : P2756-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-06062024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/11/2024
Supervised By : Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 01:14:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

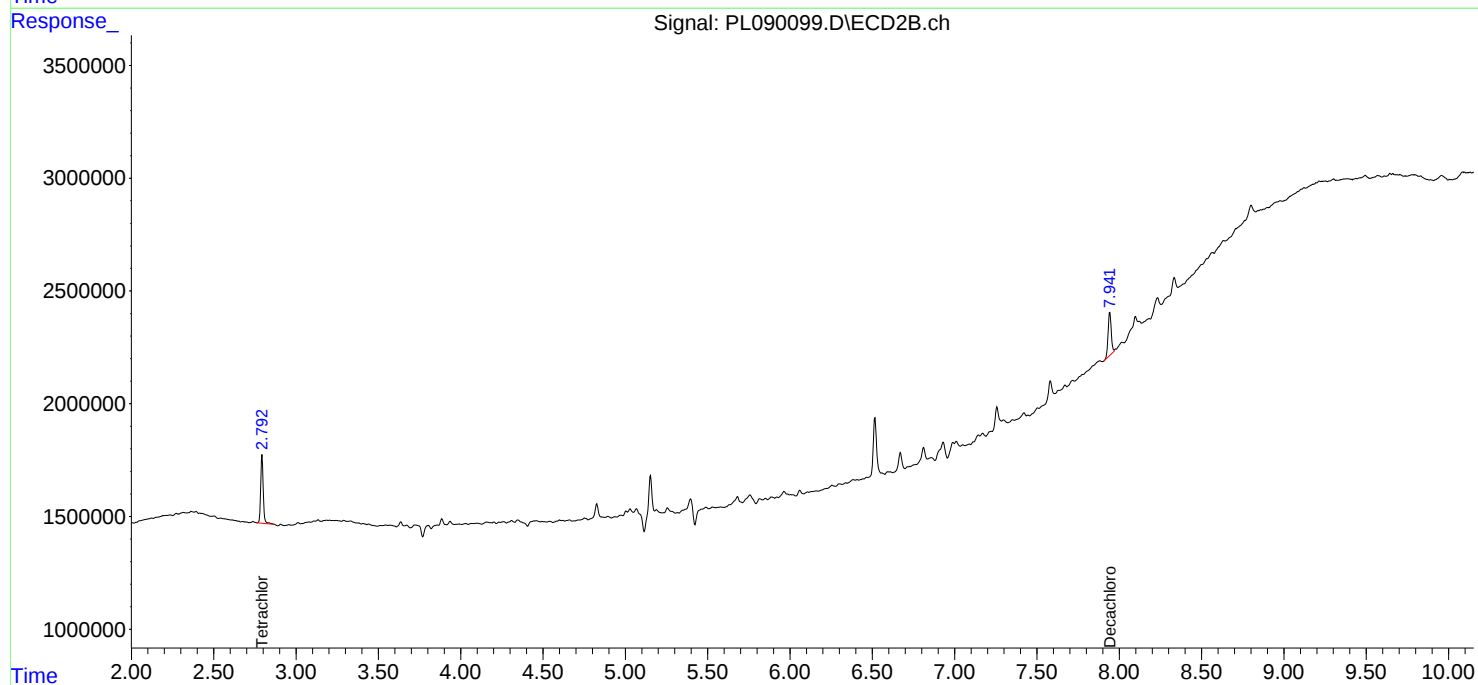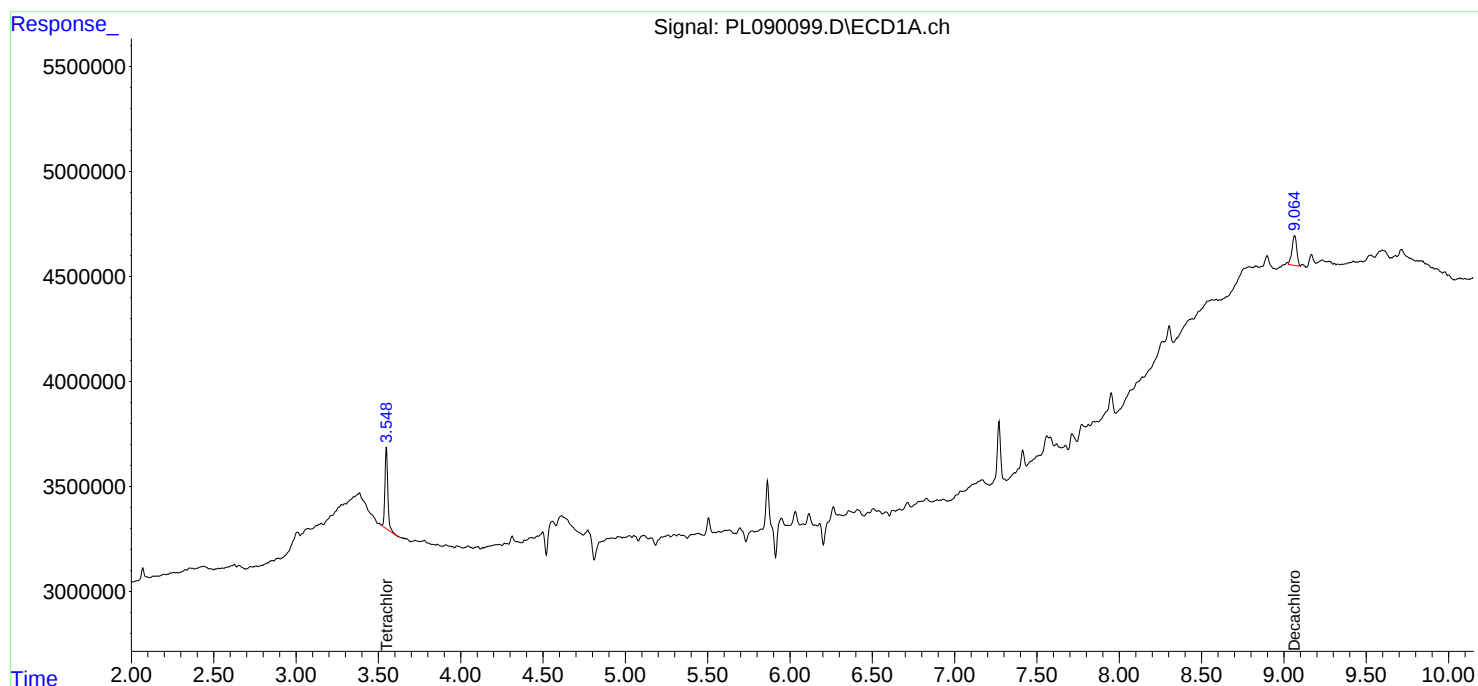

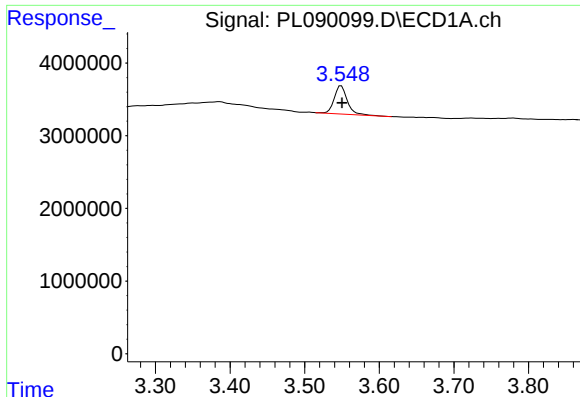


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.002 min
Response: 4794332
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-06062024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/11/2024
Supervised By :Ankita Jodhani 06/11/2024

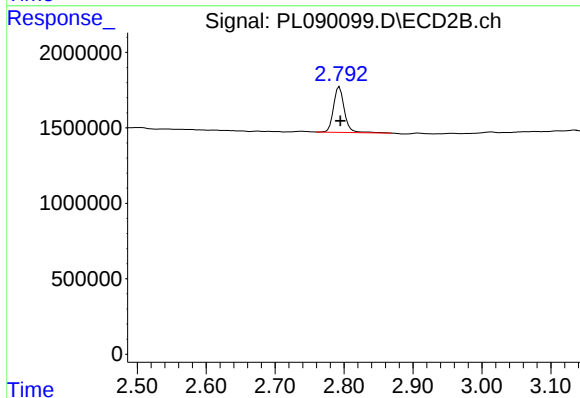


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.001 min
Response: 3277003
Conc: 2.29 ng/ml

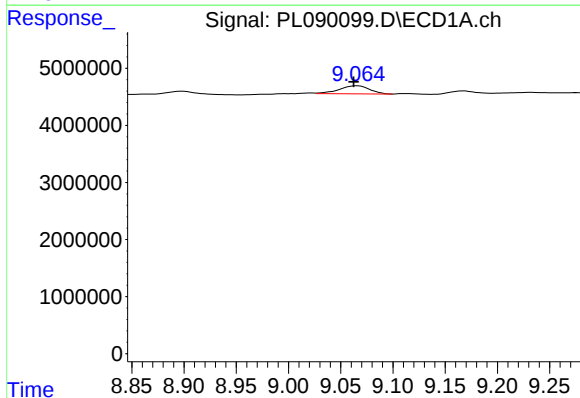

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.003 min
Response: 2829251
Conc: 1.92 ng/ml

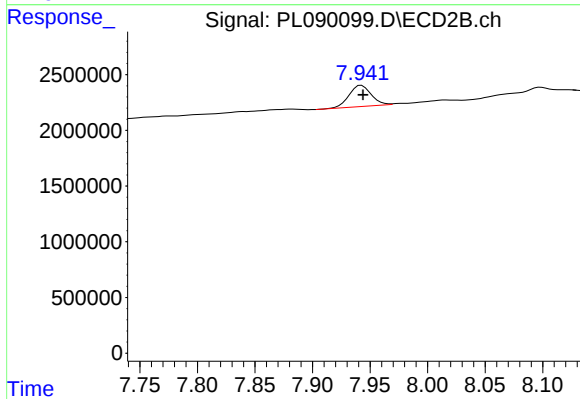

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: -0.001 min
Response: 2533470
Conc: 1.70 ng/ml