

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
 Data File : PL049414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 12:12
 Operator : SM\AJ
 Sample : WATER IDOC BL
 Misc : FOR RC
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WATER IDOC BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:10:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.330	3.937	247.1E6	67145644	22.429	23.241
28) SA Decachlor...	7.998	8.975	220.0E6	65187034	17.304	19.519

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
Data File : PL049414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 12:12
Operator : SM\AJ
Sample : WATER IDOC BL
Misc : FOR RC
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WATER IDOC BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:10:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

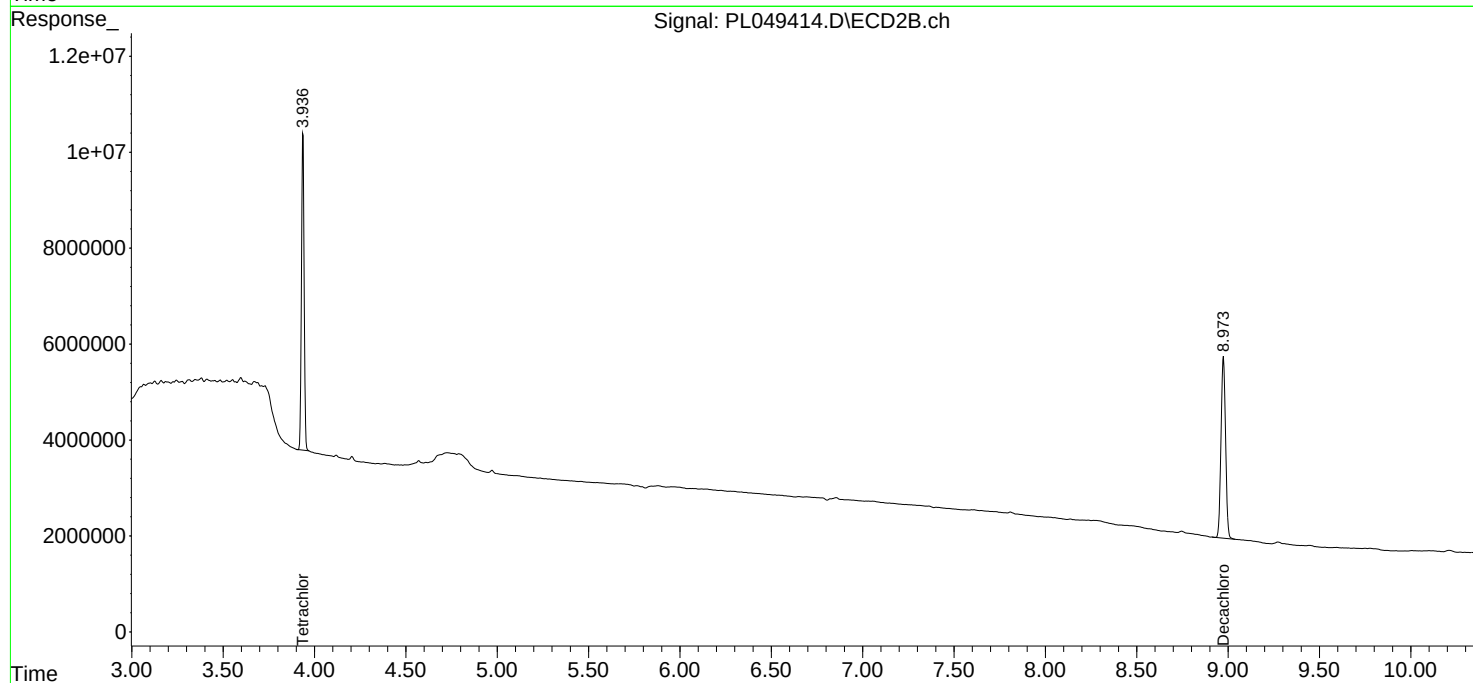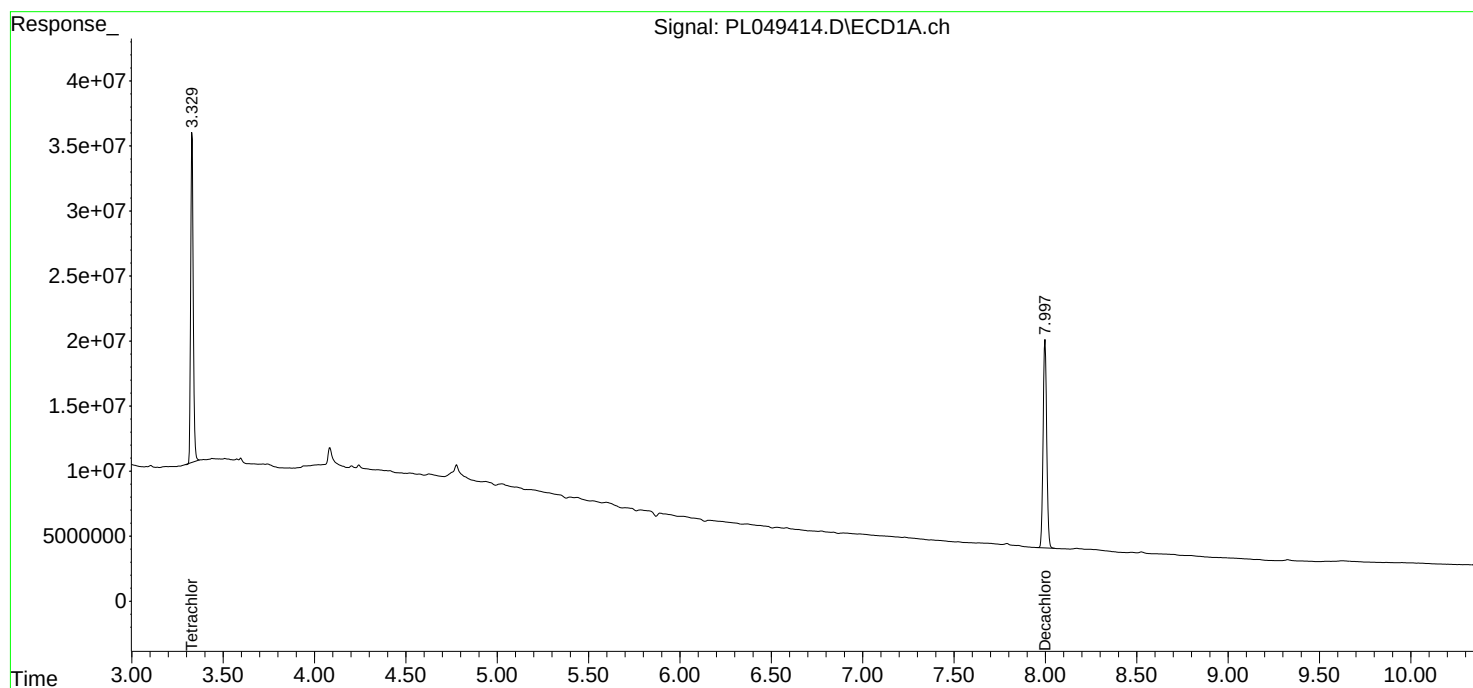


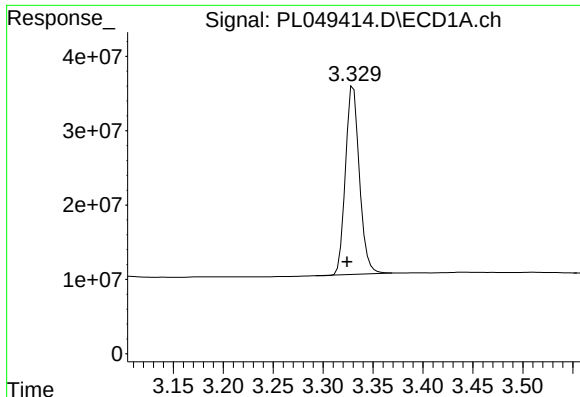

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.006 min
Response: 247145036
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
WATER IDOC BL

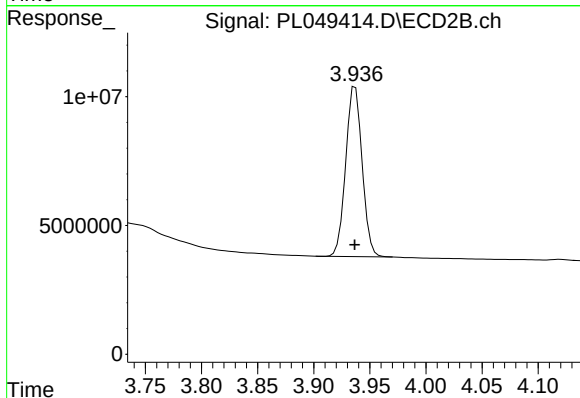


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 67145644
Conc: 23.24 ng/ml

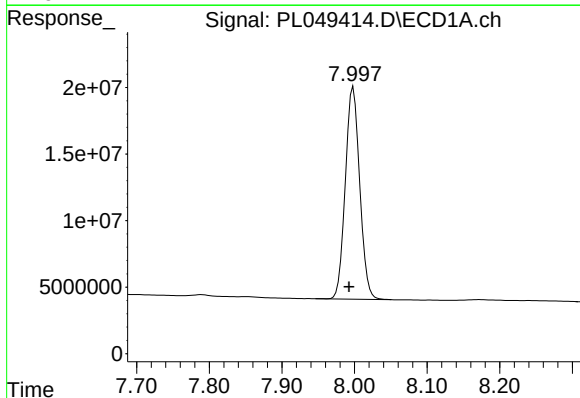

#28 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: 0.006 min
Response: 220029135
Conc: 17.30 ng/ml

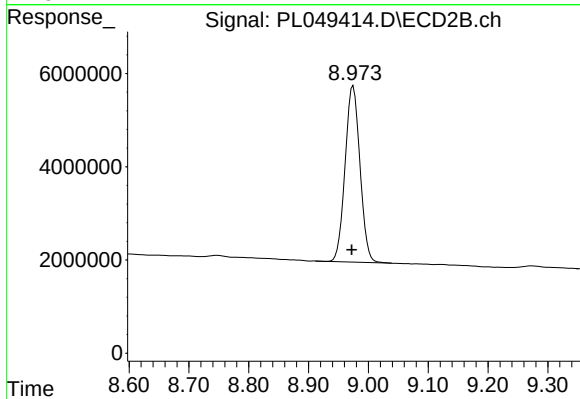

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.002 min
Response: 65187034
Conc: 19.52 ng/ml