

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
 Data File : PL049423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 14:28
 Operator : SM\AJ
 Sample : K3282-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 25082-2022

Manual Integrations
 APPROVED

Ankita
 6/12/2019 9:19:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:12:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.936	190.0E6	52598830	17.247	18.206
28)	SA Decachlor...	7.991	8.972	108.4E6	36798769	8.521	11.019 #
Target Compounds							
10)	B gamma-Chl...	5.210	6.031	12713390	4574840	0.796m	1.323m#
11)	B alpha-Chl...	5.267	6.107	24344394	8373632	1.558	2.414 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
Data File : PL049423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 14:28
Operator : SM\AJ
Sample : K3282-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
25082-2022


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:12:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

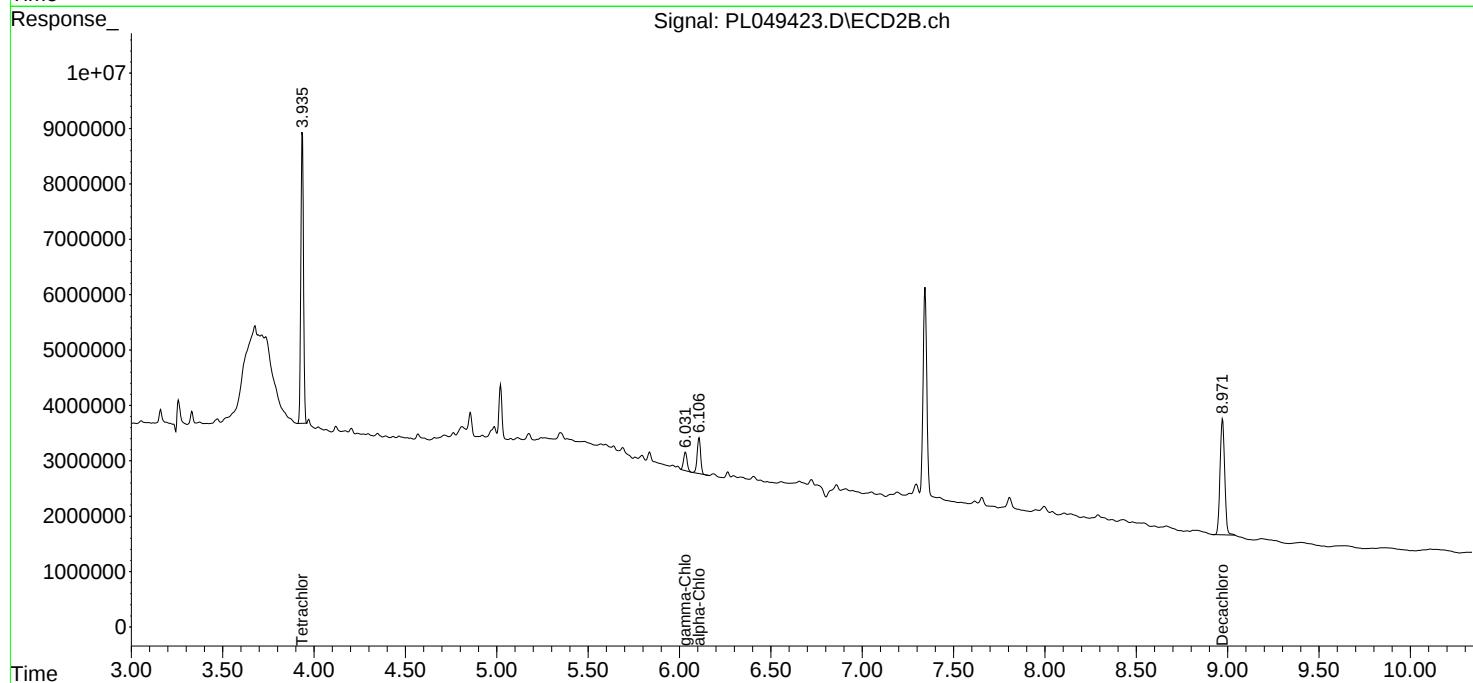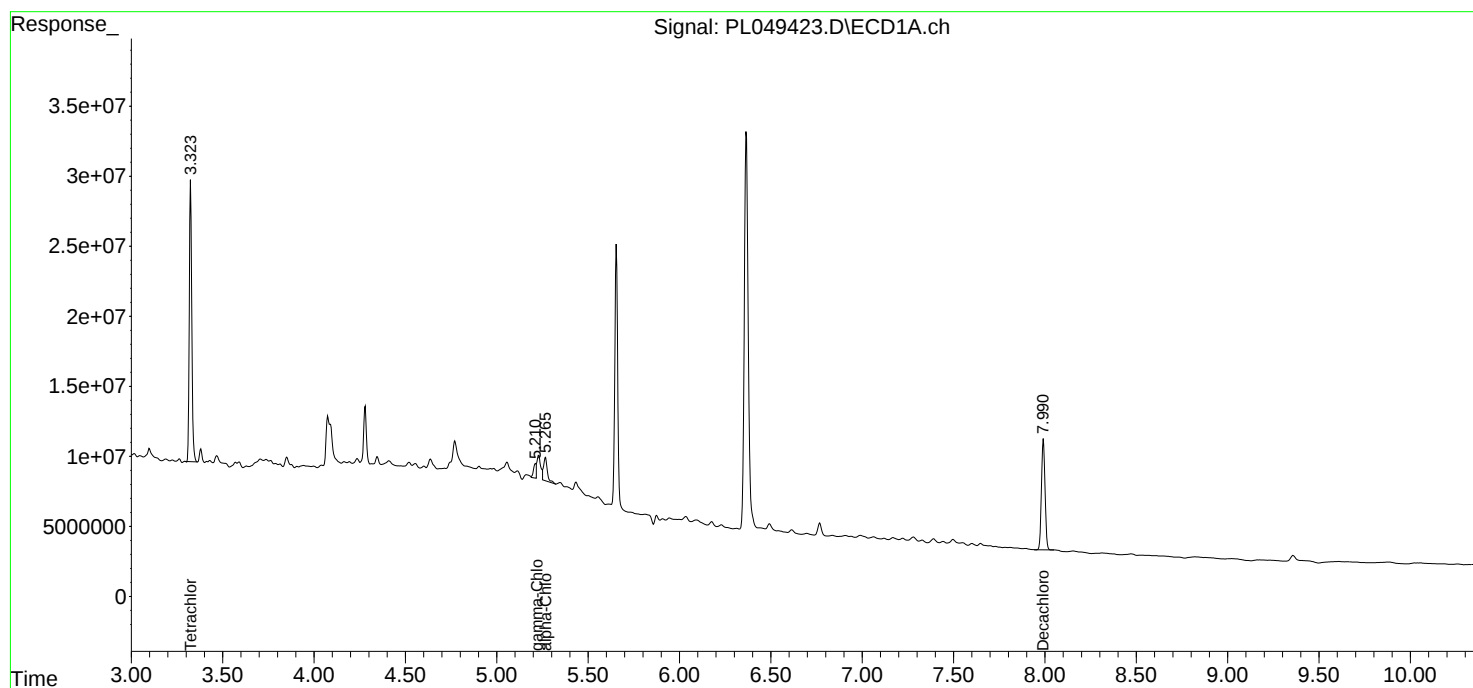

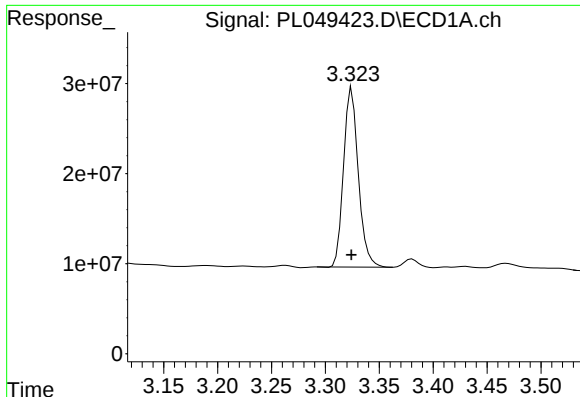


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 190038791
Conc: 17.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
25082-2022


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:39 AM

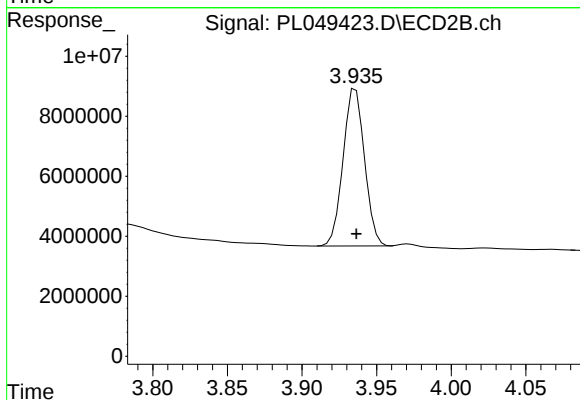


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 52598830
Conc: 18.21 ng/ml

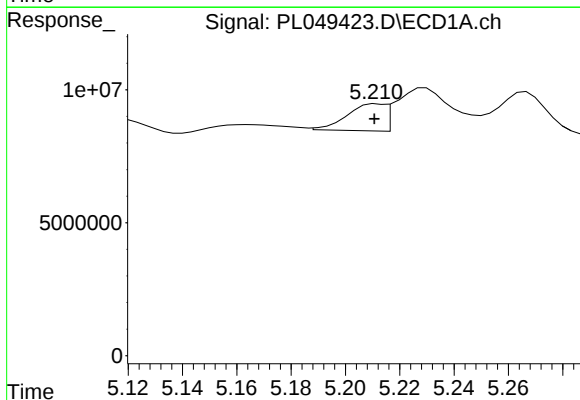


#10 gamma-Chlordane

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 12713390
Conc: 0.80 ng/ml m

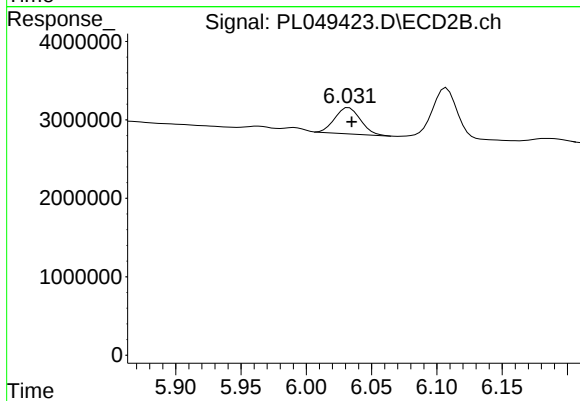

#10 gamma-Chlordane

R.T.: 6.031 min
Delta R.T.: -0.003 min
Response: 4574840
Conc: 1.32 ng/ml m

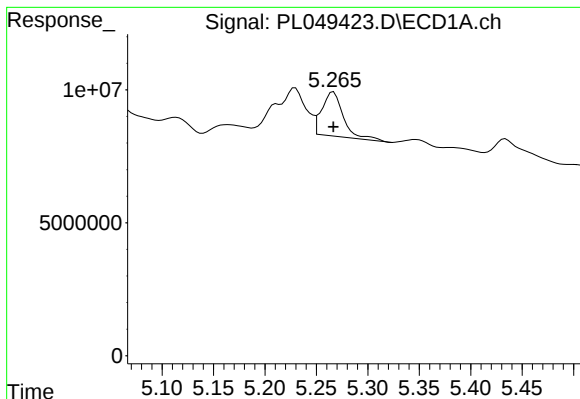


#11 alpha-Chlordane

R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 24344394
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
25082-2022


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:39 AM

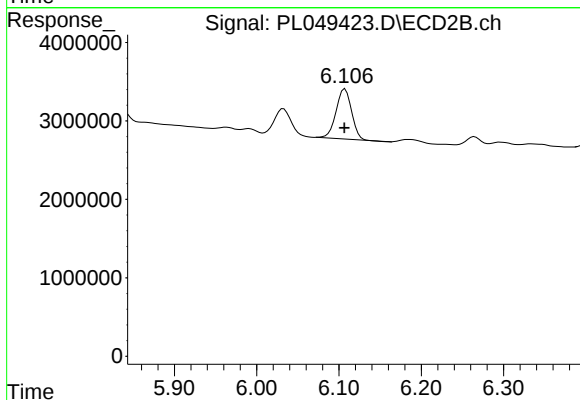


#11 alpha-Chlordane

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 8373632
Conc: 2.41 ng/ml

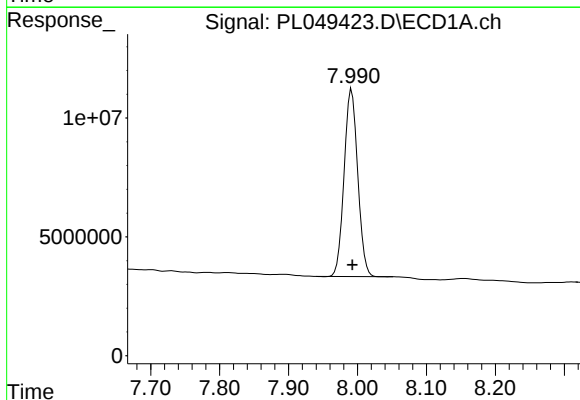

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 108351722
Conc: 8.52 ng/ml

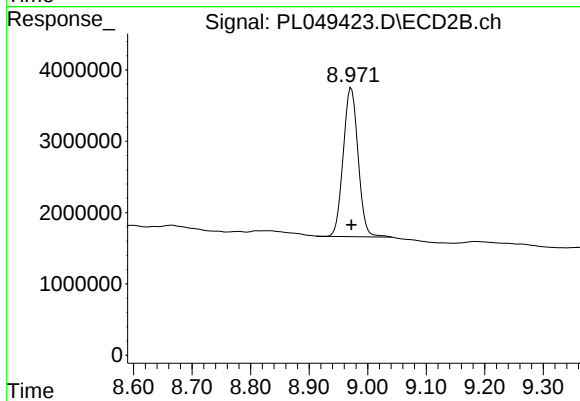

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 36798769
Conc: 11.02 ng/ml