

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
 Data File : PL049424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2019 14:43
 Operator : SM\AJ
 Sample : K3283-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 200030-200034

Manual Integrations
 APPROVED

Ankita
 6/12/2019 9:19:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 01:12:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.936	135.1E6	37130543	12.263	12.852
28)	SA Decachlor...	7.991	8.972	109.1E6	35699765	8.584	10.690
Target Compounds							
12)	B 4,4'-DDE	5.434	6.265	60070650	13339413	3.840	4.064
17)	MA 4,4'-DDT	6.177	7.053	36971459	9885315	3.003m	3.526

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061119\
Data File : PL049424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2019 14:43
Operator : SM\AJ
Sample : K3283-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
200030-200034


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 01:12:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

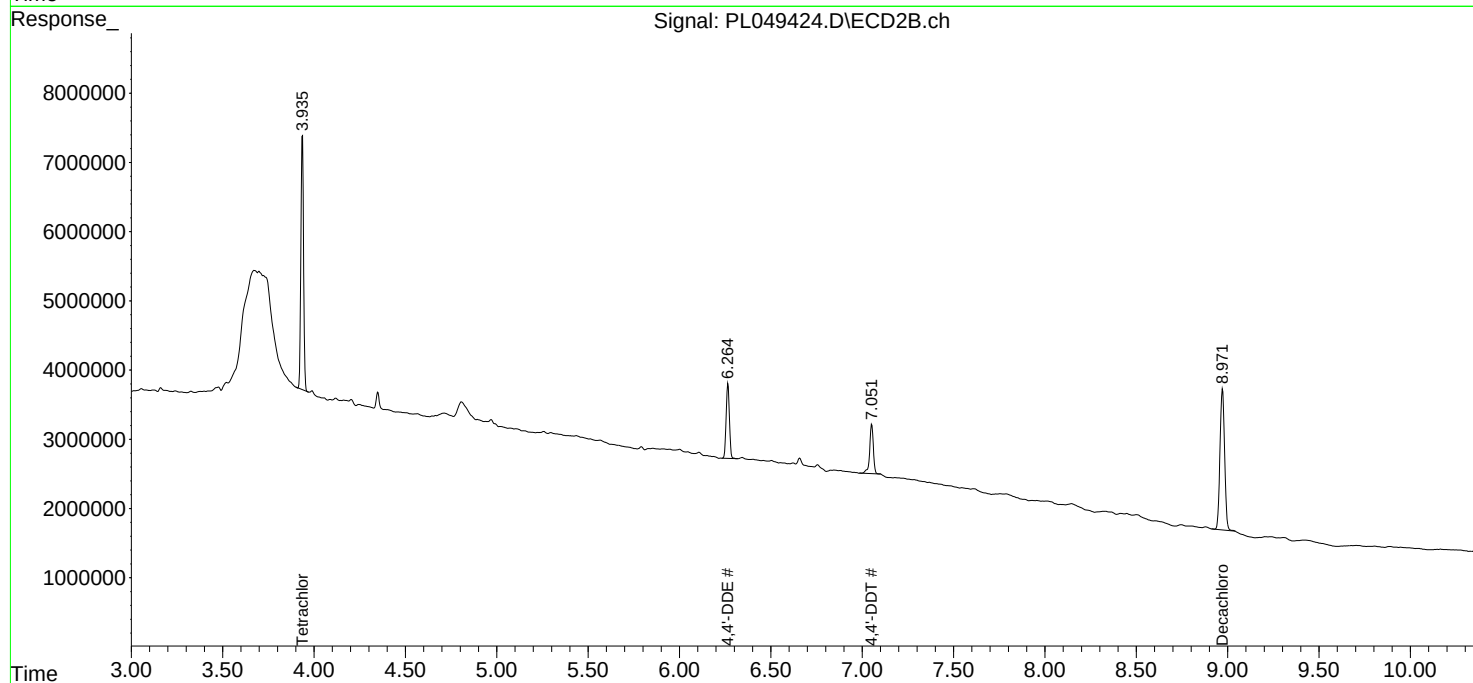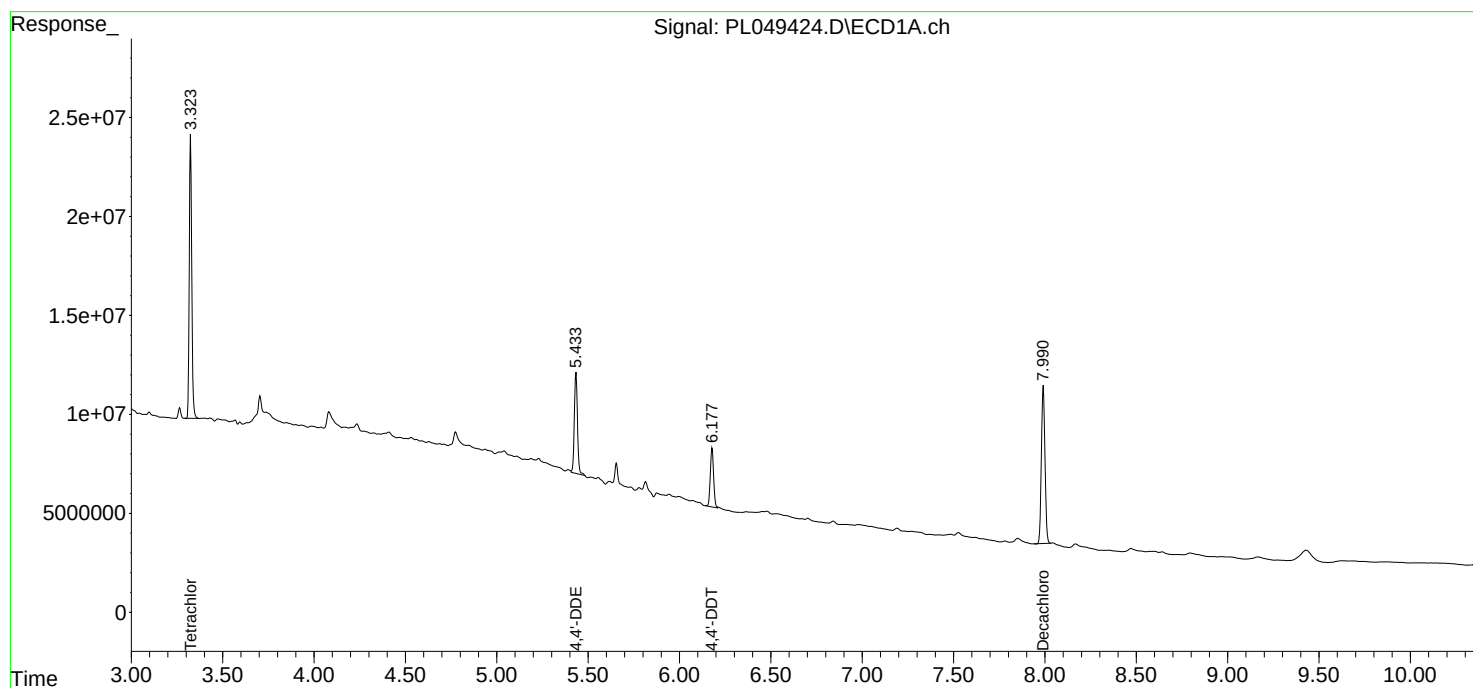

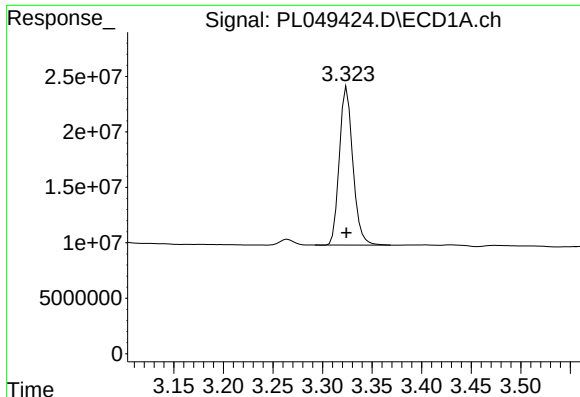


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.000 min
Response: 135121459
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
200030-200034


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:41 AM

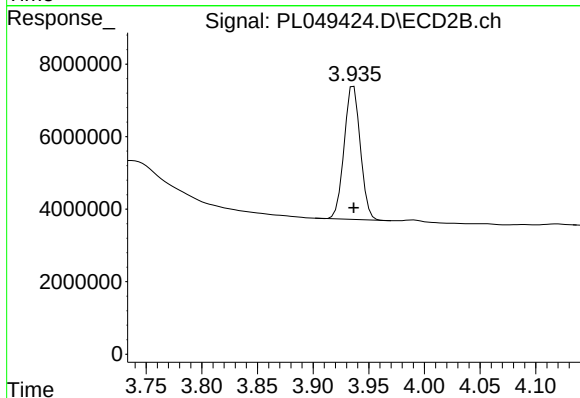


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 37130543
Conc: 12.85 ng/ml

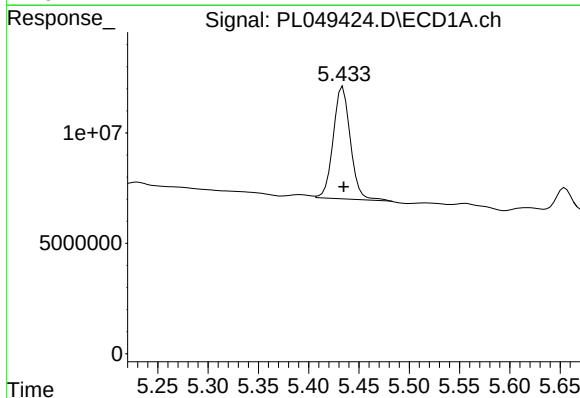


#12 4,4'-DDE

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 60070650
Conc: 3.84 ng/ml

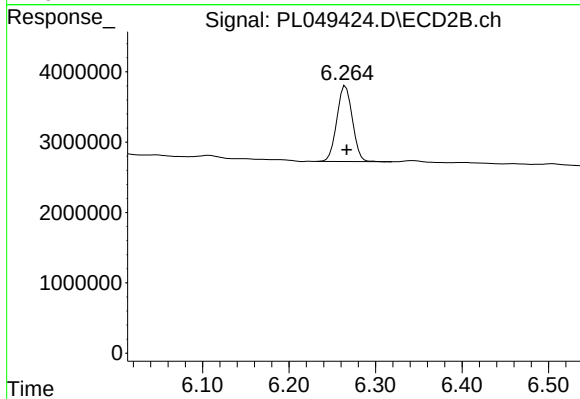

#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.001 min
Response: 13339413
Conc: 4.06 ng/ml

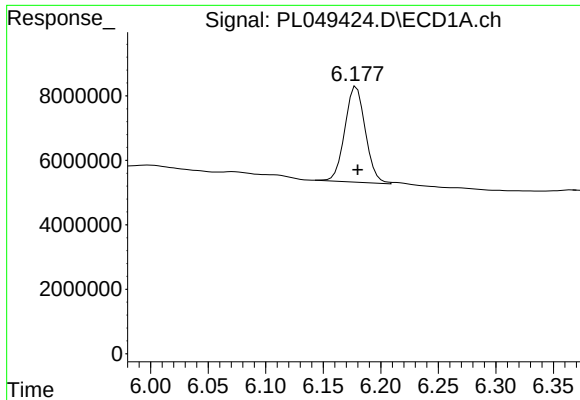


#17 4,4'-DDT

R.T.: 6.177 min
Delta R.T.: -0.003 min
Response: 36971459
Conc: 3.00 ng/ml m

Instrument :
ECD_L
ClientSampleId :
200030-200034


Manual Integrations
APPROVED

Ankita
6/12/2019 9:19:41 AM

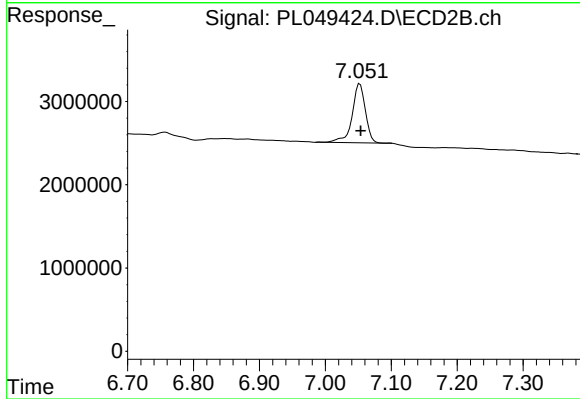


#17 4,4'-DDT

R.T.: 7.053 min
Delta R.T.: -0.001 min
Response: 9885315
Conc: 3.53 ng/ml

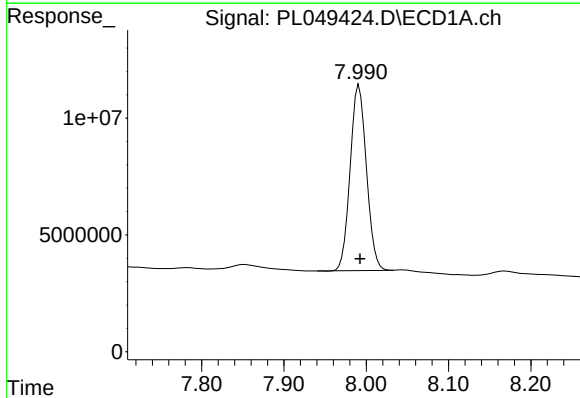

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.001 min
Response: 109146021
Conc: 8.58 ng/ml

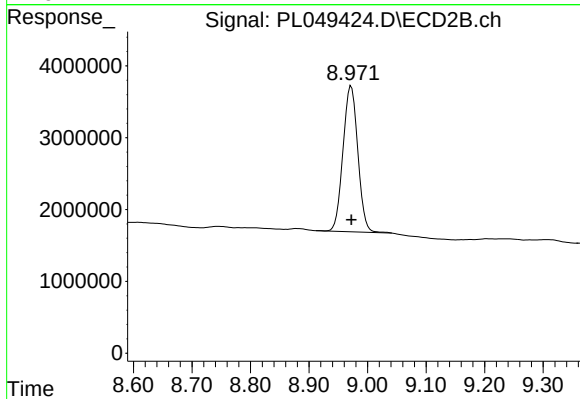

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 35699765
Conc: 10.69 ng/ml