

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
 Data File : PL096006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 10:55
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 13:45:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 13:41:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.883	226.8E6	383.6E6	74.669	75.054
28)	SA Decachlor...	9.111	8.065	170.6E6	362.0E6	75.688	76.392
Target Compounds							
23)	Chlordane-1	4.737	3.900	131.6E6	149.0E6	748.300	754.247
24)	Chlordane-2	5.264	4.481	138.3E6	162.5E6	753.351	756.148
25)	Chlordane-3	5.970	5.117	551.0E6	542.2E6	760.011	760.981
26)	Chlordane-4	6.055	5.181	644.6E6	469.9E6	757.204	762.620
27)	Chlordane-5	6.896	6.079	111.8E6	196.8E6	757.261	762.165



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
Data File : PL096006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 10:55
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 13:45:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 13:41:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

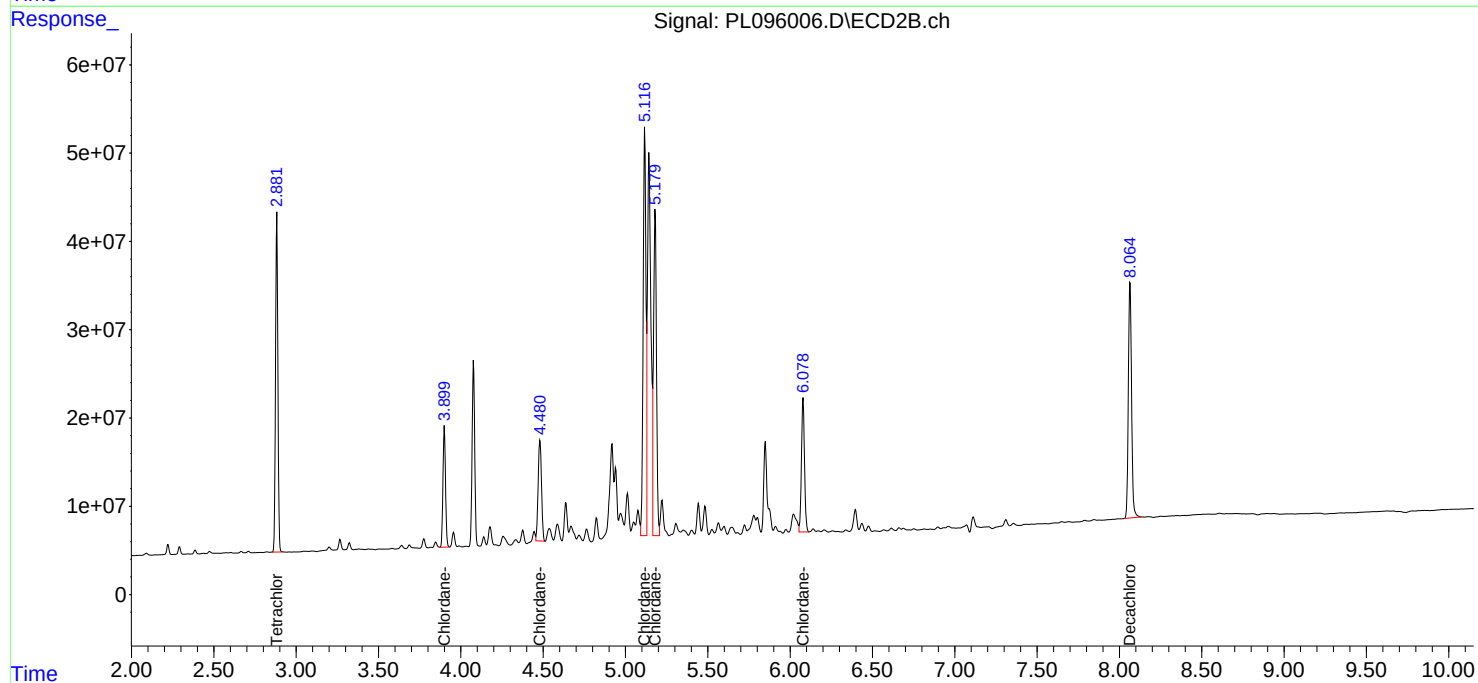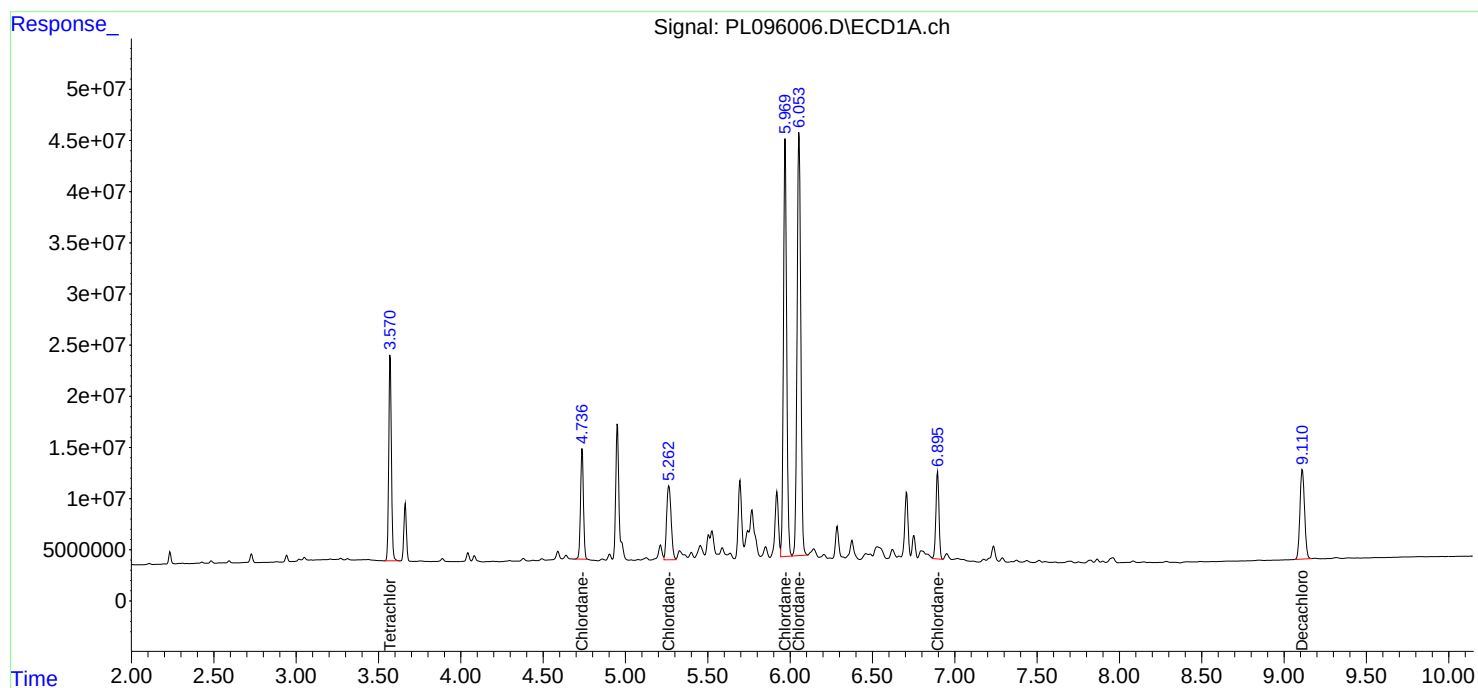


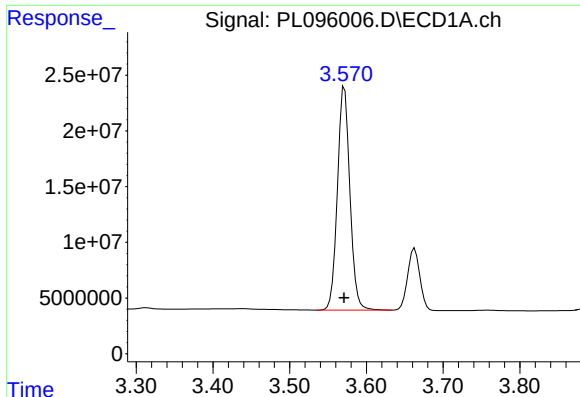

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 226788580
Conc: 74.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

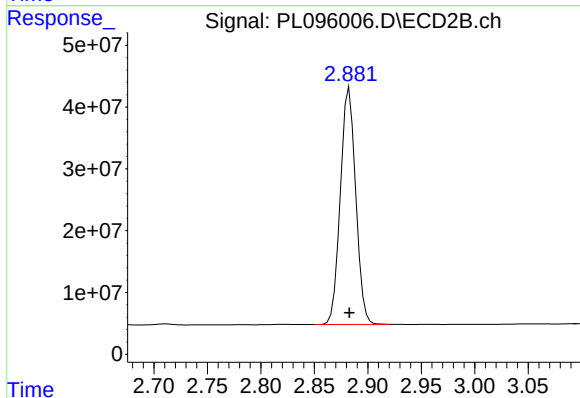


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 383593576
Conc: 75.05 ng/ml

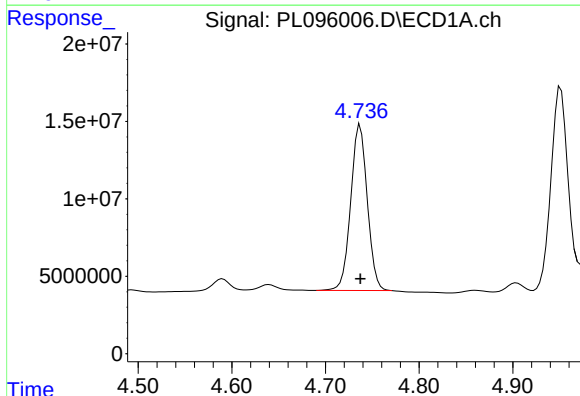


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 131558737
Conc: 748.30 ng/ml

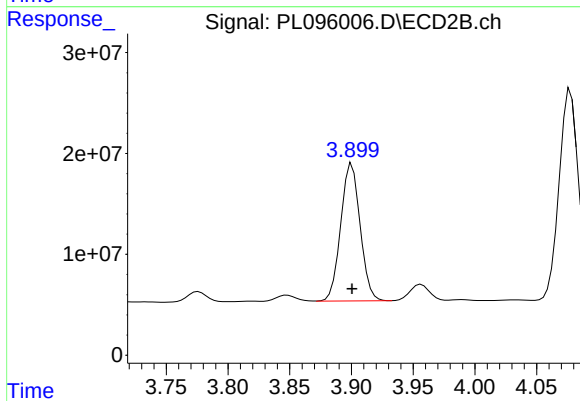

#23 Chlordane-1


R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 149006900
Conc: 754.25 ng/ml

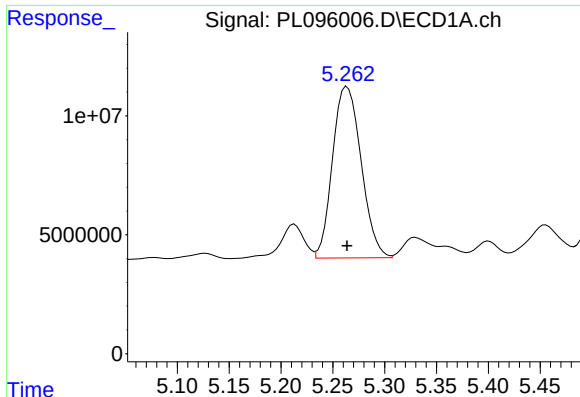

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 138348546
Conc: 753.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

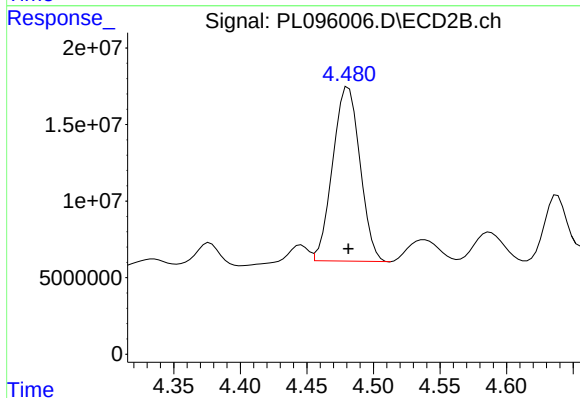


#24 Chlordane-2

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 162518705
Conc: 756.15 ng/ml

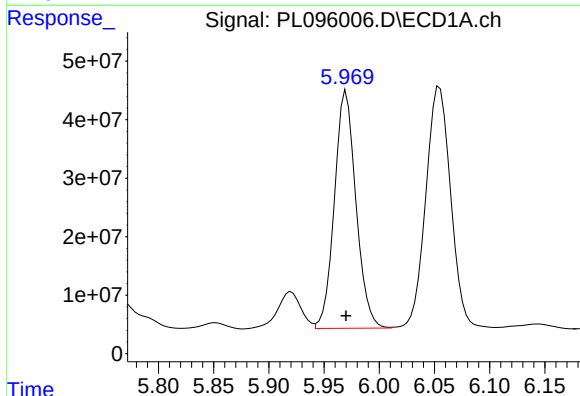


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 550965148
Conc: 760.01 ng/ml

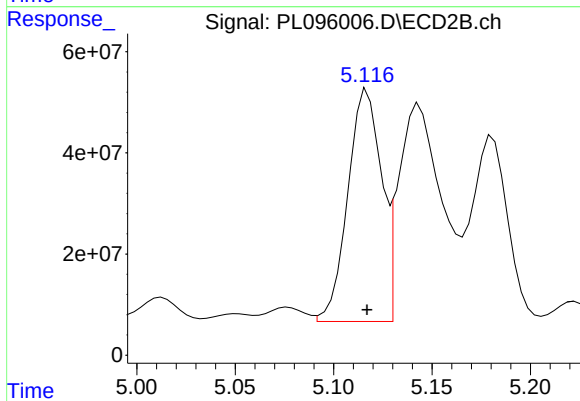

#25 Chlordane-3


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 542234847
Conc: 760.98 ng/ml

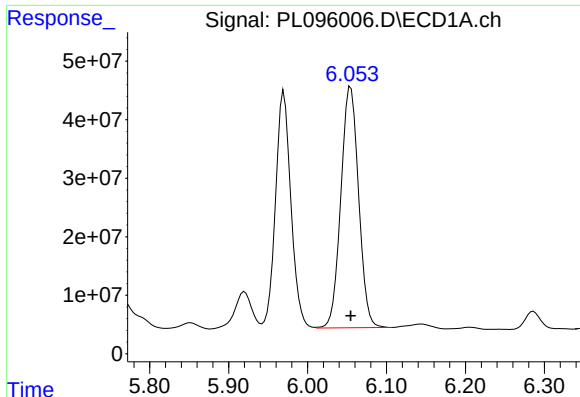

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 644631334
Conc: 757.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

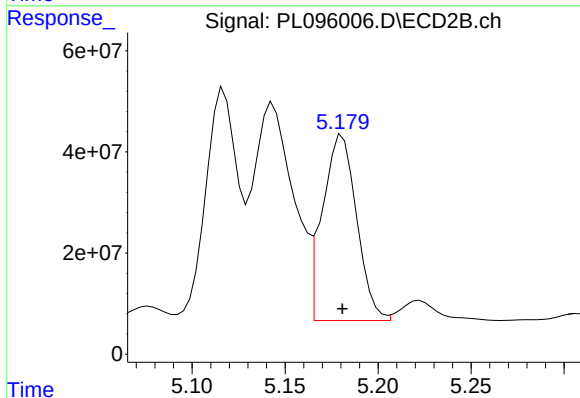


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 469867749
Conc: 762.62 ng/ml

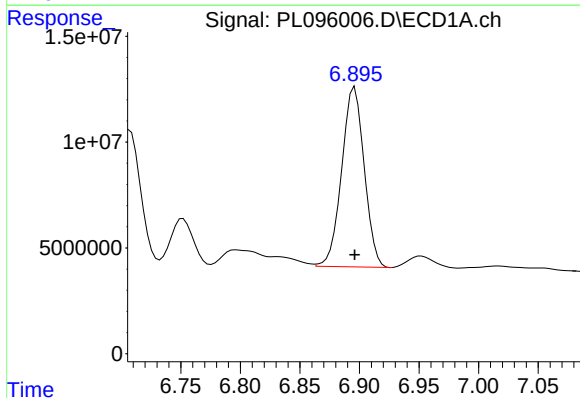


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 111807622
Conc: 757.26 ng/ml

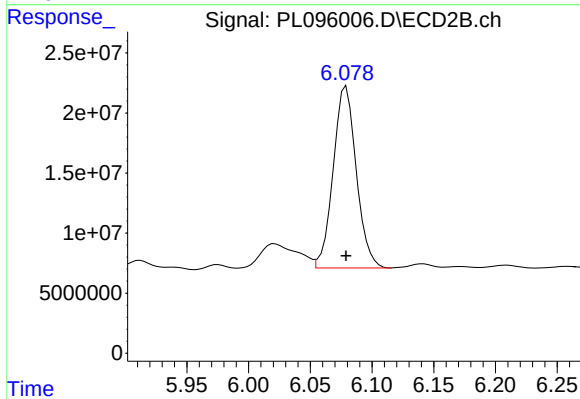

#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 196836416
Conc: 762.16 ng/ml

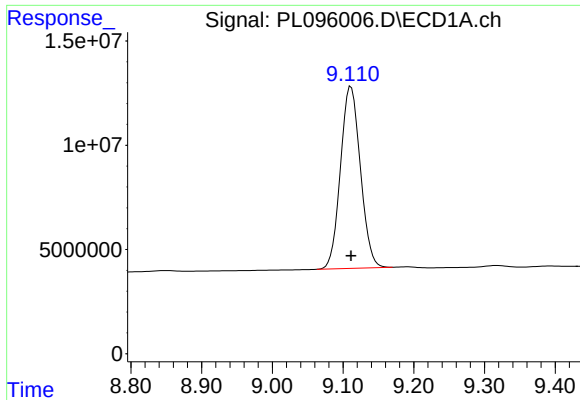

#28 Decachlorobiphenyl


R.T.: 9.111 min

Delta R.T.: 0.000 min

Response: 170632974

Conc: 75.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

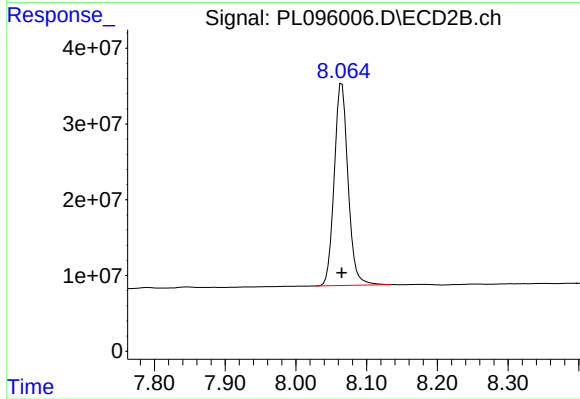

#28 Decachlorobiphenyl

R.T.: 8.065 min

Delta R.T.: 0.000 min

Response: 362037943

Conc: 76.39 ng/ml