

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
 Data File : PL096005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 10:41
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 13:43:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 13:41:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.883	308.4E6	520.7E6	101.318	101.908
28)	SA Decachlor...	9.112	8.065	223.5E6	472.0E6	99.576	100.536
Target Compounds							
23)	Chlordane-1	4.737	3.901	178.6E6	202.7E6	1014.985	1029.101
24)	Chlordane-2	5.265	4.482	183.9E6	217.4E6	1003.546	1015.434
25)	Chlordane-3	5.970	5.118	737.8E6	733.0E6	1024.598	1036.319
26)	Chlordane-4	6.055	5.182	867.6E6	628.4E6	1024.021	1028.509
27)	Chlordane-5	6.896	6.079	148.9E6	265.4E6	1013.067	1036.182



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
Data File : PL096005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 10:41
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 13:43:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 13:41:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

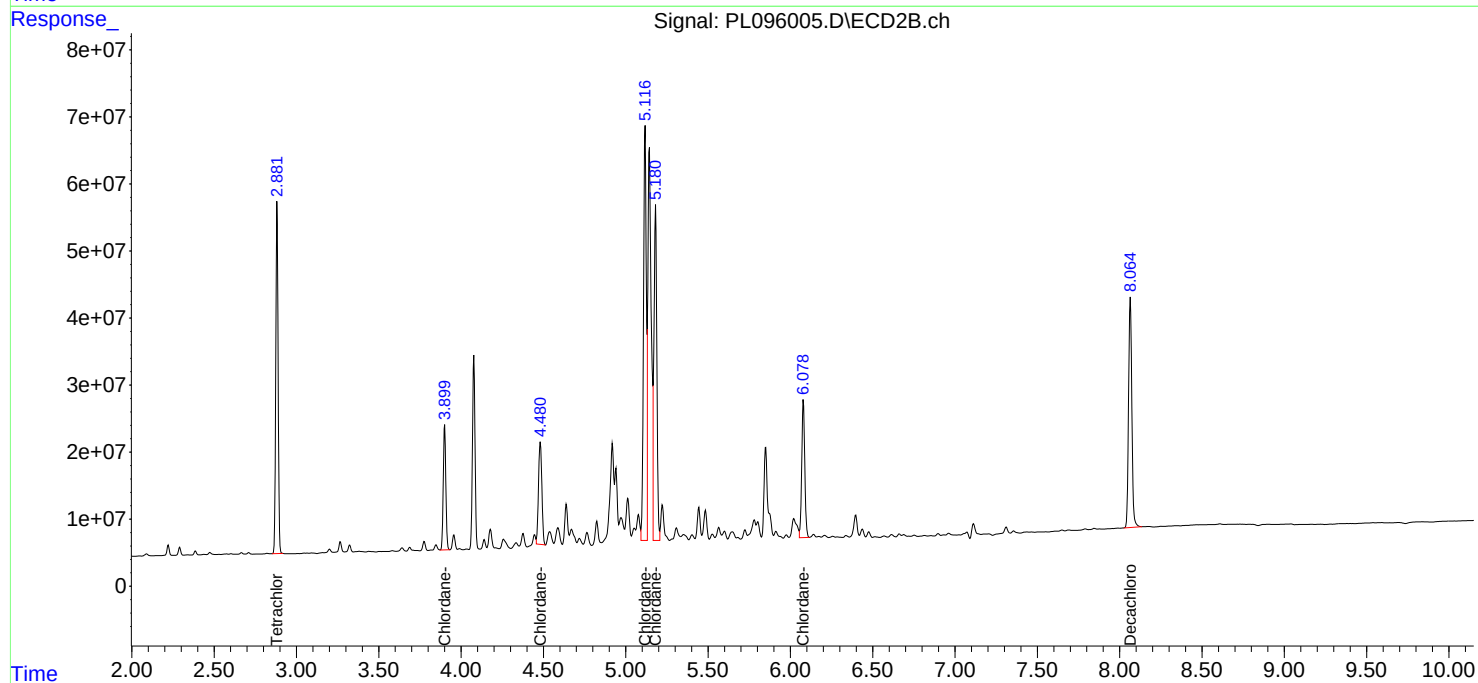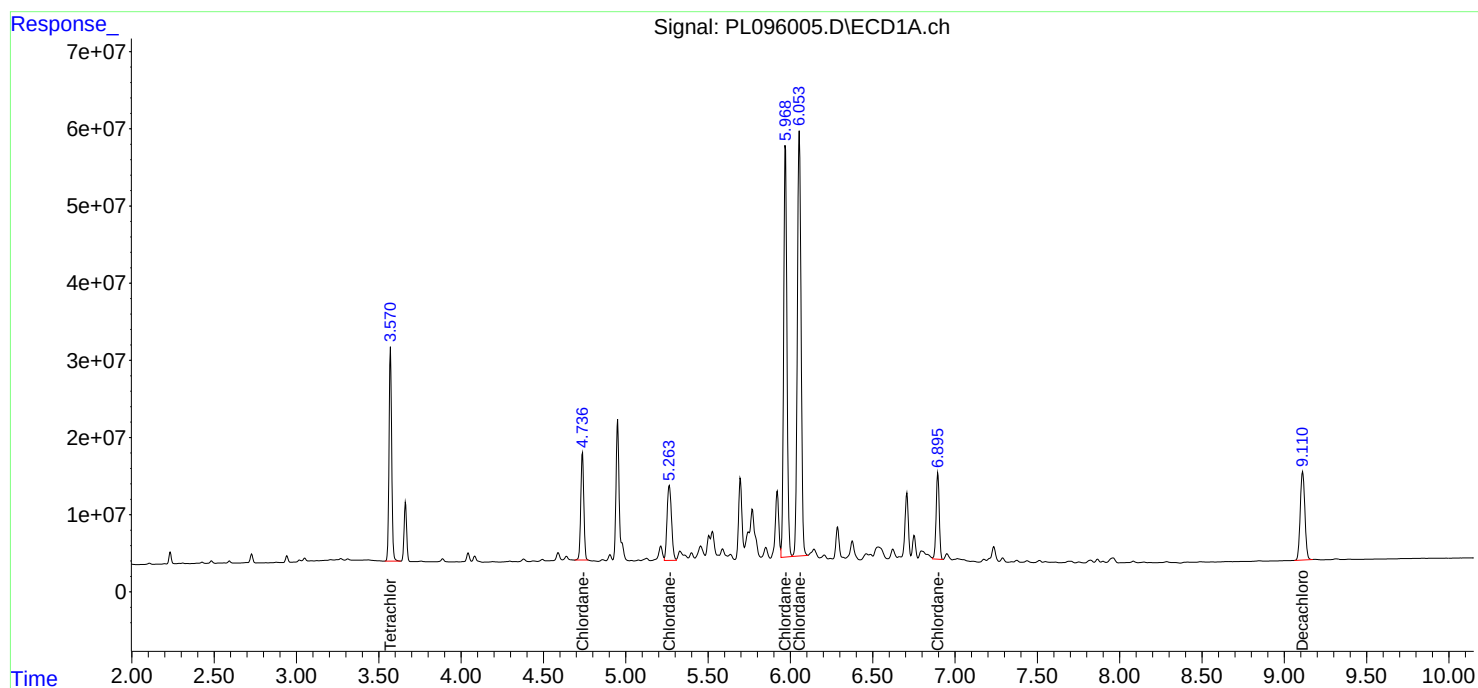


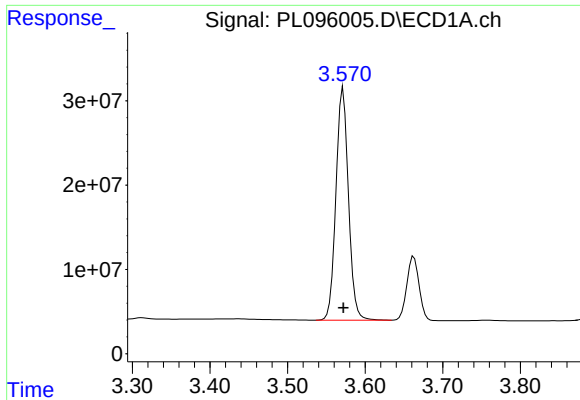

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: 0.000 min
Response: 308405475
Conc: 101.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

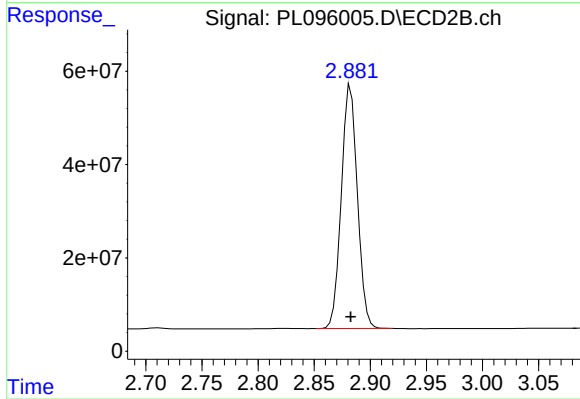


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 520653985
Conc: 101.91 ng/ml

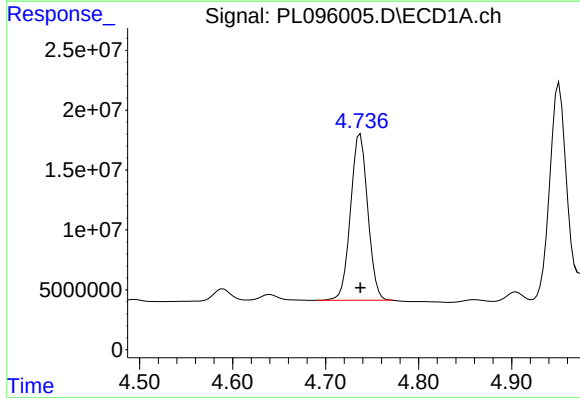


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 178646782
Conc: 1014.98 ng/ml

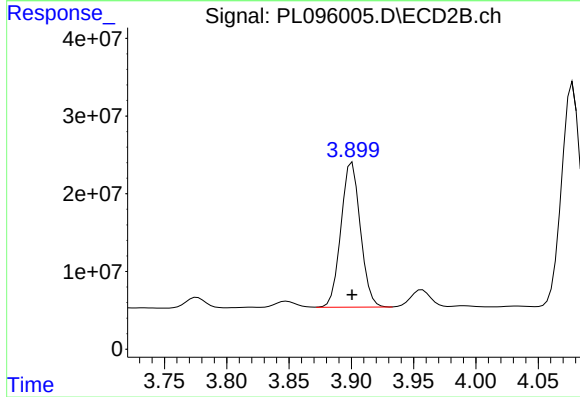

#23 Chlordane-1


R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 202730837
Conc: 1029.10 ng/ml

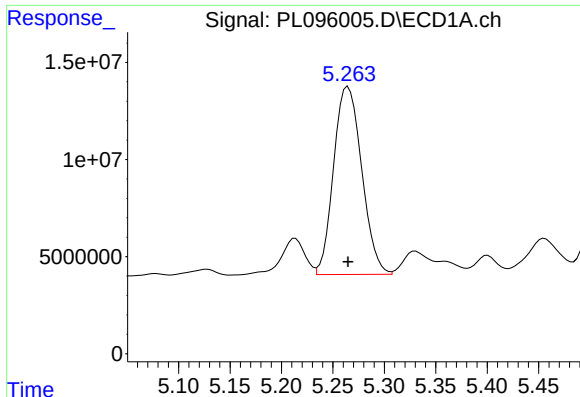

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 183883730
Conc: 1003.55 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

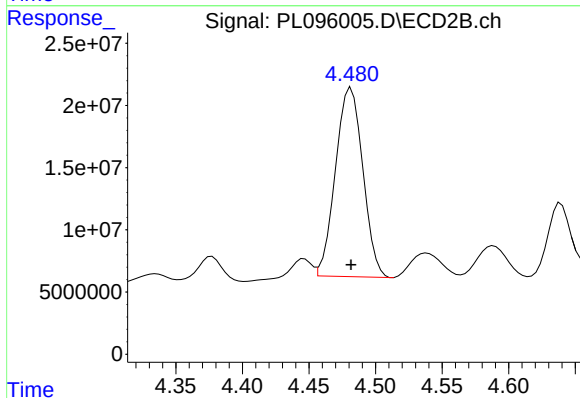


#24 Chlordane-2

R.T.: 4.482 min
Delta R.T.: 0.000 min
Response: 217352247
Conc: 1015.43 ng/ml

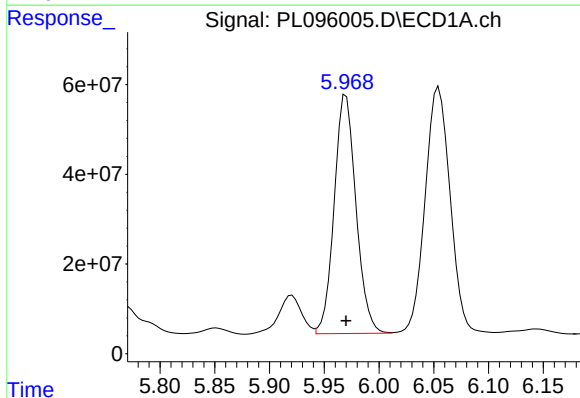


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 737817685
Conc: 1024.60 ng/ml

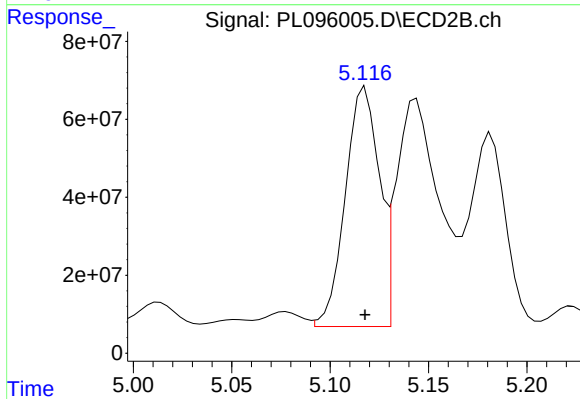

#25 Chlordane-3


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 733019465
Conc: 1036.32 ng/ml

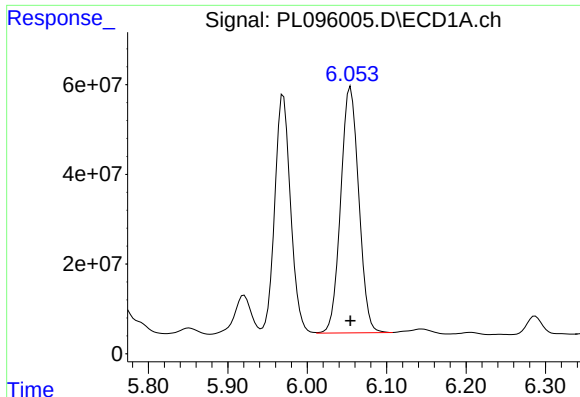

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 867593938
Conc: 1024.02 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

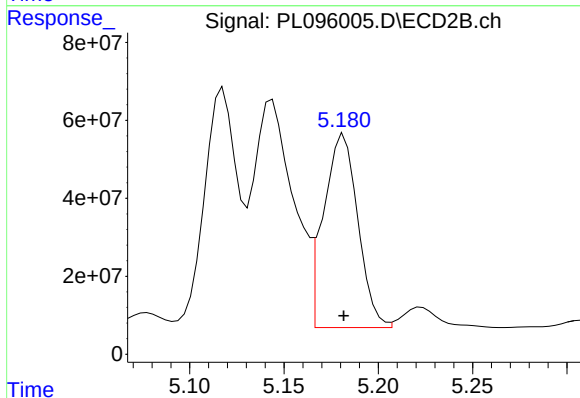


#26 Chlordane-4

R.T.: 5.182 min
Delta R.T.: 0.000 min
Response: 628357173
Conc: 1028.51 ng/ml

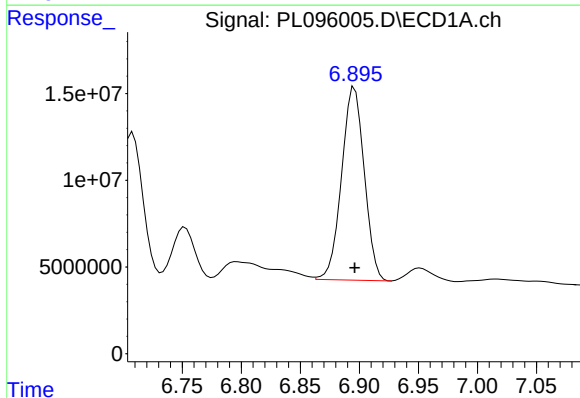


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 148852582
Conc: 1013.07 ng/ml

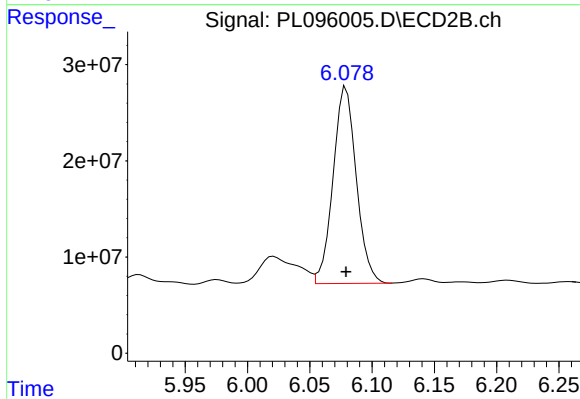

#27 Chlordane-5


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 265433852
Conc: 1036.18 ng/ml

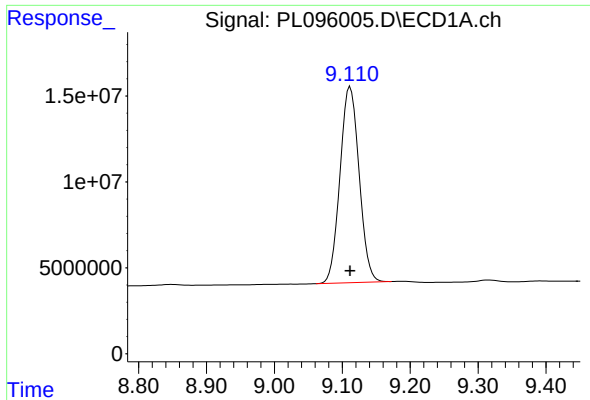

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 223458116
Conc: 99.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

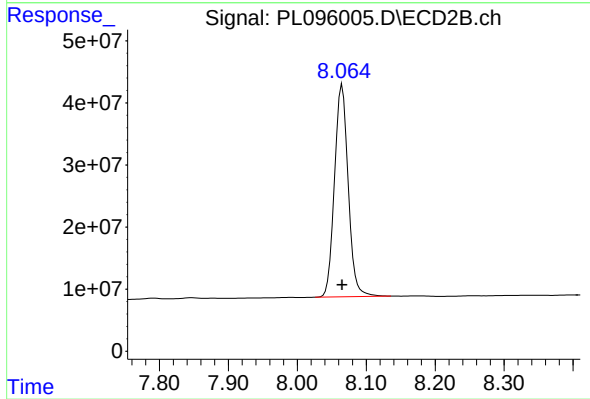

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 472040757
Conc: 100.54 ng/ml