

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
 Data File : PL096008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 11:22
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 13:47:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 13:41:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.882	78974428	127.8E6	25.744	24.999
28)	SA Decachlor...	9.114	8.065	61448113	122.4E6	26.655	25.621
Target Compounds							
23)	Chlordane-1	4.737	3.901	45821835	48677834	257.891	247.289
24)	Chlordane-2	5.264	4.482	48881663	55826583	261.939	257.237
25)	Chlordane-3	5.970	5.117	180.4E6	172.6E6	249.093	244.177
26)	Chlordane-4	6.055	5.181	214.8E6	153.5E6	251.733	249.322
27)	Chlordane-5	6.896	6.079	38443049	62748513	257.698	244.688



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
Data File : PL096008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 11:22
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 13:47:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 13:41:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

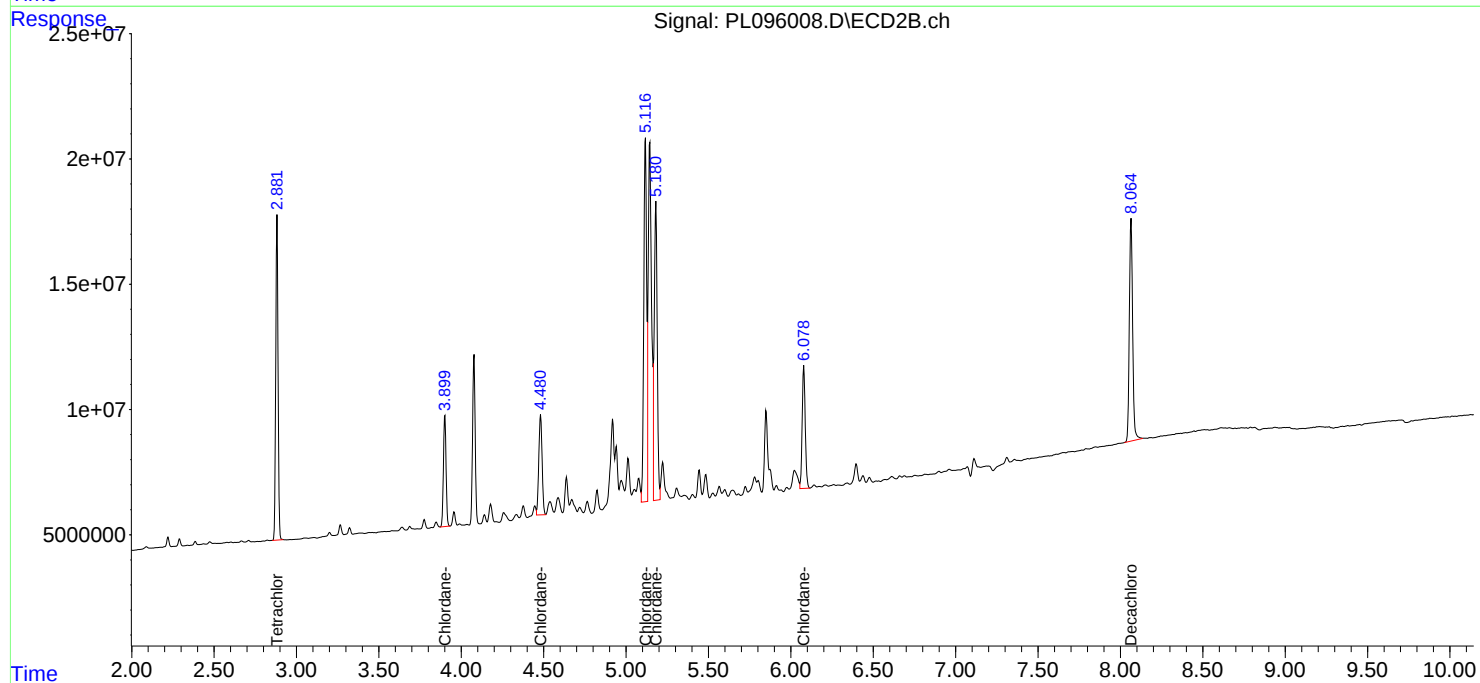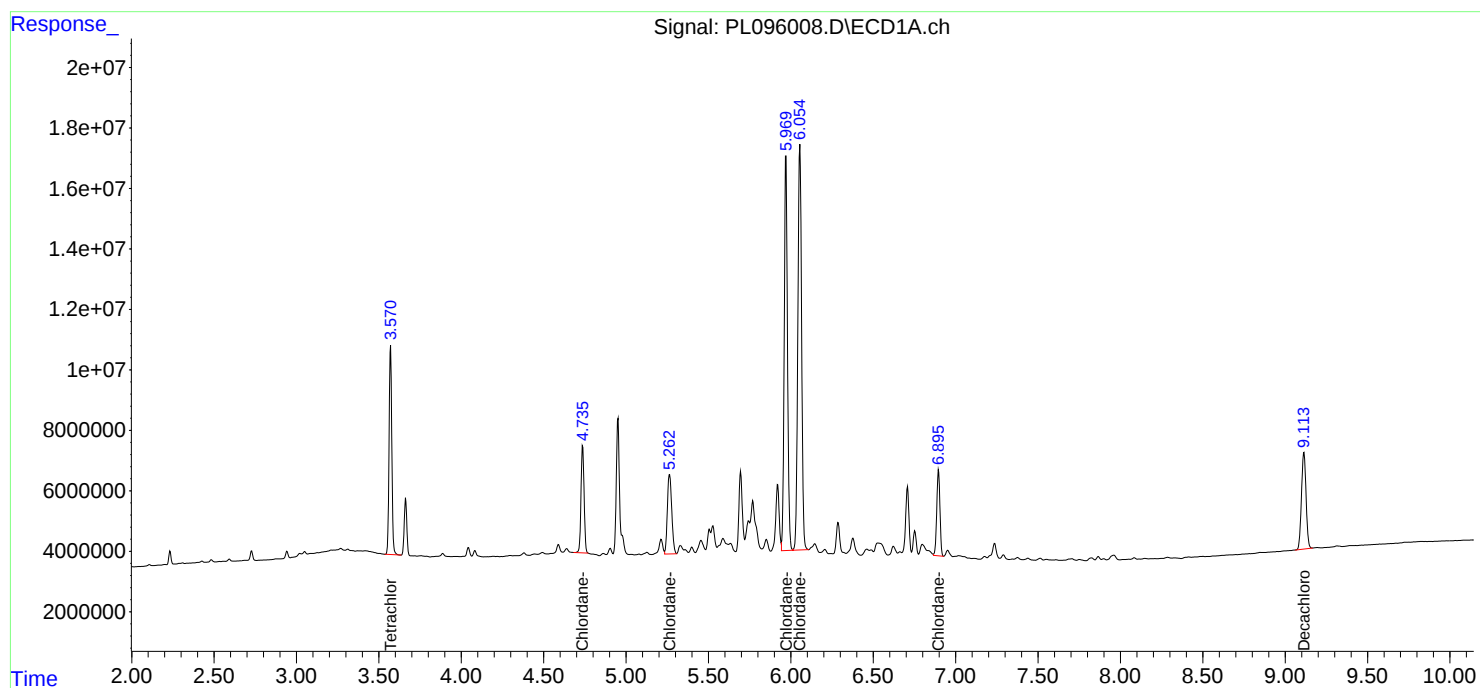


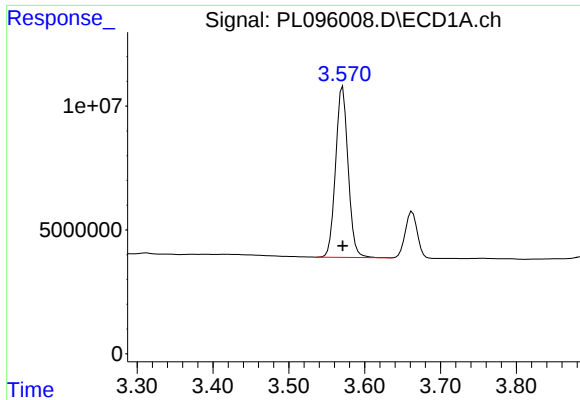

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 78974428
Conc: 25.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

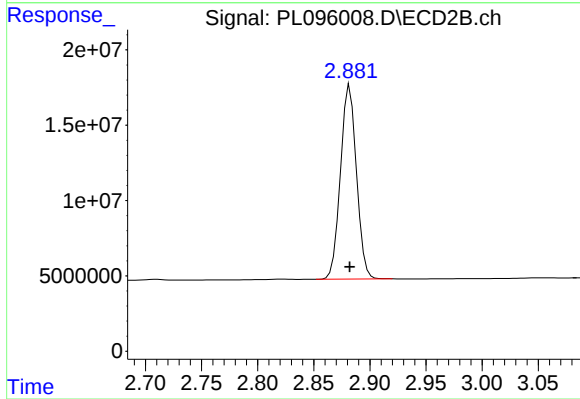


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 127765742
Conc: 25.00 ng/ml

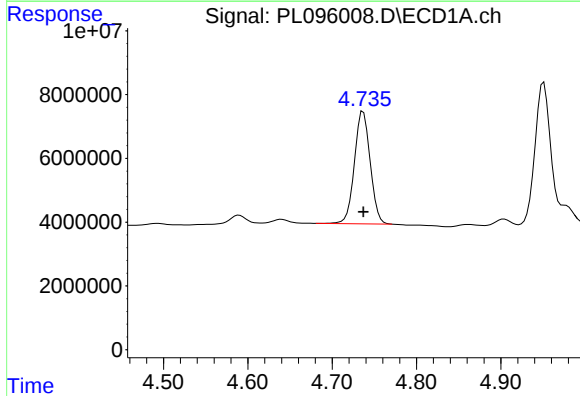


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 45821835
Conc: 257.89 ng/ml

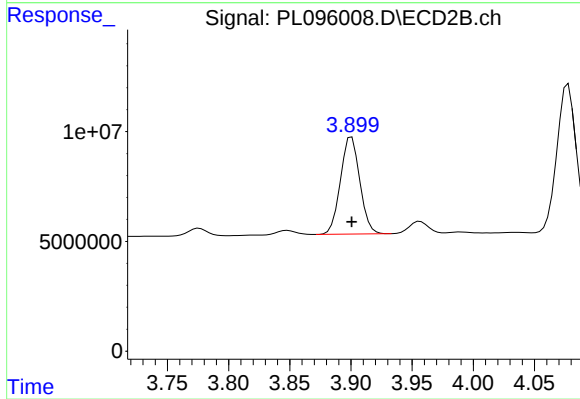

#23 Chlordane-1


R.T.: 3.901 min
Delta R.T.: 0.000 min
Response: 48677834
Conc: 247.29 ng/ml

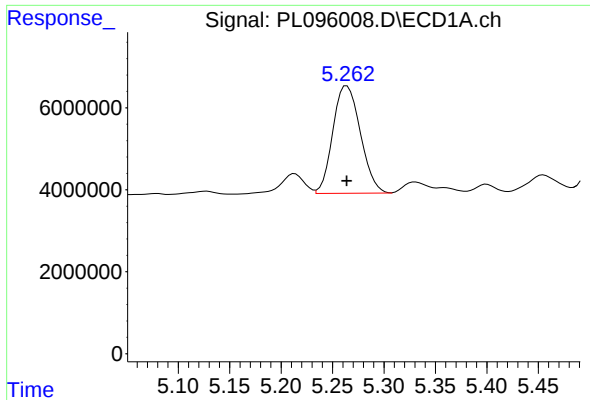

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 48881663
Conc: 261.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

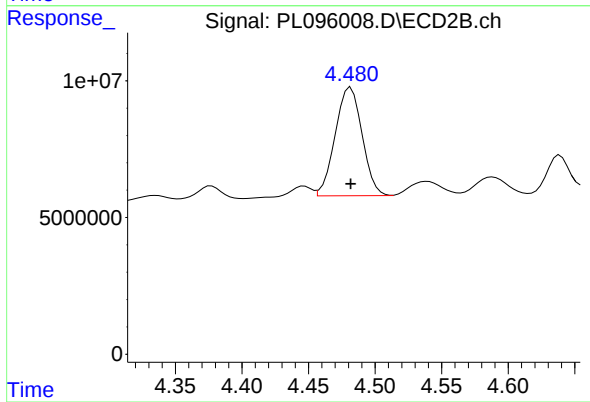


#24 Chlordane-2

R.T.: 4.482 min
Delta R.T.: 0.000 min
Response: 55826583
Conc: 257.24 ng/ml

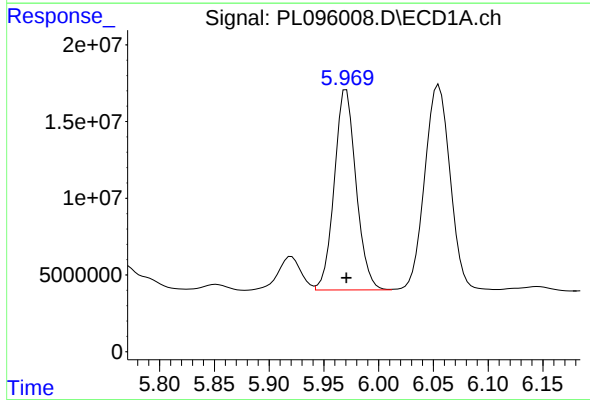


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 180360509
Conc: 249.09 ng/ml

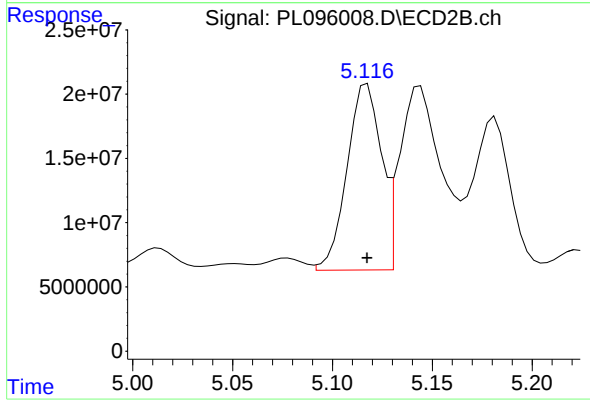

#25 Chlordane-3


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 172646859
Conc: 244.18 ng/ml

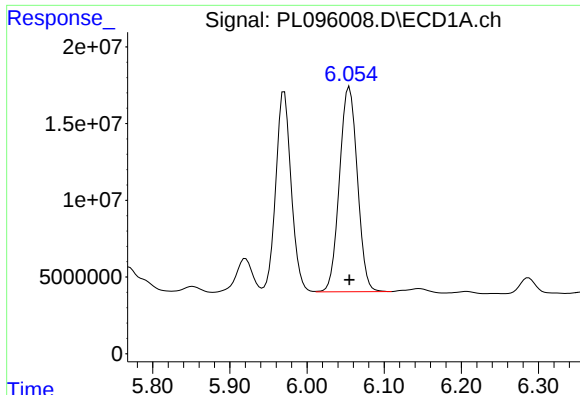

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 214804738
Conc: 251.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

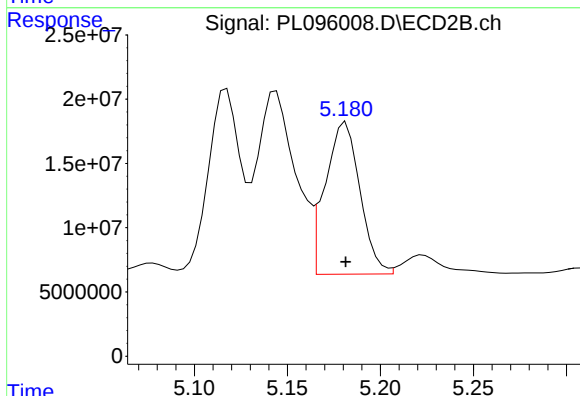


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 153474689
Conc: 249.32 ng/ml

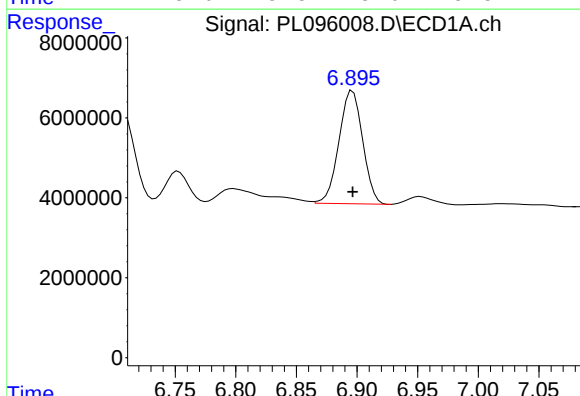


#27 Chlordane-5

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 38443049
Conc: 257.70 ng/ml

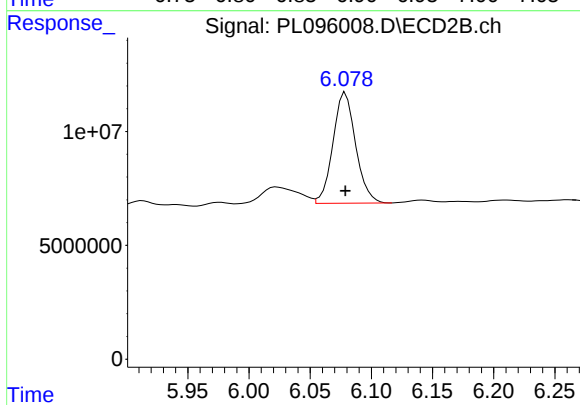

#27 Chlordane-5


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 62748513
Conc: 244.69 ng/ml

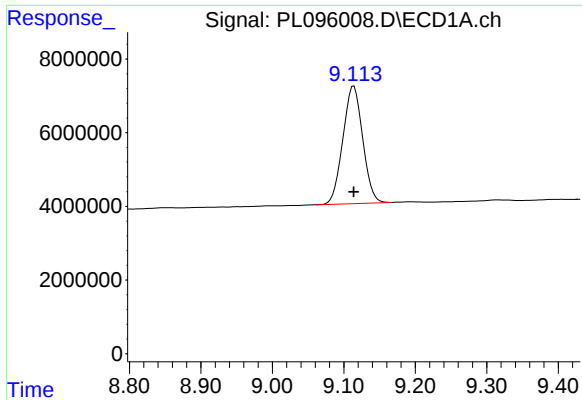

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 61448113
Conc: 26.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

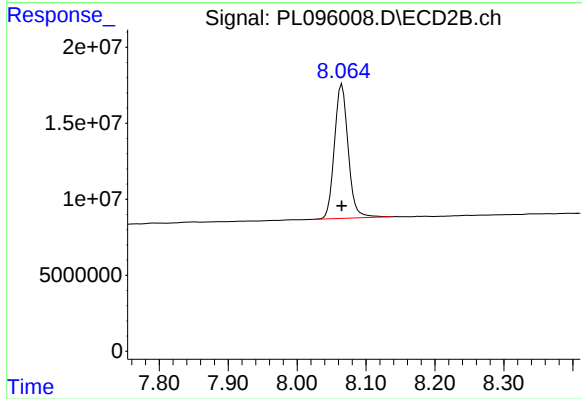

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 122438918
Conc: 25.62 ng/ml