

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
 Data File : PL096016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 13:11
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL061125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 13:51:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 11 13:50:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.882	151.2E6	250.5E6	48.500	48.945
28)	SA Decachlor...	9.112	8.065	115.2E6	235.0E6	48.672	48.418
Target Compounds							
23)	Chlordane-1	4.737	3.900	87024542	95398411	480.817	482.644
24)	Chlordane-2	5.264	4.481	92055177	105.4E6	478.584	481.586
25)	Chlordane-3	5.970	5.117	353.2E6	343.6E6	484.055	493.940
26)	Chlordane-4	6.054	5.181	415.9E6	294.8E6	480.800	481.576
27)	Chlordane-5	6.895	6.078	73540042	122.8E6	486.654	477.422



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061125\
Data File : PL096016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 13:11
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL061125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 13:51:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061125.M
Quant Title : GC Extractables
QLast Update : Wed Jun 11 13:50:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

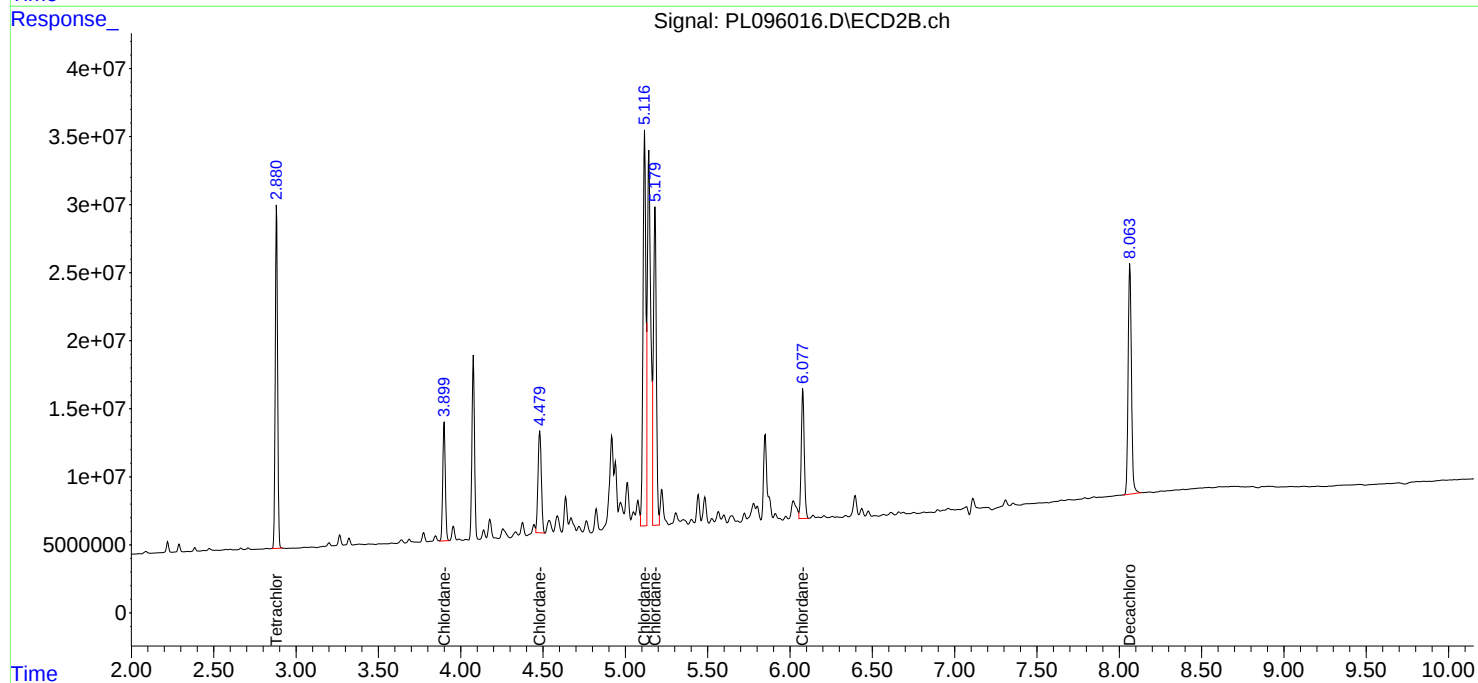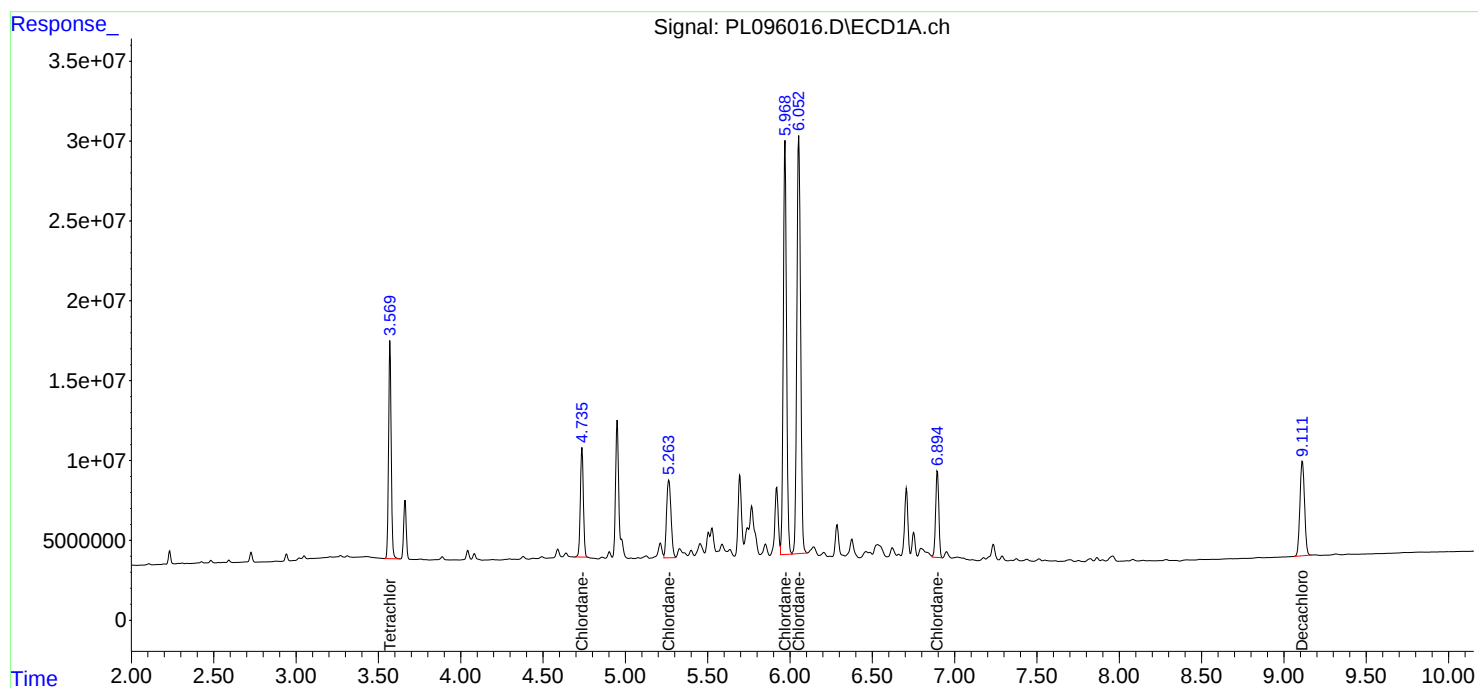


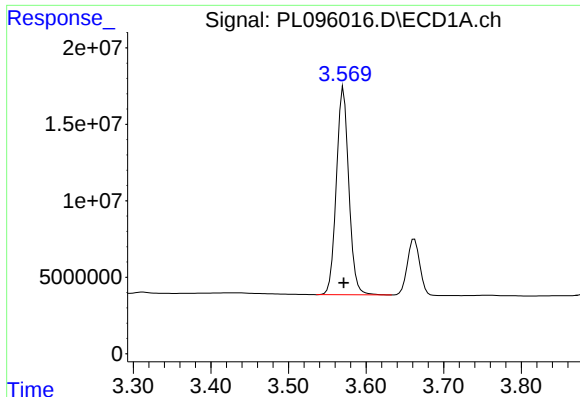

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 151163310
Conc: 48.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061125

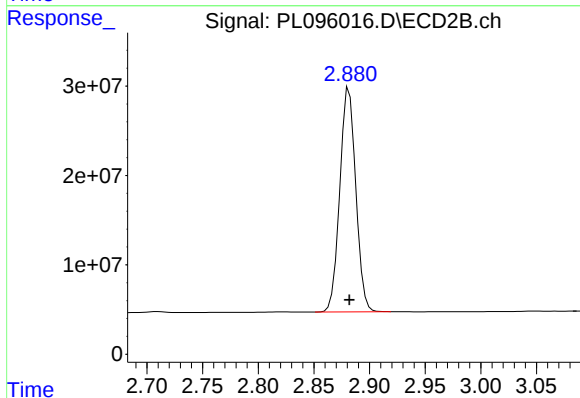


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 250463104
Conc: 48.94 ng/ml

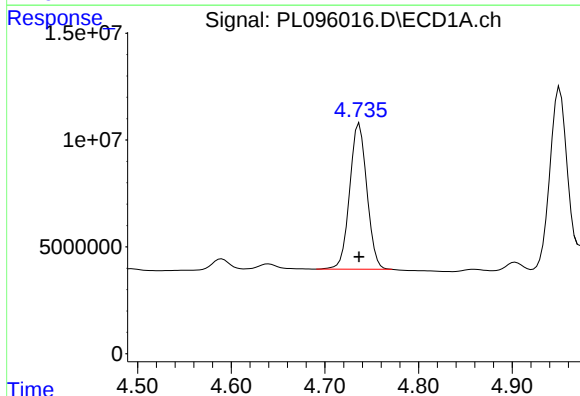


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 87024542
Conc: 480.82 ng/ml

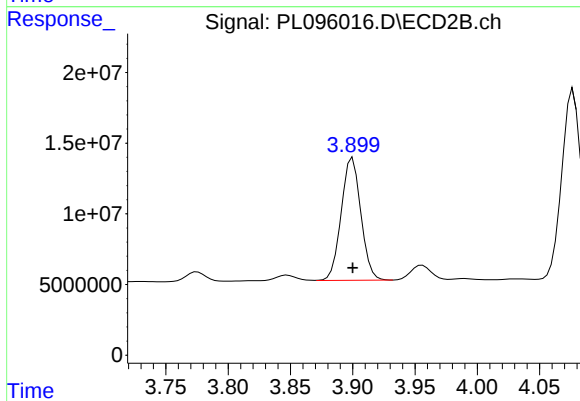

#23 Chlordane-1


R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 95398411
Conc: 482.64 ng/ml

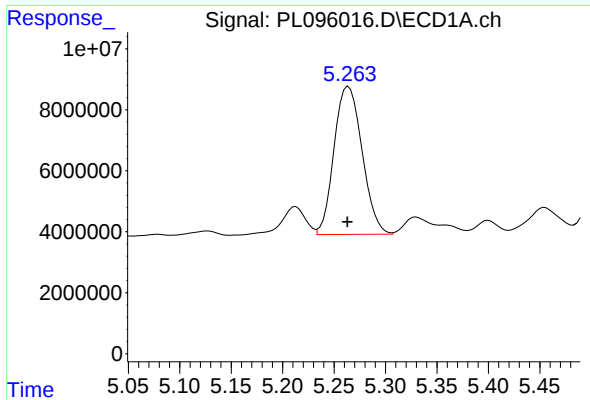

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.001 min
Response: 92055177
Conc: 478.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061125

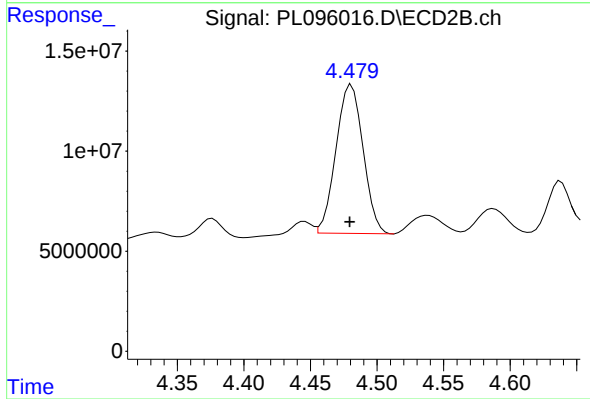


#24 Chlordane-2

R.T.: 4.481 min
Delta R.T.: 0.001 min
Response: 105396392
Conc: 481.59 ng/ml

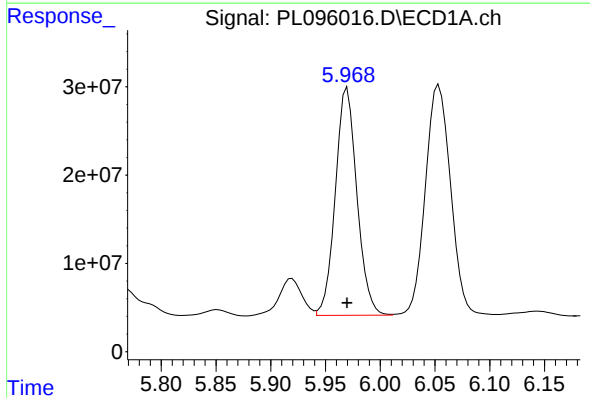


#25 Chlordane-3

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 353193482
Conc: 484.05 ng/ml

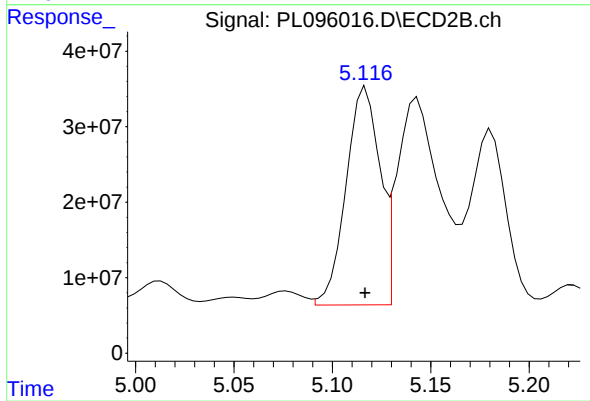

#25 Chlordane-3


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 343589876
Conc: 493.94 ng/ml

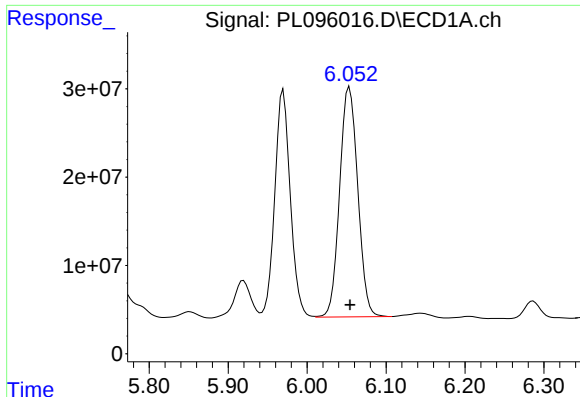

#26 Chlordane-4


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 415939530
Conc: 480.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061125

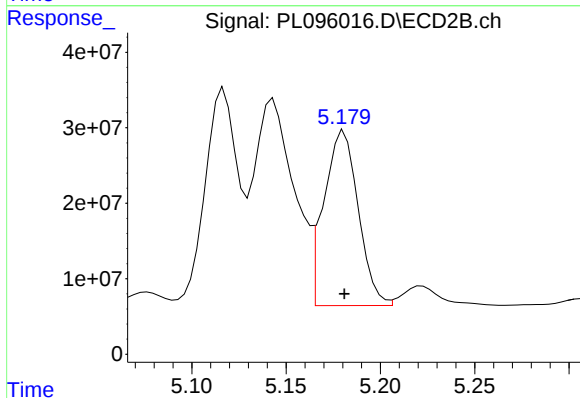


#26 Chlordane-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 294767008
Conc: 481.58 ng/ml

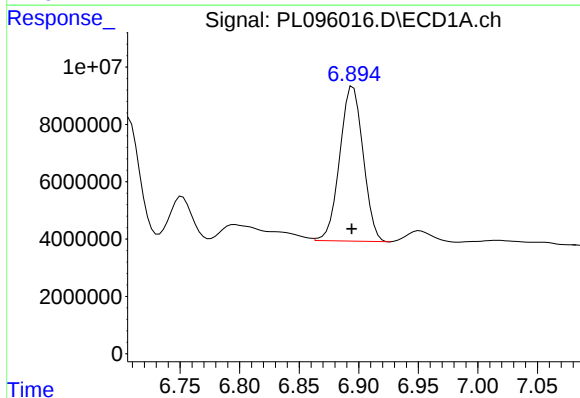


#27 Chlordane-5

R.T.: 6.895 min
Delta R.T.: 0.001 min
Response: 73540042
Conc: 486.65 ng/ml

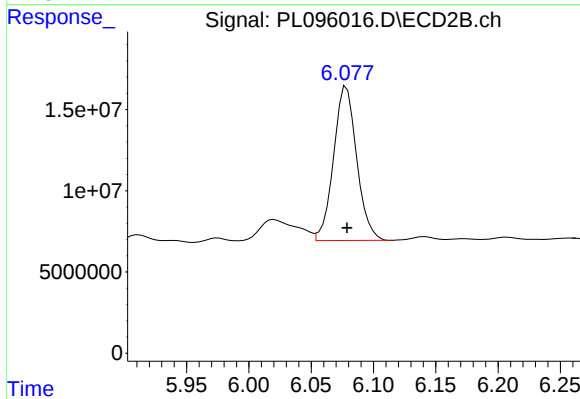

#27 Chlordane-5


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 122807630
Conc: 477.42 ng/ml

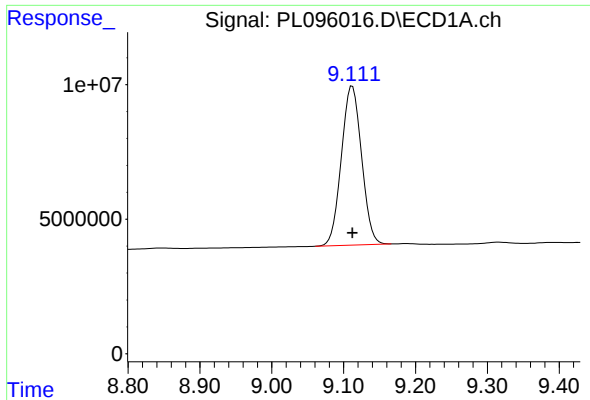

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 115214881
Conc: 48.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL061125

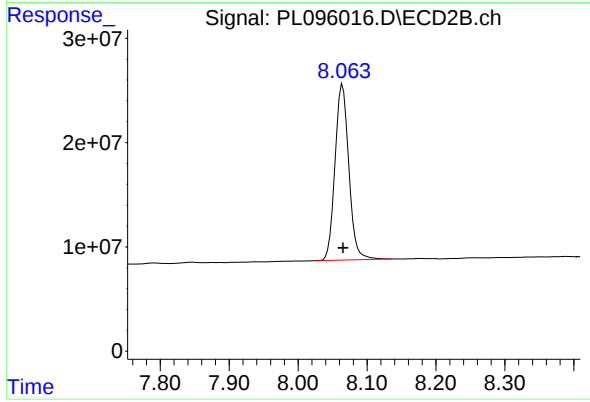

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 234951222
Conc: 48.42 ng/ml